


LB118341

7471B

INSTRUMENT ID: CV1

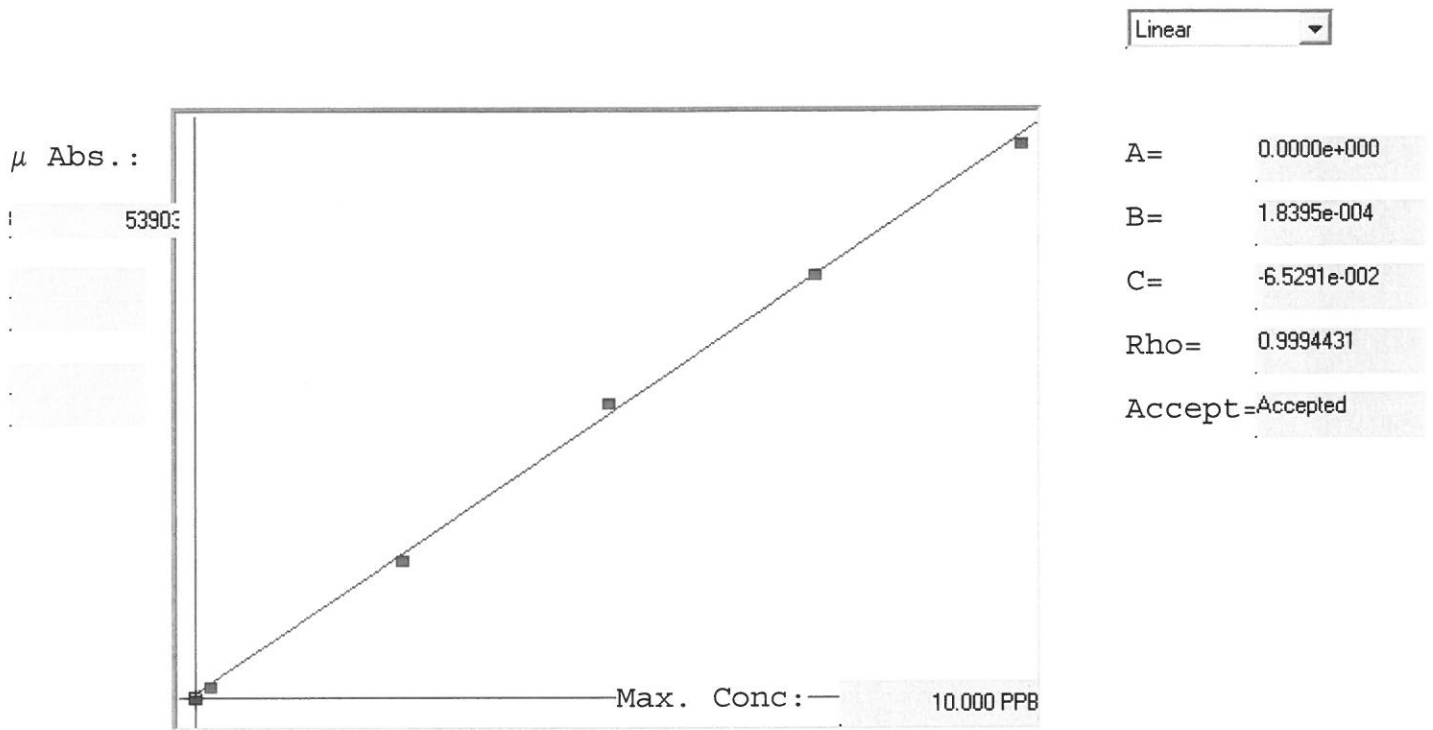

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.036	-0.036	159	0.000	159					-
0.2	0.200	0.161	-0.039	1229	0.0 %	1229					-20
2.5	2.500	2.433	-0.067	13583	0.0 %	13583					-3
5.0	5.000	5.243	0.243	28855	0.0 %	28855					5
7.5	7.500	7.549	0.049	41393	0.0 %	41393					1
10.0	10.000	9.850	-0.150	53903	0.0 %	53903					-2

LB118341 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 24 Jan 2022 11:21:06					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	159	-	0.0000	7471B	PPB	24 Jan 2022 11:27:31	S	Std
0.2 - 1	50.2	1229	-	0.2000	7471B	PPB	24 Jan 2022 11:29:48	S	Std
2.5 - 1	52.5	13583	-	2.5000	7471B	PPB	24 Jan 2022 11:32:05	S	Std
5.0 - 1	55	28855	-	5.0000	7471B	PPB	24 Jan 2022 11:34:22	S	Std
7.5 - 1	57.5	41393	-	7.5000	7471B	PPB	24 Jan 2022 11:36:39	S	Std
10.0 - 1	510	53903	-	10.0000	7471B	PPB	24 Jan 2022 11:44:03	S	Std
ICV55 - 1	ICV55	21316	3.8558	-	7471B	PPB	24 Jan 2022 11:50:04	U	SMPL
ICB55 - 1	ICB55	108	-0.0454	-	7471B	PPB	24 Jan 2022 11:52:19	U	SMPL
CCV48 - 1	CCV48	26816	4.8676	-	7471B	PPB	24 Jan 2022 11:54:33	U	SMPL
CCB48 - 1	CCB48	99	-0.0471	-	7471B	PPB	24 Jan 2022 11:56:49	U	SMPL
CRA - 1	CRA	1136	0.1437	-	7471B	PPB	24 Jan 2022 12:01:42	U	SMPL
HighStd - 1	HighStd	52446	9.5822	-	7471B	PPB	24 Jan 2022 12:03:57	U	SMPL
ChkStd - 1	ChkStd	35568	6.4775	-	7471B	PPB	24 Jan 2022 12:06:13	U	SMPL
PB142216BL - 1	PBS	46	-0.0568	-	7471B	PPB	24 Jan 2022 12:08:30	U	SMPL
PB142216BS - 1	LCSS	21153	3.8258	-	7471B	PPB	24 Jan 2022 12:15:10	U	SMPL
N1210-01 - 1	20220027-KEANSBURG-1-COMPOSITE	8466	1.4920	-	7471B	PPB	24 Jan 2022 12:17:26	U	SMPL
N1214-01 - 1	EO-02-012022	1040	0.1260	-	7471B	PPB	24 Jan 2022 12:19:42	U	SMPL
N1217-06 - 1	72-72017	12902	2.3081	-	7471B	PPB	24 Jan 2022 12:21:59	U	SMPL
N1217-08 - 1	VNJ-242	258	-0.0178	-	7471B	PPB	24 Jan 2022 12:24:16	U	SMPL
N1218-01 - 1	EAST-BOILER-PIT-WASTE-CLASS	96049	17.6031	-	7471B	PPB	24 Jan 2022 12:26:32	U	SMPL
CCV49 - 1	CCV49	26042	4.7252	-	7471B	PPB	24 Jan 2022 12:28:47	U	SMPL
CCB49 - 1	CCB49	39	-0.0581	-	7471B	PPB	24 Jan 2022 12:31:06	U	SMPL
N1224-07 - 1	AREA-2-COMPOSITE	1782	0.2625	-	7471B	PPB	24 Jan 2022 12:33:22	U	SMPL
N1224-07DUP - 1	AREA-2-COMPOSITEDUP	2004	0.3033	-	7471B	PPB	24 Jan 2022 12:38:12	U	SMPL
N1224-07MS - 1	AREA-2-COMPOSITEMS	21366	3.8650	-	7471B	PPB	24 Jan 2022 12:42:57	U	SMPL
N1224-07MSD - 1	AREA-2-COMPOSITMSD	22727	4.1154	-	7471B	PPB	24 Jan 2022 12:45:12	U	SMPL
N1224-15 - 1	AREA-1-COMPOSITE	1881	0.2807	-	7471B	PPB	24 Jan 2022 12:47:29	U	SMPL
N1224-07LX5 - 1		504	0.0274	-	7471B	PPB	24 Jan 2022 12:49:45	U	SMPL
N1224-07A - 1		22933	4.1533	-	7471B	PPB	24 Jan 2022 12:52:02	U	SMPL
M1218-01DLX5 - 1		21302	3.8533	-	7471B	PPB	24 Jan 2022 12:54:19	U	SMPL
CCV50 - 1	CCV50	25827	4.6856	-	7471B	PPB	24 Jan 2022 12:56:36	U	SMPL
CCB50 - 1	CCB50	90	-0.0487	-	7471B	PPB	24 Jan 2022 12:58:52	U	SMPL