

=====

213118413
=====

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

1/27/2022 16:25
=====

Test: Total CN

Sample Id	Result ^{mg/L}	Dil. 1 +	Response	Errors
ICV1	93.088	0.0	0.077	
ICB1	0.535	0.0	0.001	
CCV1	236.753	0.0	0.195	
CCB1	0.490	0.0	0.001	
PB142311BL	0.458	0.0	0.001	
PB142311BS	94.610	0.0	0.078	
MIDPB142311	240.016	0.0	0.197	96% (90-110)
N1202-01	2.071	0.0	0.003	
N1287-03	2.608	0.0	0.003	
N1287-03DUP	2.459	0.0	0.003	12 01/27/22
N1287-03MS	30.910	0.0	0.026	
N1287-03MSD	30.770	0.0	0.026	
CCV2	244.515	0.0	0.201	
CCB2	0.426	0.0	0.001	
N1287-03A	39.715	0.0	0.033	
CCV3	250.886	0.0	0.206	
CCB3	0.158	0.0	0.001	

N	17
Mean	74.733
SD	100.7964
CV%	134.87

Aquakem v. 7.2AQ1

Results from time period:

Thu Jan 27 15:47:23 2022

Thu Jan 27 16:17:41 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.3433	µg/l	1/27/2022 11:34:19	
5.OPPBCN	A	Total CN	P	4.8375	µg/l	1/27/2022 11:34:20	
10PPBCN	A	Total CN	P	9.9089	µg/l	1/27/2022 11:34:21	
50PPBCN	A	Total CN	P	49.7237	µg/l	1/27/2022 11:34:22	
100PPBCN	A	Total CN	P	99.3896	µg/l	1/27/2022 11:34:23	
250PPBCN	A	Total CN	P	251.2876	µg/l	1/27/2022 11:34:24	
500PPBCN	A	Total CN	P	499.5093	µg/l	1/27/2022 11:34:25	
ICV1	S	Total CN	P	93.0877	µg/l	1/27/2022 15:47:23	
ICB1	S	Total CN	P	0.5353	µg/l	1/27/2022 15:47:24	
CCV1	S	Total CN	P	236.7529	µg/l	1/27/2022 15:47:25	
CCB1	S	Total CN	P	0.4903	µg/l	1/27/2022 15:47:26	
PB142311BL	S	Total CN	P	0.4577	µg/l	1/27/2022 15:47:27	
PB142311BS	S	Total CN	P	94.6095	µg/l	1/27/2022 15:47:28	
MIDPB142311	S	Total CN	P	240.0155	µg/l	1/27/2022 15:47:29	
N1202-01	S	Total CN	P	2.0709	µg/l	1/27/2022 15:47:30	
N1287-03	S	Total CN	P	2.6076	µg/l	1/27/2022 15:47:31	
N1287-03DUP	S	Total CN	P	2.4591	µg/l	1/27/2022 15:47:32	
N1287-03MS	S	Total CN	P	30.9097	µg/l	1/27/2022 15:47:33	
N1287-03MSD	S	Total CN	P	30.7702	µg/l	1/27/2022 15:54:06	
CCV2	S	Total CN	P	244.5151	µg/l	1/27/2022 15:54:09	
CCB2	S	Total CN	P	0.4258	µg/l	1/27/2022 15:54:10	
N1287-03A	S	Total CN	P	39.715	µg/l	1/27/2022 16:17:36	
CCV3	S	Total CN	P	250.886	µg/l	1/27/2022 16:17:39	
CCB3	S	Total CN	P	0.1583	µg/l	1/27/2022 16:17:41	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

1/27/2022 11:38


Test Total CN

Accepted 1/27/2022 11:38

Factor 1222
Bias 0.001

Coeff. of det. 0.999988

Errors

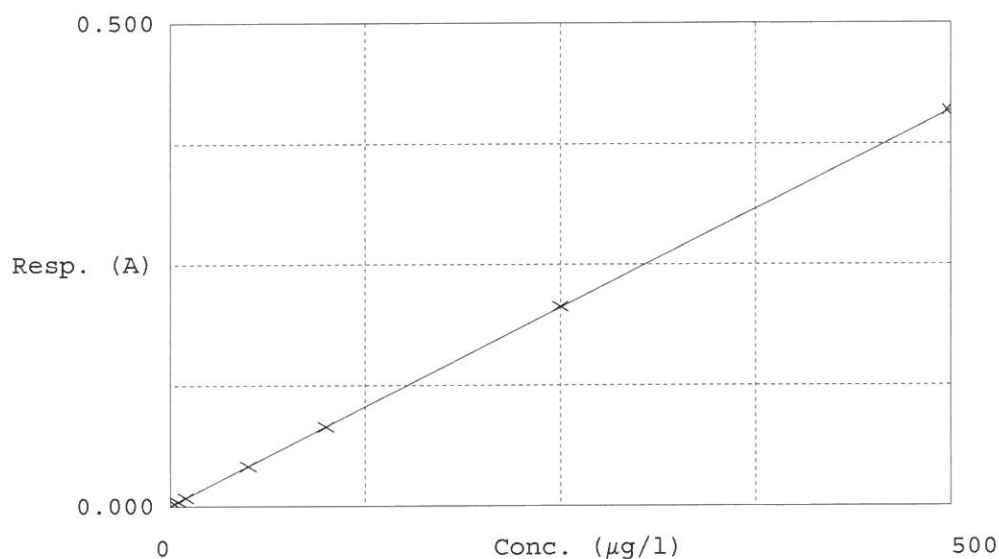

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.3433	0.0000	—
2	5.0PPBCN	0.005	4.8375	5.0000	-3.2
3	10PPBCN	0.009	9.9089	10.0000	-0.9
4	50PPBCN	0.042	49.7237	50.0000	-0.6
5	100PPBCN	0.082	99.3896	100.0000	-0.6
6	250PPBCN	0.206	251.2876	250.0000	0.5
7	500PPBCN	0.410	499.5093	500.0000	-0.1

01/27/22