

LB118432

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

1/28/2022 16:00

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.070	0.0	0.078	
ICB1	1.190	0.0	0.001	
CCV1	240.157	0.0	0.198	
CCB1	1.290	0.0	0.001	
PB142362BL	1.183	0.0	0.001	
PB142362BS	95.052	0.0	0.078	
LOWPB142362	10.100	0.0	0.008	
HIGHPB142362	478.935	0.0	0.394	
N1303-01	4.312	0.0	0.004	
N1303-01DUP	4.207	0.0	0.004	
N1303-01MS	35.848	0.0	0.030	
N1303-01MSD	35.557	0.0	0.029	
N1303-03	5.033	0.0	0.004	
N1303-05	0.876	0.0	0.001	
CCV2	238.737	0.0	0.196	
CCB2	1.105	0.0	0.001	
N1303-07	1.152	0.0	0.001	
N1303-09	0.666	0.0	0.001	
N1303-11	0.902	0.0	0.001	
N1313-01	2.179	0.0	0.002	
CCV3	246.811	0.0	0.203	
CCB3	1.557	0.0	0.001	

N	23
Mean	67.103
SD	121.3412
CV%	180.83

Aquakem v. 7.2AQ1

Results from time period:

Fri Jan 28 15:44:07 2022

Fri Jan 28 15:58:00 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.9843	µg/l	1/28/2022 10:50:27	
5.0PPBCN	A	Total CN	P	5.2505	µg/l	1/28/2022 10:50:28	
10PPBCN	A	Total CN	P	10.026	µg/l	1/28/2022 10:50:29	
50PPBCN	A	Total CN	P	49.1775	µg/l	1/28/2022 10:50:30	
100PPBCN	A	Total CN	P	99.154	µg/l	1/28/2022 10:50:31	
250PPBCN	A	Total CN	P	250.3185	µg/l	1/28/2022 10:50:32	
500PPBCN	A	Total CN	P	500.0892	µg/l	1/28/2022 10:50:33	
ICV1	S	Total CN	P	95.0699	µg/l	1/28/2022 15:44:08	
ICB1	S	Total CN	P	1.1898	µg/l	1/28/2022 15:44:09	
CCV1	S	Total CN	P	240.1565	µg/l	1/28/2022 15:44:11	
CCB1	S	Total CN	P	1.29	µg/l	1/28/2022 15:44:14	
PB142362BL	S	Total CN	P	1.1834	µg/l	1/28/2022 15:44:15	
PB142362BS	S	Total CN	P	95.0522	µg/l	1/28/2022 15:44:16	
LOWPB142362	S	Total CN	P	10.0998	µg/l	1/28/2022 15:44:17	
HIGHPB142362	S	Total CN	P	478.935	µg/l	1/28/2022 15:51:43	
N1303-01	S	Total CN	P	4.3118	µg/l	1/28/2022 15:51:44	
N1303-01DUP	S	Total CN	P	4.2073	µg/l	1/28/2022 15:51:45	
N1303-01MS	S	Total CN	P	35.8481	µg/l	1/28/2022 15:51:48	
N1303-01MSD	S	Total CN	P	35.5572	µg/l	1/28/2022 15:51:49	
N1303-03	S	Total CN	P	5.0327	µg/l	1/28/2022 15:51:50	
N1303-05	S	Total CN	P	0.8761	µg/l	1/28/2022 15:51:51	
CCV2	S	Total CN	P	238.7372	µg/l	1/28/2022 15:51:52	
CCB2	S	Total CN	P	1.1046	µg/l	1/28/2022 15:57:53	
N1303-07	S	Total CN	P	1.1524	µg/l	1/28/2022 15:57:54	
N1303-09	S	Total CN	P	0.6662	µg/l	1/28/2022 15:57:55	
N1303-11	S	Total CN	P	0.9017	µg/l	1/28/2022 15:57:56	
N1313-01	S	Total CN	P	2.1787	µg/l	1/28/2022 15:57:57	
CCV3	S	Total CN	P	246.8113	µg/l	1/28/2022 15:57:58	
CCB3	S	Total CN	P	1.5569	µg/l	1/28/2022 15:57:59	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

1/28/2022 10:57

Test Total CN


Accepted 1/28/2022 10:57

Factor 1217

Bias 0

Coeff. of det. 0.999988

Errors

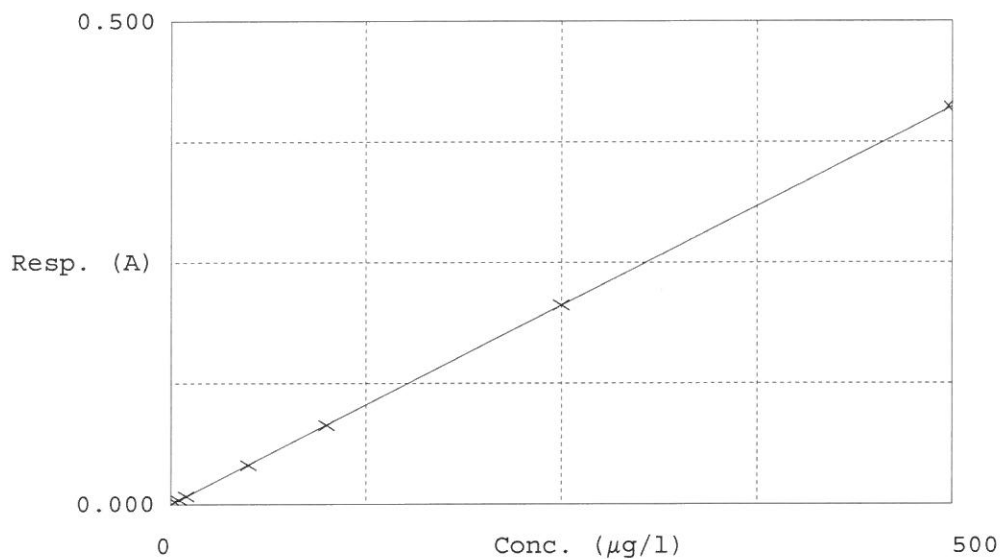

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.9843	0.0000	-
2	5.0PPBCN	0.004	5.2505	5.0000	5.0
3	10PPBCN	0.008	10.0260	10.0000	0.3
4	50PPBCN	0.041	49.1775	50.0000	-1.6
5	100PPBCN	0.082	99.1540	100.0000	-0.8
6	250PPBCN	0.206	250.3185	250.0000	0.1
7	500PPBCN	0.411	500.0892	500.0000	0.0

12 01/28/22