

LB118451


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

38332

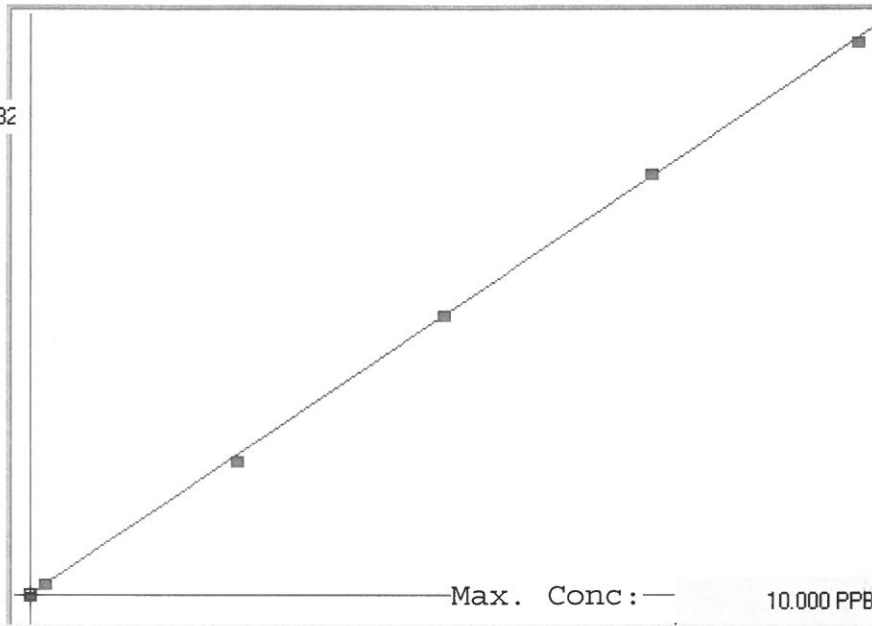

A= 0.0000e+000

B= 2.5940e-004

C= -4.7961e-003

Rho= 0.9998992

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	90D
0.0	0.000	0.009	0.009	53	0.000	53					-
0.2	0.200	0.205	0.005	810	0.0 %	810					2
2.5	2.500	2.428	-0.072	9380	0.0 %	9380					-3
5.0	5.000	5.046	0.046	19471	0.0 %	19471					1
7.5	7.500	7.573	0.073	29213	0.0 %	29213					1
10.0	10.000	9.938	-0.062	38332	0.0 %	38332					-1

LB118451 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 31 Jan 2022 10:54:23

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	53	-	0.0000	7470A	PPB	31 Jan 2022 11:03:08	S	Std
0.2 - 1	50.2	810	-	0.2000	7470A	PPB	31 Jan 2022 11:05:25	S	Std
2.5 - 1	52.5	9380	-	2.5000	7470A	PPB	31 Jan 2022 11:07:42	S	Std
5.0 - 1	55	19471	-	5.0000	7470A	PPB	31 Jan 2022 11:09:59	S	Std
7.5 - 1	57.5	29213	-	7.5000	7470A	PPB	31 Jan 2022 11:12:16	S	Std
10.0 - 1	510	38332	-	10.0000	7470A	PPB	31 Jan 2022 11:17:11	S	Std
ICV66 - 1	ICV66	14497	3.7557	-	7470A	PPB	31 Jan 2022 11:19:56	U	SMPL
ICB66 - 1	ICB66	17	-0.0004	-	7470A	PPB	31 Jan 2022 11:22:10	U	SMPL
CCV89 - 1	CCV89	18508	4.7961	-	7470A	PPB	31 Jan 2022 11:24:25	U	SMPL
CCB89 - 1	CCB89	14	-0.0012	-	7470A	PPB	31 Jan 2022 11:26:41	U	SMPL
CRA - 1	CRA	836	0.2121	-	7470A	PPB	31 Jan 2022 11:28:56	U	SMPL
HighStd - 1	HighStd	38177	9.8982	-	7470A	PPB	31 Jan 2022 11:31:11	U	SMPL
ChkStd - 1	ChkStd	26578	6.8895	-	7470A	PPB	31 Jan 2022 11:33:26	U	SMPL
PB142360BL - 1	PBW	-31	-0.0128	-	7470A	PPB	31 Jan 2022 11:35:43	U	SMPL
PB142360BS - 1	LCSW	13877	3.5949	-	7470A	PPB	31 Jan 2022 11:38:00	U	SMPL
N1282-06 - 1	B-3-COMPOSITE	20	0.0004	-	7470A	PPB	31 Jan 2022 11:40:16	U	SMPL
N1284-02 - 1	S-1	62	0.0113	-	7470A	PPB	31 Jan 2022 11:42:32	U	SMPL
N1287-02 - 1	WASTE-CHARACTER	56	0.0097	-	7470A	PPB	31 Jan 2022 11:44:49	U	SMPL
N1303-02 - 1	CC-5	115	0.0250	-	7470A	PPB	31 Jan 2022 11:47:06	U	SMPL
N1303-04 - 1	CC-6	484	0.1208	-	7470A	PPB	31 Jan 2022 11:49:21	U	SMPL
CCV90 - 1	CCV90	18621	4.8255	-	7470A	PPB	31 Jan 2022 11:51:37	U	SMPL
CCB90 - 1	CCB90	-47	-0.0170	-	7470A	PPB	31 Jan 2022 11:53:52	U	SMPL
N1303-06 - 1	CC-7	479	0.1195	-	7470A	PPB	31 Jan 2022 11:56:08	U	SMPL
N1303-08 - 1	CC-8	75	0.0147	-	7470A	PPB	31 Jan 2022 11:58:24	U	SMPL
N1303-10 - 1	CC-9	932	0.2370	-	7470A	PPB	31 Jan 2022 12:00:40	U	SMPL
N1313-02 - 1	17B-MISC-A	66	0.0123	-	7470A	PPB	31 Jan 2022 12:02:56	U	SMPL
N1319-02 - 1	MH-1S	66	0.0123	-	7470A	PPB	31 Jan 2022 12:05:12	U	SMPL
N1319-05 - 1	MH-1D	63	0.0115	-	7470A	PPB	31 Jan 2022 12:07:28	U	SMPL
N1319-08 - 1	MH-2S	56	0.0097	-	7470A	PPB	31 Jan 2022 12:09:45	U	SMPL
N1319-11 - 1	MH-2D	52	0.0087	-	7470A	PPB	31 Jan 2022 12:12:01	U	SMPL
N1319-11DUP - 1	MH-2DDUP	56	0.0097	-	7470A	PPB	31 Jan 2022 12:14:20	U	SMPL
N1319-11MS - 1	MH-2DMS	13811	3.5777	-	7470A	PPB	31 Jan 2022 12:16:35	U	SMPL
CCV91 - 1	CCV91	18969	4.9157	-	7470A	PPB	31 Jan 2022 12:18:51	U	SMPL
CCB91 - 1	CCB91	-13	-0.0082	-	7470A	PPB	31 Jan 2022 12:21:06	U	SMPL
N1319-11MSD - 1	MH-2DMSD	13892	3.5988	-	7470A	PPB	31 Jan 2022 12:23:22	U	SMPL
PB142361BL - 1	PBW	-5	-0.0061	-	7470A	PPB	31 Jan 2022 12:25:37	U	SMPL
PB142361BS - 1	LCSW	13828	3.5822	-	7470A	PPB	31 Jan 2022 12:27:53	U	SMPL
N1245-15 - 1	FB	12	-0.0017	-	7470A	PPB	31 Jan 2022 12:30:10	U	SMPL
PB142315TB - 1	PB142315TB	38	0.0051	-	7470A	PPB	31 Jan 2022 12:32:26	U	SMPL
N1319-11LX5 - 1		-3	-0.0056	-	7470A	PPB	31 Jan 2022 12:36:53	U	SMPL
N1319-11A - 1		14052	3.6403	-	7470A	PPB	31 Jan 2022 12:39:09	U	SMPL
CCV92 - 1	CCV92	18924	4.9040	-	7470A	PPB	31 Jan 2022 12:41:26	U	SMPL
CCB92 - 1	CCB92	-7	-0.0066	-	7470A	PPB	31 Jan 2022 12:43:43	U	SMPL