

LB 118457

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

1/31/2022 16:02

Test: Phenolics-

Sample Id	<i>mp/l</i> Result	Dil. 1 +	Response	Errors
ICV1	0.914	0.0	0.106	
ICB1	0.013	0.0	0.005	
CCV1	0.984	0.0	0.114	
CCB1	0.012	0.0	0.005	
PB142332BL	0.013	0.0	0.005	
N1202-01	0.358	0.0	0.044	
N1202-01DUP	0.356	0.0	0.043	
N1202-01MS	1.294	0.0	0.149	
N1202-01MSD	1.318	0.0	0.152	
N1301-01	0.047	0.0	0.009	
PB142332BS	0.972	0.0	0.113	
CCV2	0.982	0.0	0.114	
CCB2	0.011	0.0	0.005	

N 13
Mean 0.560
SD 0.5252
CV% 93.87

Aquakem v. 7.2AQ1

Results from time period:

Mon Jan 31 14:47:53 2022

Mon Jan 31 15:54:03 2022

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0127	mg/l	1/31/2022 14:47:53	
0.05PPM	A	Phenolics-	P	0.0601	mg/l	1/31/2022 14:47:54	
0.1PPM	A	Phenolics-	P	0.1099	mg/l	1/31/2022 14:47:55	
0.25PPM	A	Phenolics-	P	0.2557	mg/l	1/31/2022 14:47:56	
0.50PPM	A	Phenolics-	P	0.4884	mg/l	1/31/2022 14:47:57	
1.0PPM	A	Phenolics-	P	0.9435	mg/l	1/31/2022 14:47:58	
2.0PPM	A	Phenolics-	P	2.0297	mg/l	1/31/2022 14:47:59	
ICV1	S	Phenolics-	P	0.9137	mg/l	1/31/2022 15:11:01	
ICB1	S	Phenolics-	P	0.0125	mg/l	1/31/2022 15:11:03	
CCV1	S	Phenolics-	P	0.9843	mg/l	1/31/2022 15:11:05	
CCB1	S	Phenolics-	P	0.0124	mg/l	1/31/2022 15:11:06	
PB142332BL	S	Phenolics-	P	0.0129	mg/l	1/31/2022 15:11:08	
N1202-01	S	Phenolics-	P	0.3581	mg/l	1/31/2022 15:11:10	
N1202-01DUP	S	Phenolics-	P	0.3564	mg/l	1/31/2022 15:11:11	
N1202-01MS	S	Phenolics-	P	1.2945	mg/l	1/31/2022 15:16:22	
N1202-01MSD	S	Phenolics-	P	1.3176	mg/l	1/31/2022 15:16:23	
N1301-01	S	Phenolics-	P	0.0473	mg/l	1/31/2022 15:16:24	
PB142332BS	S	Phenolics-	P	0.9716	mg/l	1/31/2022 15:32:56	
CCV2	S	Phenolics-	P	0.9815	mg/l	1/31/2022 15:32:58	
CCB2	S	Phenolics-	P	0.0114	mg/l	1/31/2022 15:32:59	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

1/31/2022 14:49


Test Phenolics-

Accepted 1/31/2022 14:49

Factor 8.872
Bias 0.003

Coeff. of det. 0.998544

Errors

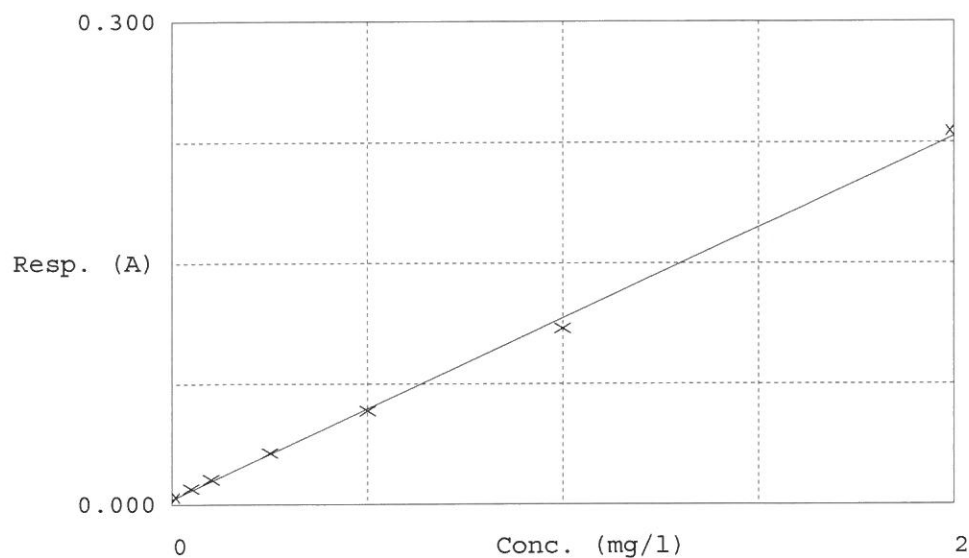

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.005	0.0127	0.0000	-
2	Phenol-2	0.010	0.0601	0.0500	20.2
3	Phenol-2	0.016	0.1099	0.1000	9.9
4	Phenol-2	0.032	0.2557	0.2500	2.3
5	Phenol-2	0.058	0.4884	0.5000	-2.3
6	Phenol-2	0.110	0.9435	1.0000	-5.7
7	Phenol-2	0.232	2.0297	2.0000	1.5

12

01/31/22