


LB112497

7471B

INSTRUMENT ID: CV2

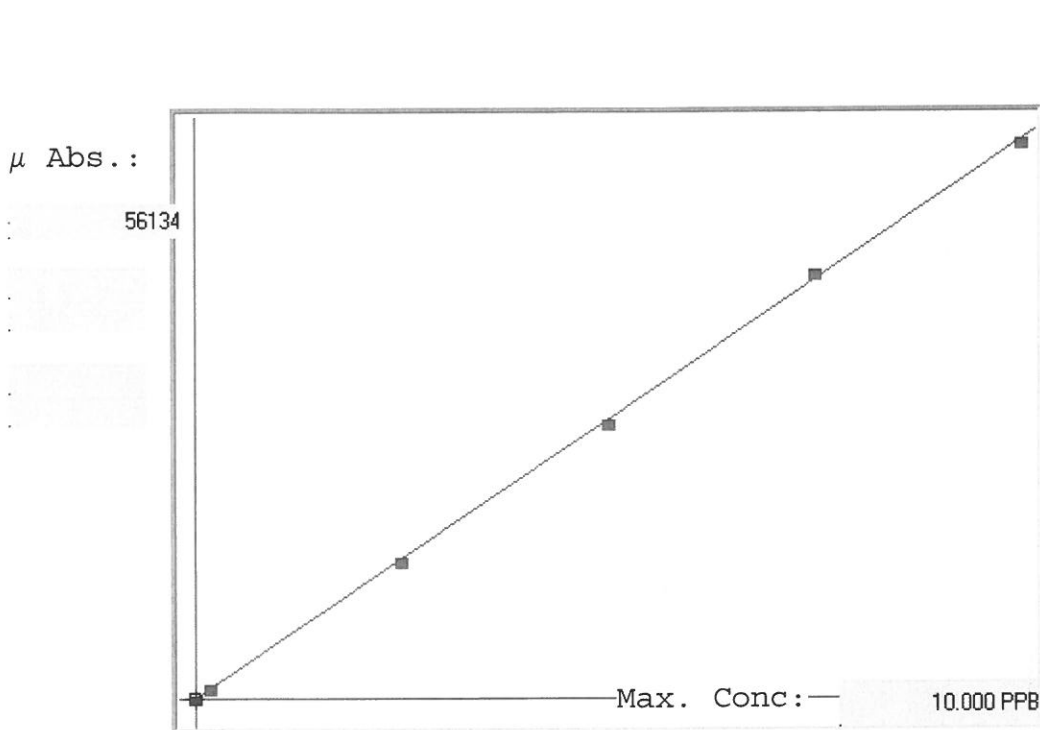

Linear

A= 0.0000e+000

B= 1.7690e-004

C= 8.4752e-003

Rho= 0.9998753

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.016	0.016	45	0.000	45					-
0.2	0.200	0.194	-0.006	1051	0.0 %	1051					-3
2.5	2.500	2.480	-0.020	13973	0.0 %	13973					-1
5.0	5.000	4.953	-0.047	27952	0.0 %	27952					-1
7.5	7.500	7.617	0.117	43011	0.0 %	43011					2
10.0	10.000	9.939	-0.061	56134	0.0 %	56134					-1

LB118497 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 02 Feb 2022 15:42:57

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	45	-	0.0000	7471B	PPB	02 Feb 2022 15:43:59	S	Std
0.2 - 1	50.2	1051	-	0.2000	7471B	PPB	02 Feb 2022 15:46:16	S	Std
2.5 - 1	52.5	13973	-	2.5000	7471B	PPB	02 Feb 2022 15:48:33	S	Std
5.0 - 1	55	27952	-	5.0000	7471B	PPB	02 Feb 2022 15:50:50	S	Std
7.5 - 1	57.5	43011	-	7.5000	7471B	PPB	02 Feb 2022 15:53:07	S	Std
10.0 - 1	510	56134	-	10.0000	7471B	PPB	02 Feb 2022 16:00:28	S	Std
ICV70 - 1	ICV70	20886	3.7032	-	7471B	PPB	02 Feb 2022 16:03:06	U	SMPL
ICB70 - 1	ICB70	-25	0.0041	-	7471B	PPB	02 Feb 2022 16:05:21	U	SMPL
CCV11 - 1	CCV11	26369	4.6731	-	7471B	PPB	02 Feb 2022 16:07:36	U	SMPL
CCB11 - 1	CCB11	-30	0.0032	-	7471B	PPB	02 Feb 2022 16:09:51	U	SMPL
CRA - 1	CRA	978	0.1815	-	7471B	PPB	02 Feb 2022 16:12:08	U	SMPL
HighStd - 1	HighStd	57529	10.1853	-	7471B	PPB	02 Feb 2022 16:14:23	U	SMPL
ChkStd - 1	ChkStd	38453	6.8108	-	7471B	PPB	02 Feb 2022 16:16:39	U	SMPL
PB142447BL - 1	PBS	-67	-0.0034	-	7471B	PPB	02 Feb 2022 16:18:56	U	SMPL
PB142447BS - 1	LCSS	20809	3.6896	-	7471B	PPB	02 Feb 2022 16:21:13	U	SMPL
N1356-01 - 1	F-PHC	39272	6.9557	-	7471B	PPB	02 Feb 2022 16:23:29	U	SMPL
N1356-01DUP - 1	F-PHCDUP	38856	6.8821	-	7471B	PPB	02 Feb 2022 16:25:46	U	SMPL
N1356-01MS - 1	F-PHCMS	40211	7.1218	-	7471B	PPB	02 Feb 2022 16:28:03	U	SMPL
N1356-01MSD - 1	F-PHCMSD	42779	7.5761	-	7471B	PPB	02 Feb 2022 16:30:21	U	SMPL
N1356-03 - 1	M-PHC	17708	3.1410	-	7471B	PPB	02 Feb 2022 16:32:37	U	SMPL
CCV12 - 1	CCV12	26202	4.6436	-	7471B	PPB	02 Feb 2022 16:34:53	U	SMPL
CCB12 - 1	CCB12	-36	0.0021	-	7471B	PPB	02 Feb 2022 16:37:08	U	SMPL
N1356-05 - 1	B-PHC	8671	1.5424	-	7471B	PPB	02 Feb 2022 16:39:23	U	SMPL
N1358-01 - 1	BU-2-020122	1696	0.3085	-	7471B	PPB	02 Feb 2022 16:41:38	U	SMPL
N1356-01LX5 - 1		7244	1.2899	-	7471B	PPB	02 Feb 2022 16:43:54	U	SMPL
N1356-01A - 1		62917	11.1385	-	7471B	PPB	02 Feb 2022 16:46:10	U	SMPL
CCV13 - 1	CCV13	26416	4.6815	-	7471B	PPB	02 Feb 2022 16:48:26	U	SMPL
CCB13 - 1	CCB13	-27	0.0037	-	7471B	PPB	02 Feb 2022 16:50:44	U	SMPL