

LB 118566

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092Reviewed by : 12 Instrument ID : Konelab

2/7/2022 12:09

Test: ~~Total~~ ^{Reactive} CN

Sample Id	Result ^{mg/L}	Dil. 1 +	Response	Errors
ICV1	94.246	0.0	0.079	
ICB1	0.969	0.0	0.001	
CCV1	242.429	0.0	0.204	
CCB1	0.721	0.0	0.001	
PB142521BL	0.769	0.0	0.001	
N1400-02	0.716	0.0	0.001	
N1400-02DUP	0.724	0.0	0.001	
PB142520BL	0.559	0.0	0.001	
N1400-01	0.637	0.0	0.001	
N1400-01DUP	0.636	0.0	0.001	
N1419-02	0.803	0.0	0.001	
CCV2	246.922	0.0	0.208	
CCB2	0.653	0.0	0.001	

N	13
Mean	45.445
SD	92.0968
CV%	202.66

Aquakem v. 7.2AQ1

Results from time period:

Mon Feb 07 10:55:02 2022

Mon Feb 07 11:58:45 2022

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	REACTIVE CN P		0.8748	µg/l	2/7/2022 11:19:46	
5.0PPBCN	A	REACTIVE CN P		5.2705	µg/l	2/7/2022 11:19:47	
10PPBCN	A	REACTIVE CN P		10.3178	µg/l	2/7/2022 11:19:48	
50PPBCN	A	REACTIVE CN P		49.5178	µg/l	2/7/2022 11:19:49	
100PPBCN	A	REACTIVE CN P		100.0016	µg/l	2/7/2022 11:19:50	
250PPBCN	A	REACTIVE CN P		247.9573	µg/l	2/7/2022 11:19:51	
500PPBCN	A	REACTIVE CN P		501.0602	µg/l	2/7/2022 11:19:52	
ICV1	S	REACTIVE CN P		94.2464	µg/l	2/7/2022 11:52:28	
ICB1	S	REACTIVE CN P		0.9691	µg/l	2/7/2022 11:52:29	
CCV1	S	REACTIVE CN P		242.429	µg/l	2/7/2022 11:52:31	
CCB1	S	REACTIVE CN P		0.7213	µg/l	2/7/2022 11:52:35	
PB142521BL	S	REACTIVE CN P		0.7688	µg/l	2/7/2022 11:52:36	
N1400-02	S	REACTIVE CN P		0.7157	µg/l	2/7/2022 11:52:37	
N1400-02DUP	S	REACTIVE CN P		0.7243	µg/l	2/7/2022 11:58:38	
PB142520BL	S	REACTIVE CN P		0.559	µg/l	2/7/2022 11:58:40	
N1400-01	S	REACTIVE CN P		0.637	µg/l	2/7/2022 11:58:41	
N1400-01DUP	S	REACTIVE CN P		0.6361	µg/l	2/7/2022 11:58:42	
N1419-02	S	REACTIVE CN P		0.8029	µg/l	2/7/2022 11:58:43	
CCV2	S	REACTIVE CN P		246.9224	µg/l	2/7/2022 11:58:44	
CCB2	S	REACTIVE CN P		0.6534	µg/l	2/7/2022 11:58:45	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

2/7/2022 11:22


Test Total CN

Accepted 2/7/2022 11:22

Factor 1190
Bias 0

Coeff. of det. 0.999969

Errors

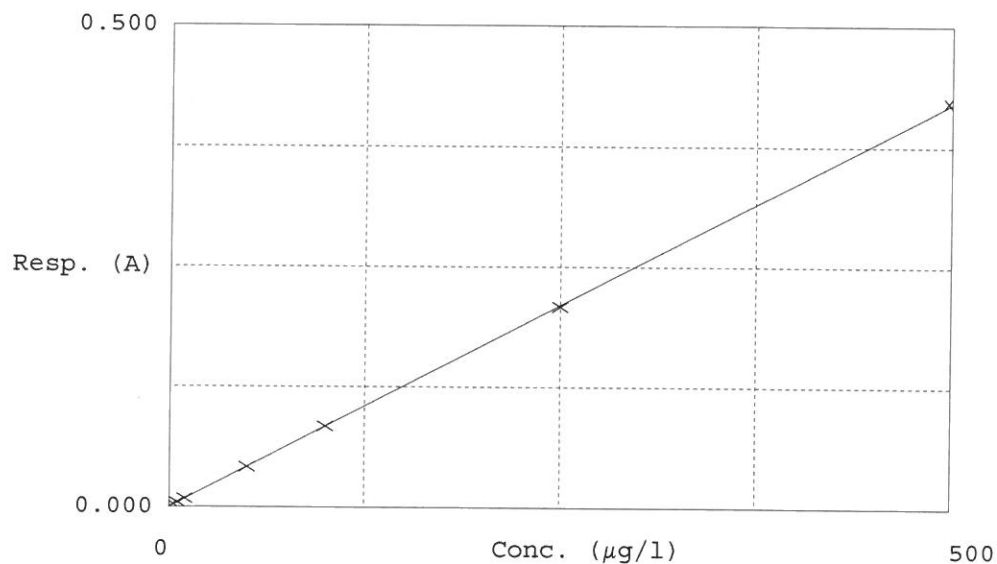

	Calibrator	Response	Calc. con.	Conc.	^{Re} Errors
1	0.0PPBCN	0.001	0.8748	0.0000	-
2	5.0PPBCN	0.005	5.2705	5.0000	5.4
3	10PPBCN	0.009	10.3178	10.0000	3.2
4	50PPBCN	0.042	49.5178	50.0000	-1.0
5	100PPBCN	0.084	100.0016	100.0000	0.0
6	250PPBCN	0.209	247.9573	250.0000	-0.8
7	500PPBCN	0.421	501.0602	500.0000	0.2

12 02/07/22