


LB11859a

7471B

INSTRUMENT ID: CV1

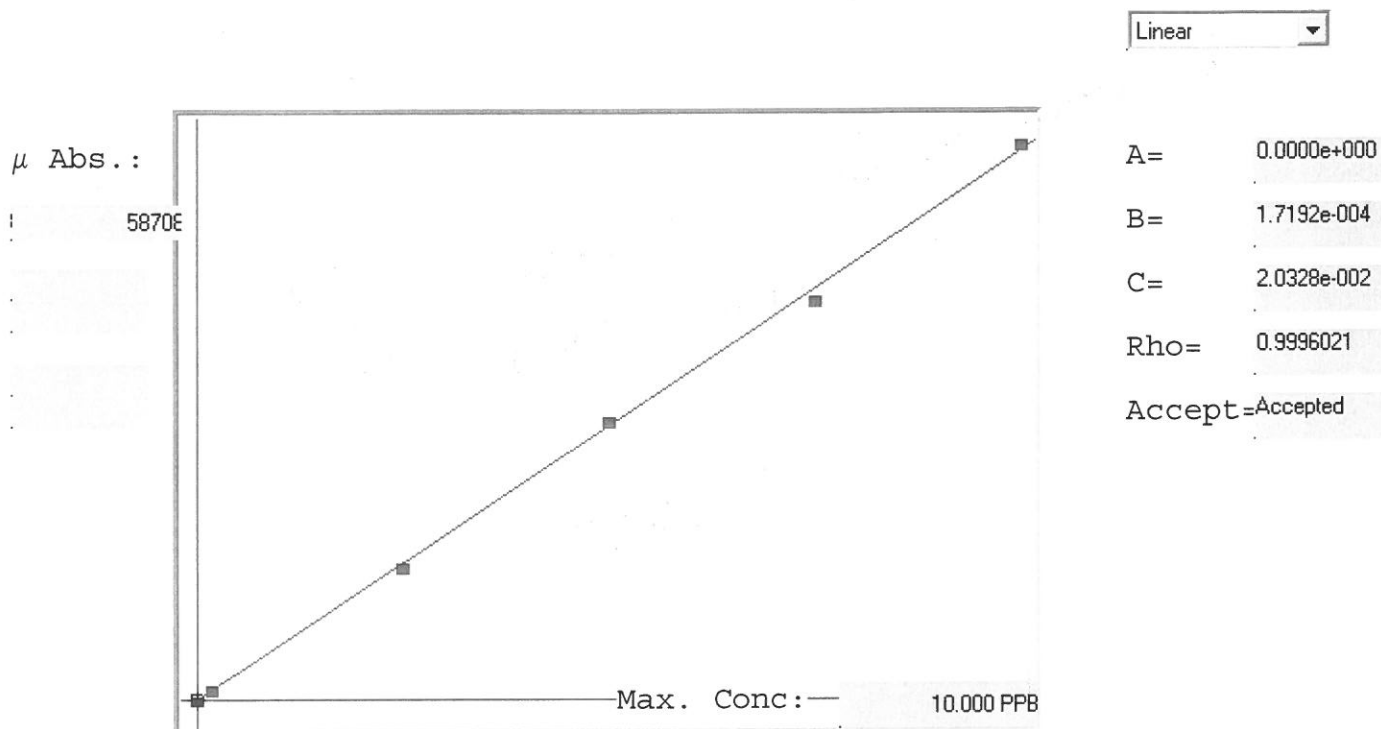

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.033	0.033	74	0.000	74				
0.2	0.200	0.210	0.010	1104	0.0 %	1104				
2.5	2.500	2.462	-0.038	14204	0.0 %	14204				
5.0	5.000	5.086	0.086	29466	0.0 %	29466				
7.5	7.500	7.295	-0.205	42313	0.0 %	42313				
10.0	10.000	10.114	0.114	58708	0.0 %	58708				

LB118590 INSTRUMENT ID:CV1

Method: 7471B

Operator: Admin

Date of Analysis: 09 Feb 2022 09:40:12

Sample ID	Extended ID	μ Abs.	Conc.	Std. Conc	Method	Units	Date	Type	Type
0.0 - 1	50	74	-	0.0000	7471B	PPB	09 Feb 2022 10:51:41	S	Std
0.2 - 1	50-2	1104	-	0.2000	7471B	PPB	09 Feb 2022 10:53:58	S	Std
2.5 - 1	52.5	14204	-	2.5000	7471B	PPB	09 Feb 2022 10:56:15	S	Std
5.0 - 1	55	29466	-	5.0000	7471B	PPB	09 Feb 2022 10:58:32	S	Std
7.5 - 1	57.5	42313	-	7.5000	7471B	PPB	09 Feb 2022 11:00:49	S	Std
10.0 - 1	510	58708	-	10.0000	7471B	PPB	09 Feb 2022 11:03:06	S	Std
ICV81 - 1	ICV81	21381	3.6962	-	7471B	PPB	09 Feb 2022 11:10:32	U	SMPL
ICB81 - 1	ICB81	-22	0.0165	-	7471B	PPB	09 Feb 2022 11:12:47	U	SMPL
CCV048 - 1	CCV048	28998	5.0057	-	7471B	PPB	09 Feb 2022 11:19:22	U	SMPL
CCB048 - 1	CCB048	-21	0.0167	-	7471B	PPB	09 Feb 2022 11:21:37	U	SMPL
CRA - 1	CRA	1088	0.2074	-	7471B	PPB	09 Feb 2022 11:23:52	U	SMPL
HighStd - 1	HighStd	56280	9.6961	-	7471B	PPB	09 Feb 2022 11:26:07	U	SMPL
ChkStd - 1	ChkStd	39462	6.8047	-	7471B	PPB	09 Feb 2022 11:28:22	U	SMPL
PB142540BL - 1	PBS	-78	0.0069	-	7471B	PPB	09 Feb 2022 11:30:40	U	SMPL
PB142540BS - 1	LCSS	21523	3.7206	-	7471B	PPB	09 Feb 2022 11:37:59	U	SMPL
N1422-01 - 1	BP-2	10483	1.8226	-	7471B	PPB	09 Feb 2022 11:40:15	U	SMPL
N1423-02 - 1	TP-21	812	0.1599	-	7471B	PPB	09 Feb 2022 11:42:32	U	SMPL
N1423-02DUP - 1	TP-21DUP	803	0.1584	-	7471B	PPB	09 Feb 2022 11:44:49	U	SMPL
CCV049 - 1	CCV049	28658	4.9473	-	7471B	PPB	09 Feb 2022 11:51:36	U	SMPL
CCB049 - 1	CCB049	-46	0.0124	-	7471B	PPB	09 Feb 2022 11:53:51	U	SMPL
N1423-04 - 1	TP-22	940	0.1819	-	7471B	PPB	09 Feb 2022 11:56:07	U	SMPL
N1423-06 - 1	TP-23	1223	0.2306	-	7471B	PPB	09 Feb 2022 11:58:22	U	SMPL
N1423-08 - 1	TP-24	737	0.1470	-	7471B	PPB	09 Feb 2022 12:00:38	U	SMPL
N1423-10 - 1	TP-25	660	0.1338	-	7471B	PPB	09 Feb 2022 12:02:54	U	SMPL
N1426-01 - 1	POST-EX-01-0207	-9	0.0188	-	7471B	PPB	09 Feb 2022 12:05:10	U	SMPL
N1426-02 - 1	POST-EX-02-0207	886	0.1727	-	7471B	PPB	09 Feb 2022 12:07:26	U	SMPL
N1426-03 - 1	POST-EX-03-0207	0	0.0203	-	7471B	PPB	09 Feb 2022 12:09:43	U	SMPL
N1426-04 - 1	POST-EX-04-0207	7897	1.3780	-	7471B	PPB	09 Feb 2022 12:16:57	U	SMPL
N1426-05 - 1	POST-EX-05-0207	402	0.0894	-	7471B	PPB	09 Feb 2022 12:19:15	U	SMPL
N1427-01 - 1	VAUH-03-WASTE	37015	6.3840	-	7471B	PPB	09 Feb 2022 12:21:31	U	SMPL
CCV050 - 1	CCV050	29545	5.0998	-	7471B	PPB	09 Feb 2022 12:25:31	U	SMPL
CCB050 - 1	CCB050	-27	0.0157	-	7471B	PPB	09 Feb 2022 12:27:46	U	SMPL
N1432-01 - 1	SP-1	794	0.1568	-	7471B	PPB	09 Feb 2022 12:30:01	U	SMPL
N1432-04 - 1	SP-2	4573	0.8065	-	7471B	PPB	09 Feb 2022 12:32:17	U	SMPL
N1432-07 - 1	SP-3	1546	0.2861	-	7471B	PPB	09 Feb 2022 12:34:32	U	SMPL
N1432-10 - 1	SP-4	4539	0.8007	-	7471B	PPB	09 Feb 2022 12:36:48	U	SMPL
N1432-13 - 1	SP-5	2447	0.4410	-	7471B	PPB	09 Feb 2022 12:39:04	U	SMPL
N1432-16 - 1	SP-6	547	0.1144	-	7471B	PPB	09 Feb 2022 12:41:20	U	SMPL
N1432-19 - 1	SP-7	1637	0.3018	-	7471B	PPB	09 Feb 2022 12:43:37	U	SMPL
N1432-02MS - 1	TP-21MS	21808	3.7696	-	7471B	PPB	09 Feb 2022 12:45:54	U	SMPL
N1432-02MSD - 1	TP-21MSD	22009	3.8042	-	7471B	PPB	09 Feb 2022 12:48:11	U	SMPL
N1432-02LX5 - 1	TP-21L	26	0.0248	-	7471B	PPB	09 Feb 2022 12:53:46	U	SMPL
CCV051 - 1	CCV051	29724	5.1305	-	7471B	PPB	09 Feb 2022 12:56:01	U	SMPL
CCB051 - 1	CCB051	-26	0.0159	-	7471B	PPB	09 Feb 2022 12:58:17	U	SMPL