

LB118611

=====

Test results	Aquakem 7.2AQ1	Page: 1
--------------	----------------	---------

=====

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

2/10/2022 10:54

Test: Phenolics-

Sample Id	^{mg/L} Result	Dil. 1 +	Response	Errors
ICV1	1.025	0.0	0.117	
ICB1	0.001	0.0	0.005	
CCV1	0.989	0.0	0.113	
CCB1	0.001	0.0	0.005	
PB142574BL	0.002	0.0	0.005	
PB142574BS	1.048	0.0	0.120	
N1431-01	0.035	0.0	0.009	
N1431-01DUP	0.038	0.0	0.009	
N1431-01MS	1.048	0.0	0.120	
N1431-01MSD	1.071	0.0	0.122	
N1431-02	0.008	0.0	0.006	
CCV2	0.980	0.0	0.113	
CCB2	-0.000	0.0	0.005	

N	13
Mean	0.480
SD	0.5271
CV%	109.75

Aquakem v. 7.2AQ1

Results from time period:

Thu Feb 10 09:37:57 2022

Thu Feb 10 10:45:58 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0003	mg/l	2/10/2022 10:06:04	
0.05PPM	A	Phenolics-	P	0.0569	mg/l	2/10/2022 10:06:05	
0.1PPM	A	Phenolics-	P	0.109	mg/l	2/10/2022 10:06:06	
0.25PPM	A	Phenolics-	P	0.2507	mg/l	2/10/2022 10:06:07	
0.50PPM	A	Phenolics-	P	0.4875	mg/l	2/10/2022 10:06:08	
1.0PPM	A	Phenolics-	P	0.9863	mg/l	2/10/2022 10:06:09	
2.0PPM	A	Phenolics-	P	2.0093	mg/l	2/10/2022 10:06:10	
ICV1	S	Phenolics-	P	1.0246	mg/l	2/10/2022 10:39:34	
ICB1	S	Phenolics-	P	0.0012	mg/l	2/10/2022 10:39:36	
CCV1	S	Phenolics-	P	0.9886	mg/l	2/10/2022 10:39:38	
CCB1	S	Phenolics-	P	0.0008	mg/l	2/10/2022 10:39:41	
PB142574BL	S	Phenolics-	P	0.0018	mg/l	2/10/2022 10:39:43	
PB142574BS	S	Phenolics-	P	1.048	mg/l	2/10/2022 10:39:44	
N1431-01	S	Phenolics-	P	0.0354	mg/l	2/10/2022 10:45:52	
N1431-01DUP	S	Phenolics-	P	0.0376	mg/l	2/10/2022 10:45:53	
N1431-01MS	S	Phenolics-	P	1.0482	mg/l	2/10/2022 10:45:54	
N1431-01MSD	S	Phenolics-	P	1.0706	mg/l	2/10/2022 10:45:55	
N1431-02	S	Phenolics-	P	0.0075	mg/l	2/10/2022 10:45:56	
CCV2	S	Phenolics-	P	0.98	mg/l	2/10/2022 10:45:57	
CCB2	S	Phenolics-	P	-0.0004	mg/l	2/10/2022 10:45:58	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

2/10/2022 10:09

Reviewed by : 12 Instrument ID : Konelab


Test Phenolics-

Accepted 2/10/2022 10:09

Factor 9.091
Bias 0.005

Coeff. of det. 0.999822

Errors

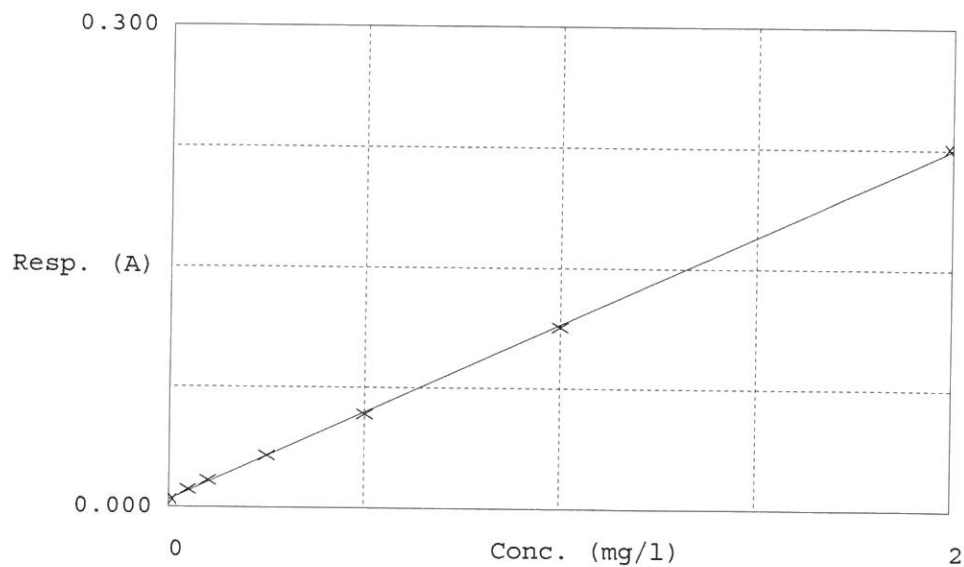

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.005	0.0003	0.0000	-
2	Phenol-2	0.011	0.0569	0.0500	13.8
3	Phenol-2	0.017	0.1090	0.1000	9
4	Phenol-2	0.032	0.2507	0.2500	2.3
5	Phenol-2	0.058	0.4875	0.5000	-2.5
6	Phenol-2	0.113	0.9863	1.0000	-1.4
7	Phenol-2	0.226	2.0093	2.0000	0.5

12
02/10/22