

LB 118697

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

2/16/2022 13:37

Test: CNEPA-NEW

Sample Id	^{ug/L} Result	Dil. 1 +	Response	Errors
ICV001 ICV001	92.305	0.0	0.105	
ICB001 ICB001	1.268	0.0	0.012	
CCV001 CCV001	237.003	0.0	0.252	
CCB001 CCB001	1.965	0.0	0.013	
PB142699BL PBS699	1.716	0.0	0.012	
NB331-04 MDL - SOIL-QT1-2022-02	6.093	0.0	0.017	
PB142700BL PBW700	0.706	0.0	0.011	
NB331-02 MDL - WATER-QT1-2022-02	5.887	0.0	0.017	
CCV002 CCV002	240.749	0.0	0.256	
CCB002 CCB002	1.580	0.0	0.012	

N	10
Mean	58.927
SD	98.8882
CV%	167.81

12
02/16/22

Aquakem v. 7.2AQ1

Results from time period:

Wed Feb 16 12:21:06 2022

Wed Feb 16 13:31:08 2022

Sample Id	Sam/Ct	Test short r	Test typ	Result	Result un	Result date and time
S0.0	A	CNEPA-NEV	P	-0.909	µg/l	2/16/2022 12:58:33
S5.0	A	CNEPA-NEV	P	5.787	µg/l	2/16/2022 12:58:34
S10.0	A	CNEPA-NEV	P	10.9922	µg/l	2/16/2022 12:58:35
S100.0	A	CNEPA-NEV	P	98.6294	µg/l	2/16/2022 12:58:36
S250.0	A	CNEPA-NEV	P	250.5081	µg/l	2/16/2022 12:58:37
S500.0	A	CNEPA-NEV	P	499.9924	µg/l	2/16/2022 12:58:38
ICV001 ICV001	S	CNEPA-NEV	P	92.3052	µg/l	2/16/2022 13:24:22
ICB001 ICB001	S	CNEPA-NEV	P	1.2683	µg/l	2/16/2022 13:24:23
CCV001 CCV001	S	CNEPA-NEV	P	237.0031	µg/l	2/16/2022 13:24:26
CCB001 CCB001	S	CNEPA-NEV	P	1.9655	µg/l	2/16/2022 13:24:27
PB142699BL PBS699	S	CNEPA-NEV	P	1.7158	µg/l	2/16/2022 13:24:29
N1331-04 MDL-SOIL-QT1-2022-02	S	CNEPA-NEV	P	6.0925	µg/l	2/16/2022 13:31:00
PB142700BL PBW700	S	CNEPA-NEV	P	0.706	µg/l	2/16/2022 13:31:02
N1331-02 MDL-WATER-QT1-2022-02	S	CNEPA-NEV	P	5.8865	µg/l	2/16/2022 13:31:04
CCV002 CCV002	S	CNEPA-NEV	P	240.7491	µg/l	2/16/2022 13:31:05
CCB002 CCB002	S	CNEPA-NEV	P	1.5797	µg/l	2/16/2022 13:31:08

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

2/16/2022 12:59

Test CNEPA-NEW


Accepted 2/16/2022 12:59

~~Factor slope~~ 981.6 0.001019
~~Bias Y Intercept~~ 0.011

12 02/18/22

Coeff. of det. 0.999977

Errors

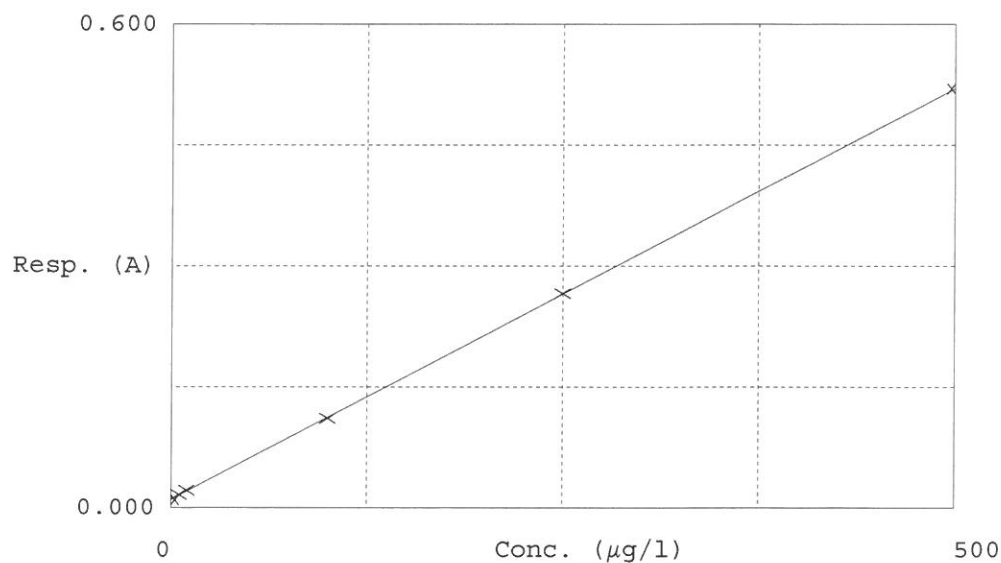

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.010	-0.9090	0.0000	-
2	5.0PPBCN	0.016	5.7870	5.0000	15.7
3	10PPBCN	0.022	10.9922	10.0000	9.9
4	100PPBCN	0.111	98.6294	100.0000	-1.4
5	250PPBCN	0.266	250.5081	250.0000	0.2
6	500PPBCN	0.520	499.9924	500.0000	0.0

12 02/16/22