

Clear table

| Instrument ID: IC-2      Analyst :      IZ      Method:      300.0 / 9056A |                      |                       |                       |                       |                       |                        |                       |             |               |                          |         |
|----------------------------------------------------------------------------|----------------------|-----------------------|-----------------------|-----------------------|-----------------------|------------------------|-----------------------|-------------|---------------|--------------------------|---------|
| ident                                                                      | concentra<br>tion F- | concentratio<br>n CL- | concentrati<br>on NO2 | concentrati<br>on BR- | concentrati<br>on NO3 | concentrati<br>on HPO4 | concentrati<br>on SO4 | file name   | date time     | Initial wt/<br>Final Vol | Analyst |
| STD1                                                                       | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2022-02-09_ | 2/9/22 10:14  |                          | IZ/AP   |
| STD2                                                                       | 0.4180               | 0.6650                | 0.6690                | 2.3100                | 0.5670                | 0.9300                 | 3.5030                | 2022-02-09_ | 2/9/22 10:44  |                          | IZ/AP   |
| STD3                                                                       | 0.8230               | 1.2010                | 1.2010                | 4.0240                | 1.0070                | 2.1230                 | 6.0660                | 2022-02-09_ | 2/9/22 11:12  |                          | IZ/AP   |
| STD4                                                                       | 0.9690               | 1.4880                | 1.4890                | 4.9210                | 1.2340                | 2.5290                 | 7.3890                | 2022-02-09_ | 2/9/22 11:41  |                          | IZ/AP   |
| STD5                                                                       | 1.9550               | 2.9440                | 2.9380                | 9.6950                | 2.4360                | 5.0230                 | 14.4840               | 2022-02-09_ | 2/9/22 12:10  |                          | IZ/AP   |
| STD6                                                                       | 4.0970               | 5.9230                | 5.9210                | 19.7690               | 4.9330                | 9.6840                 | 29.5340               | 2022-02-09_ | 2/9/22 12:39  |                          | IZ/AP   |
| STD7                                                                       | 4.9380               | 7.5780                | 7.5820                | 25.2810               | 6.3230                | 12.7100                | 38.0230               | 2022-02-09_ | 2/9/22 13:08  |                          | IZ/AP   |
| ICV                                                                        | 2.0620               | 2.9470                | 2.9280                | 9.6150                | 2.8870                | 5.4380                 | 14.5570               | 2022-02-09_ | 2/9/22 14:26  |                          | IZ/AP   |
| ICB                                                                        | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2022-02-09_ | 2/9/22 15:12  |                          | IZ/AP   |
| CCV                                                                        | 2.1070               | 2.8460                | 2.7660                | 9.3350                | 2.3530                | 5.3690                 | 14.0130               | 2022-02-17_ | 2/17/22 9:05  |                          | IZ/AP   |
| CCB                                                                        | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2022-02-17_ | 2/17/22 9:36  |                          | IZ/AP   |
| LB118714BLW                                                                | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2022-02-17_ | 2/17/22 10:05 |                          | IZ/AP   |
| LB118714BSW                                                                | 2.0450               | 2.8150                | 2.7590                | 9.2370                | 2.3300                | 5.3900                 | 13.8750               | 2022-02-17_ | 2/17/22 10:35 |                          | IZ/AP   |
| N1565-01X10                                                                | 0.0000               | 141.4610              | 0.0000                | 0.9600                | 0.0000                | 0.0000                 | 1.9520                | 2022-02-17_ | 2/17/22 11:04 |                          | IZ/AP   |
| N1565-01DLX300                                                             | 0.0000               | 3.4040                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2022-02-17_ | 2/17/22 11:33 |                          | IZ/AP   |
| N1565-01MSX10                                                              | 0.2940               | 135.8310              | 0.2670                | 1.8390                | 0.3530                | 1.1740                 | 3.2210                | 2022-02-17_ | 2/17/22 12:02 |                          | IZ/AP   |
| N1565-01MSDX10                                                             | 0.2690               | 135.1870              | 0.2650                | 1.8340                | 0.3530                | 1.1670                 | 3.1990                | 2022-02-17_ | 2/17/22 12:31 |                          | IZ/AP   |
| CCV                                                                        | 2.0160               | 2.8670                | 2.8170                | 9.3890                | 2.3620                | 5.8800                 | 14.0820               | 2022-02-17_ | 2/17/22 13:00 |                          | IZ/AP   |
| CCB                                                                        | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2022-02-17_ | 2/17/22 13:29 |                          | IZ/AP   |

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A


| ident | concentra<br>tion F- | concentratio<br>n CL- | concentrati<br>on NO2 | concentrati<br>on BR- | concentrati<br>on NO3 | concentrati<br>on HPO4 | concentrati<br>on SO4 | file name   | date time    | Initial wt/<br>Final Vol | Analyst |
|-------|----------------------|-----------------------|-----------------------|-----------------------|-----------------------|------------------------|-----------------------|-------------|--------------|--------------------------|---------|
| STD1  | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2022-02-09_ | 2/9/22 10:14 |                          | IZ/AP   |
| STD2  | 0.4180               | 0.6650                | 0.6690                | 2.3100                | 0.5670                | 0.9300                 | 3.5030                | 2022-02-09_ | 2/9/22 10:44 |                          | IZ/AP   |
| STD3  | 0.8230               | 1.2010                | 1.2010                | 4.0240                | 1.0070                | 2.1230                 | 6.0660                | 2022-02-09_ | 2/9/22 11:12 |                          | IZ/AP   |
| STD4  | 0.9690               | 1.4880                | 1.4890                | 4.9210                | 1.2340                | 2.5290                 | 7.3890                | 2022-02-09_ | 2/9/22 11:41 |                          | IZ/AP   |
| STD5  | 1.9550               | 2.9440                | 2.9380                | 9.6950                | 2.4360                | 5.0230                 | 14.4840               | 2022-02-09_ | 2/9/22 12:10 |                          | IZ/AP   |
| STD6  | 4.0970               | 5.9230                | 5.9210                | 19.7690               | 4.9330                | 9.6840                 | 29.5340               | 2022-02-09_ | 2/9/22 12:39 |                          | IZ/AP   |
| STD7  | 4.9380               | 7.5780                | 7.5820                | 25.2810               | 6.3230                | 12.7100                | 38.0230               | 2022-02-09_ | 2/9/22 13:08 |                          | IZ/AP   |

| ident | True Value F- | True Value CL- | True Value NO2 | True Value BR- | True Value NO3 | True Value HPO4 | True Value SO4 |
|-------|---------------|----------------|----------------|----------------|----------------|-----------------|----------------|
| STD1  | 0.0000        | 0.0000         | 0.0000         | 0.0000         | 0.0000         | 0.0000          | 0.0000         |
| STD2  | 0.4000        | 0.6000         | 0.6000         | 2.0000         | 0.5000         | 1.0000          | 3.0000         |
| STD3  | 0.8000        | 1.2000         | 1.2000         | 4.0000         | 1.0000         | 2.0000          | 6.0000         |
| STD4  | 1.0000        | 1.5000         | 1.5000         | 5.0000         | 1.2500         | 2.5000          | 7.5000         |
| STD5  | 2.0000        | 3.0000         | 3.0000         | 10.0000        | 2.5000         | 5.0000          | 15.0000        |
| STD6  | 4.0000        | 6.0000         | 6.0000         | 20.0000        | 5.0000         | 10.0000         | 30.0000        |
| STD7  | 5.0000        | 7.5000         | 7.5000         | 25.0000        | 6.2500         | 12.5000         | 37.0000        |

| ident | Relative Error F- | Relative Error CL- | Relative Error NO2 | Relative Error BR- | Relative Error NO3 | Relative Error HPO4 | Relative Error SO4 |
|-------|-------------------|--------------------|--------------------|--------------------|--------------------|---------------------|--------------------|
| STD1  |                   |                    |                    |                    |                    |                     |                    |
| STD2  | 4.5000            | 10.8333            | 11.5000            | 15.5000            | 13.4000            | -7.0000             | 16.7667            |
| STD3  | 2.8750            | 0.0833             | 0.0833             | 0.6000             | 0.7000             | 6.1500              | 1.1000             |
| STD4  | -3.1000           | -0.8000            | -0.7333            | -1.5800            | -1.2800            | 1.1600              | -1.4800            |
| STD5  | -2.2500           | -1.8667            | -2.0667            | -3.0500            | -2.5600            | 0.4600              | -3.4400            |
| STD6  | 2.4250            | -1.2833            | -1.3167            | -1.1550            | -1.3400            | -3.1600             | -1.5533            |
| STD7  | -1.2400           | 1.0400             | 1.0933             | 1.1240             | 1.1680             | 1.6800              | 2.7649             |

# CALIBRATION OF COMPONENT F-

Method: AnionsIC2-020922.mtw  
 Equation:  $Q = 0.0764573 \cdot A + 1.88372$   
 RSD: 2.976 %  
 Correlation coefficient: 0.999517

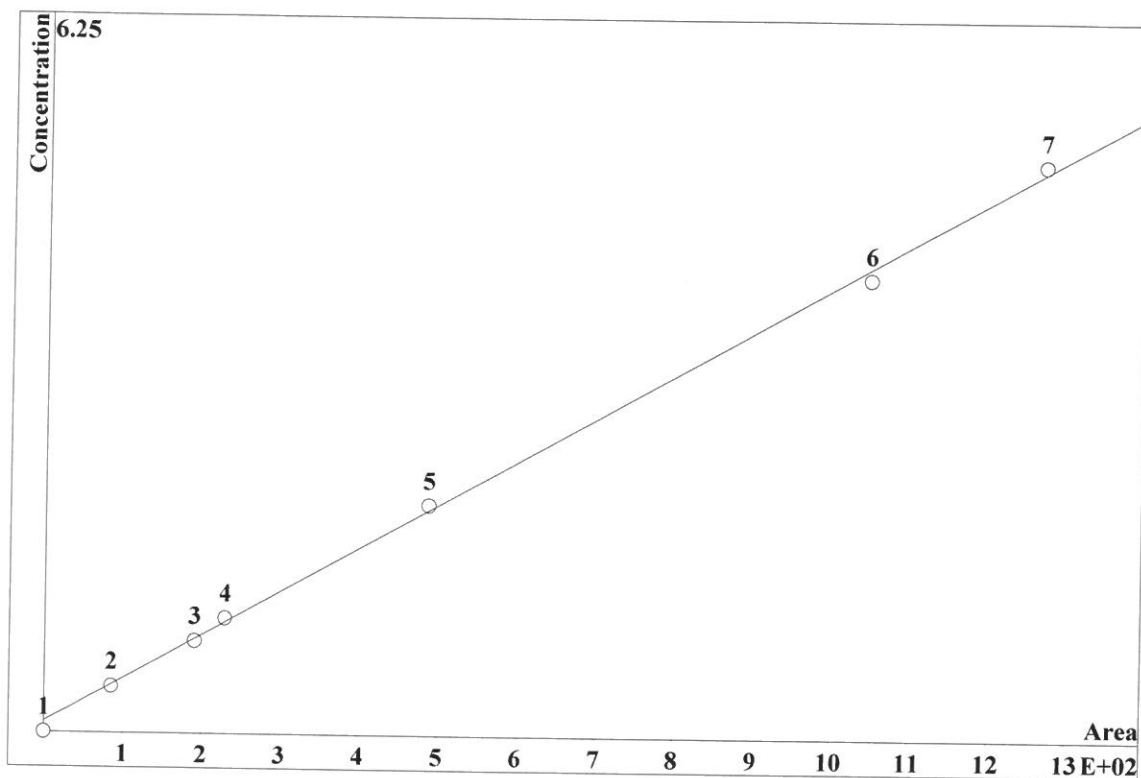


K3 = 0      K2 = 0      K1 = 0.0764573      K0 = 1.88372  
 Base: Area  
 Ref.channel: ch1  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used File |
|-------|--------|-------|-------|---------|-----------|-----------|
| 1     | 0      | 0     | 0     | 0       | 0         | 0         |
| 2     | 3.083  | 84.81 | 0.4   | 20      | 5.653     |           |
| 3     | 7.04   | 190.6 | 0.8   | 20      | 5.653     |           |
| 4     | 7.797  | 228.7 | 1     | 20      | 5.653     |           |
| 5     | 19.23  | 486.8 | 2     | 20      | 5.653     |           |
| 6     | 42.9   | 1047  | 4     | 20      | 5.653     |           |
| 7     | 49.77  | 1267  | 5     | 20      | 5.653     |           |

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-020922.mtw  
 Equation:  $Q = 0.117378 \cdot A + 2.12854$   
 RSD: 2.113 %  
 Correlation coefficient: 0.999757

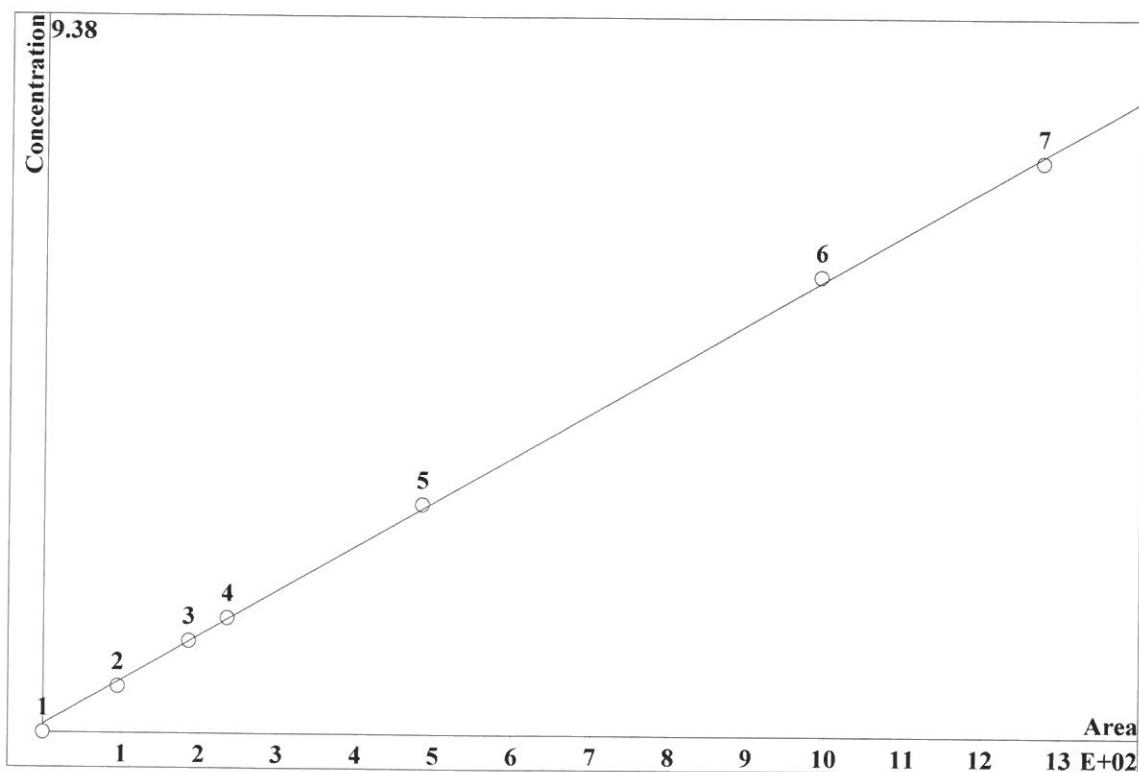


K3 = 0      K2 = 0      K1 = 0.117378      K0 = 2.12854  
 Base: Area  
 Ref.channel: ch1  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      | 0     | 0     | 0       | 0         |      |      |
| 2     | 6.463  | 95.21 | 0.6   | 20      | 8.643     |      |      |
| 3     | 12.62  | 186.5 | 1.2   | 20      | 8.643     |      |      |
| 4     | 15.96  | 235.5 | 1.5   | 20      | 8.643     |      |      |
| 5     | 33.32  | 483.5 | 3     | 20      | 8.643     |      |      |
| 6     | 68.88  | 991.1 | 6     | 20      | 8.643     |      |      |
| 7     | 89.91  | 1273  | 7.5   | 20      | 8.643     |      |      |

# CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-020922.mtw  
 Equation:  $Q = 0.051054 \cdot A + 2.56076$   
 RSD: 2.235 %  
 Correlation coefficient: 0.999728

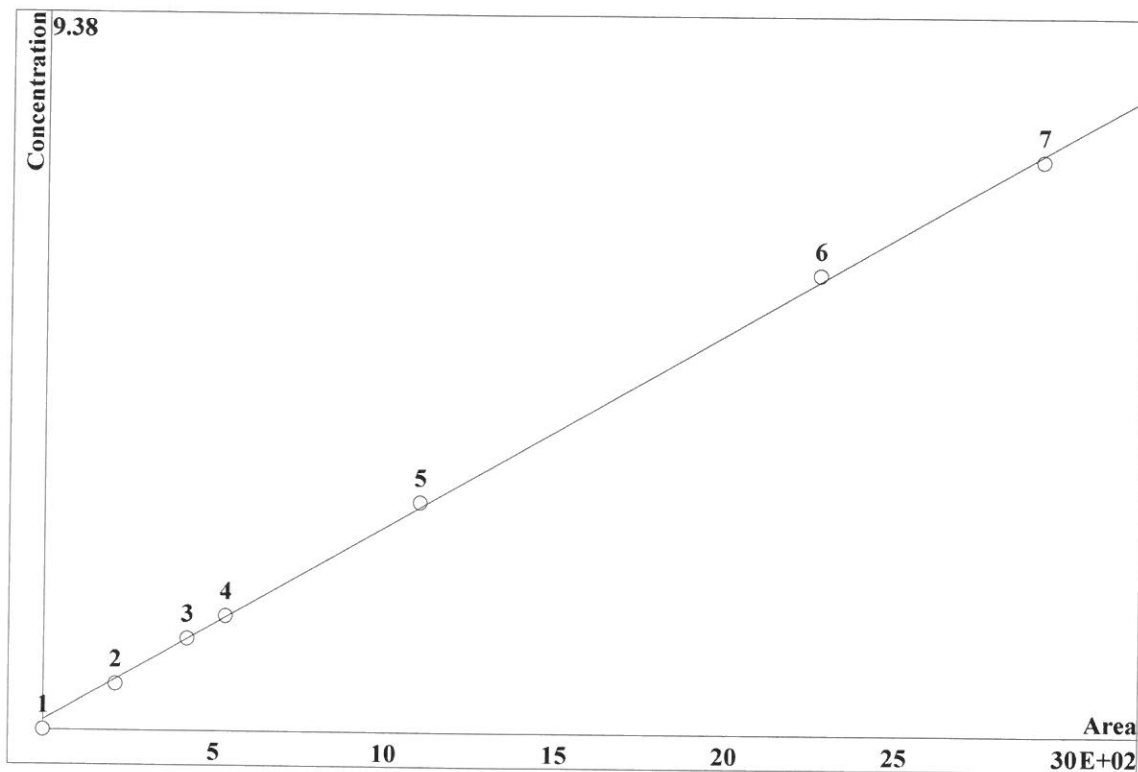


K3 = 0      K2 = 0      K1 = 0.051054      K0 = 2.56076  
 Base: Area  
 Ref.channel: ch1  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      | 0     | 0     | 0       | 0         |      |      |
| 2     | 11.63  | 212   | 0.6   | 20      | 10.46     |      |      |
| 3     | 23.16  | 420.4 | 1.2   | 20      | 10.46     |      |      |
| 4     | 29.36  | 533.1 | 1.5   | 20      | 10.46     |      |      |
| 5     | 59.9   | 1101  | 3     | 20      | 10.46     |      |      |
| 6     | 121.8  | 2269  | 6     | 20      | 10.46     |      |      |
| 7     | 155.4  | 2920  | 7.5   | 20      | 10.46     |      |      |

\*□

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-020922.mtw  
 Equation:  $Q = 0.255164 \cdot A + 11.0743$   
 RSD: 2.607 %  
 Correlation coefficient: 0.999630

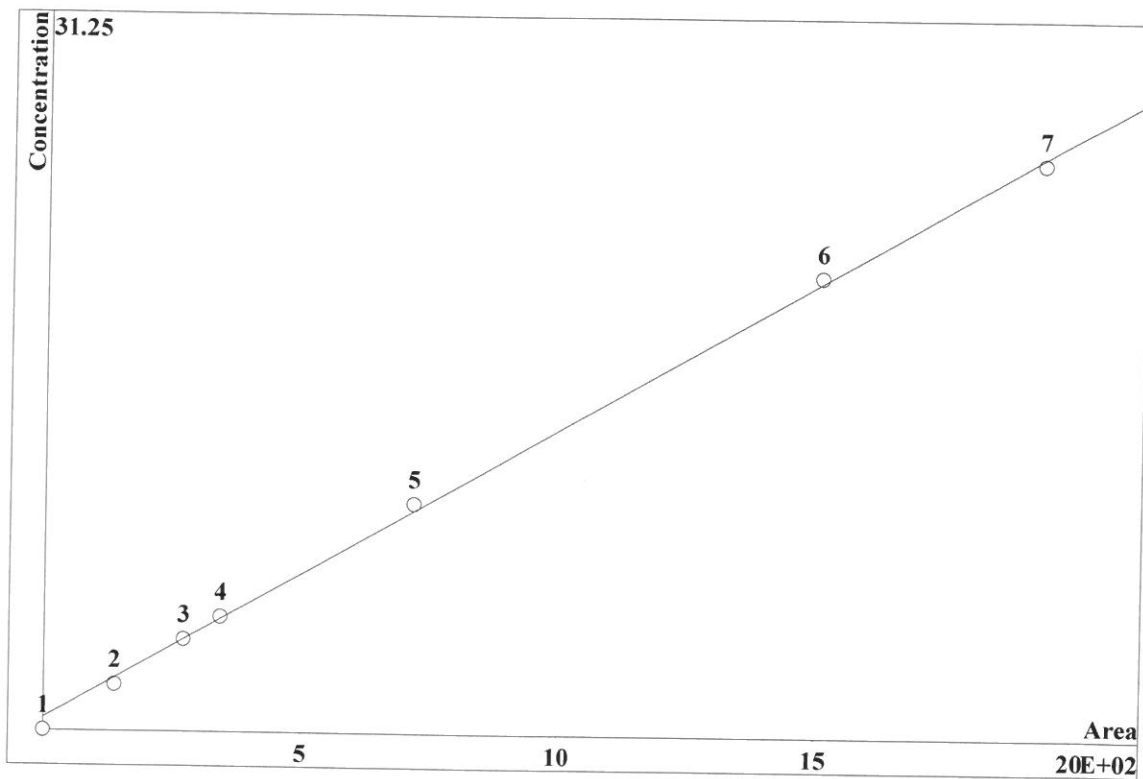


K3 = 0      K2 = 0      K1 = 0.255164      K0 = 11.0743  
 Base: Area  
 Ref.channel: ch1  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      |       | 0     | 0       | 0         |      | 0    |
| 2     | 6.658  | 137.7 | 2     | 20      | 13.53     |      |      |
| 3     | 13.38  | 272   | 4     | 20      | 13.53     |      |      |
| 4     | 17.03  | 342.3 | 5     | 20      | 13.53     |      |      |
| 5     | 35.75  | 716.5 | 10    | 20      | 13.53     |      |      |
| 6     | 74.76  | 1506  | 20    | 20      | 13.53     |      |      |
| 7     | 96.87  | 1938  | 25    | 20      | 13.53     |      |      |

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-020922.mtw  
 Equation:  $Q = 0.0456384 \cdot A + 2.3263$   
 RSD: 2.481 %  
 Correlation coefficient: 0.999664

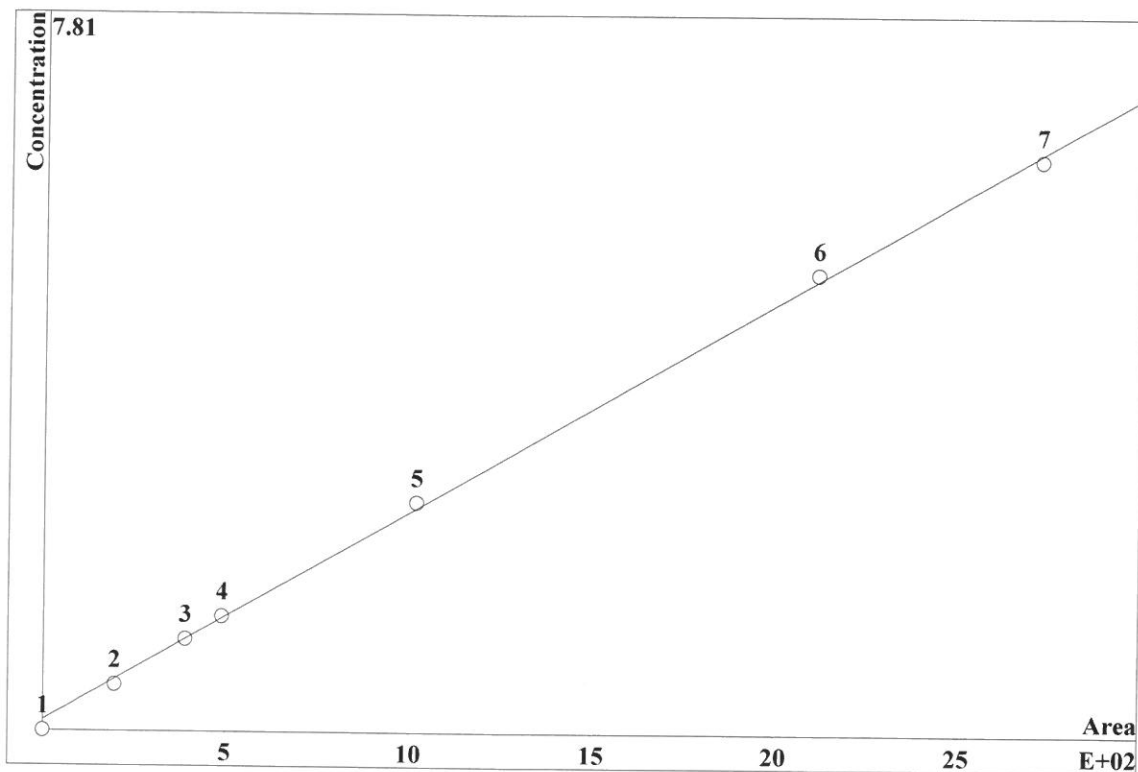


K3 = 0      K2 = 0      K1 = 0.0456384      K0 = 2.3263  
 Base: Area  
 Ref.channel: chl  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      | 0     | 0     | 0       | 0         |      | 0    |
| 2     | 8.047  | 197.3 | 0.5   | 20      | 15.58     |      |      |
| 3     | 16.02  | 390.5 | 1     | 20      | 15.58     |      |      |
| 4     | 20.32  | 489.8 | 1.25  | 20      | 15.58     |      |      |
| 5     | 42.36  | 1017  | 2.5   | 20      | 15.58     |      |      |
| 6     | 88.55  | 2111  | 5     | 20      | 15.58     |      |      |
| 7     | 115.1  | 2720  | 6.25  | 20      | 15.58     |      |      |

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-020922.mtw  
 Equation:  $Q = 0.0815612 \cdot A - 3.88126$   
 RSD: 3.697 %  
 Correlation coefficient: 0.999255

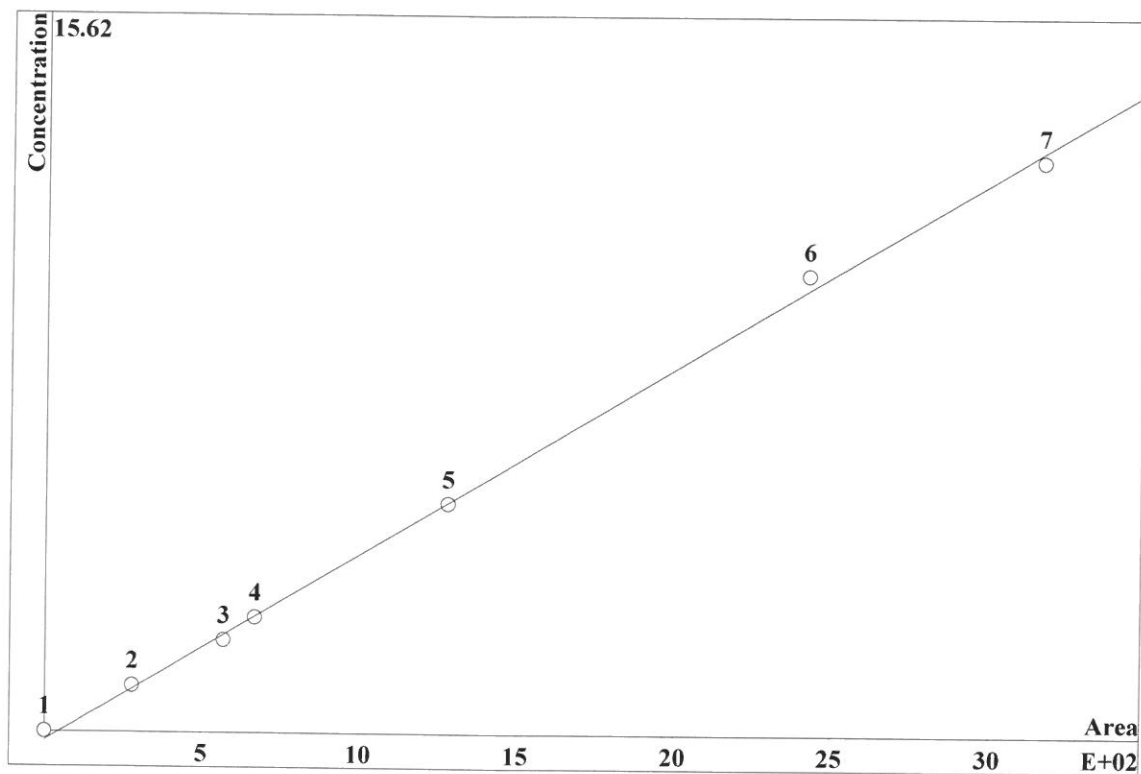


K3 = 0      K2 = 0      K1 = 0.0815612      K0 = -3.88126  
 Base: Area  
 Ref.channel: ch1  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File  |
|-------|--------|-------|-------|---------|-----------|------|-------|
| 1     |        | 0     | 0     | 0       |           |      | 0     |
| 2     | 7.423  | 275.7 |       | 1       | 20        |      | 20.18 |
| 3     | 15.55  | 568.3 |       | 2       | 20        |      | 20.18 |
| 4     | 18.32  | 667.7 |       | 2.5     | 20        |      | 20.18 |
| 5     | 37.46  | 1279  |       | 5       | 20        |      | 20.18 |
| 6     | 72.93  | 2422  |       | 10      | 20        |      | 20.18 |
| 7     | 88.68  | 3164  |       | 12.5    | 20        |      | 20.18 |

## CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-020922.mtw  
 Equation:  $Q = 0.148372 \cdot A + 17.1343$   
 RSD: 3.070 %  
 Correlation coefficient: 0.999486

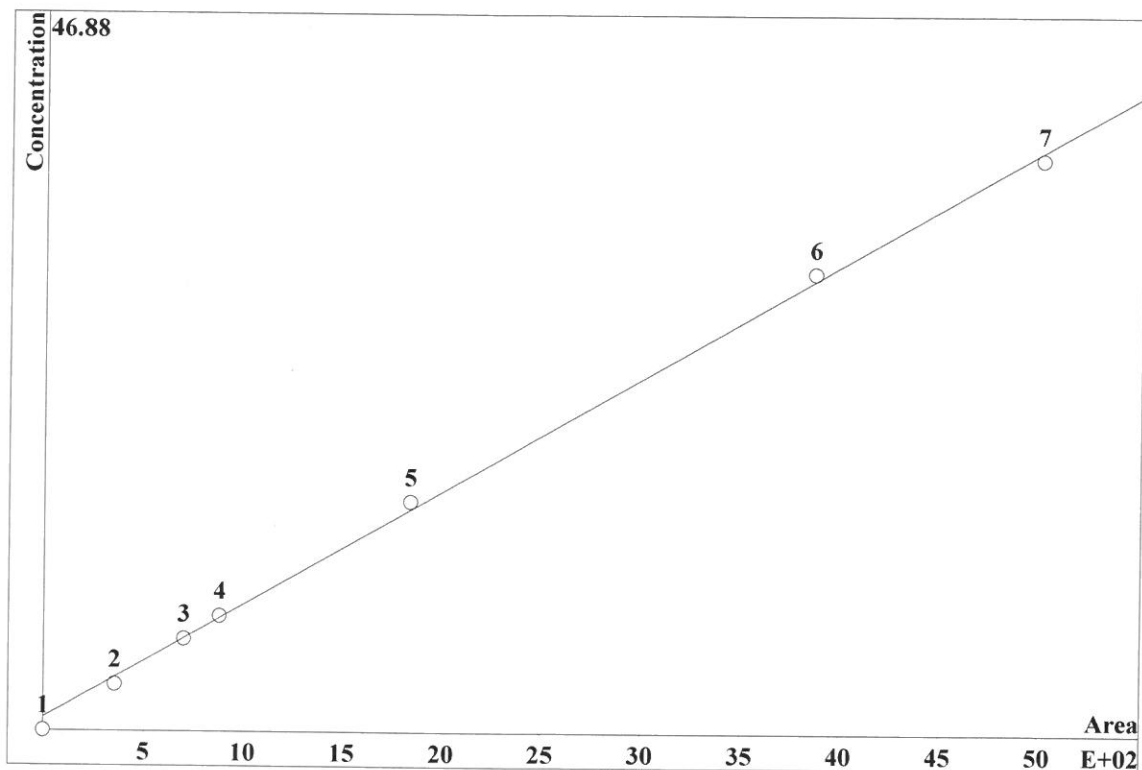

K3 = 0      K2 = 0      K1 = 0.148372      K0 = 17.1343  
 Base: Area  
 Ref.channel: ch1  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used File |
|-------|--------|-------|-------|---------|-----------|-----------|
| 1     | 0      | 0     | 0     | 0       | 0         | 0         |
| 2     | 11.82  | 356.7 | 3     | 20      | 23.09     |           |
| 3     | 23.46  | 702.2 | 6     | 20      | 23.09     |           |
| 4     | 29.62  | 880.6 | 7.5   | 20      | 23.09     |           |
| 5     | 62.43  | 1837  | 15    | 20      | 23.09     |           |
| 6     | 134    | 3866  | 30    | 20      | 23.09     |           |
| 7     | 175    | 5010  | 37.5  | 20      | 23.09     |           |

Report date: 2/11/2022 9:12:12 AM  
Printed by: wet


Ident: STD1  
Analysis from: 2/9/2022 10:14:56 AM  
File: \_2022-02-09\_

Last save: 2/9/2022 1:45:42 PM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30021

Last save: 2/9/2022 1:43:1

SAMPLE:  
: IZ/AP  
Vial number: 2  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

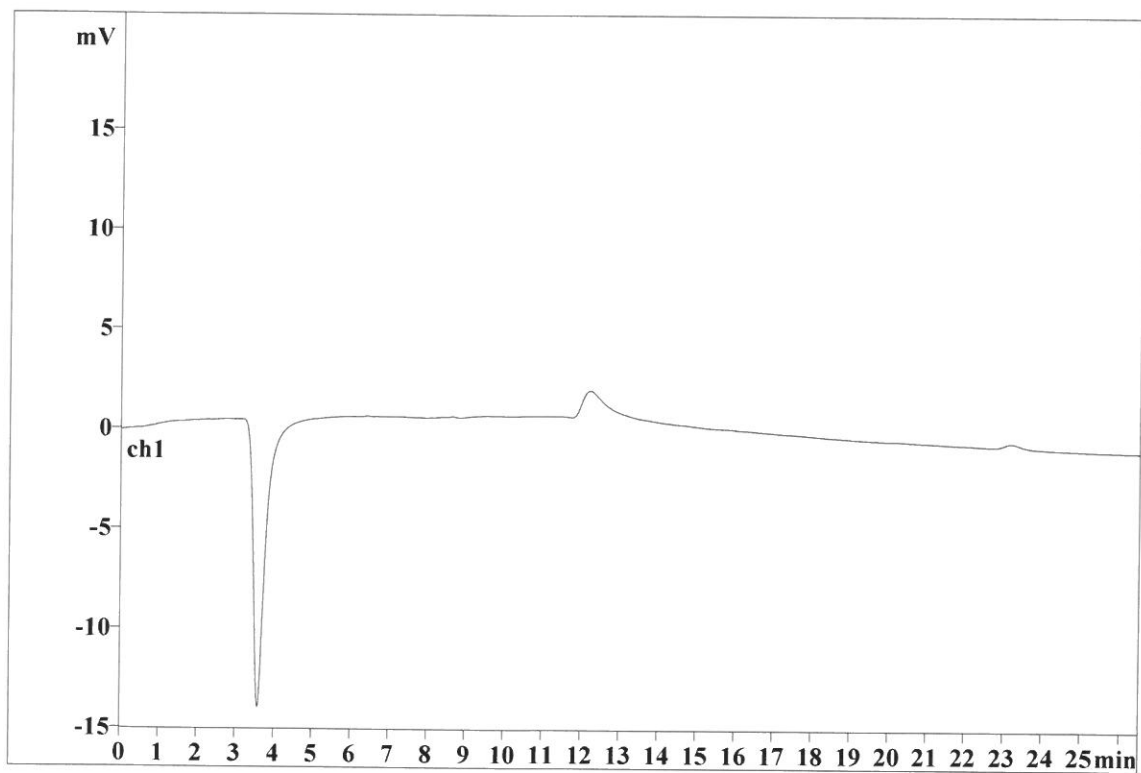

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 2/11/2022 9:15:38 AM  
Printed by: wet


Ident: STD2  
Analysis from: 2/9/2022 10:44:04 AM  
File: \_2022-02-09\_

Last save: 2/11/2022 9:13:06 AM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30022

Last save: 2/9/2022 1:43:1

SAMPLE:  
: IZ/AP  
Vial number: 3  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

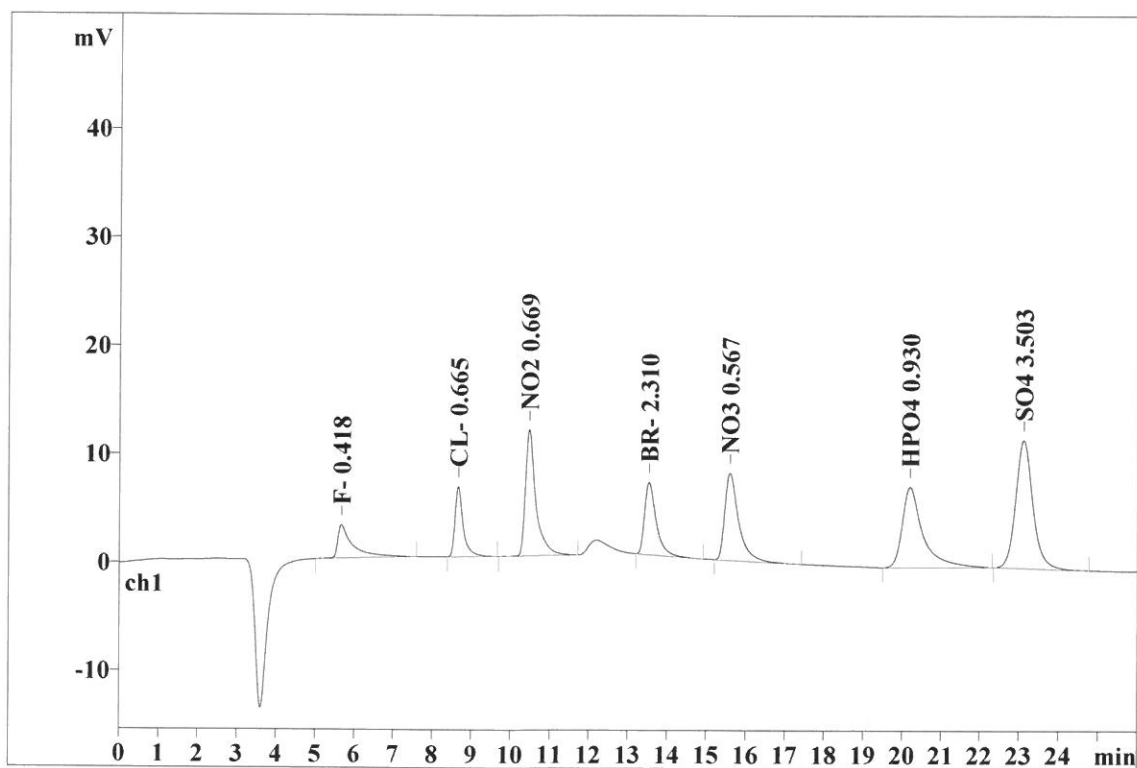

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.65             | 0.310          | 3.08         | 5.59        | 84.812         | 6.24      |
| 2  | 8.64             | 0.203          | 6.46         | 11.73       | 95.209         | 7.00      |
| 3  | 10.46            | 0.244          | 11.63        | 21.10       | 212.013        | 15.59     |
| 4  | 13.53            | 0.297          | 6.66         | 12.08       | 137.697        | 10.13     |
| 5  | 15.58            | 0.350          | 8.05         | 14.60       | 197.333        | 14.51     |
| 6  | 20.18            | 0.488          | 7.42         | 13.47       | 275.747        | 20.28     |
| 7  | 23.09            | 0.442          | 11.81        | 21.43       | 356.702        | 26.24     |
| 7  | 26.00            | 0.334          | 55.12        | 99.99       | 1359.513       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/11/2022 9:16:00 AM  
Printed by: wet


Ident: STD3  
Analysis from: 2/9/2022 11:12:41 AM  
File: \_2022-02-09\_

Last save: 2/11/2022 9:13:06 AM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30023

Last save: 2/9/2022 1:43:1

SAMPLE:  
: IZ/AP  
Vial number: 4  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

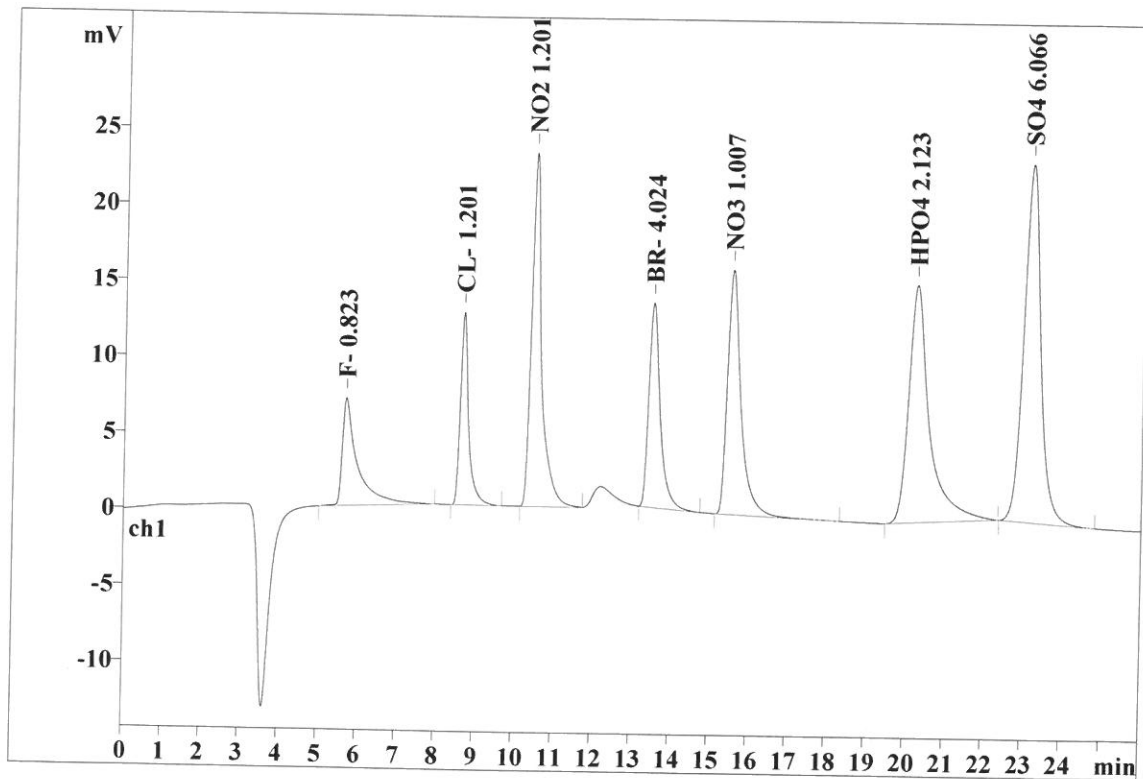

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.67             | 0.312          | 7.04         | 6.33        | 190.598        | 6.98      |
| 2  | 8.65             | 0.203          | 12.62        | 11.35       | 186.486        | 6.83      |
| 3  | 10.45            | 0.241          | 23.16        | 20.82       | 420.441        | 15.40     |
| 4  | 13.51            | 0.294          | 13.38        | 12.03       | 272.020        | 9.96      |
| 5  | 15.52            | 0.347          | 16.02        | 14.40       | 390.458        | 14.30     |
| 6  | 20.22            | 0.480          | 15.55        | 13.98       | 568.297        | 20.81     |
| 7  | 23.14            | 0.439          | 23.46        | 21.09       | 702.248        | 25.72     |
| 7  | 26.00            | 0.331          | 111.23       | 99.99       | 2730.549       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/11/2022 9:16:11 AM  
Printed by: wet


Ident: STD4  
Analysis from: 2/9/2022 11:41:19 AM  
File: \_2022-02-09\_

Last save: 2/11/2022 9:13:06 AM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30024

Last save: 2/9/2022 1:43:1

SAMPLE:  
: IZ/AP  
Vial number: 5  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

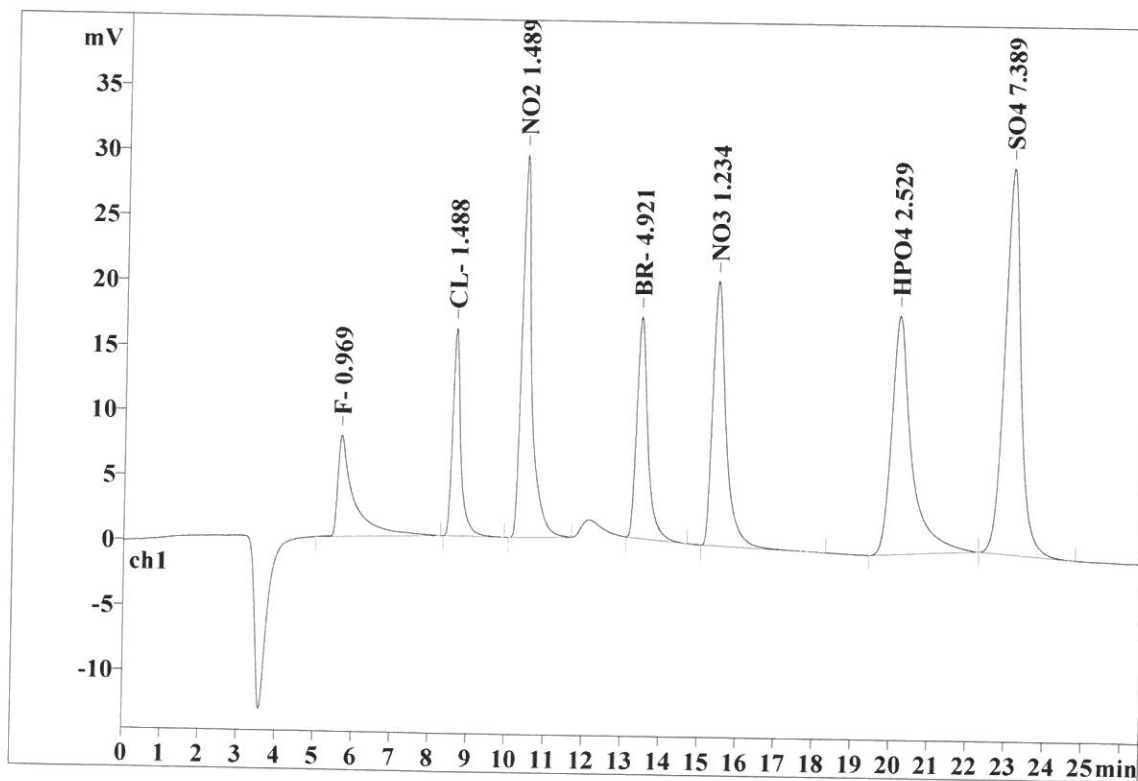

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.65             | 0.323          | 7.79         | 5.63        | 228.707        | 6.77      |
| 2  | 8.61             | 0.203          | 15.96        | 11.53       | 235.452        | 6.97      |
| 3  | 10.39            | 0.242          | 29.36        | 21.21       | 533.132        | 15.78     |
| 4  | 13.41            | 0.290          | 17.03        | 12.30       | 342.291        | 10.13     |
| 5  | 15.40            | 0.343          | 20.32        | 14.68       | 489.764        | 14.50     |
| 6  | 20.14            | 0.479          | 18.31        | 13.23       | 667.688        | 19.77     |
| 7  | 23.06            | 0.435          | 29.62        | 21.40       | 880.586        | 26.07     |
| 7  | 26.50            | 0.331          | 138.40       | 99.99       | 3377.621       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/11/2022 9:16:19 AM  
Printed by: wet


Ident: STD5  
Analysis from: 2/9/2022 12:10:27 PM  
File: \_2022-02-09\_

Last save: 2/11/2022 9:13:06 AM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30025

Last save: 2/9/2022 1:43:1

SAMPLE:  
: IZ/AP  
Vial number: 6  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

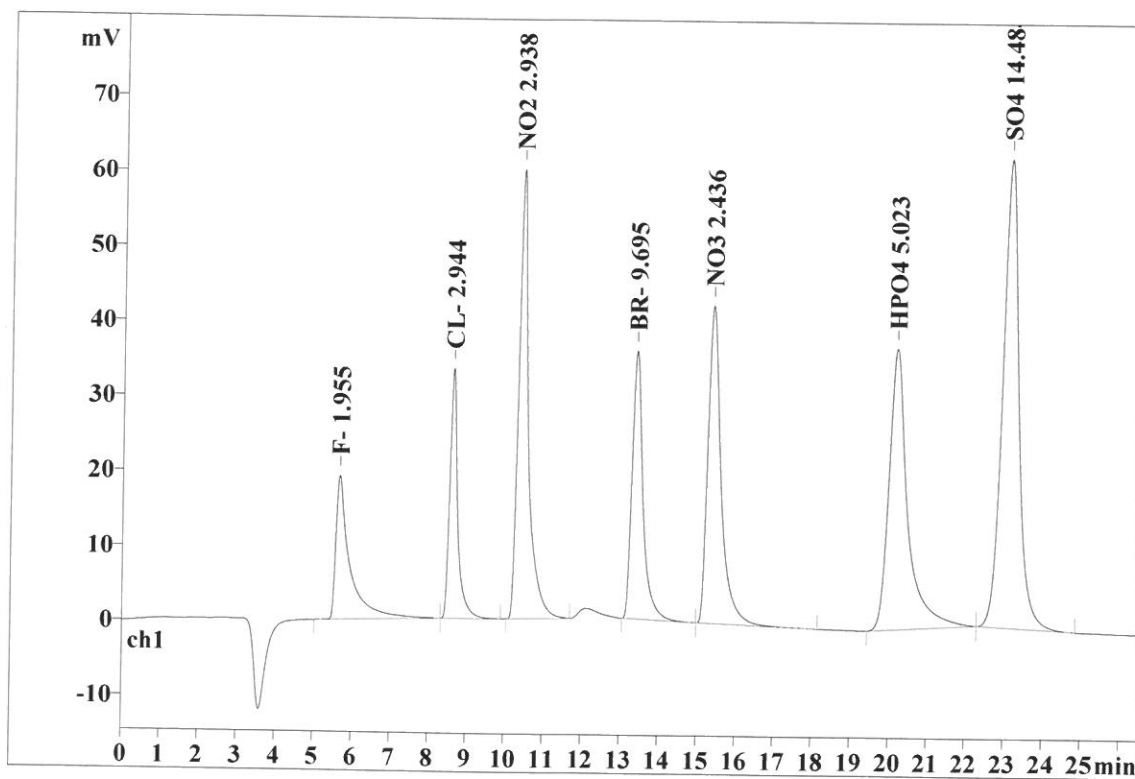

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.65             | 0.291          | 19.23        | 6.62        | 486.802        | 7.03      |
| 2  | 8.60             | 0.199          | 33.32        | 11.47       | 483.534        | 6.99      |
| 3  | 10.38            | 0.246          | 59.90        | 20.62       | 1100.787       | 15.91     |
| 4  | 13.38            | 0.286          | 35.74        | 12.31       | 716.475        | 10.35     |
| 5  | 15.34            | 0.340          | 42.36        | 14.58       | 1016.745       | 14.69     |
| 6  | 20.13            | 0.453          | 37.46        | 12.90       | 1279.215       | 18.48     |
| 7  | 23.07            | 0.429          | 62.43        | 21.50       | 1836.939       | 26.54     |
| 7  | 26.50            | 0.320          | 290.44       | 100.00      | 6920.497       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/11/2022 9:16:35 AM  
Printed by: wet


Ident: STD6  
Analysis from: 2/9/2022 12:39:35 PM  
File: \_2022-02-09\_

Last save: 2/11/2022 9:13:06 AM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30026

Last save: 2/9/2022 1:43:1

SAMPLE:  
: IZ/AP  
Vial number: 7  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

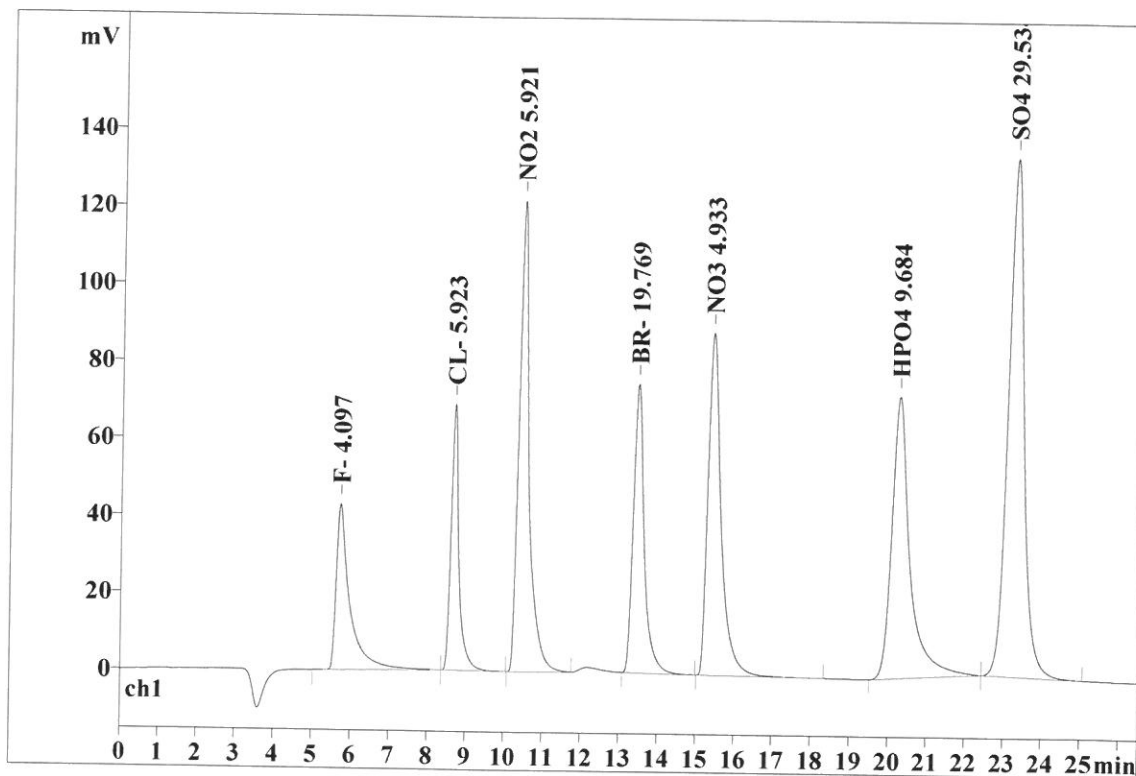

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.70             | 0.301          | 42.90        | 7.10        | 1047.105       | 7.37      |
| 2  | 8.65             | 0.197          | 68.88        | 11.41       | 991.148        | 6.97      |
| 3  | 10.41            | 0.250          | 121.81       | 20.17       | 2269.207       | 15.97     |
| 4  | 13.44            | 0.290          | 74.76        | 12.38       | 1506.105       | 10.60     |
| 5  | 15.38            | 0.338          | 88.55        | 14.67       | 2110.715       | 14.85     |
| 6  | 20.22            | 0.444          | 72.92        | 12.08       | 2422.309       | 17.04     |
| 7  | 23.23            | 0.422          | 133.96       | 22.19       | 3865.583       | 27.20     |
| 7  | 26.50            | 0.320          | 603.78       | 100.00      | 14212.172      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/11/2022 9:16:47 AM  
Printed by: wet


Ident: STD7  
Analysis from: 2/9/2022 1:08:43 PM  
File: \_2022-02-09\_

Last save: 2/11/2022 9:13:06 AM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30027

Last save: 2/9/2022 1:43:1

SAMPLE:  
: IZ/AP  
Vial number: 8  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

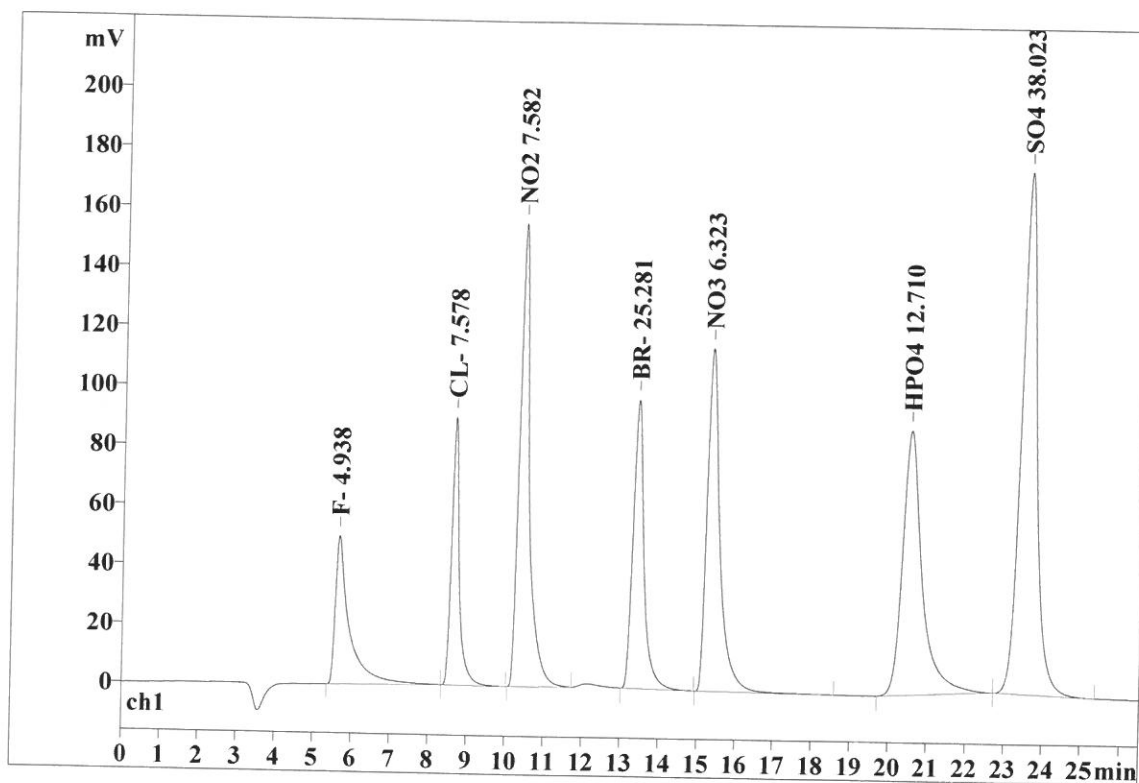

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.65             | 0.299          | 49.77        | 6.46        | 1267.058       | 6.93      |
| 2  | 8.63             | 0.193          | 89.91        | 11.67       | 1273.069       | 6.96      |
| 3  | 10.37            | 0.253          | 155.41       | 20.16       | 2919.971       | 15.96     |
| 4  | 13.39            | 0.287          | 96.87        | 12.57       | 1938.144       | 10.60     |
| 5  | 15.30            | 0.334          | 115.06       | 14.93       | 2719.910       | 14.87     |
| 6  | 20.51            | 0.489          | 88.68        | 11.51       | 3164.352       | 17.30     |
| 7  | 23.52            | 0.418          | 174.99       | 22.71       | 5009.882       | 27.39     |
| 7  | 26.50            | 0.325          | 770.69       | 100.00      | 18292.386      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/11/2022 9:17:11 AM  
Printed by: wet


Ident: ICV  
Analysis from: 2/9/2022 2:26:08 PM  
File: \_2022-02-09\_

Last save: 2/9/2022 2:52:38 PM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30029

Last save: 2/9/2022 1:45:3

SAMPLE:  
:  
Vial number: 9  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

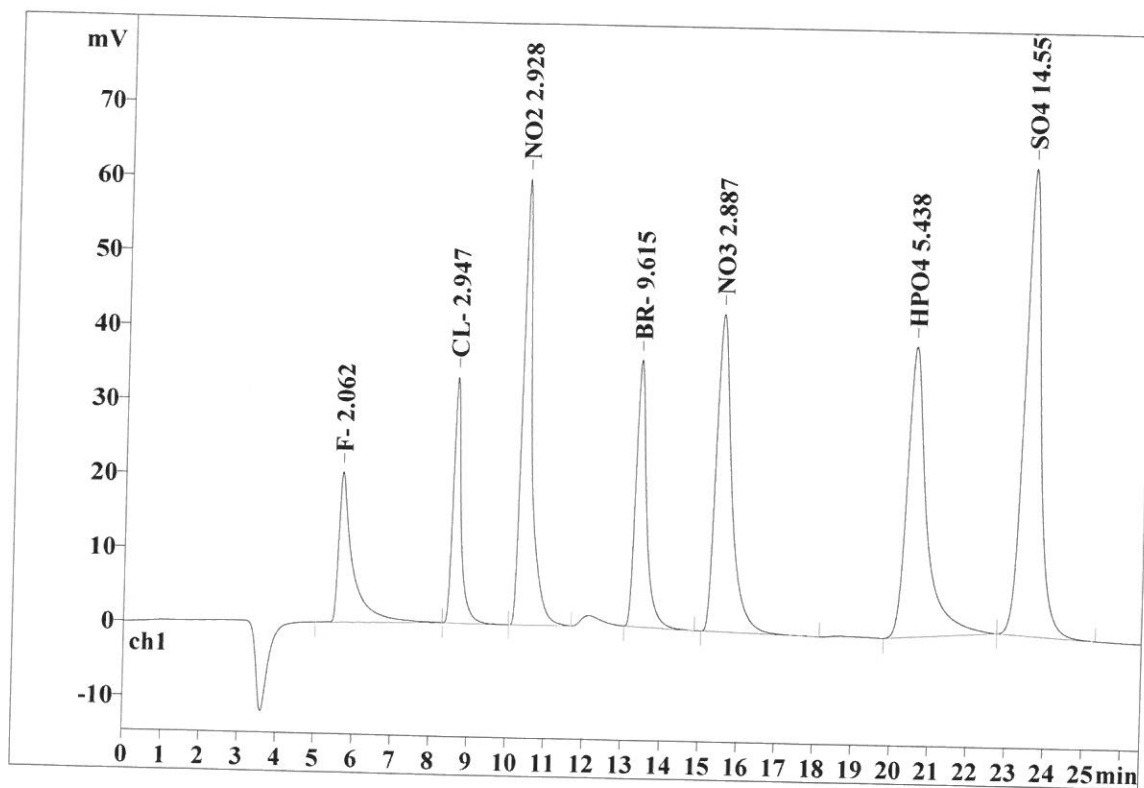

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.66             | 0.303          | 20.21        | 6.88        | 514.757        | 7.10      |
| 2  | 8.60             | 0.201          | 33.10        | 11.27       | 483.930        | 6.68      |
| 3  | 10.37            | 0.242          | 60.01        | 20.43       | 1096.792       | 15.13     |
| 4  | 13.37            | 0.285          | 35.89        | 12.22       | 710.194        | 9.80      |
| 5  | 15.48            | 0.411          | 42.71        | 14.54       | 1214.409       | 16.76     |
| 6  | 20.52            | 0.468          | 39.06        | 13.29       | 1381.008       | 19.05     |
| 7  | 23.53            | 0.430          | 62.82        | 21.38       | 1846.770       | 25.48     |
| 7  | 26.50            | 0.334          | 293.80       | 100.00      | 7247.860       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/11/2022 9:18:03 AM  
Printed by: wet


Ident: ICB  
Analysis from: 2/9/2022 3:12:21 PM  
File: \_2022-02-09\_

Last save: 2/9/2022 3:38:51 PM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30030

Last save: 2/9/2022 1:45:3

SAMPLE:  
:  
Vial number: 10  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

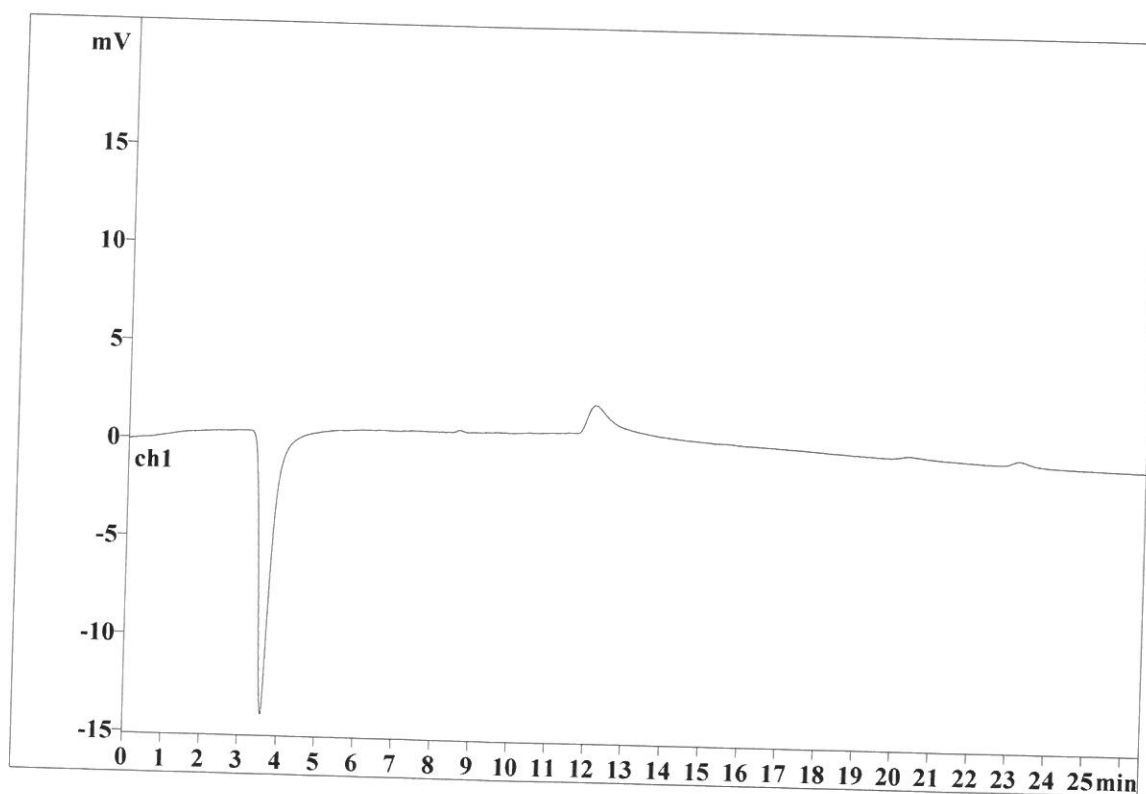

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 2/17/2022 3:20:56 PM  
Printed by: wet


Ident: CCV  
Analysis from: 2/17/2022 9:05:16 AM  
File: \_2022-02-17\_

Last save: 2/17/2022 9:31:46 AM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30097

Last save: 2/9/2022 1:45:3

SAMPLE:  
: IZ/AP  
Vial number: 11  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

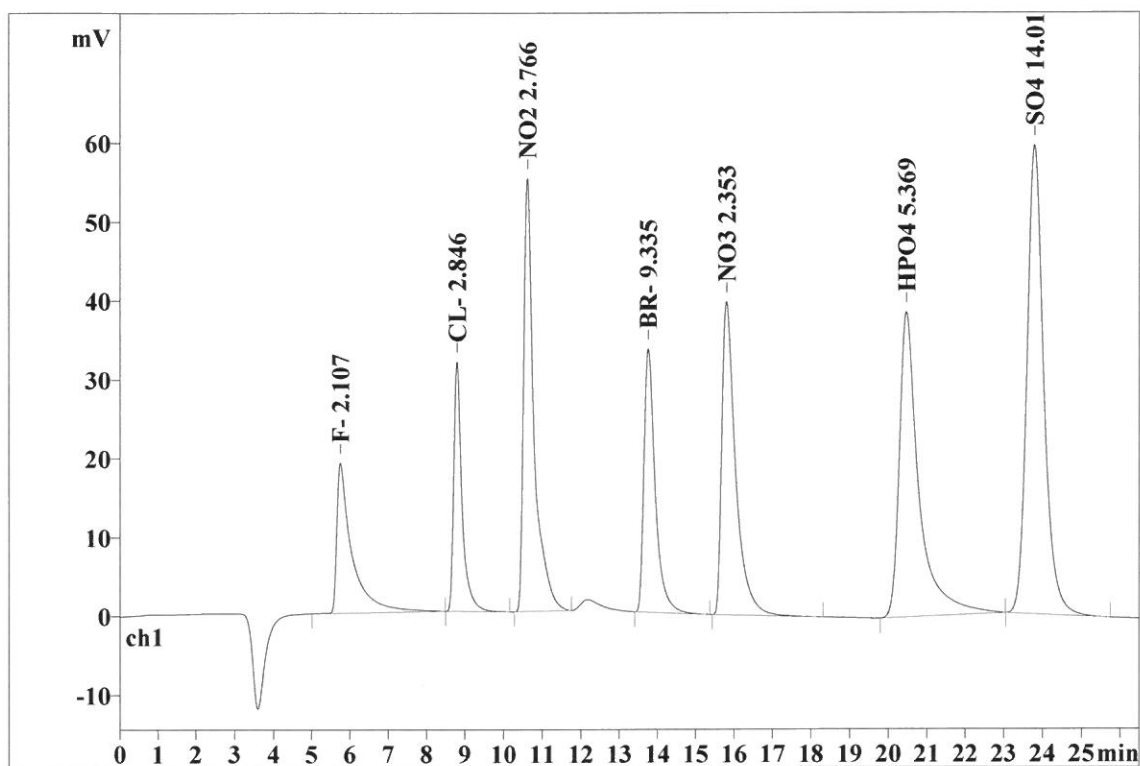

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.75             | 0.330          | 19.06        | 6.88        | 526.435        | 7.70      |
| 2  | 8.79             | 0.202          | 31.67        | 11.43       | 466.712        | 6.83      |
| 3  | 10.61            | 0.246          | 54.95        | 19.84       | 1033.514       | 15.13     |
| 4  | 13.75            | 0.296          | 33.40        | 12.06       | 688.310        | 10.07     |
| 5  | 15.81            | 0.352          | 39.71        | 14.34       | 980.340        | 14.35     |
| 6  | 20.47            | 0.460          | 38.70        | 13.97       | 1364.235       | 19.97     |
| 7  | 23.79            | 0.438          | 59.50        | 21.48       | 1773.364       | 25.95     |
| 7  | 26.50            | 0.332          | 276.99       | 100.00      | 6832.910       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/17/2022 3:21:06 PM  
Printed by: wet


Ident: CCB  
Analysis from: 2/17/2022 9:36:46 AM  
File: \_2022-02-17\_

Last save: 2/17/2022 10:03:16 AM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30098

Last save: 2/9/2022 1:45:3

SAMPLE:  
: IZ/AP  
Vial number: 12  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

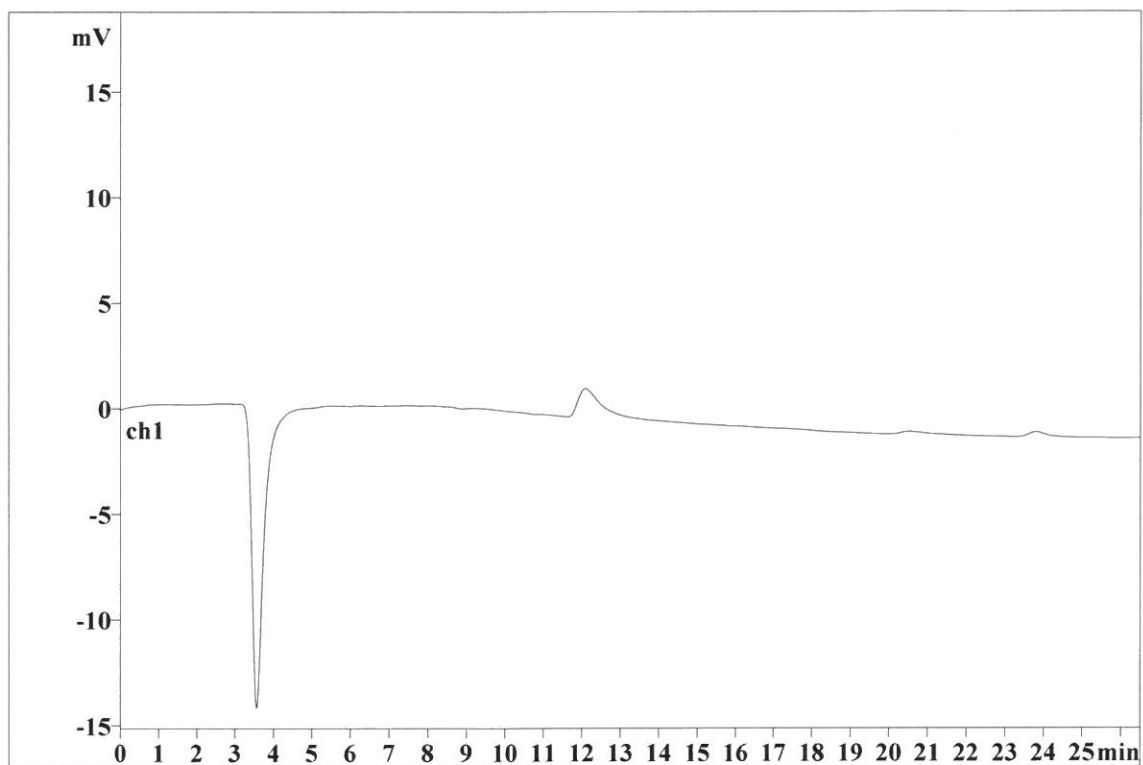

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 2/17/2022 3:21:16 PM  
Printed by: wet


Ident: LB118714BLW  
Analysis from: 2/17/2022 10:05:54 AM  
File: \_2022-02-17\_

Last save: 2/17/2022 11:50:20 AM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30099

Last save: 2/9/2022 1:45:3

SAMPLE:  
: IZ/AP  
Vial number: 13  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

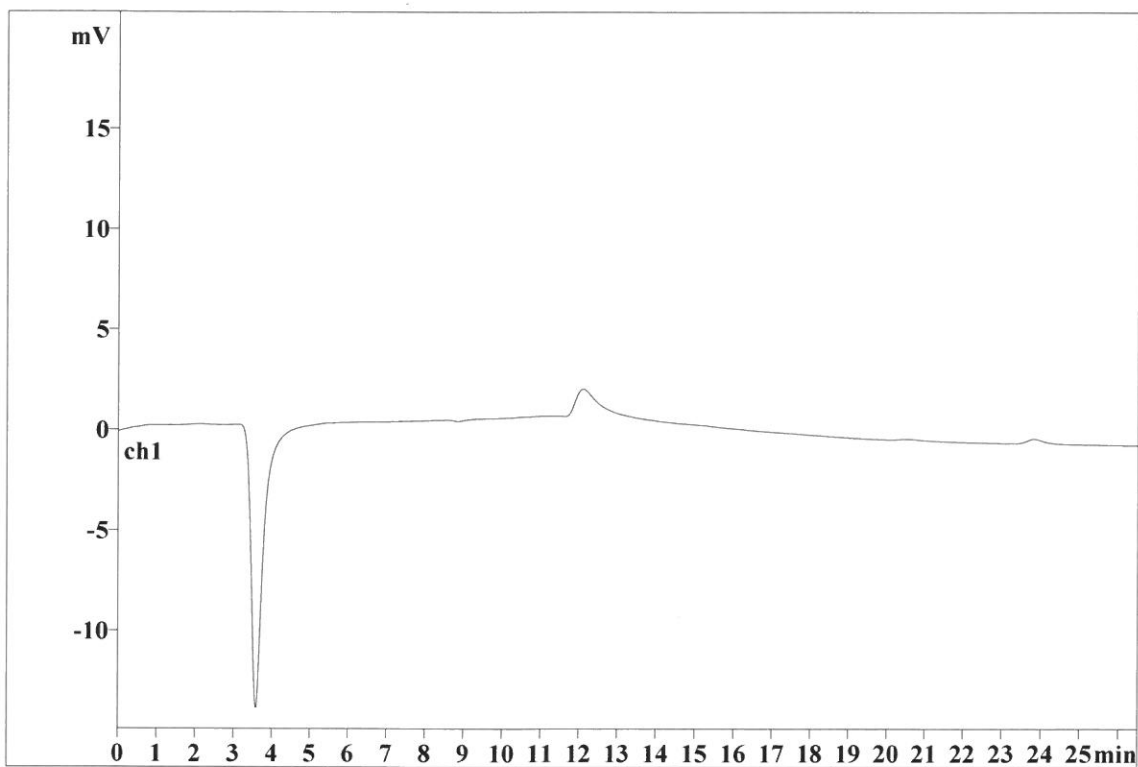

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 2/17/2022 3:21:26 PM  
Printed by: wet


Ident: LB118714BSW  
Analysis from: 2/17/2022 10:35:02 AM  
File: \_2022-02-17\_

Last save: 2/17/2022 11:50:20 AM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30100

Last save: 2/9/2022 1:45:3

SAMPLE:  
: IZ/AP  
Vial number: 14  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

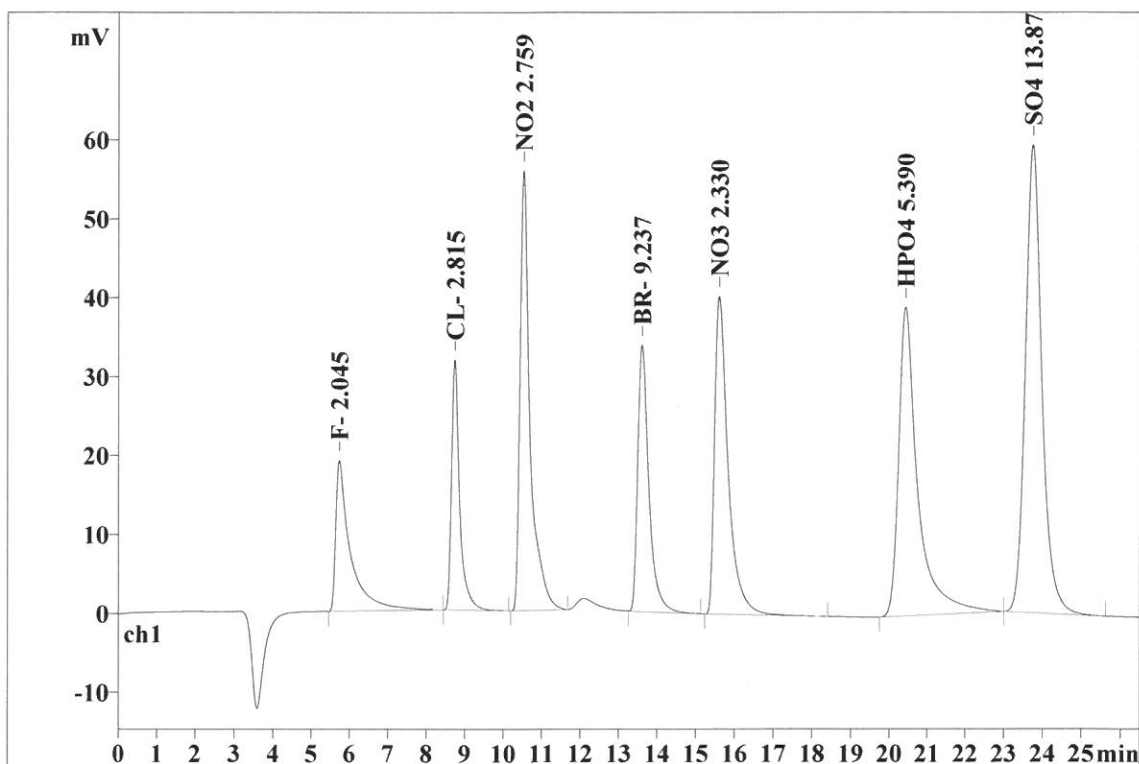

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.73             | 0.319          | 19.10        | 6.84        | 510.342        | 7.53      |
| 2  | 8.73             | 0.200          | 31.68        | 11.35       | 461.532        | 6.81      |
| 3  | 10.52            | 0.243          | 55.76        | 19.98       | 1030.696       | 15.21     |
| 4  | 13.60            | 0.290          | 33.80        | 12.11       | 680.588        | 10.04     |
| 5  | 15.60            | 0.343          | 40.29        | 14.44       | 970.294        | 14.32     |
| 6  | 20.43            | 0.457          | 39.14        | 14.02       | 1369.266       | 20.20     |
| 7  | 23.74            | 0.435          | 59.32        | 21.25       | 1754.875       | 25.89     |
| 7  | 26.50            | 0.327          | 279.08       | 100.00      | 6777.593       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/17/2022 3:22:45 PM  
Printed by: wet


Ident: N1565-01X10  
Analysis from: 2/17/2022 11:04:10 AM  
File: \_2022-02-17\_

Last save: 2/17/2022 12:06:22 PM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30101

Last save: 2/9/2022 1:45:3

SAMPLE:  
: IZ/AP  
Vial number: 15  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

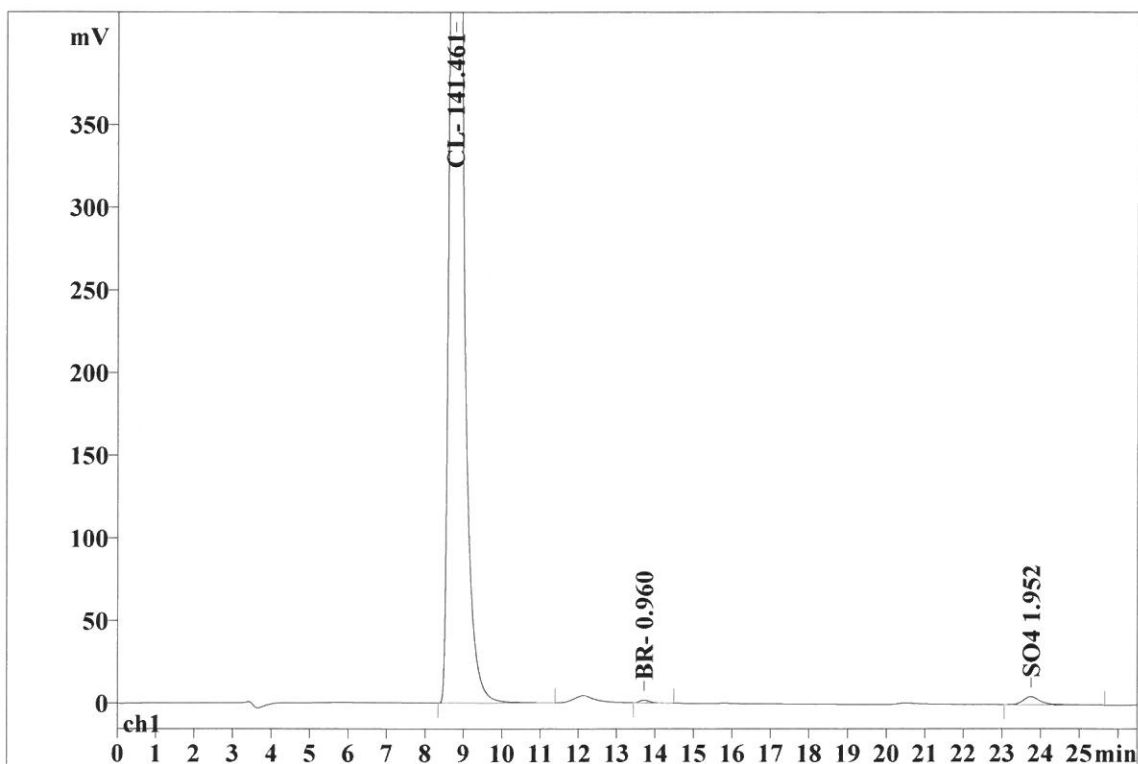

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.75             | 0.250          | 1341.55      | 99.51       | 24085.337      | 99.26     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 13.71            | 0.269          | 1.77         | 0.13        | 31.860         | 0.13      |
| 5  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 23.75            | 0.443          | 4.87         | 0.36        | 147.586        | 0.61      |
| 7  | 26.50            | 0.137          | 1348.19      | 100.00      | 24264.782      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/17/2022 3:23:03 PM  
Printed by: wet


Ident: N1565-01DLX300  
Analysis from: 2/17/2022 11:33:18 AM  
File: \_2022-02-17\_

Last save: 2/17/2022 11:59:48 AM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30102

Last save: 2/9/2022 1:45:3

SAMPLE:  
: IZ/AP  
Vial number: 16  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

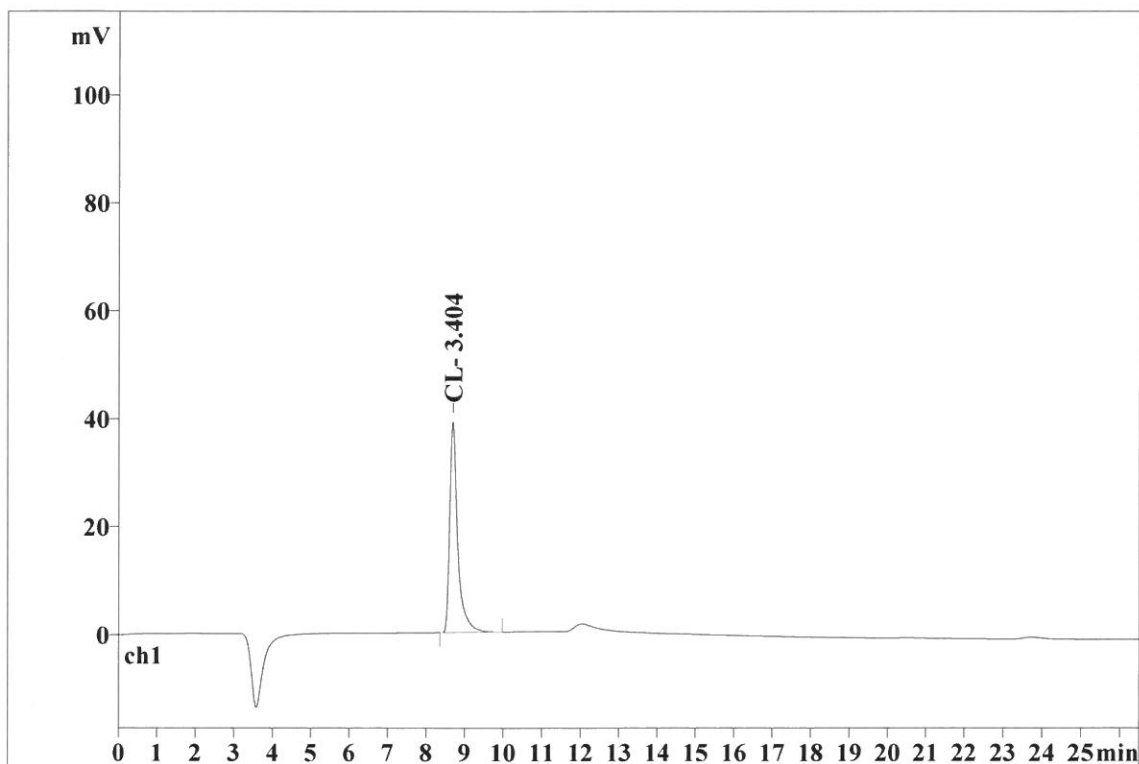

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.68             | 0.196          | 38.98        | 100.00      | 561.841        | 100.00    |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 26.50            | 0.028          | 38.98        | 100.00      | 561.841        | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/17/2022 3:23:21 PM  
Printed by: wet


Ident: N1565-01MSX10  
Analysis from: 2/17/2022 12:02:27 PM  
File: \_2022-02-17\_

Last save: 2/17/2022 12:28:56 PM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30103

Last save: 2/9/2022 1:45:3

SAMPLE:  
: IZ/AP  
Vial number: 17  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

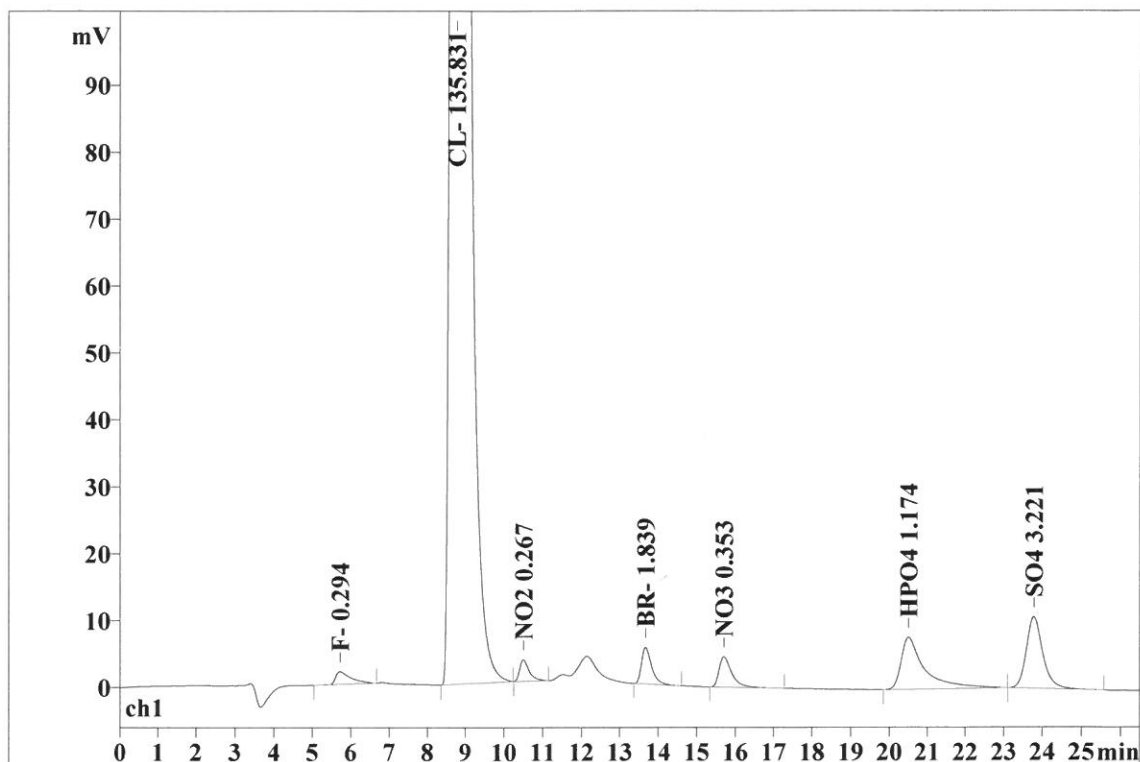

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.72             | 0.394          | 1.91         | 0.14        | 52.201         | 0.22      |
| 2  | 8.75             | 0.244          | 1326.15      | 97.52       | 23125.978      | 95.99     |
| 3  | 10.51            | 0.243          | 3.24         | 0.24        | 54.298         | 0.23      |
| 4  | 13.67            | 0.269          | 5.49         | 0.40        | 100.745        | 0.42      |
| 5  | 15.71            | 0.327          | 4.55         | 0.33        | 103.503        | 0.43      |
| 6  | 20.50            | 0.529          | 7.80         | 0.57        | 335.471        | 1.39      |
| 7  | 23.78            | 0.438          | 10.74        | 0.79        | 318.631        | 1.32      |
| 7  | 26.50            | 0.349          | 1359.88      | 100.00      | 24090.827      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/17/2022 3:23:35 PM  
Printed by: wet


Ident: N1565-01MSDX10  
Analysis from: 2/17/2022 12:31:34 PM  
File: \_2022-02-17\_

Last save: 2/17/2022 12:58:04 PM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30104

Last save: 2/9/2022 1:45:3

SAMPLE:  
: IZ/AP  
Vial number: 18  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

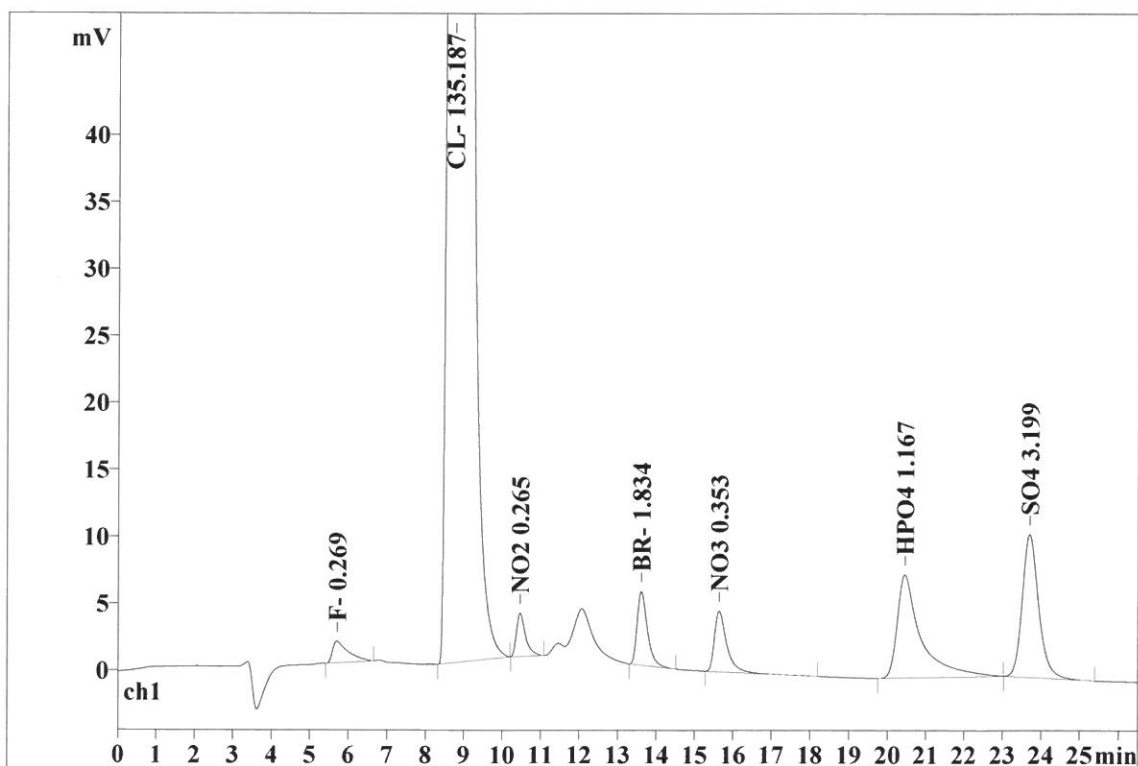

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.70             | 0.416          | 1.61         | 0.12        | 45.665         | 0.19      |
| 2  | 8.72             | 0.243          | 1325.66      | 97.55       | 23016.323      | 96.02     |
| 3  | 10.46            | 0.241          | 3.24         | 0.24        | 53.741         | 0.22      |
| 4  | 13.61            | 0.268          | 5.50         | 0.40        | 100.374        | 0.42      |
| 5  | 15.64            | 0.325          | 4.54         | 0.33        | 103.506        | 0.43      |
| 6  | 20.44            | 0.531          | 7.72         | 0.57        | 333.737        | 1.39      |
| 7  | 23.70            | 0.436          | 10.69        | 0.79        | 315.762        | 1.32      |
| 7  | 26.50            | 0.352          | 1358.95      | 100.00      | 23969.106      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/17/2022 3:23:42 PM  
Printed by: wet


Ident: CCV  
Analysis from: 2/17/2022 1:00:45 PM  
File: \_2022-02-17\_

Last save: 2/17/2022 1:27:15 PM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30105

Last save: 2/9/2022 1:45:3

SAMPLE:  
: IZ/AP  
Vial number: 11  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

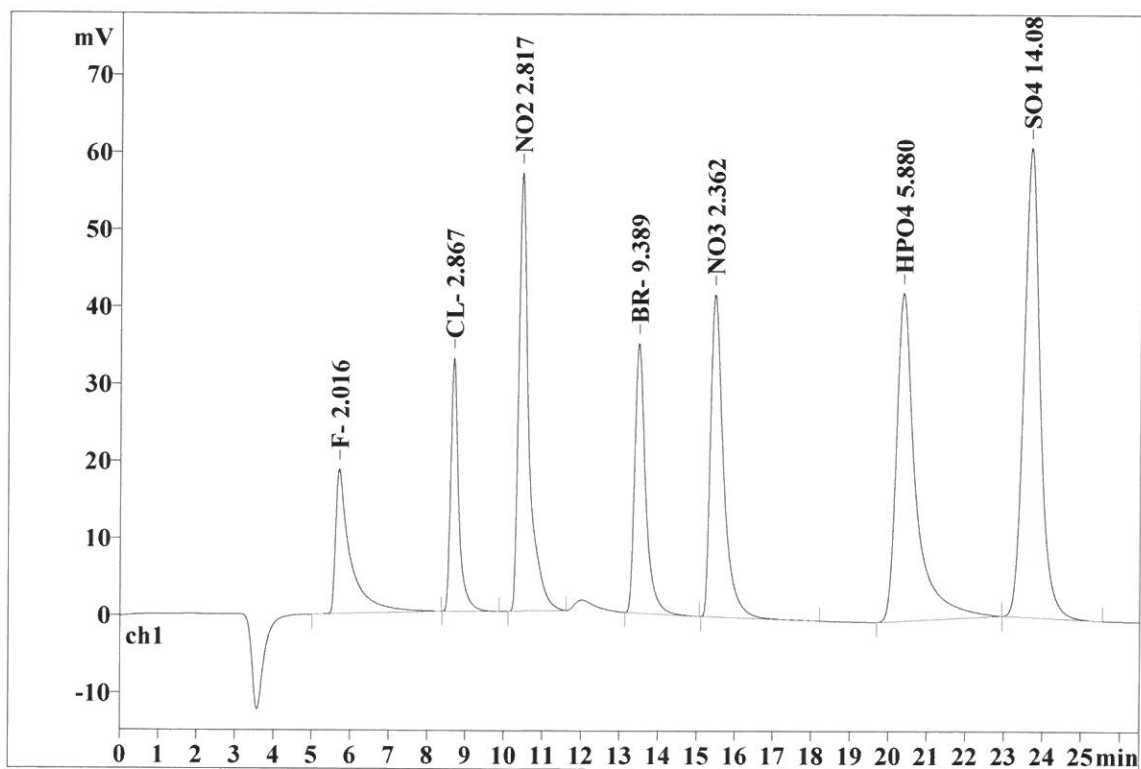

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.70             | 0.314          | 18.74        | 6.50        | 502.588        | 7.21      |
| 2  | 8.67             | 0.198          | 32.82        | 11.38       | 470.349        | 6.74      |
| 3  | 10.45            | 0.246          | 56.78        | 19.69       | 1053.417       | 15.10     |
| 4  | 13.47            | 0.285          | 34.94        | 12.12       | 692.481        | 9.93      |
| 5  | 15.46            | 0.337          | 41.77        | 14.48       | 984.072        | 14.11     |
| 6  | 20.36            | 0.455          | 42.49        | 14.73       | 1489.431       | 21.35     |
| 7  | 23.67            | 0.431          | 60.83        | 21.10       | 1782.703       | 25.56     |
| 7  | 26.50            | 0.324          | 288.36       | 100.00      | 6975.041       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/17/2022 3:23:50 PM  
Printed by: wet


Ident: CCB  
Analysis from: 2/17/2022 1:29:53 PM  
File: \_2022-02-17\_

Last save: 2/17/2022 1:56:23 PM

Method: AnionsIC2-020922.mtw  
Run operator: wet  
Analysis number: 30106

Last save: 2/9/2022 1:45:3

SAMPLE:  
: IZ/AP  
Vial number: 12  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

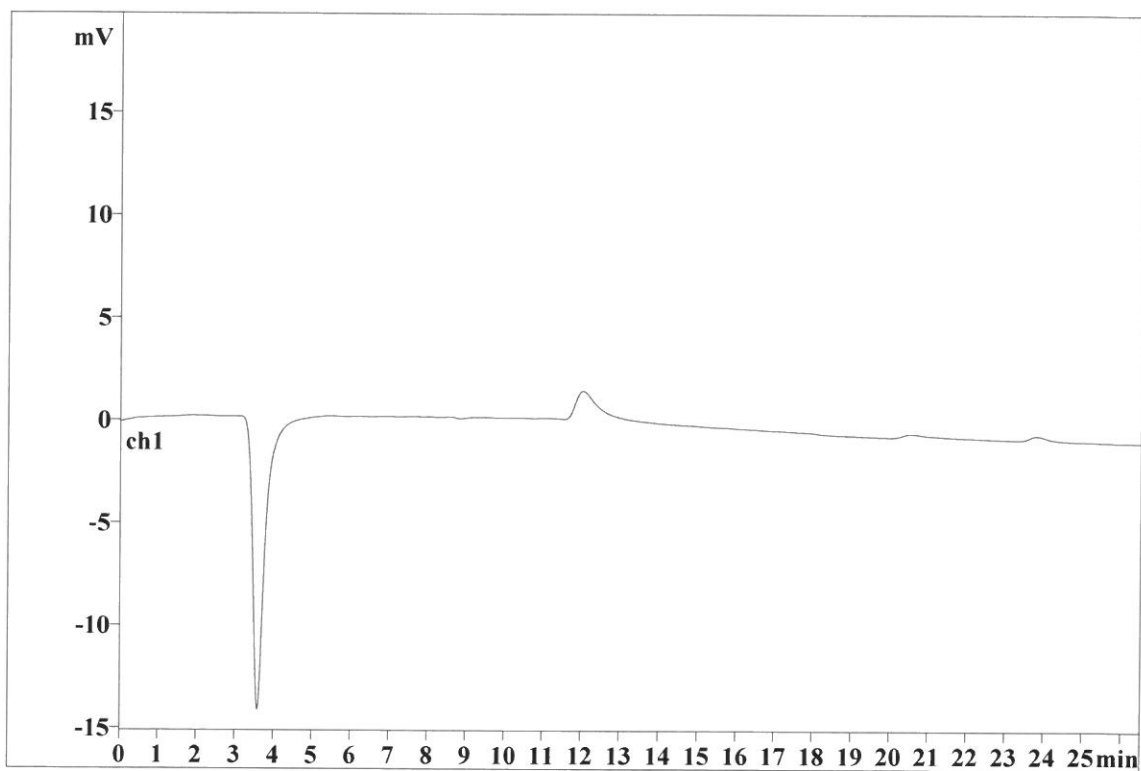

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD