

Clear table

Instrument ID: IC-2				Analyst : IZ		Method: 300.0 / 9056A					
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-02-09_	2/9/22 10:14		IZ/AP
STD2	0.4180	0.6650	0.6690	2.3100	0.5670	0.9300	3.5030	2022-02-09_	2/9/22 10:44		IZ/AP
STD3	0.8230	1.2010	1.2010	4.0240	1.0070	2.1230	6.0660	2022-02-09_	2/9/22 11:12		IZ/AP
STD4	0.9690	1.4880	1.4890	4.9210	1.2340	2.5290	7.3890	2022-02-09_	2/9/22 11:41		IZ/AP
STD5	1.9550	2.9440	2.9380	9.6950	2.4360	5.0230	14.4840	2022-02-09_	2/9/22 12:10		IZ/AP
STD6	4.0970	5.9230	5.9210	19.7690	4.9330	9.6840	29.5340	2022-02-09_	2/9/22 12:39		IZ/AP
STD7	4.9380	7.5780	7.5820	25.2810	6.3230	12.7100	38.0230	2022-02-09_	2/9/22 13:08		IZ/AP
ICV	2.1550	3.0390	2.9850	9.8860	2.5180	5.6190	14.8780	2022-02-10_	2/10/22 9:45		IZ/AP
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-02-10_	2/10/22 10:14		IZ/AP
CCV	2.0090	2.8120	2.7460	9.2220	2.3060	5.3320	13.8110	2022-02-18_	2/18/22 9:42		IZ/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-02-18_	2/18/22 10:12		IZ/AP
LB118748BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-02-18_	2/18/22 10:41		IZ/AP
LB118748BSW	1.9760	2.8050	2.7590	9.2060	2.3120	5.3430	13.7990	2022-02-18_	2/18/22 11:10		IZ/AP
N1603-02	0.0000	670.0170	0.0000	0.8350	1.2000	0.8630	16.1480	2022-02-18_	2/18/22 13:49		IZ/AP
N1604-01	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-02-18_	2/18/22 14:18		IZ/AP
N1604-02	0.0000	374.9070	0.0000	0.0000	0.3540	0.3350	9.4260	2022-02-18_	2/18/22 14:47		IZ/AP
N1604-04	0.0000	374.9670	0.0000	0.0000	0.3540	0.3390	9.4630	2022-02-18_	2/18/22 15:16		IZ/AP
N1613-01	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-02-18_	2/18/22 15:46		IZ/AP
N1613-01MS	2.1890	3.0070	2.9280	9.7970	2.4880	5.8180	14.7350	2022-02-18_	2/18/22 16:15		IZ/AP
N1613-01MSD	1.9590	2.8810	2.8320	9.4200	2.4010	5.4220	14.1620	2022-02-18_	2/18/22 16:44		IZ/AP
CCV	2.0110	2.8290	2.7830	9.2860	2.3420	5.5410	13.9250	2022-02-18_	2/18/22 17:13		IZ/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-02-18_	2/18/22 17:42		IZ/AP

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A


ident	concentratio tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-02-09_	2/9/22 10:14		IZ/AP
STD2	0.4180	0.6650	0.6690	2.3100	0.5670	0.9300	3.5030	2022-02-09_	2/9/22 10:44		IZ/AP
STD3	0.8230	1.2010	1.2010	4.0240	1.0070	2.1230	6.0660	2022-02-09_	2/9/22 11:12		IZ/AP
STD4	0.9690	1.4880	1.4890	4.9210	1.2340	2.5290	7.3890	2022-02-09_	2/9/22 11:41		IZ/AP
STD5	1.9550	2.9440	2.9380	9.6950	2.4360	5.0230	14.4840	2022-02-09_	2/9/22 12:10		IZ/AP
STD6	4.0970	5.9230	5.9210	19.7690	4.9330	9.6840	29.5340	2022-02-09_	2/9/22 12:39		IZ/AP
STD7	4.9380	7.5780	7.5820	25.2810	6.3230	12.7100	38.0230	2022-02-09_	2/9/22 13:08		IZ/AP

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1							
STD2	4.5000	10.8333	11.5000	15.5000	13.4000	-7.0000	16.7667
STD3	2.8750	0.0833	0.0833	0.6000	0.7000	6.1500	1.1000
STD4	-3.1000	-0.8000	-0.7333	-1.5800	-1.2800	1.1600	-1.4800
STD5	-2.2500	-1.8667	-2.0667	-3.0500	-2.5600	0.4600	-3.4400
STD6	2.4250	-1.2833	-1.3167	-1.1550	-1.3400	-3.1600	-1.5533
STD7	-1.2400	1.0400	1.0933	1.1240	1.1680	1.6800	2.7649

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-020922.mtw
 Equation: $Q = 0.0764573 \cdot A + 1.88372$
 RSD: 2.976 %
 Correlation coefficient: 0.999517

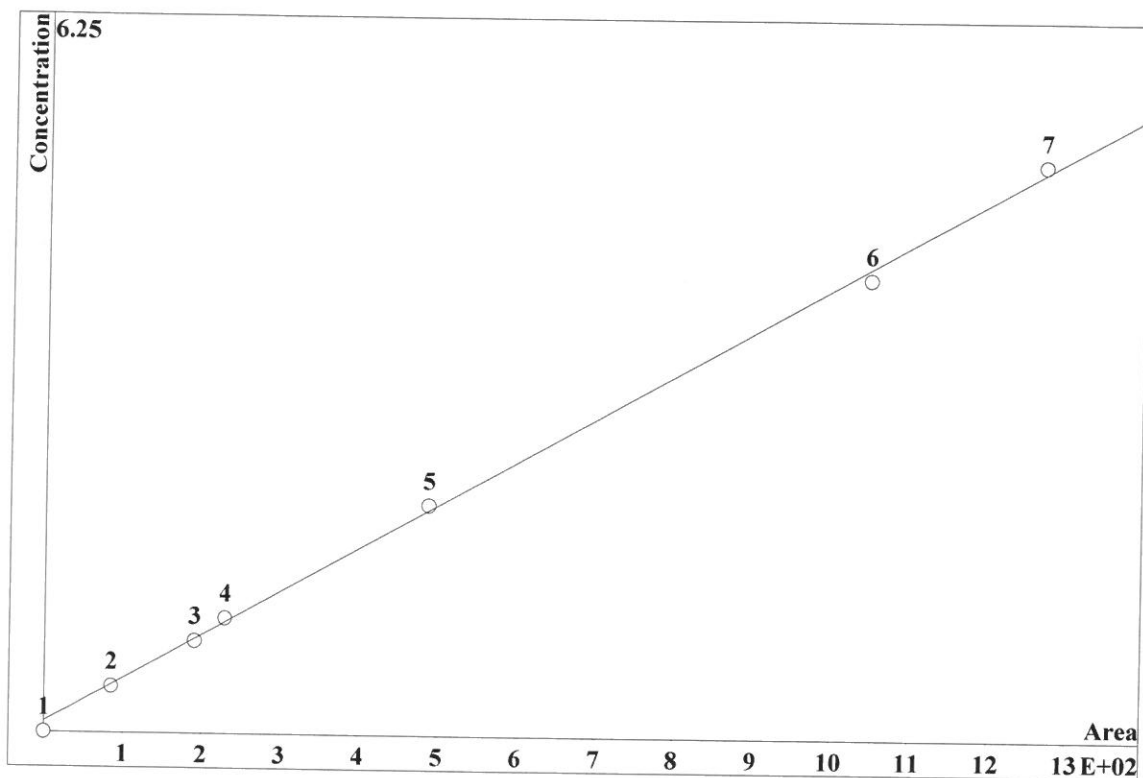


K3 = 0 K2 = 0 K1 = 0.0764573 K0 = 1.88372
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	3.083	84.81	0.4	20	5.653	
3	7.04	190.6	0.8	20	5.653	
4	7.797	228.7	1	20	5.653	
5	19.23	486.8	2	20	5.653	
6	42.9	1047	4	20	5.653	
7	49.77	1267	5	20	5.653	

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-020922.mtw
 Equation: $Q = 0.117378 \cdot A + 2.12854$
 RSD: 2.113 %
 Correlation coefficient: 0.999757

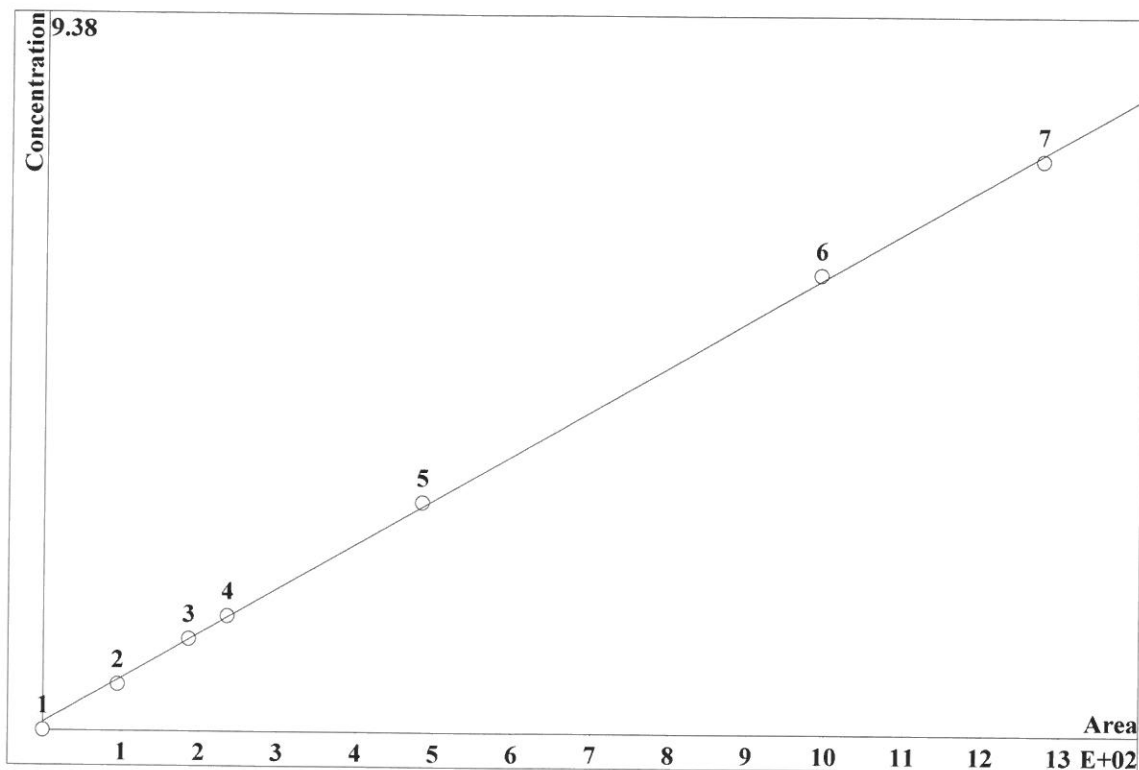


K3 = 0 K2 = 0 K1 = 0.117378 K0 = 2.12854
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	6.463	95.21	0.6	20	8.643		
3	12.62	186.5	1.2	20	8.643		
4	15.96	235.5	1.5	20	8.643		
5	33.32	483.5	3	20	8.643		
6	68.88	991.1	6	20	8.643		
7	89.91	1273	7.5	20	8.643		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-020922.mtw
 Equation: $Q = 0.051054 \cdot A + 2.56076$
 RSD: 2.235 %
 Correlation coefficient: 0.999728

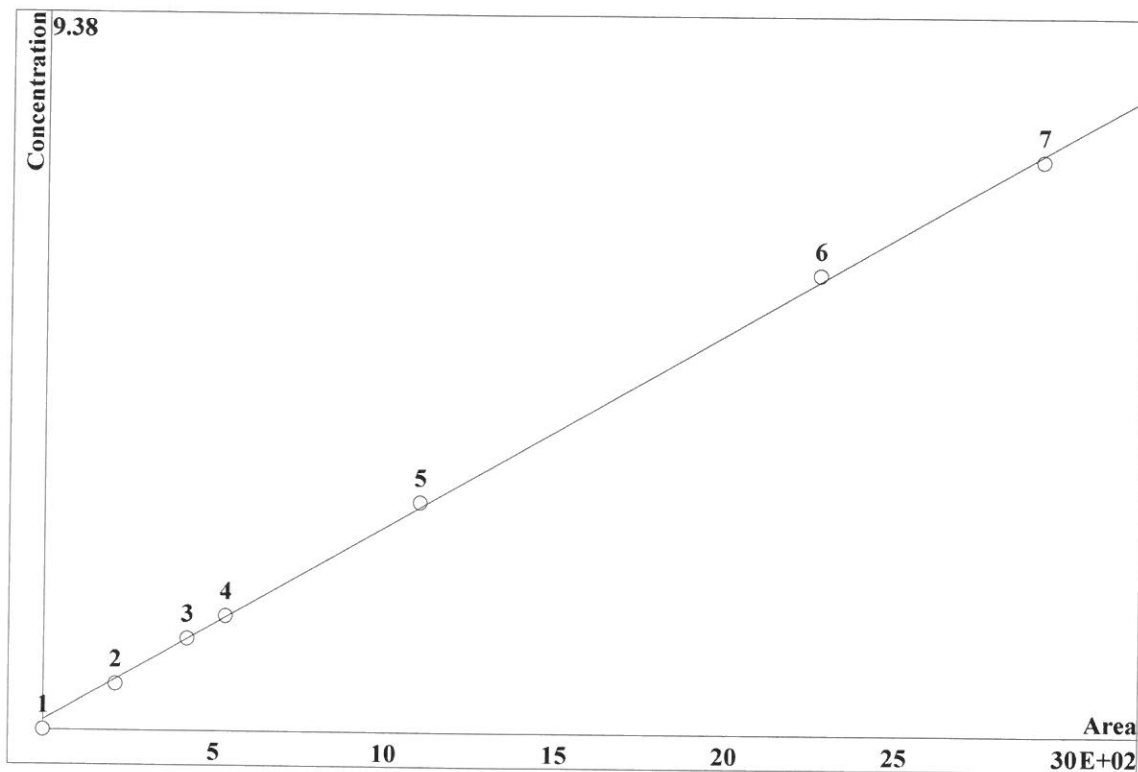


K3 = 0 K2 = 0 K1 = 0.051054 K0 = 2.56076
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	11.63	212	0.6	20	10.46		
3	23.16	420.4	1.2	20	10.46		
4	29.36	533.1	1.5	20	10.46		
5	59.9	1101	3	20	10.46		
6	121.8	2269	6	20	10.46		
7	155.4	2920	7.5	20	10.46		

*□

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-020922.mtw
 Equation: $Q = 0.255164 \cdot A + 11.0743$
 RSD: 2.607 %
 Correlation coefficient: 0.999630

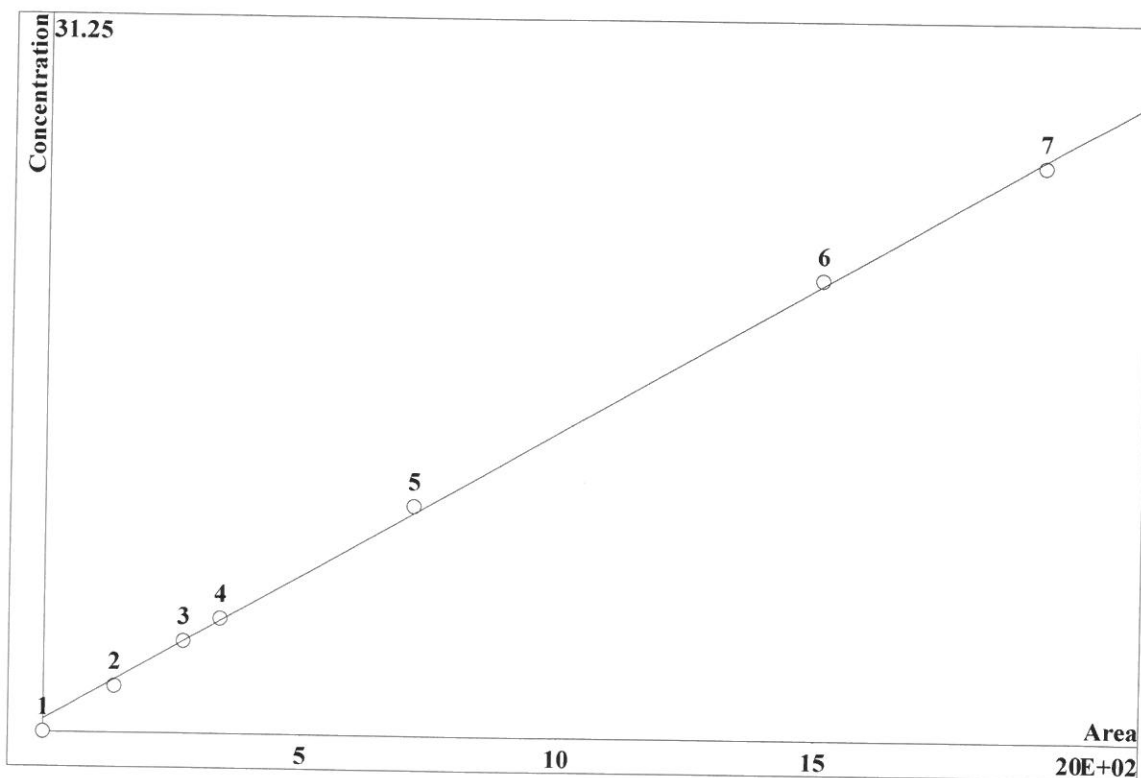


K3 = 0 K2 = 0 K1 = 0.255164 K0 = 11.0743
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.658	137.7	2	20	13.53		
3	13.38	272	4	20	13.53		
4	17.03	342.3	5	20	13.53		
5	35.75	716.5	10	20	13.53		
6	74.76	1506	20	20	13.53		
7	96.87	1938	25	20	13.53		

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-020922.mtw
 Equation: $Q = 0.0456384 \cdot A + 2.3263$
 RSD: 2.481 %
 Correlation coefficient: 0.999664

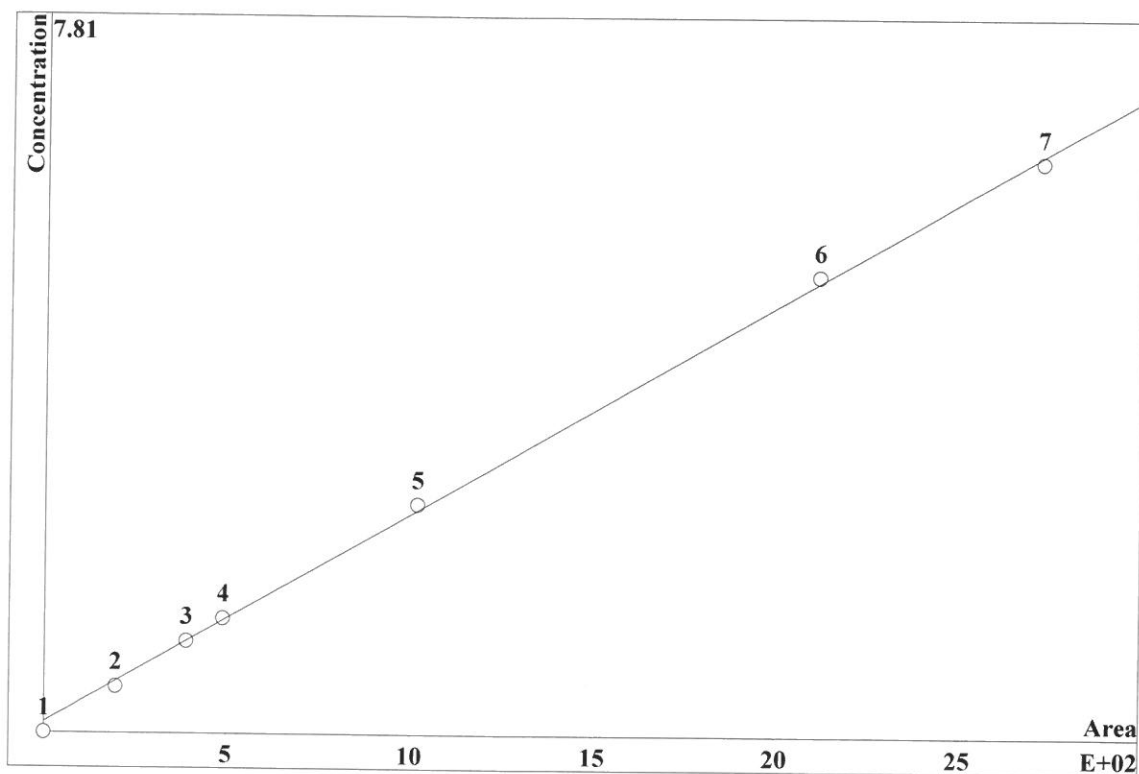


K3 = 0 K2 = 0 K1 = 0.0456384 K0 = 2.3263
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	8.047	197.3	0.5	20	15.58		
3	16.02	390.5	1	20	15.58		
4	20.32	489.8	1.25	20	15.58		
5	42.36	1017	2.5	20	15.58		
6	88.55	2111	5	20	15.58		
7	115.1	2720	6.25	20	15.58		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-020922.mtw
 Equation: $Q = 0.0815612 \cdot A - 3.88126$
 RSD: 3.697 %
 Correlation coefficient: 0.999255

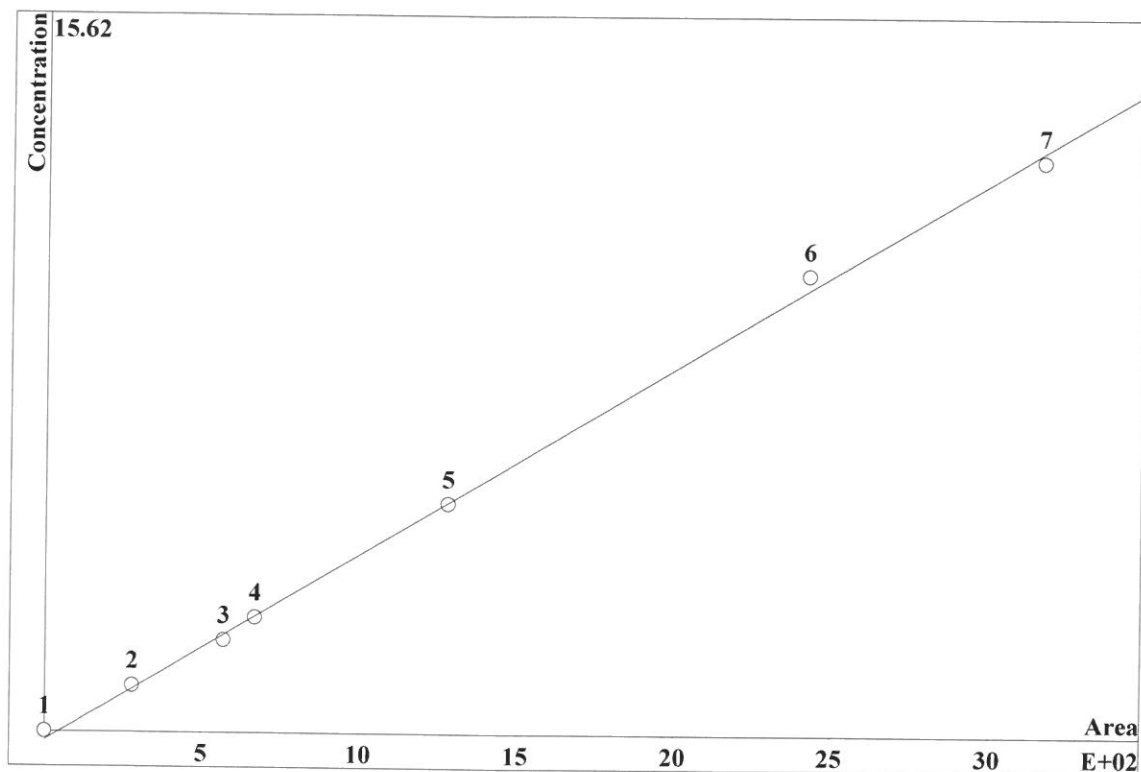


K3 = 0 K2 = 0 K1 = 0.0815612 K0 = -3.88126
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	7.423	275.7	1	20	20.18		
3	15.55	568.3	2	20	20.18		
4	18.32	667.7	2.5	20	20.18		
5	37.46	1279	5	20	20.18		
6	72.93	2422	10	20	20.18		
7	88.68	3164	12.5	20	20.18		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-020922.mtw
 Equation: $Q = 0.148372 \cdot A + 17.1343$
 RSD: 3.070 %
 Correlation coefficient: 0.999486

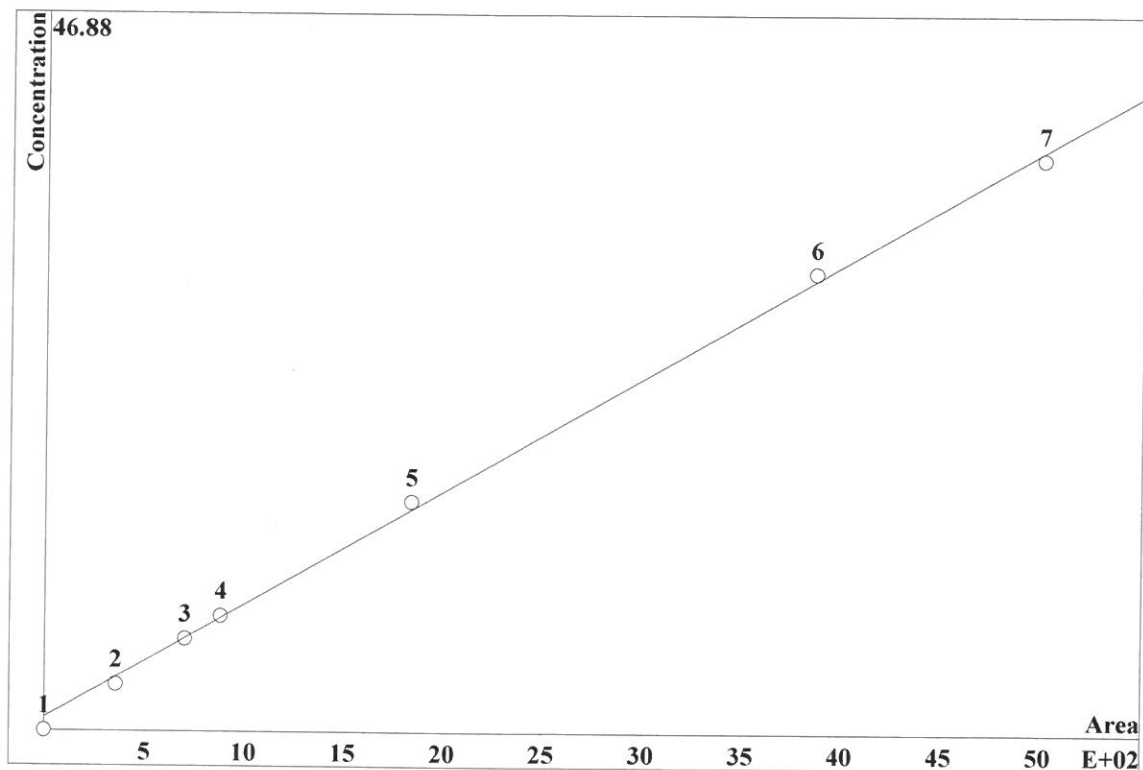

K3 = 0 K2 = 0 K1 = 0.148372 K0 = 17.1343
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	11.82	356.7	3	20	23.09		
3	23.46	702.2	6	20	23.09		
4	29.62	880.6	7.5	20	23.09		
5	62.43	1837	15	20	23.09		
6	134	3866	30	20	23.09		
7	175	5010	37.5	20	23.09		

Report date: 2/11/2022 9:12:12 AM
Printed by: wet


Ident: STD1
Analysis from: 2/9/2022 10:14:56 AM
File: _2022-02-09_

Last save: 2/9/2022 1:45:42 PM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30021

Last save: 2/9/2022 1:43:1

SAMPLE:
: IZ/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

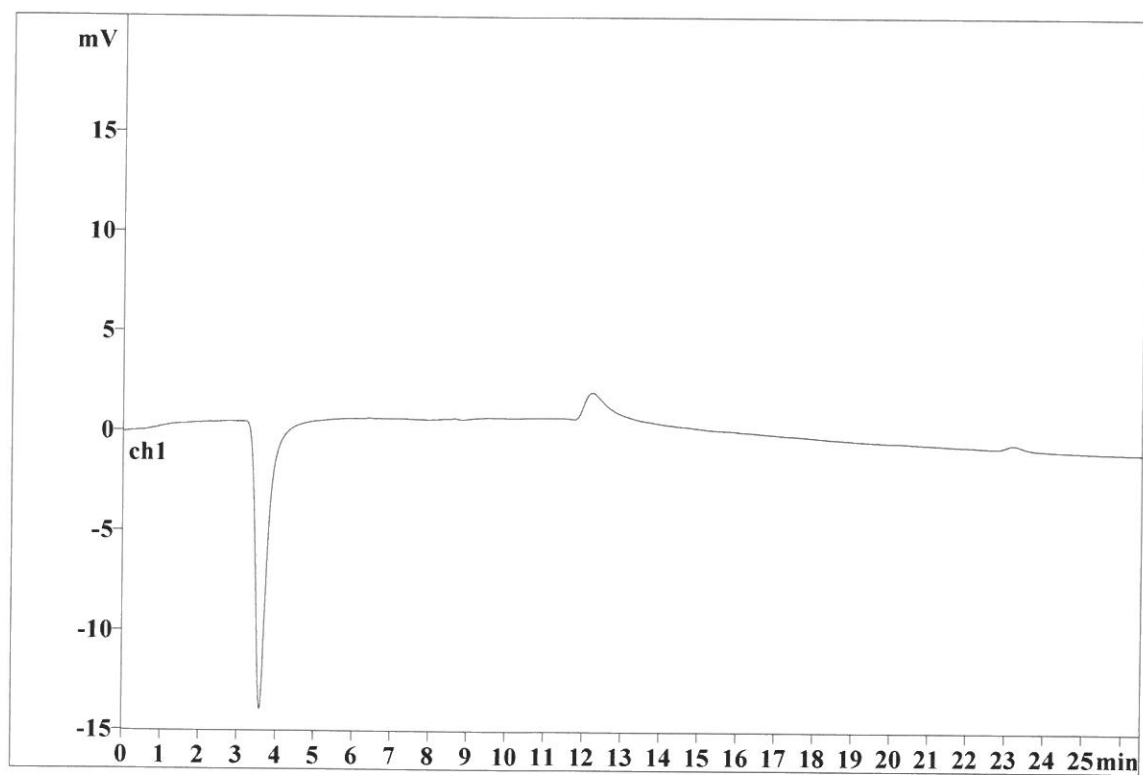

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 2/11/2022 9:15:38 AM
Printed by: wet


Ident: STD2
Analysis from: 2/9/2022 10:44:04 AM
File: _2022-02-09_

Last save: 2/11/2022 9:13:06 AM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30022

Last save: 2/9/2022 1:43:1

SAMPLE:
: IZ/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

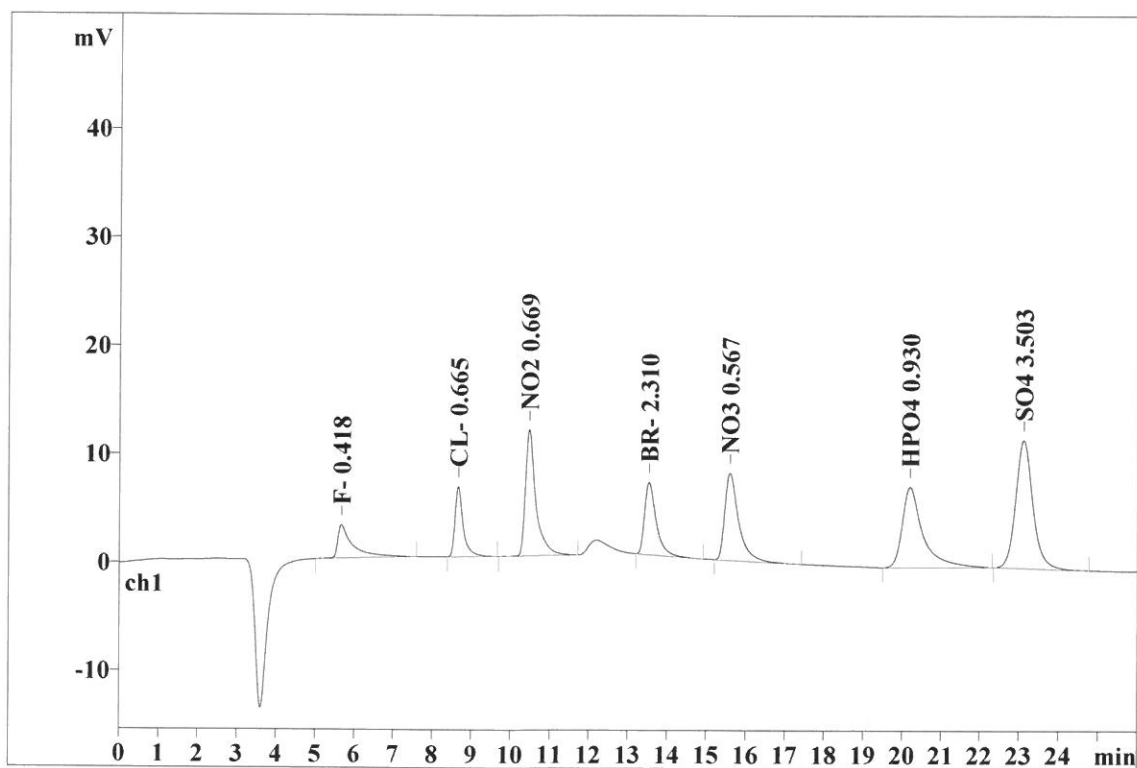

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.65	0.310	3.08	5.59	84.812	6.24
2	8.64	0.203	6.46	11.73	95.209	7.00
3	10.46	0.244	11.63	21.10	212.013	15.59
4	13.53	0.297	6.66	12.08	137.697	10.13
5	15.58	0.350	8.05	14.60	197.333	14.51
6	20.18	0.488	7.42	13.47	275.747	20.28
7	23.09	0.442	11.81	21.43	356.702	26.24
7	26.00	0.334	55.12	99.99	1359.513	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/11/2022 9:16:00 AM
Printed by: wet


Ident: STD3
Analysis from: 2/9/2022 11:12:41 AM
File: _2022-02-09_

Last save: 2/11/2022 9:13:06 AM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30023

Last save: 2/9/2022 1:43:1

SAMPLE:
: IZ/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

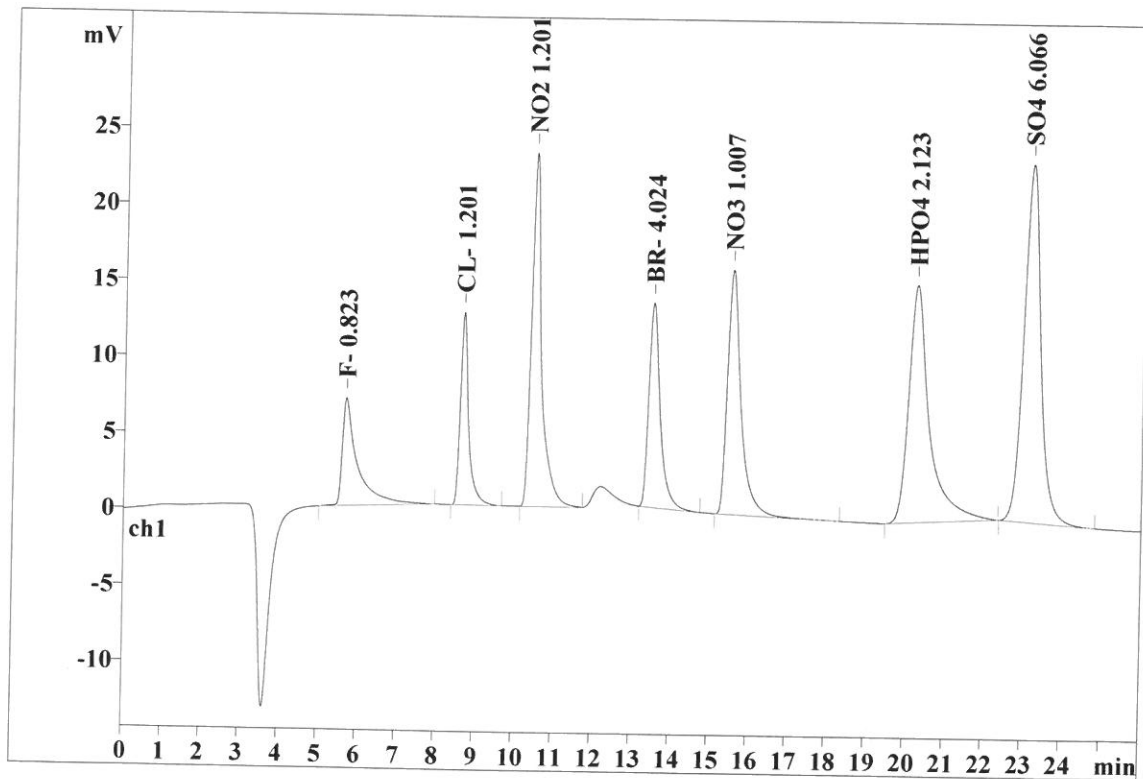

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.67	0.312	7.04	6.33	190.598	6.98
2	8.65	0.203	12.62	11.35	186.486	6.83
3	10.45	0.241	23.16	20.82	420.441	15.40
4	13.51	0.294	13.38	12.03	272.020	9.96
5	15.52	0.347	16.02	14.40	390.458	14.30
6	20.22	0.480	15.55	13.98	568.297	20.81
7	23.14	0.439	23.46	21.09	702.248	25.72
7	26.00	0.331	111.23	99.99	2730.549	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/11/2022 9:16:11 AM
Printed by: wet


Ident: STD4
Analysis from: 2/9/2022 11:41:19 AM
File: _2022-02-09_

Last save: 2/11/2022 9:13:06 AM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30024

Last save: 2/9/2022 1:43:1

SAMPLE:
: IZ/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

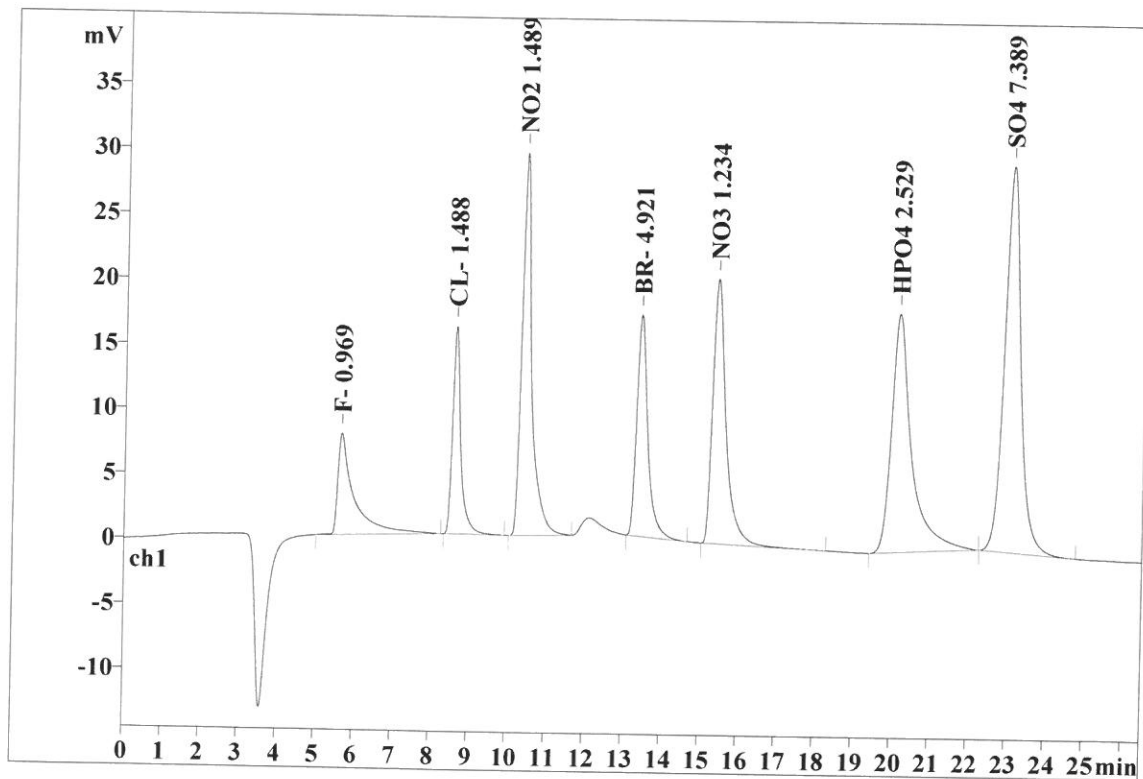

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.65	0.323	7.79	5.63	228.707	6.77
2	8.61	0.203	15.96	11.53	235.452	6.97
3	10.39	0.242	29.36	21.21	533.132	15.78
4	13.41	0.290	17.03	12.30	342.291	10.13
5	15.40	0.343	20.32	14.68	489.764	14.50
6	20.14	0.479	18.31	13.23	667.688	19.77
7	23.06	0.435	29.62	21.40	880.586	26.07
7	26.50	0.331	138.40	99.99	3377.621	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/11/2022 9:16:19 AM
Printed by: wet


Ident: STD5
Analysis from: 2/9/2022 12:10:27 PM
File: _2022-02-09_

Last save: 2/11/2022 9:13:06 AM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30025

Last save: 2/9/2022 1:43:1

SAMPLE:
: IZ/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

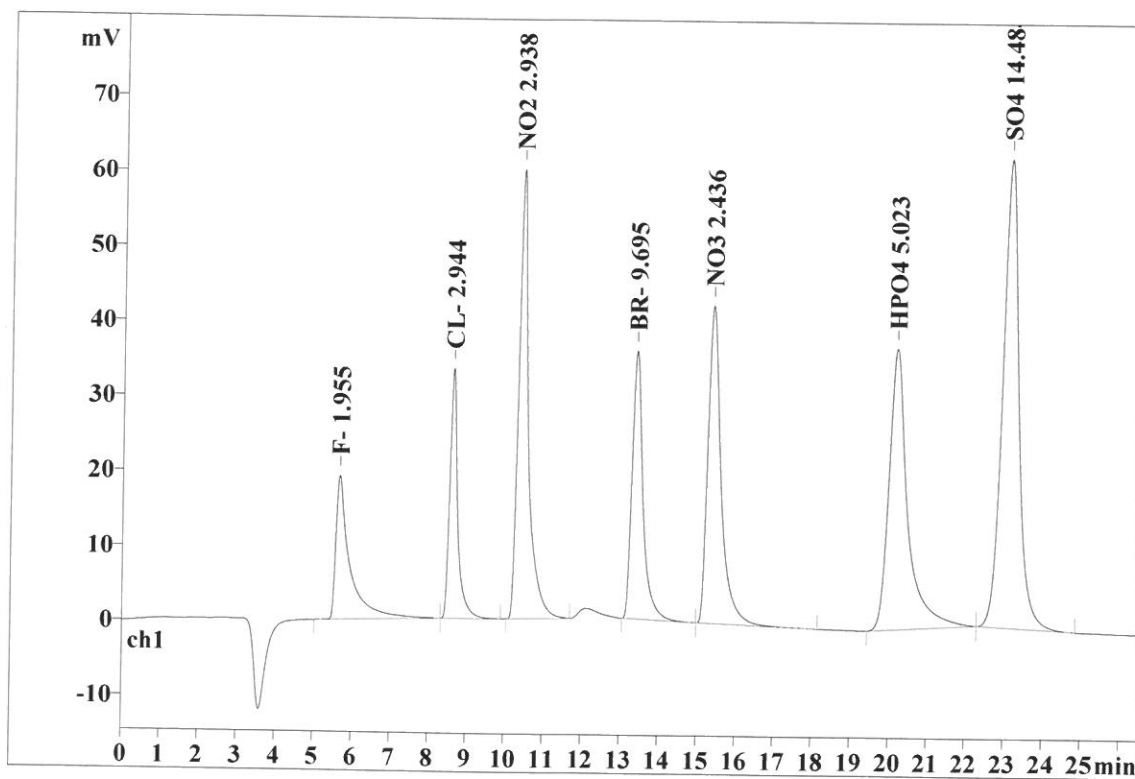

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.65	0.291	19.23	6.62	486.802	7.03
2	8.60	0.199	33.32	11.47	483.534	6.99
3	10.38	0.246	59.90	20.62	1100.787	15.91
4	13.38	0.286	35.74	12.31	716.475	10.35
5	15.34	0.340	42.36	14.58	1016.745	14.69
6	20.13	0.453	37.46	12.90	1279.215	18.48
7	23.07	0.429	62.43	21.50	1836.939	26.54
7	26.50	0.320	290.44	100.00	6920.497	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/11/2022 9:16:35 AM
Printed by: wet


Ident: STD6
Analysis from: 2/9/2022 12:39:35 PM
File: _2022-02-09_

Last save: 2/11/2022 9:13:06 AM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30026

Last save: 2/9/2022 1:43:1

SAMPLE:
: IZ/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

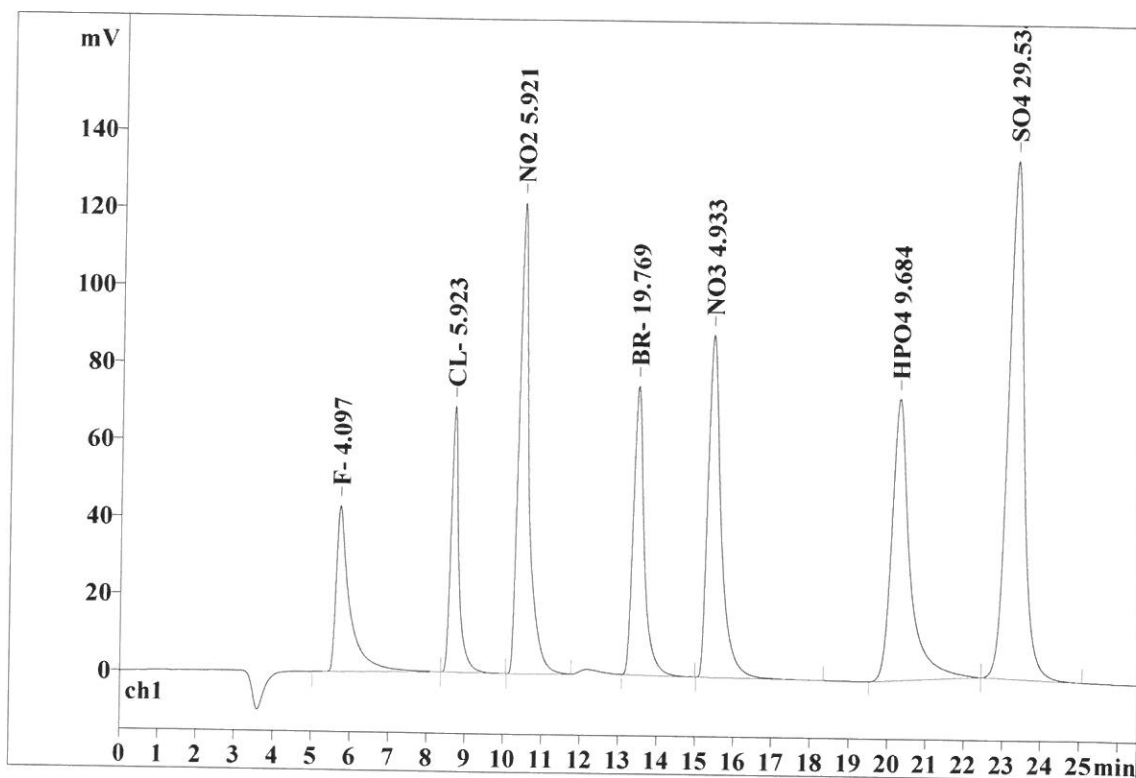

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.70	0.301	42.90	7.10	1047.105	7.37
2	8.65	0.197	68.88	11.41	991.148	6.97
3	10.41	0.250	121.81	20.17	2269.207	15.97
4	13.44	0.290	74.76	12.38	1506.105	10.60
5	15.38	0.338	88.55	14.67	2110.715	14.85
6	20.22	0.444	72.92	12.08	2422.309	17.04
7	23.23	0.422	133.96	22.19	3865.583	27.20
7	26.50	0.320	603.78	100.00	14212.172	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/11/2022 9:16:47 AM
Printed by: wet


Ident: STD7
Analysis from: 2/9/2022 1:08:43 PM
File: _2022-02-09_

Last save: 2/11/2022 9:13:06 AM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30027

Last save: 2/9/2022 1:43:1

SAMPLE:
: IZ/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

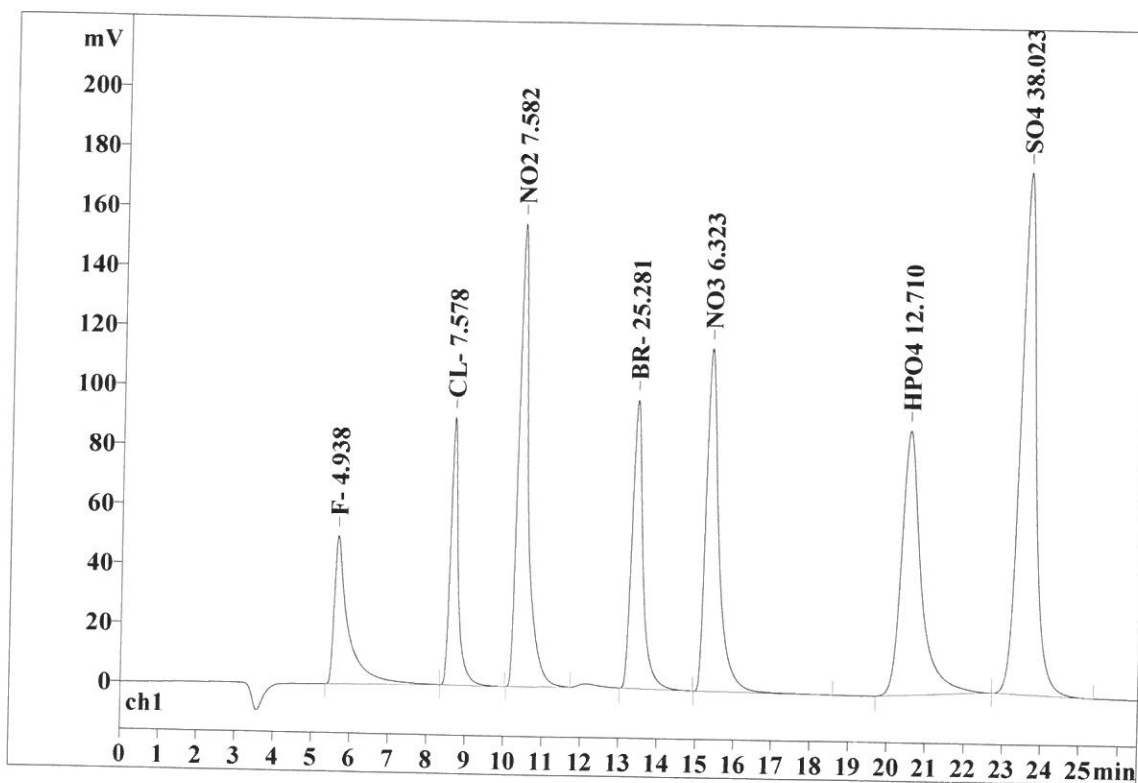

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.65	0.299	49.77	6.46	1267.058	6.93
2	8.63	0.193	89.91	11.67	1273.069	6.96
3	10.37	0.253	155.41	20.16	2919.971	15.96
4	13.39	0.287	96.87	12.57	1938.144	10.60
5	15.30	0.334	115.06	14.93	2719.910	14.87
6	20.51	0.489	88.68	11.51	3164.352	17.30
7	23.52	0.418	174.99	22.71	5009.882	27.39
7	26.50	0.325	770.69	100.00	18292.386	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/24/2022 8:23:58 AM
Printed by: wet


Ident: ICV
Analysis from: 2/10/2022 9:45:21 AM
File: _2022-02-10_

Last save: 2/24/2022 8:23:26 AM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30037

Last save: 2/9/2022 1:45:3

SAMPLE:
: IZ/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

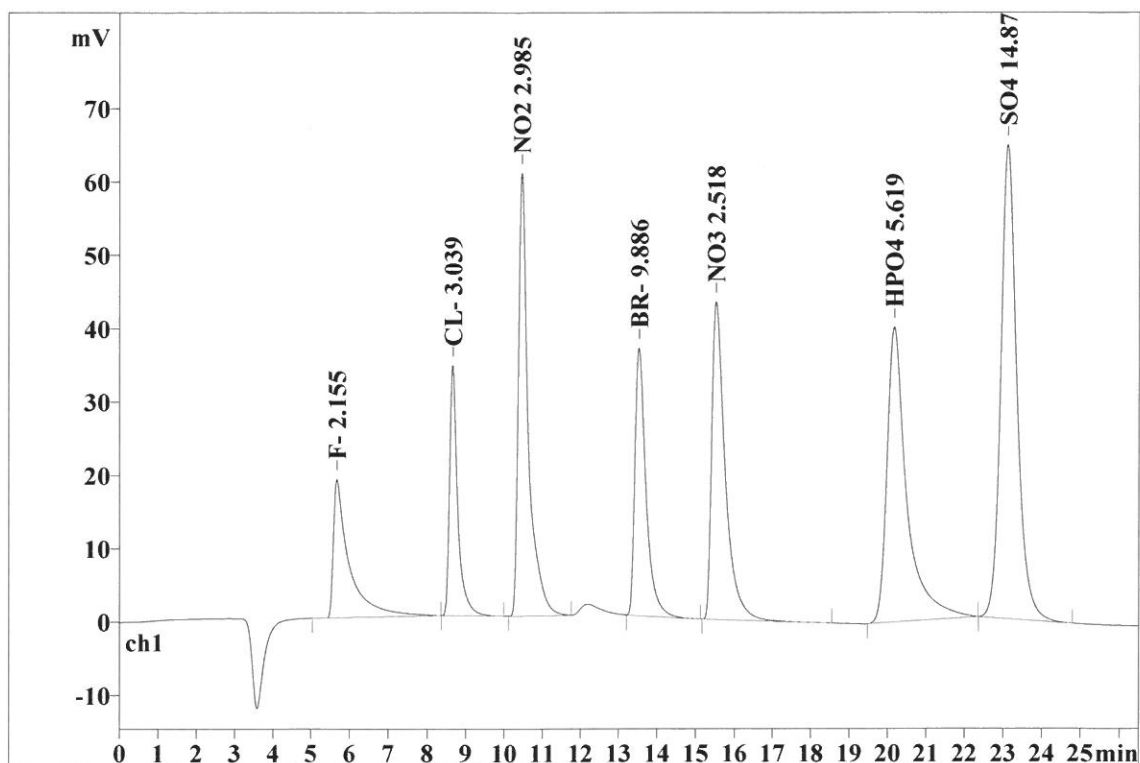

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.68	0.330	18.85	6.33	539.176	7.43
2	8.66	0.200	34.09	11.44	499.748	6.89
3	10.46	0.243	60.39	20.27	1119.178	15.42
4	13.54	0.288	36.49	12.25	731.456	10.08
5	15.53	0.345	43.30	14.53	1052.599	14.50
6	20.17	0.466	40.20	13.49	1425.503	19.64
7	23.12	0.429	64.59	21.68	1890.083	26.04
7	26.50	0.329	297.91	100.00	7257.743	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/24/2022 8:24:17 AM
Printed by: wet


Ident: ICB
Analysis from: 2/10/2022 10:14:31 AM
File: _2022-02-10_

Last save: 2/24/2022 8:23:26 AM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30038

Last save: 2/9/2022 1:45:3

SAMPLE:
: IZ/AP
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

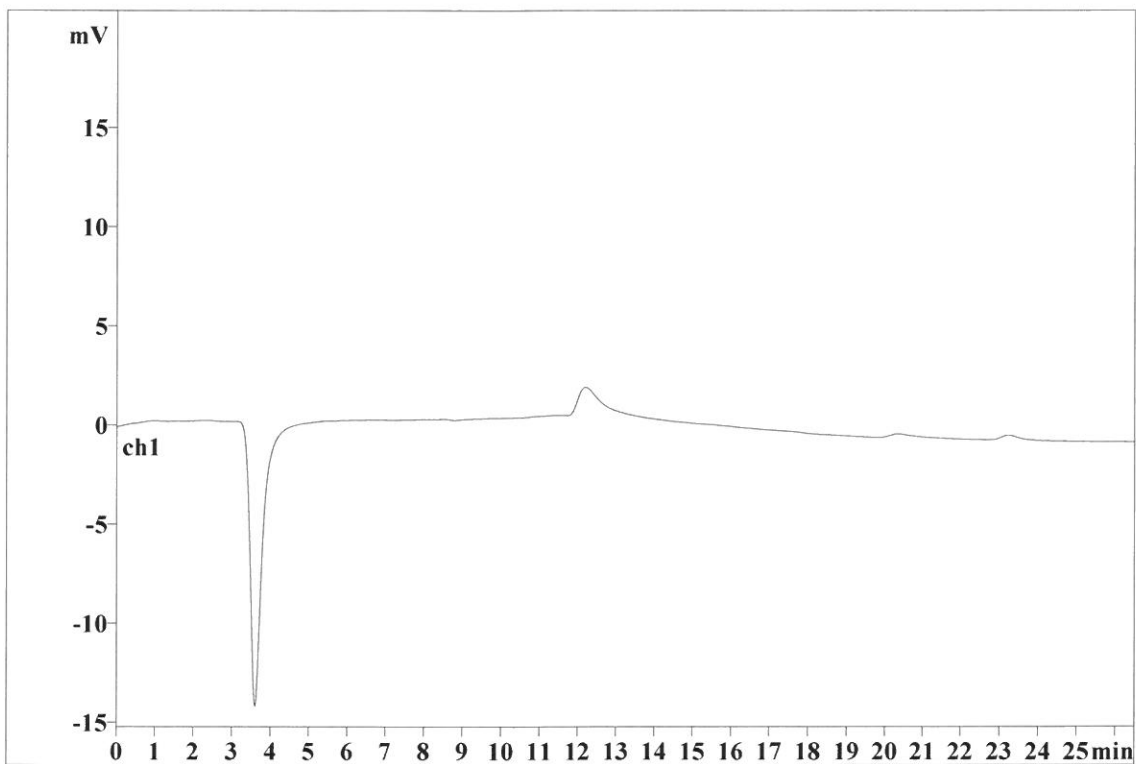

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 2/18/2022 4:31:12 PM
Printed by: wet


Ident: CCV
Analysis from: 2/18/2022 9:42:59 AM
File: _2022-02-18_

Last save: 2/18/2022 10:09:29 AM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30109

Last save: 2/9/2022 1:45:3

SAMPLE:
: IZ/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

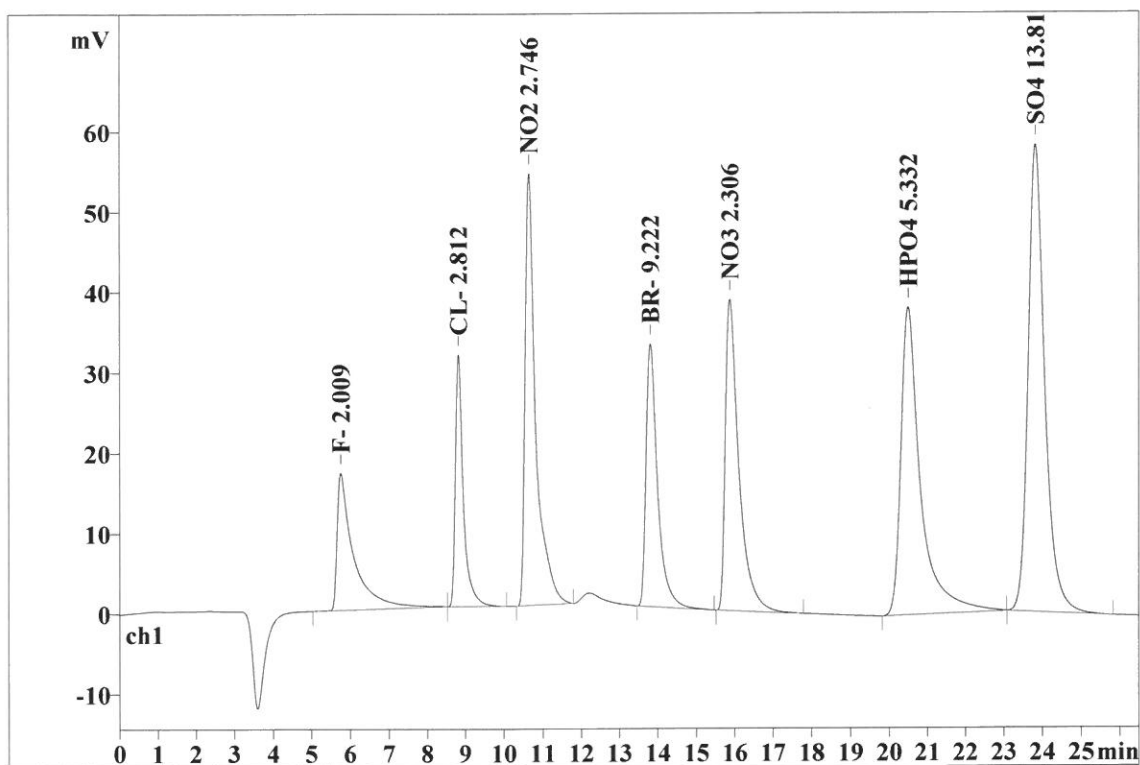

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.76	0.344	17.07	6.33	500.904	7.45
2	8.81	0.201	31.29	11.59	461.006	6.85
3	10.65	0.251	53.75	19.91	1025.663	15.25
4	13.81	0.297	32.65	12.10	679.414	10.10
5	15.88	0.353	38.70	14.34	959.487	14.26
6	20.49	0.462	38.28	14.18	1355.176	20.14
7	23.83	0.439	58.16	21.55	1746.145	25.95
7	26.50	0.335	269.89	100.00	6727.795	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/18/2022 4:31:29 PM
Printed by: wet


Ident: CCB
Analysis from: 2/18/2022 10:12:11 AM
File: _2022-02-18_

Last save: 2/18/2022 10:38:42 AM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30110

Last save: 2/9/2022 1:45:3

SAMPLE:
: IZ/AP
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

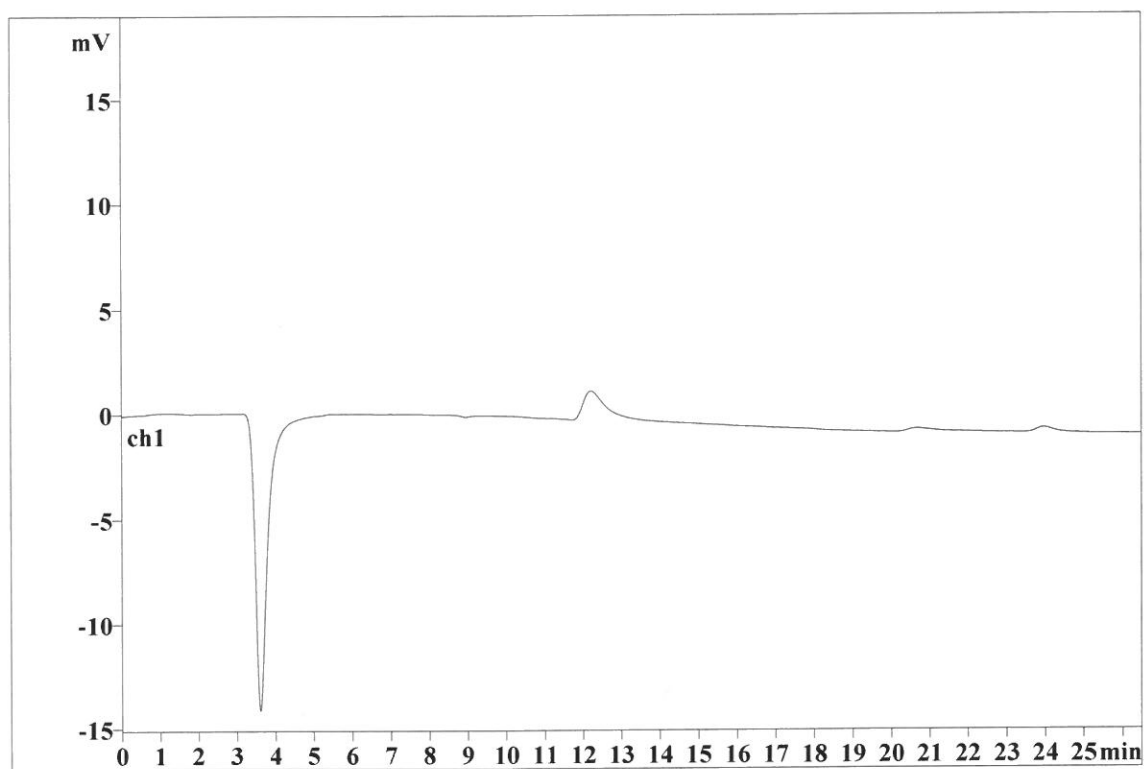

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 2/18/2022 4:31:40 PM
Printed by: wet


Ident: LB118748BLW
Analysis from: 2/18/2022 10:41:21 AM
File: _2022-02-18_

Last save: 2/18/2022 4:20:41 PM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30111

Last save: 2/9/2022 1:45:3

SAMPLE:
: IZ/AP
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

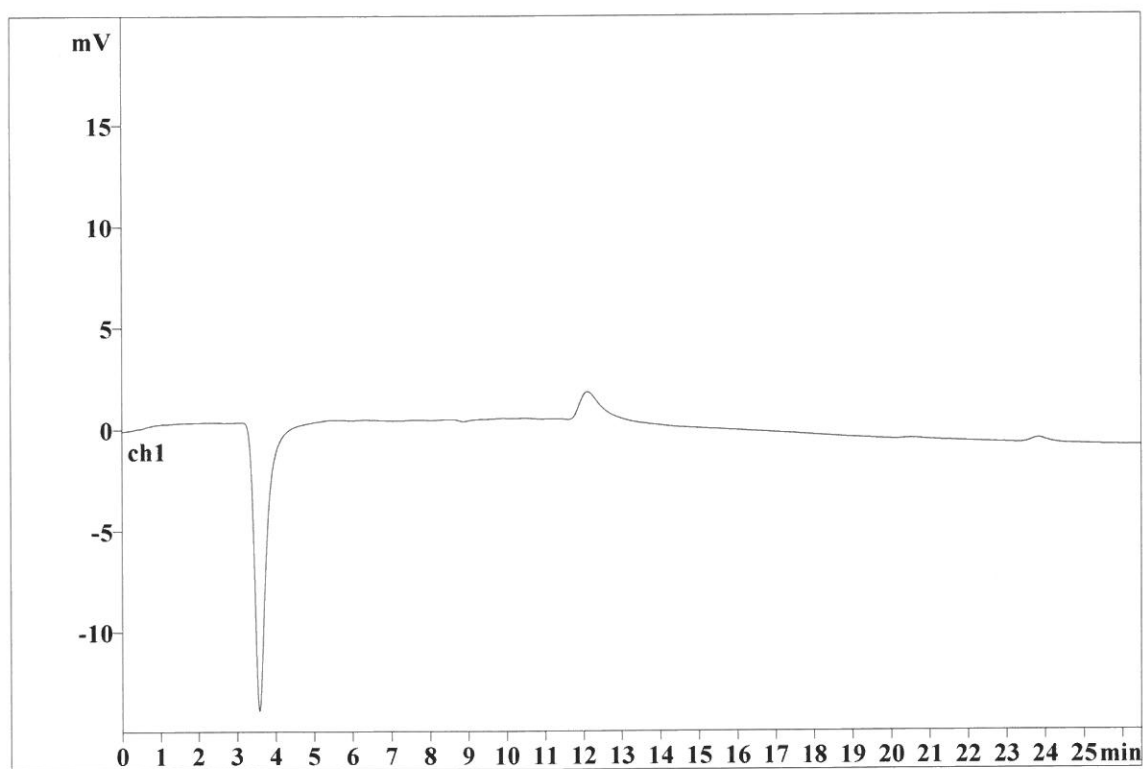

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 2/18/2022 4:31:53 PM
Printed by: wet


Ident: LB118748BSW
Analysis from: 2/18/2022 11:10:29 AM
File: _2022-02-18_

Last save: 2/18/2022 4:20:41 PM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30112

Last save: 2/9/2022 1:45:3

SAMPLE:
: IZ/AP
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

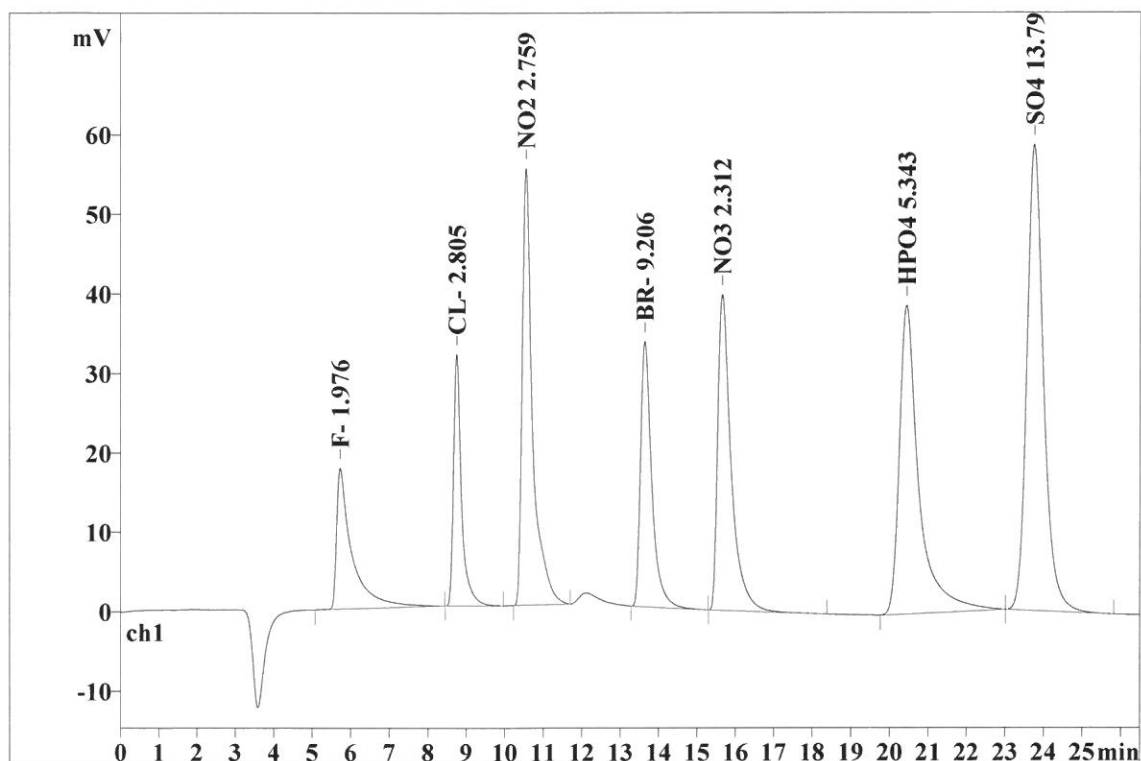

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.73	0.323	17.73	6.45	492.253	7.32
2	8.74	0.198	31.69	11.52	459.888	6.84
3	10.54	0.246	54.98	19.99	1030.737	15.32
4	13.63	0.290	33.39	12.14	678.177	10.08
5	15.66	0.344	39.75	14.45	962.392	14.31
6	20.43	0.456	38.85	14.12	1357.871	20.19
7	23.76	0.436	58.65	21.32	1744.633	25.94
7	26.50	0.328	275.04	100.00	6725.953	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/18/2022 4:32:15 PM
Printed by: wet


Ident: N1603-02
Analysis from: 2/18/2022 1:49:33 PM
File: _2022-02-18_

Last save: 2/18/2022 4:10:45 PM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30115

Last save: 2/9/2022 1:45:3

SAMPLE:
: IZ/AP
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

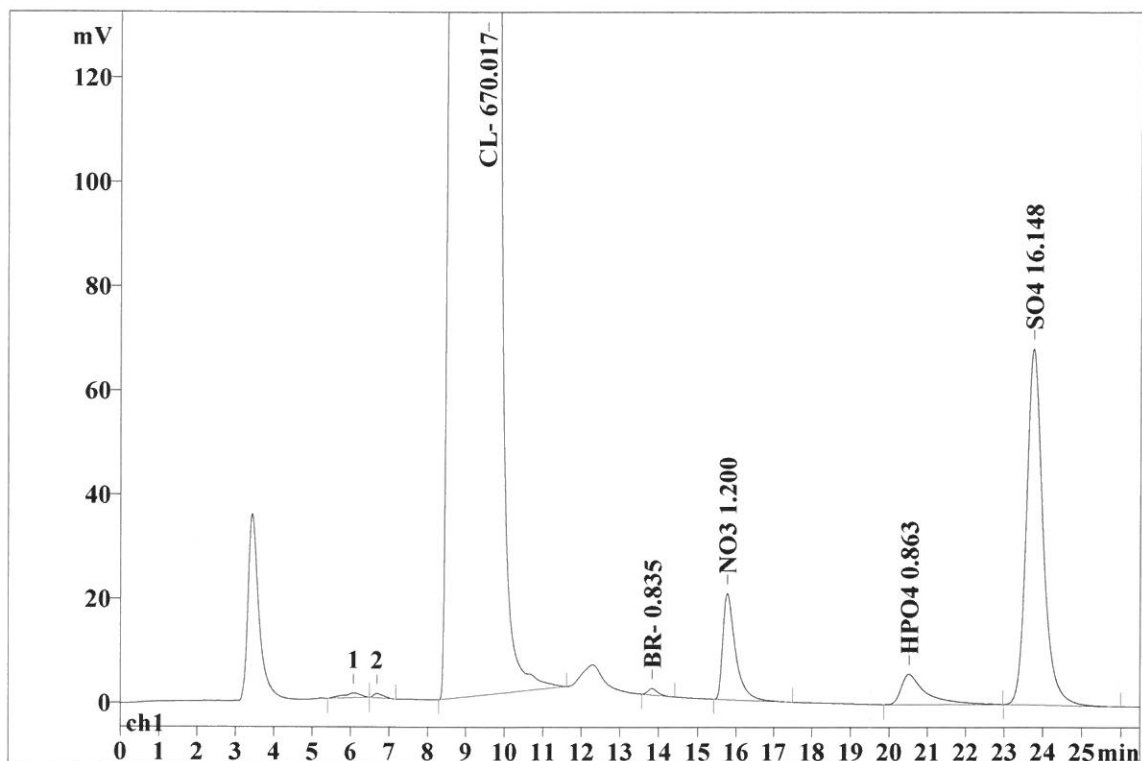

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.50	1.129	1700.83	94.57	114145.379	97.55
3	0.00	0.000	0.00	0.00	0.000	0.00
4	13.83	0.271	1.25	0.07	22.083	0.02
5	15.77	0.332	20.41	1.13	474.710	0.41
6	20.52	0.561	5.83	0.32	259.218	0.22
7	23.75	0.440	68.35	3.80	2061.205	1.76
7	26.50	0.390	1796.67	99.90	116962.594	99.96

This report has been created by IC Net
METROHM LTD

Report date: 2/18/2022 4:32:25 PM
Printed by: wet


Ident: N1604-01
Analysis from: 2/18/2022 2:18:41 PM
File: _2022-02-18_

Last save: 2/18/2022 2:45:12 PM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30116

Last save: 2/9/2022 1:45:3

SAMPLE:
: IZ/AP
Vial number: 16
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

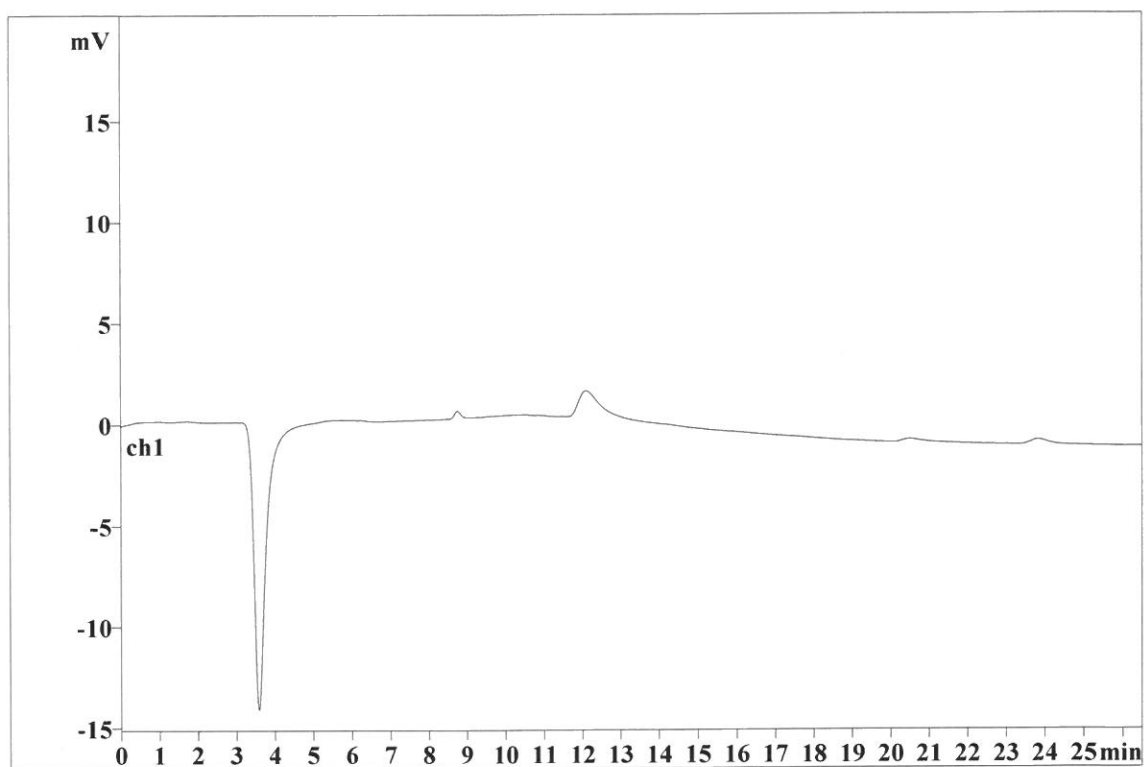

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 2/18/2022 4:32:44 PM
Printed by: wet


Ident: N1604-02
Analysis from: 2/18/2022 2:47:50 PM
File: _2022-02-18_

Last save: 2/18/2022 4:09:55 PM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30117

Last save: 2/9/2022 1:45:3

SAMPLE:
: IZ/AP
Vial number: 17
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

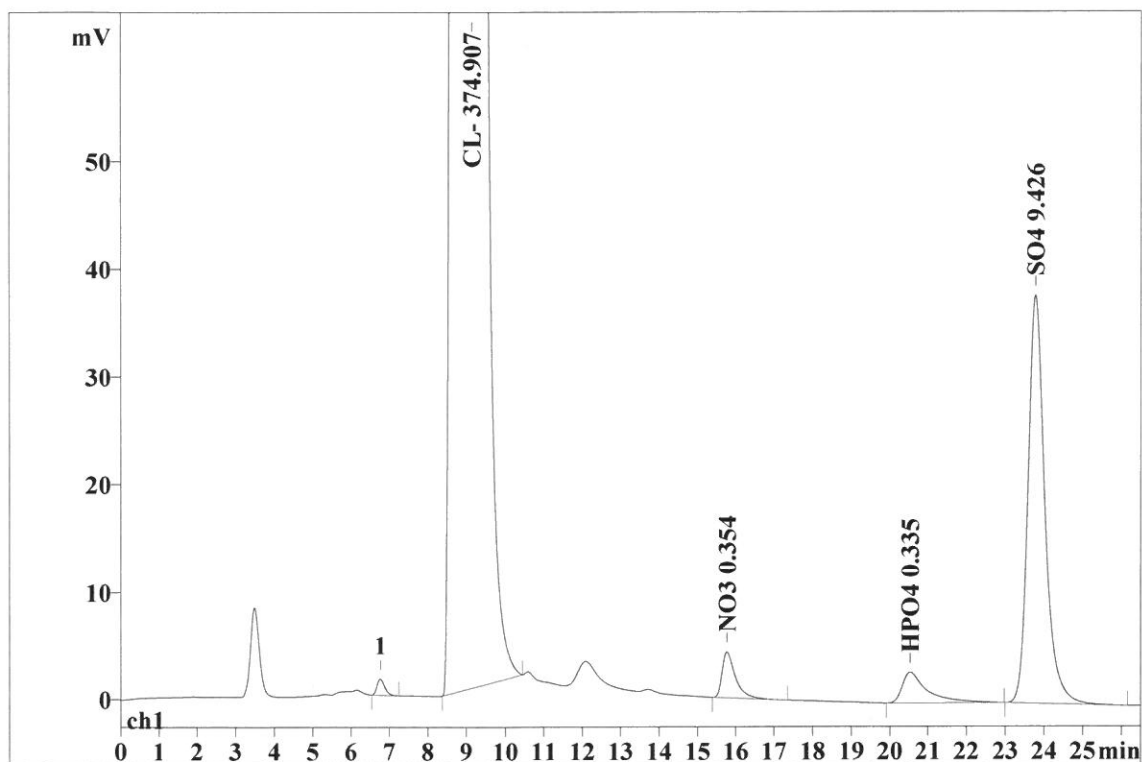

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.12	0.638	1648.33	97.25	63861.911	97.84
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.78	0.348	4.29	0.25	103.954	0.16
6	20.54	0.575	2.87	0.17	129.669	0.20
7	23.78	0.444	37.96	2.24	1155.068	1.77
7	26.50	0.286	1693.45	99.91	65250.602	99.97

This report has been created by IC Net
METROHM LTD

Report date: 2/18/2022 4:32:58 PM
 Printed by: wet


Ident: N1604-04
 Analysis from: 2/18/2022 3:16:58 PM
 File: _2022-02-18_

Last save: 2/18/2022 4:11:14 PM

Method: AnionsIC2-020922.mtw
 Run operator: wet
 Analysis number: 30118

Last save: 2/9/2022 1:45:3

SAMPLE:
 : IZ/AP
 Vial number: 18
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

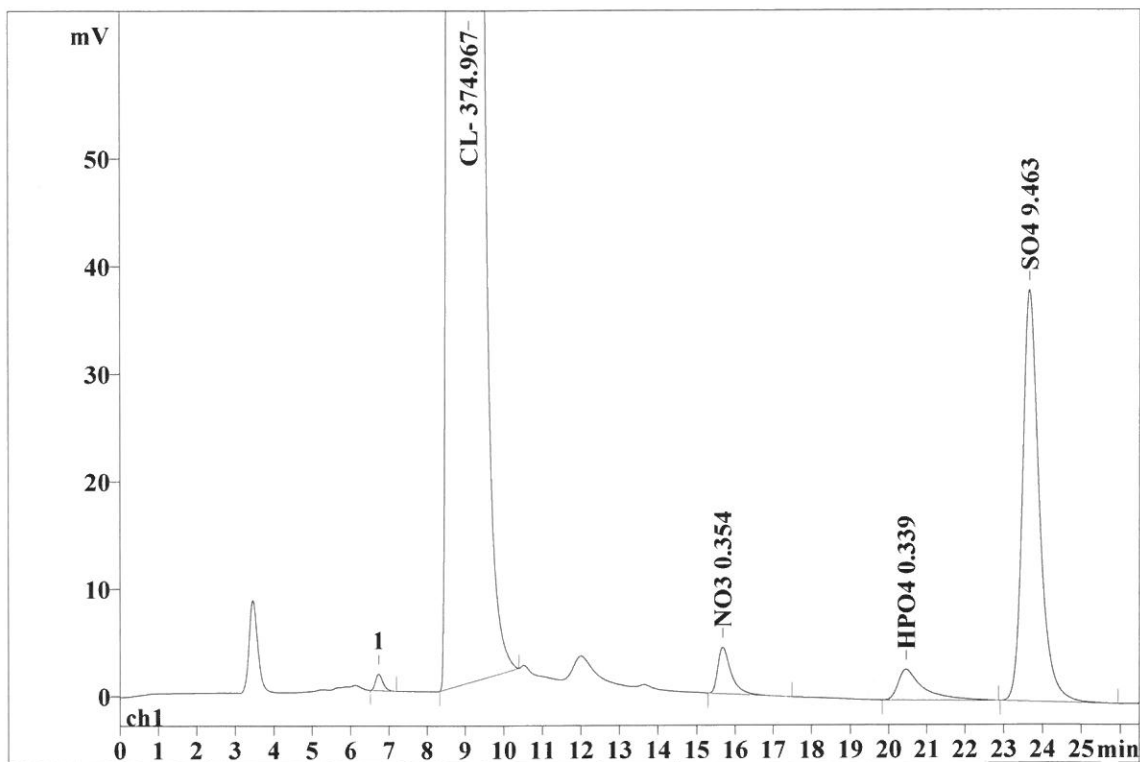

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.07	0.638	1648.58	97.23	63872.178	97.83
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.68	0.346	4.32	0.26	104.356	0.16
6	20.45	0.581	2.87	0.17	130.783	0.20
7	23.68	0.443	38.26	2.26	1160.139	1.78
7	26.50	0.287	1694.03	99.91	65267.457	99.97

This report has been created by IC Net
 METROHM LTD

Report date: 2/18/2022 4:33:08 PM
Printed by: wet


Ident: N1613-01
Analysis from: 2/18/2022 3:46:06 PM
File: _2022-02-18_

Last save: 2/18/2022 4:12:37 PM

Method: AnionsIC2-020922.mtw
Run operator: wet
Analysis number: 30119

Last save: 2/9/2022 1:45:3

SAMPLE:
: IZ/AP
Vial number: 19
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

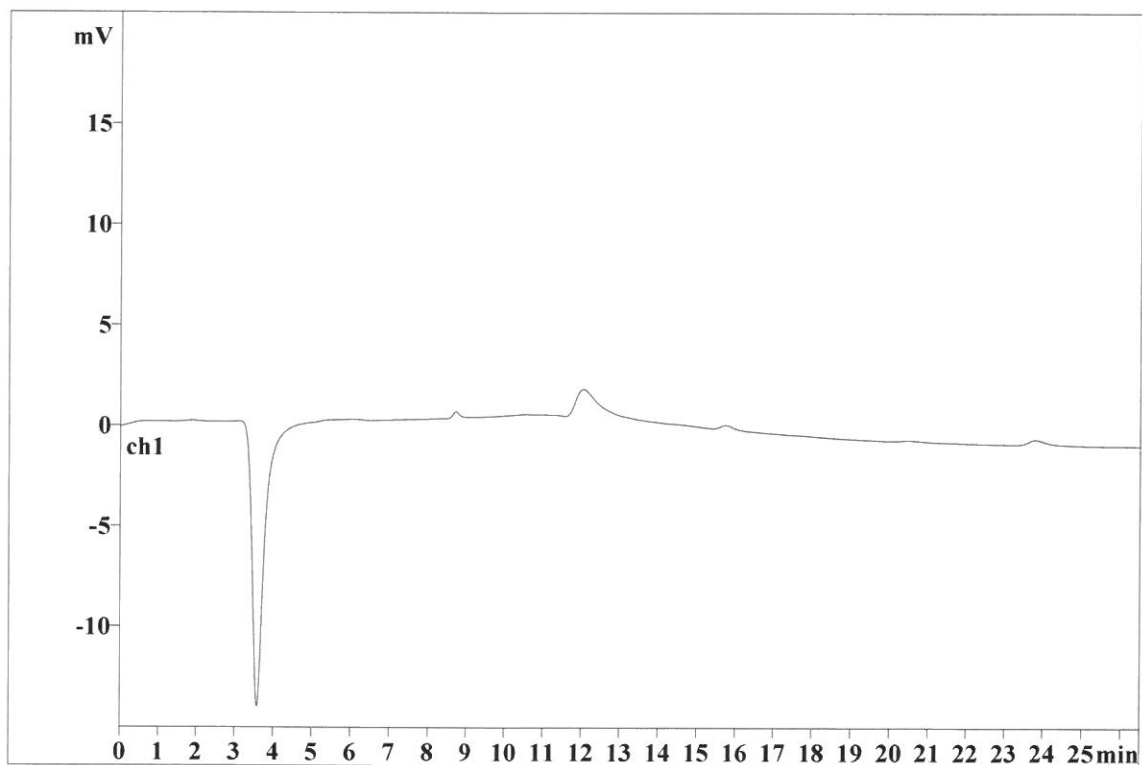

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD