


LB118759

7470A

INSTRUMENT ID: CV1

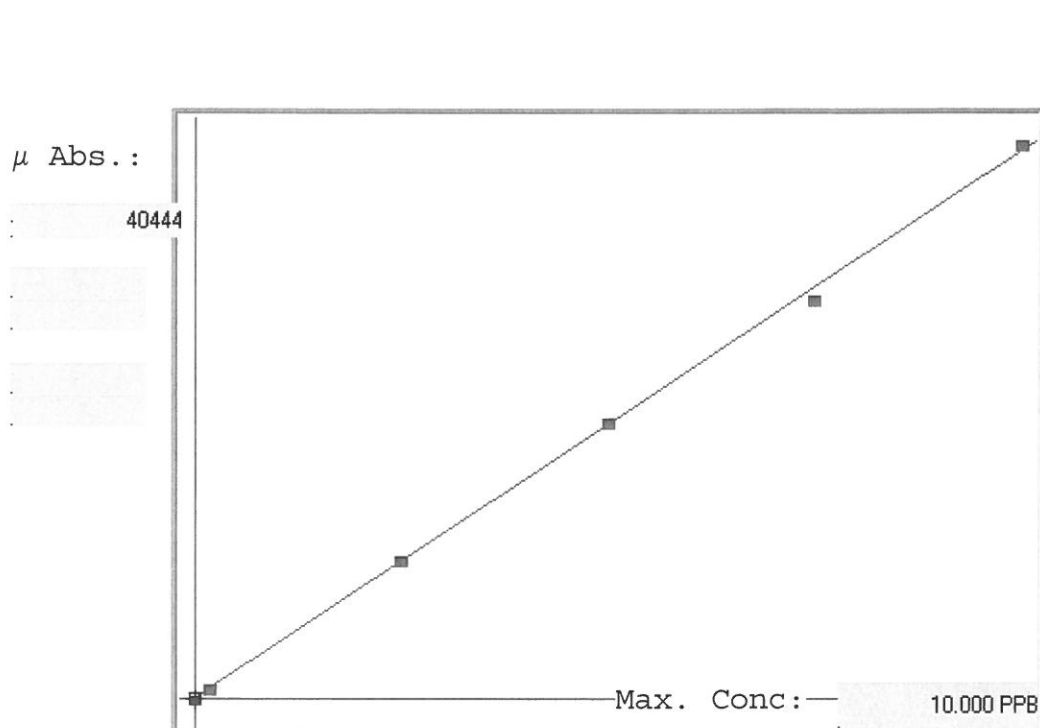

Linear

A= 0.0000e+000

B= 2.5006e-004

C= -5.0552e-003

Rho= 0.9996586

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0 D
0.0	0.000	-0.002	-0.002	14	0.000	14					1
0.2	0.200	0.202	0.002	828	0.0 %	828					2
2.5	2.500	2.539	0.039	10173	0.0 %	10173					1
5.0	5.000	5.052	0.052	20223	0.0 %	20223					1
7.5	7.500	7.300	-0.200	29215	0.0 %	29215					-3
10.0	10.000	10.108	0.108	40444	0.0 %	40444					1

LB118759 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 20 Feb 2022 14:15:42

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	14	-	0.0000	7470A	PPB	20 Feb 2022 14:19:27	S	Std
0.2 - 1	50.2	828	-	0.2000	7470A	PPB	20 Feb 2022 14:21:44	S	Std
2.5 - 1	52.5	10173	-	2.5000	7470A	PPB	20 Feb 2022 14:24:02	S	Std
5.0 - 1	55	20223	-	5.0000	7470A	PPB	20 Feb 2022 14:26:19	S	Std
7.5 - 1	57.5	29215	-	7.5000	7470A	PPB	20 Feb 2022 14:28:35	S	Std
10.0 - 1	510	40444	-	10.0000	7470A	PPB	20 Feb 2022 14:30:51	S	Std
ICV97 - 1	ICV97	14534	3.6293	-	7470A	PPB	20 Feb 2022 14:33:50	U	SMPL
ICB97 - 1	ICB97	-32	-0.0131	-	7470A	PPB	20 Feb 2022 14:36:05	U	SMPL
CCV16 - 1	CCV16	20005	4.9974	-	7470A	PPB	20 Feb 2022 14:38:21	U	SMPL
CCB16 - 1	CCB16	-43	-0.0158	-	7470A	PPB	20 Feb 2022 14:40:36	U	SMPL
CRA - 1	CRA	801	0.1952	-	7470A	PPB	20 Feb 2022 14:42:52	U	SMPL
HighStd - 1	HighStd	39973	9.9906	-	7470A	PPB	20 Feb 2022 14:45:07	U	SMPL
ChkStd - 1	ChkStd	26556	6.6355	-	7470A	PPB	20 Feb 2022 14:47:23	U	SMPL
PB142823BL - 1	PBW	-67	-0.0218	-	7470A	PPB	20 Feb 2022 14:49:39	U	SMPL
PB142823BS - 1	LCSW	14391	3.5936	-	7470A	PPB	20 Feb 2022 14:54:26	U	SMPL
N1481-01 - 1	RW7B-GW-20220209	-23	-0.0108	-	7470A	PPB	20 Feb 2022 14:56:42	U	SMPL
N1481-01DUP - 1	RW7B-GW-20220209DUP	8	-0.0031	-	7470A	PPB	20 Feb 2022 14:58:59	U	SMPL
N1481-01MS - 1	RW7B-GW-20220209MS	13595	3.3945	-	7470A	PPB	20 Feb 2022 15:01:16	U	SMPL
N1481-01MSD - 1	RW7B-GW-20220209MSD	13345	3.3320	-	7470A	PPB	20 Feb 2022 15:03:33	U	SMPL
N1581-27 - 1	FB02-20220215	-30	-0.0126	-	7470A	PPB	20 Feb 2022 15:05:49	U	SMPL
CCV17 - 1	CCV17	19737	4.9304	-	7470A	PPB	20 Feb 2022 15:08:06	U	SMPL
CCB17 - 1	CCB17	-33	-0.0133	-	7470A	PPB	20 Feb 2022 15:10:22	U	SMPL
N1481-01LX5 - 1		8	-0.0031	-	7470A	PPB	20 Feb 2022 15:12:37	U	SMPL
N1481-01A - 1		14598	3.6453	-	7470A	PPB	20 Feb 2022 15:14:53	U	SMPL
CCV18 - 1	CCV18	19848	4.9581	-	7470A	PPB	20 Feb 2022 15:17:08	U	SMPL
CCB18 - 1	CCB18	-32	-0.0131	-	7470A	PPB	20 Feb 2022 15:19:24	U	SMPL