


LB118773

7470A

INSTRUMENT ID: CV1

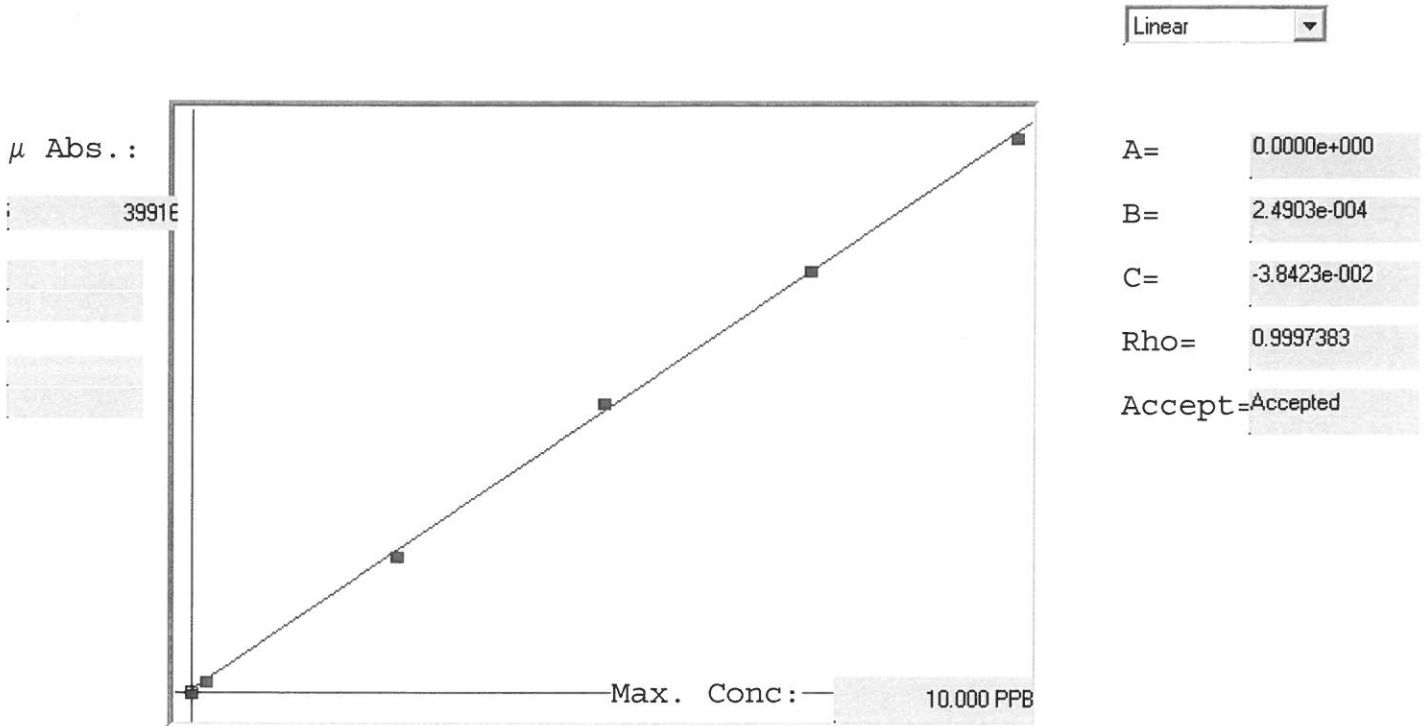

| Std ID | Conc.  | Calc.  | Dev.   | Mean  | SD or %RSD | Rep 1 | Rep 2 | Rep 3 | Rep 4 | Rep 5 | %D  |
|--------|--------|--------|--------|-------|------------|-------|-------|-------|-------|-------|-----|
| 0.0    | 0.000  | -0.015 | -0.015 | 95    | 0.000      | 95    |       |       |       |       | 1   |
| 0.2    | 0.200  | 0.177  | -0.023 | 865   | 0.0 %      | 865   |       |       |       |       | -12 |
| 2.5    | 2.500  | 2.434  | -0.066 | 9928  | 0.0 %      | 9928  |       |       |       |       | -3  |
| 5.0    | 5.000  | 5.162  | 0.162  | 20885 | 0.0 %      | 20885 |       |       |       |       | 3   |
| 7.5    | 7.500  | 7.540  | 0.040  | 30431 | 0.0 %      | 30431 |       |       |       |       | 1   |
| 10.0   | 10.000 | 9.902  | -0.098 | 39916 | 0.0 %      | 39916 |       |       |       |       | -1  |

## LB118773 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 22 Feb 2022 08:56:21

| Sample ID       | Extended ID                     | μ Abs | Conc    | Std Conc | Method | Units | Date                 | Type | Type |
|-----------------|---------------------------------|-------|---------|----------|--------|-------|----------------------|------|------|
| 0.0 - 1         | 50                              | 95    | -       | 0.0000   | 7470A  | PPB   | 22 Feb 2022 08:59:07 | S    | Std  |
| 0.2 - 1         | 50.2                            | 865   | -       | 0.2000   | 7470A  | PPB   | 22 Feb 2022 09:01:25 | S    | Std  |
| 2.5 - 1         | 52.5                            | 9928  | -       | 2.5000   | 7470A  | PPB   | 22 Feb 2022 09:03:42 | S    | Std  |
| 5.0 - 1         | 35                              | 20885 | -       | 5.0000   | 7470A  | PPB   | 22 Feb 2022 09:05:59 | S    | Std  |
| 7.5 - 1         | 33.5                            | 30431 | -       | 7.5000   | 7470A  | PPB   | 22 Feb 2022 09:08:16 | S    | Std  |
| 10.0 - 1        | 310                             | 39916 | -       | 10.0000  | 7470A  | PPB   | 22 Feb 2022 09:10:32 | S    | Std  |
| ICV01 - 1       | ICV01                           | 15600 | 3.8464  | -        | 7470A  | PPB   | 22 Feb 2022 09:13:29 | U    | SMPL |
| ICB01 - 1       | ICB01                           | -30   | -0.0459 | -        | 7470A  | PPB   | 22 Feb 2022 09:15:44 | U    | SMPL |
| CCV29 - 1       | CCV29                           | 19964 | 4.9331  | -        | 7470A  | PPB   | 22 Feb 2022 09:17:59 | U    | SMPL |
| CCB29 - 1       | CCB29                           | -35   | -0.0471 | -        | 7470A  | PPB   | 22 Feb 2022 09:20:15 | U    | SMPL |
| CRA - 1         | CRA                             | 763   | 0.1516  | -        | 7470A  | PPB   | 22 Feb 2022 09:22:30 | U    | SMPL |
| HighStd - 1     | HighStd                         | 38266 | 9.4908  | -        | 7470A  | PPB   | 22 Feb 2022 09:24:45 | U    | SMPL |
| ChkStd - 1      | ChkStd                          | 27364 | 6.7759  | -        | 7470A  | PPB   | 22 Feb 2022 09:27:01 | U    | SMPL |
| PB142850BL - 1  | PBW                             | -51   | -0.0511 | -        | 7470A  | PPB   | 22 Feb 2022 09:29:17 | U    | SMPL |
| PB142850BS - 1  | LCSW                            | 15680 | 3.8663  | -        | 7470A  | PPB   | 22 Feb 2022 09:31:34 | U    | SMPL |
| N1611-07 - 1    | 1070                            | 16    | -0.0344 | -        | 7470A  | PPB   | 22 Feb 2022 09:33:51 | U    | SMPL |
| N1611-07DUP - 1 | 1070DUP                         | 36    | -0.0295 | -        | 7470A  | PPB   | 22 Feb 2022 09:36:08 | U    | SMPL |
| N1611-07MS - 1  | 1070MS                          | 13438 | 3.3080  | -        | 7470A  | PPB   | 22 Feb 2022 09:38:25 | U    | SMPL |
| N1611-07MSD - 1 | 1070MSD                         | 13366 | 3.2901  | -        | 7470A  | PPB   | 22 Feb 2022 09:40:43 | U    | SMPL |
| N1611-08 - 1    | WATER-COMP                      | 60    | -0.0235 | -        | 7470A  | PPB   | 22 Feb 2022 09:42:59 | U    | SMPL |
| CCV30 - 1       | CCV30                           | 19793 | 4.8905  | -        | 7470A  | PPB   | 22 Feb 2022 09:45:14 | U    | SMPL |
| CCB30 - 1       | CCB30                           | -44   | -0.0494 | -        | 7470A  | PPB   | 22 Feb 2022 09:47:30 | U    | SMPL |
| N1627-01 - 1    | 20220095-BERKELEY-7-ELUTIRATE   | 108   | -0.0115 | -        | 7470A  | PPB   | 22 Feb 2022 09:49:45 | U    | SMPL |
| N1627-02 - 1    | 20220096-BERKELEY-8-ELUTRIATE   | 59    | -0.0237 | -        | 7470A  | PPB   | 22 Feb 2022 09:52:01 | U    | SMPL |
| N1627-03 - 1    | 20220092A-BERKELEY-4A-ELUTRIATE | 72    | -0.0205 | -        | 7470A  | PPB   | 22 Feb 2022 09:54:16 | U    | SMPL |
| N1611-07LX5 - 1 |                                 | -15   | -0.0422 | -        | 7470A  | PPB   | 22 Feb 2022 09:56:32 | U    | SMPL |
| N1611-07A - 1   |                                 | 15850 | 3.9086  | -        | 7470A  | PPB   | 22 Feb 2022 09:58:48 | U    | SMPL |
| CCV31 - 1       | CCV31                           | 20064 | 4.9580  | -        | 7470A  | PPB   | 22 Feb 2022 10:01:05 | U    | SMPL |
| CCB31 - 1       | CCB31                           | -30   | -0.0459 | -        | 7470A  | PPB   | 22 Feb 2022 10:03:22 | U    | SMPL |