


LB118790

7471B

INSTRUMENT ID: CV1

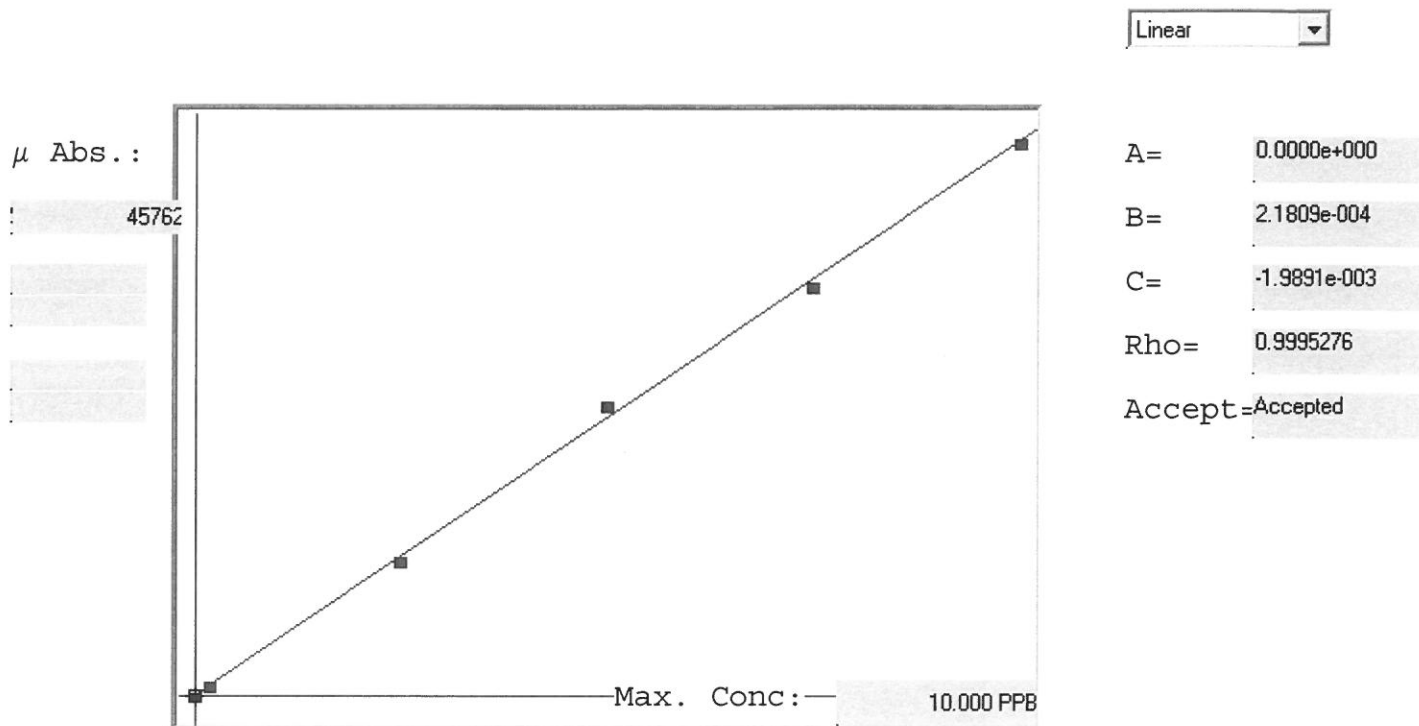

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/01
0.0	0.000	-0.005	-0.005	-15	0.000	-15					
0.2	0.200	0.171	-0.029	792	0.0 %	792					-15
2.5	2.500	2.435	-0.065	11175	0.0 %	11175					-3
5.0	5.000	5.240	0.240	24036	0.0 %	24036					5
7.5	7.500	7.381	-0.119	33856	0.0 %	33856					-2
10.0	10.000	9.978	-0.022	45762	0.0 %	45762					0

LB118790 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 23 Feb 2022 11:56:46

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-15	-	0.00007471B	PPB		23 Feb 2022 11:57:00	S	Std
0.2 - 1	50.2	792	-	0.20007471B	PPB		23 Feb 2022 11:59:18	S	Std
2.5 - 1	52.5	11175	-	2.50007471B	PPB		23 Feb 2022 12:01:35	S	Std
5.0 - 1	55	24036	-	5.00007471B	PPB		23 Feb 2022 12:03:52	S	Std
7.5 - 1	57.5	33856	-	7.50007471B	PPB		23 Feb 2022 12:06:10	S	Std
10.0 - 1	510	45762	-	10.00007471B	PPB		23 Feb 2022 12:08:28	S	Std
ICV04 - 1	ICV04	17109	3.7292	-7471B	PPB		23 Feb 2022 12:11:14	U	SMPL
ICB04 - 1	ICB04	-37	-0.0101	-7471B	PPB		23 Feb 2022 12:13:29	U	SMPL
CCV39 - 1	CCV39	23471	5.1167	-7471B	PPB		23 Feb 2022 12:15:46	U	SMPL
CCB39 - 1	CCB39	-35	-0.0096	-7471B	PPB		23 Feb 2022 12:18:01	U	SMPL
CRA - 1	CRA	869	0.1875	-7471B	PPB		23 Feb 2022 12:20:18	U	SMPL
HighStd - 1	HighStd	48291	10.5296	-7471B	PPB		23 Feb 2022 12:22:33	U	SMPL
ChkStd - 1	ChkStd	34600	7.5438	-7471B	PPB		23 Feb 2022 12:24:49	U	SMPL
PB142877BL - 1	PBS	-59	-0.0149	-7471B	PPB		23 Feb 2022 12:27:07	U	SMPL
PB142877BS - 1	LCSS	17880	3.8974	-7471B	PPB		23 Feb 2022 12:29:25	U	SMPL
N1628-01 - 1	BP-3	10933	2.3823	-7471B	PPB		23 Feb 2022 12:31:41	U	SMPL
N1634-01 - 1	20071	436	0.0931	-7471B	PPB		23 Feb 2022 12:33:59	U	SMPL
N1635-01 - 1	RO-124055	871	0.1880	-7471B	PPB		23 Feb 2022 12:36:16	U	SMPL
N1635-03 - 1	RO-124042	2191	0.4758	-7471B	PPB		23 Feb 2022 12:38:33	U	SMPL
N1635-05 - 1	RO-124019	2565	0.5574	-7471B	PPB		23 Feb 2022 12:40:49	U	SMPL
CCV40 - 1	CCV40	23882	5.2063	-7471B	PPB		23 Feb 2022 12:43:05	U	SMPL
CCB40 - 1	CCB40	-28	-0.0081	-7471B	PPB		23 Feb 2022 12:45:20	U	SMPL
N1636-01 - 1	HR-02-022222	1366	0.2959	-7471B	PPB		23 Feb 2022 12:47:37	U	SMPL
N1636-01DUP - 1	HR-02-022222DUP	1167	0.2525	-7471B	PPB		23 Feb 2022 12:49:52	U	SMPL
N1636-01MS - 1	HR-02-022222MS	20431	4.4537	-7471B	PPB		23 Feb 2022 12:52:08	U	SMPL
N1636-01MSD - 1	HR-02-022222MSD	20555	4.4807	-7471B	PPB		23 Feb 2022 12:54:24	U	SMPL
N1636-01LX5 - 1		196	0.0408	-7471B	PPB		23 Feb 2022 12:56:41	U	SMPL
N1636-01A - 1		20757	4.5248	-7471B	PPB		23 Feb 2022 12:58:59	U	SMPL
CCV41 - 1	CCV41	24544	5.3507	-7471B	PPB		23 Feb 2022 13:01:15	U	SMPL
CCB41 - 1	CCB41	-49	-0.0127	-7471B	PPB		23 Feb 2022 13:03:33	U	SMPL