

## Clear table

| Instrument ID: IC-2 |                      |                       |                        |                       |                       |                        |                       |             |               | Analyst : |  | IZ | Method: |  | 300.0 / 9056A |  | Initial wt/<br>Final Vol |       | Analyst |
|---------------------|----------------------|-----------------------|------------------------|-----------------------|-----------------------|------------------------|-----------------------|-------------|---------------|-----------|--|----|---------|--|---------------|--|--------------------------|-------|---------|
| ident               | concentra<br>tion F- | concentratio<br>n CL- | concentratio<br>on NO2 | concentrati<br>on BR- | concentrati<br>on NO3 | concentrati<br>on HPO4 | concentrati<br>on SO4 | file name   | date time     |           |  |    |         |  |               |  |                          |       |         |
| STD1                | 0.0000               | 0.0000                | 0.0000                 | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2022-02-24_ | 2/24/22 9:19  |           |  |    |         |  |               |  |                          | IZ/AP |         |
| STD2                | 0.4460               | 0.6760                | 0.6850                 | 2.3070                | 0.5830                | 0.9020                 | 3.5940                | 2022-02-24_ | 2/24/22 9:47  |           |  |    |         |  |               |  |                          | IZ/AP |         |
| STD3                | 0.8340               | 1.2230                | 1.2150                 | 4.0580                | 1.0210                | 2.0340                 | 6.1250                | 2022-02-24_ | 2/24/22 10:16 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| STD4                | 0.9640               | 1.5070                | 1.4940                 | 4.9870                | 1.2470                | 2.5640                 | 7.4540                | 2022-02-24_ | 2/24/22 10:44 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| STD5                | 1.9190               | 2.9030                | 2.9130                 | 9.6630                | 2.4010                | 5.0700                 | 14.3340               | 2022-02-24_ | 2/24/22 11:13 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| STD6                | 4.0470               | 5.8550                | 5.8620                 | 19.5320               | 4.8750                | 9.8620                 | 29.2010               | 2022-02-24_ | 2/24/22 11:42 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| STD7                | 4.9900               | 7.6360                | 7.6300                 | 25.4530               | 6.3720                | 12.5690                | 38.2920               | 2022-02-24_ | 2/24/22 12:10 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| ICV                 | 2.0180               | 2.9500                | 2.9680                 | 9.8510                | 2.4610                | 5.1030                 | 14.6150               | 2022-02-24_ | 2/24/22 13:22 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| ICB                 | 0.0000               | 0.0000                | 0.0000                 | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2022-02-24_ | 2/24/22 13:52 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| CCV                 | 2.0630               | 2.9040                | 2.8980                 | 9.6320                | 2.4120                | 6.4710                 | 14.2760               | 2022-02-24_ | 2/24/22 23:28 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| CCB                 | 0.0000               | 0.0000                | 0.0000                 | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2022-02-24_ | 2/24/22 23:56 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| N1671-01            | 0.2500               | 403.8680              | 0.0000                 | 0.0000                | 2.3870                | 0.0000                 | 29.5760               | 2022-02-25_ | 2/25/22 9:05  |           |  |    |         |  |               |  |                          | IZ/AP |         |
| N1671-03            | 0.4270               | 365.2140              | 0.0000                 | 0.7460                | 2.2510                | 0.0000                 | 21.6090               | 2022-02-25_ | 2/25/22 9:34  |           |  |    |         |  |               |  |                          | IZ/AP |         |
| N1671-05            | 0.3410               | 151.9890              | 0.0000                 | 0.0000                | 2.5030                | 0.0000                 | 16.3120               | 2022-02-25_ | 2/25/22 10:02 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| N1671-07            | 0.3700               | 360.1600              | 0.0000                 | 0.7530                | 2.2420                | 0.0000                 | 21.6350               | 2022-02-25_ | 2/25/22 10:31 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| N1671-07MS          | 3.0220               | 344.1640              | 3.0690                 | 9.9350                | 4.6190                | 10.5840                | 36.2830               | 2022-02-25_ | 2/25/22 11:00 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| N1671-07MSD         | 3.1160               | 345.5380              | 3.1230                 | 9.9660                | 4.6590                | 10.8070                | 36.3740               | 2022-02-25_ | 2/25/22 11:28 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| LB118840BLW         | 0.0000               | 0.0000                | 0.0000                 | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2022-02-25_ | 2/25/22 11:57 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| LB118840BSW         | 1.9820               | 2.8680                | 2.8700                 | 9.6110                | 2.3900                | 6.3700                 | 14.1870               | 2022-02-25_ | 2/25/22 12:26 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| CCV                 | 2.0690               | 2.8780                | 2.8670                 | 9.6100                | 2.4030                | 6.2710                 | 14.2210               | 2022-02-25_ | 2/25/22 12:54 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| CCB                 | 0.0000               | 0.0000                | 0.0000                 | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2022-02-25_ | 2/25/22 13:23 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| N1680-01            | 0.0000               | 0.0000                | 0.0000                 | 0.0000                | 0.1850                | 0.0000                 | 0.0000                | 2022-02-25_ | 2/25/22 13:52 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| N1680-02            | 0.0000               | 0.0000                | 0.0000                 | 0.0000                | 0.2360                | 0.0000                 | 0.0000                | 2022-02-25_ | 2/25/22 14:21 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| N1680-03            | 0.0000               | 0.0000                | 0.0000                 | 0.0000                | 0.1980                | 0.0000                 | 0.0000                | 2022-02-25_ | 2/25/22 14:49 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| N1671-01DLX100      | 0.0000               | 5.4540                | 0.0000                 | 0.0000                | 0.0000                | 0.0000                 | 1.3360                | 2022-02-25_ | 2/25/22 15:18 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| N1671-03DLX100      | 0.0000               | 4.0200                | 0.0000                 | 0.0000                | 0.0000                | 0.0000                 | 1.2770                | 2022-02-25_ | 2/25/22 15:46 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| N1671-05DLX50       | 0.0000               | 2.2640                | 0.0000                 | 0.0000                | 0.1900                | 0.0000                 | 1.3610                | 2022-02-25_ | 2/25/22 16:15 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| N1671-07DLX100      | 0.0000               | 4.0860                | 0.0000                 | 0.0000                | 0.0000                | 0.0000                 | 1.2770                | 2022-02-25_ | 2/25/22 16:44 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| CCV                 | 2.1020               | 2.8850                | 2.8780                 | 9.6310                | 2.4000                | 6.4660                 | 14.2680               | 2022-02-25_ | 2/25/22 17:13 |           |  |    |         |  |               |  |                          | IZ/AP |         |
| CCB                 | 0.0000               | 0.0000                | 0.0000                 | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2022-02-25_ | 2/25/22 17:41 |           |  |    |         |  |               |  |                          | IZ/AP |         |

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A


| ident | concentra<br>tion F- | concentratio<br>n CL- | concentratio<br>on NO2 | concentratio<br>on BR- | concentratio<br>on NO3 | concentratio<br>on HPO4 | concentratio<br>on SO4 | file name  | date time     | Initial wt/<br>Final Vol | Analyst |
|-------|----------------------|-----------------------|------------------------|------------------------|------------------------|-------------------------|------------------------|------------|---------------|--------------------------|---------|
| STD1  | 0.0000               | 0.0000                | 0.0000                 | 0.0000                 | 0.0000                 | 0.0000                  | 0.0000                 | 2022-02-24 | 2/24/22 9:19  |                          | IZ/AP   |
| STD2  | 0.4460               | 0.6760                | 0.6850                 | 2.3070                 | 0.5830                 | 0.9020                  | 3.5940                 | 2022-02-24 | 2/24/22 9:47  |                          | IZ/AP   |
| STD3  | 0.8340               | 1.2230                | 1.2150                 | 4.0580                 | 1.0210                 | 2.0340                  | 6.1250                 | 2022-02-24 | 2/24/22 10:16 |                          | IZ/AP   |
| STD4  | 0.9640               | 1.5070                | 1.4940                 | 4.9870                 | 1.2470                 | 2.5640                  | 7.4540                 | 2022-02-24 | 2/24/22 10:44 |                          | IZ/AP   |
| STD5  | 1.9190               | 2.9030                | 2.9130                 | 9.6630                 | 2.4010                 | 5.0700                  | 14.3340                | 2022-02-24 | 2/24/22 11:13 |                          | IZ/AP   |
| STD6  | 4.0470               | 5.8550                | 5.8620                 | 19.5320                | 4.8750                 | 9.8620                  | 29.2010                | 2022-02-24 | 2/24/22 11:42 |                          | IZ/AP   |
| STD7  | 4.9900               | 7.6360                | 7.6300                 | 25.4530                | 6.3720                 | 12.5690                 | 38.2920                | 2022-02-24 | 2/24/22 12:10 |                          | IZ/AP   |

| ident | True Value F- | True Value CL- | True Value NO2 | True Value BR- | True Value NO3 | True Value HPO4 | True Value SO4 |
|-------|---------------|----------------|----------------|----------------|----------------|-----------------|----------------|
| STD1  | 0.0000        | 0.0000         | 0.0000         | 0.0000         | 0.0000         | 0.0000          | 0.0000         |
| STD2  | 0.4000        | 0.6000         | 0.6000         | 2.0000         | 0.5000         | 1.0000          | 3.0000         |
| STD3  | 0.8000        | 1.2000         | 1.2000         | 4.0000         | 1.0000         | 2.0000          | 6.0000         |
| STD4  | 1.0000        | 1.5000         | 1.5000         | 5.0000         | 1.2500         | 2.5000          | 7.5000         |
| STD5  | 2.0000        | 3.0000         | 3.0000         | 10.0000        | 2.5000         | 5.0000          | 15.0000        |
| STD6  | 4.0000        | 6.0000         | 6.0000         | 20.0000        | 5.0000         | 10.0000         | 30.0000        |
| STD7  | 5.0000        | 7.5000         | 7.5000         | 25.0000        | 6.2500         | 12.5000         | 37.0000        |

| ident | Relative Error F- | Relative Error CL- | Relative Error NO2 | Relative Error BR- | Relative Error NO3 | Relative Error HPO4 | Relative Error SO4 |
|-------|-------------------|--------------------|--------------------|--------------------|--------------------|---------------------|--------------------|
| STD1  |                   |                    |                    |                    |                    |                     |                    |
| STD2  | 11.5000           | 12.6667            | 14.1667            | 15.3500            | 16.6000            | -9.8000             | 19.8000            |
| STD3  | 4.2500            | 1.9167             | 1.2500             | 1.4500             | 2.1000             | 1.7000              | 2.0833             |
| STD4  | -3.6000           | 0.4667             | -0.4000            | -0.2600            | -0.2400            | 2.5600              | -0.6133            |
| STD5  | -4.0500           | -3.2333            | -2.9000            | -3.3700            | -3.9600            | 1.4000              | -4.4400            |
| STD6  | 1.1750            | -2.4167            | -2.3000            | -2.3400            | -2.5000            | -1.3800             | -2.6633            |
| STD7  | -0.2000           | 1.8133             | 1.7333             | 1.8120             | 1.9520             | 0.5520              | 3.4919             |

# CALIBRATION OF COMPONENT F-

Method: AnionsIC2-022422.mtw  
 Equation:  $Q = 0.0774574 \cdot A + 2.3269$   
 RSD: 2.644 %  
 Correlation coefficient: 0.999619

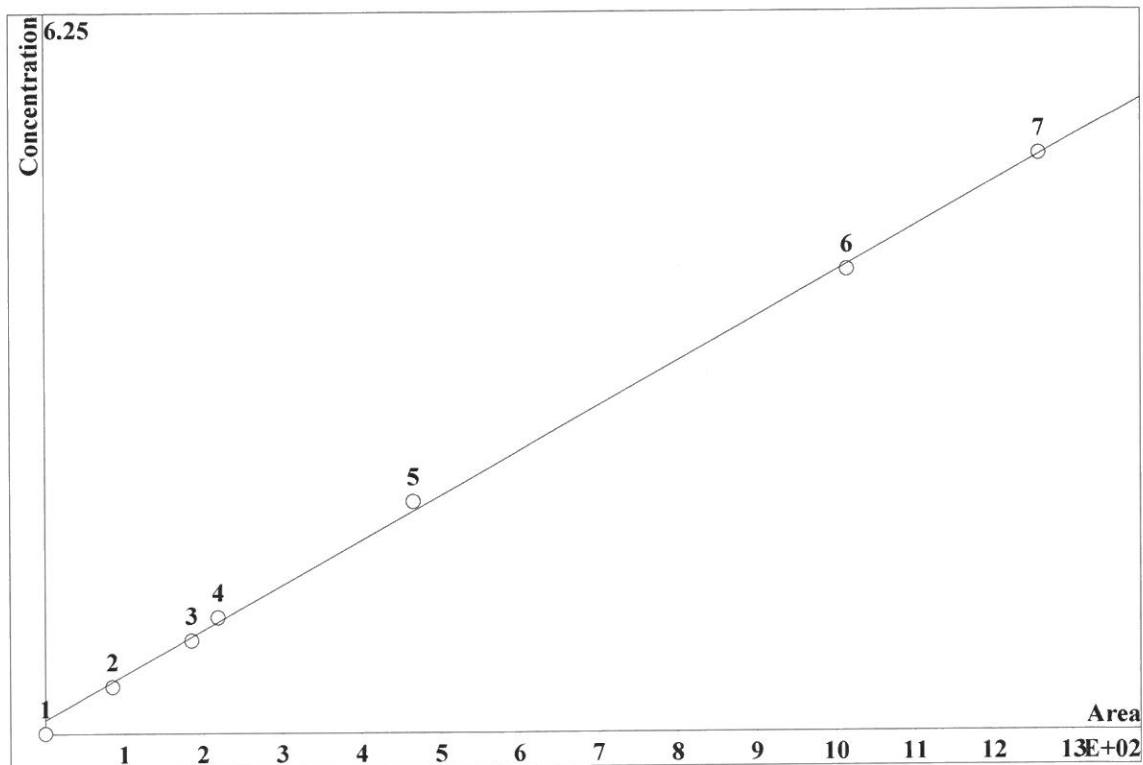


K3 = 0      K2 = 0      K1 = 0.0774574      K0 = 2.3269  
 Base: Area  
 Ref.channel: chl  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      | 0     | 0     | 0       | 0         |      | 0    |
| 2     | 2.522  | 85.15 | 0.4   | 20      | 5.653     |      |      |
| 3     | 6.096  | 185.3 | 0.8   | 20      | 5.653     |      |      |
| 4     | 7.125  | 218.7 | 1     | 20      | 5.653     |      |      |
| 5     | 16.21  | 465.4 | 2     | 20      | 5.653     |      |      |
| 6     | 38.5   | 1015  | 4     | 20      | 5.653     |      |      |
| 7     | 47.61  | 1258  | 5     | 20      | 5.653     |      |      |

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-022422.mtw  
 Equation:  $Q = 0.116052 \cdot A + 2.98439$   
 RSD: 3.571 %  
 Correlation coefficient: 0.999305

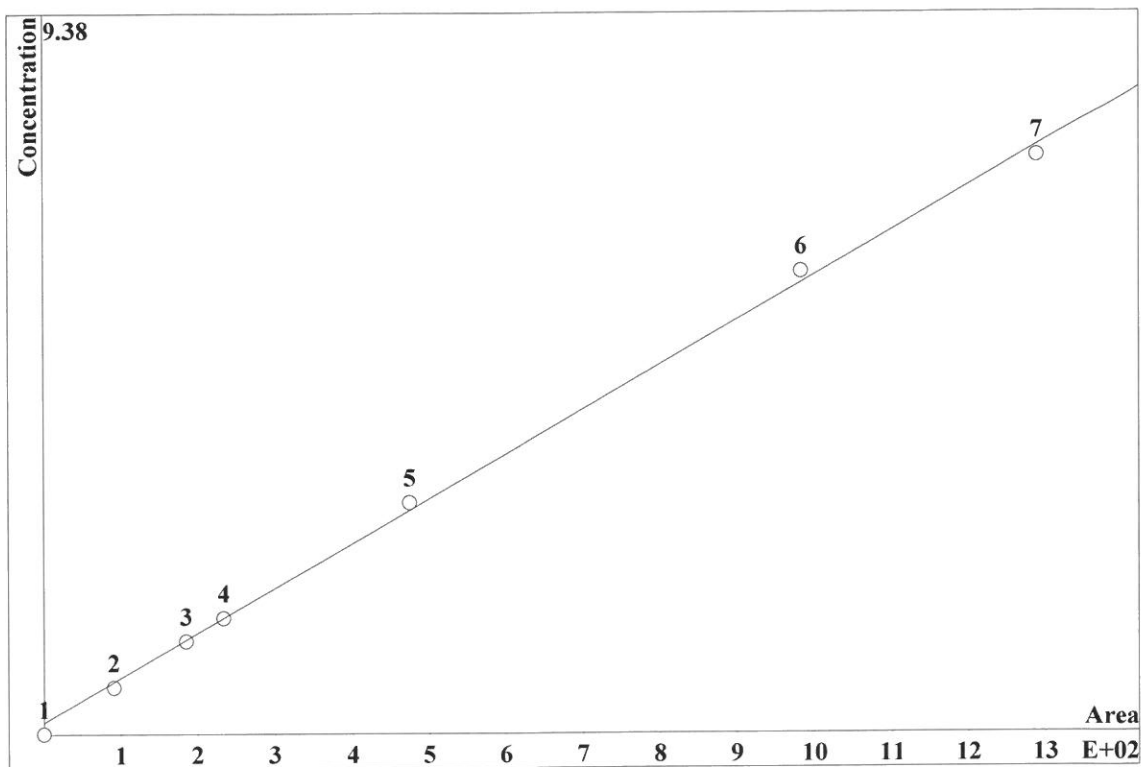


K3 = 0      K2 = 0      K1 = 0.116052      K0 = 2.98439  
 Base: Area  
 Ref.channel: chl  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      | 0     | 0     | 0       | 0         |      | 0    |
| 2     | 6.052  | 90.86 | 0.6   | 20      | 8.643     |      |      |
| 3     | 12.33  | 185   | 1.2   | 20      | 8.643     |      |      |
| 4     | 15.65  | 234   | 1.5   | 20      | 8.643     |      |      |
| 5     | 32.32  | 474.5 | 3     | 20      | 8.643     |      |      |
| 6     | 68.1   | 983.3 | 6     | 20      | 8.643     |      |      |
| 7     | 91.47  | 1290  | 7.5   | 20      | 8.643     |      |      |

## CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-022422.mtw  
 Equation:  $Q = 0.0506181 \cdot A + 3.25506$   
 RSD: 3.420 %  
 Correlation coefficient: 0.999362

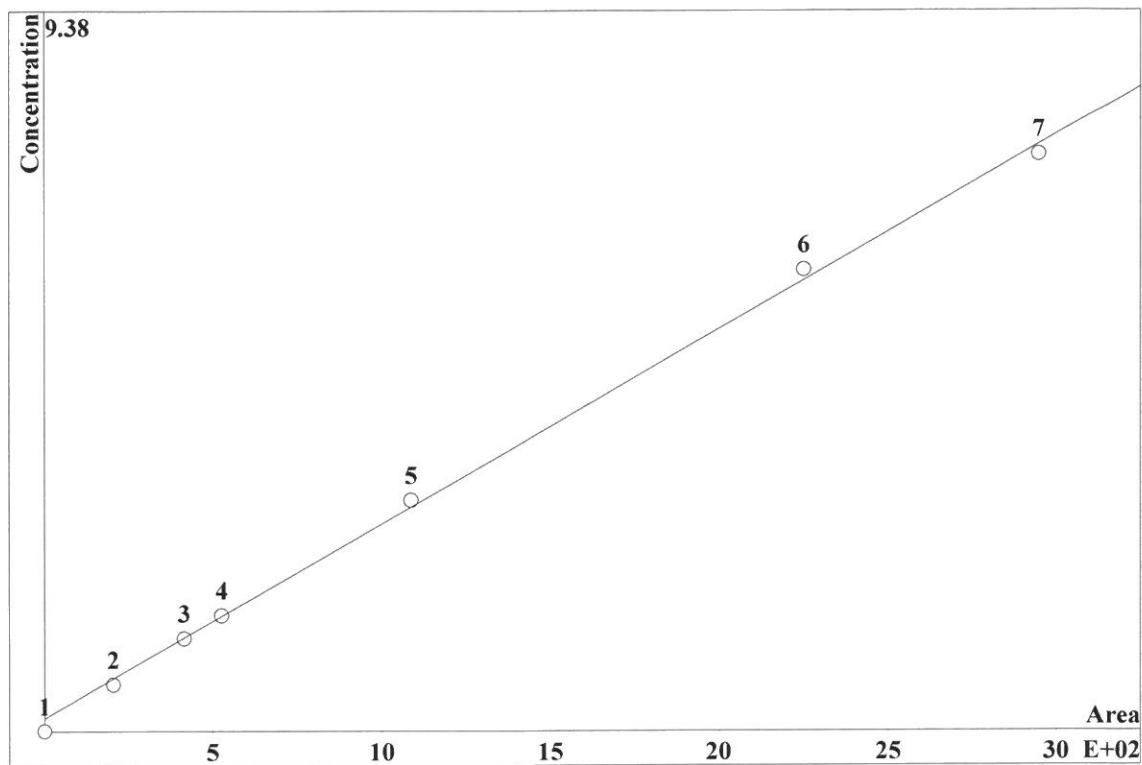


K3 = 0      K2 = 0      K1 = 0.0506181      K0 = 3.25506  
 Base: Area  
 Ref.channel: ch1  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used File |
|-------|--------|-------|-------|---------|-----------|-----------|
| 1     | 0      | 0     | 0     | 0       | 0         | 0         |
| 2     | 11.01  | 206.5 | 0.6   | 20      | 11.04     |           |
| 3     | 22.61  | 415.7 | 1.2   | 20      | 11.04     |           |
| 4     | 28.77  | 526.1 | 1.5   | 20      | 11.04     |           |
| 5     | 58     | 1087  | 3     | 20      | 11.04     |           |
| 6     | 119    | 2252  | 6     | 20      | 11.04     |           |
| 7     | 155    | 2950  | 7.5   | 20      | 10.45     |           |

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-022422.mtw  
 Equation:  $Q = 0.260136 \cdot A + 11.2471$   
 RSD: 3.624 %  
 Correlation coefficient: 0.999284

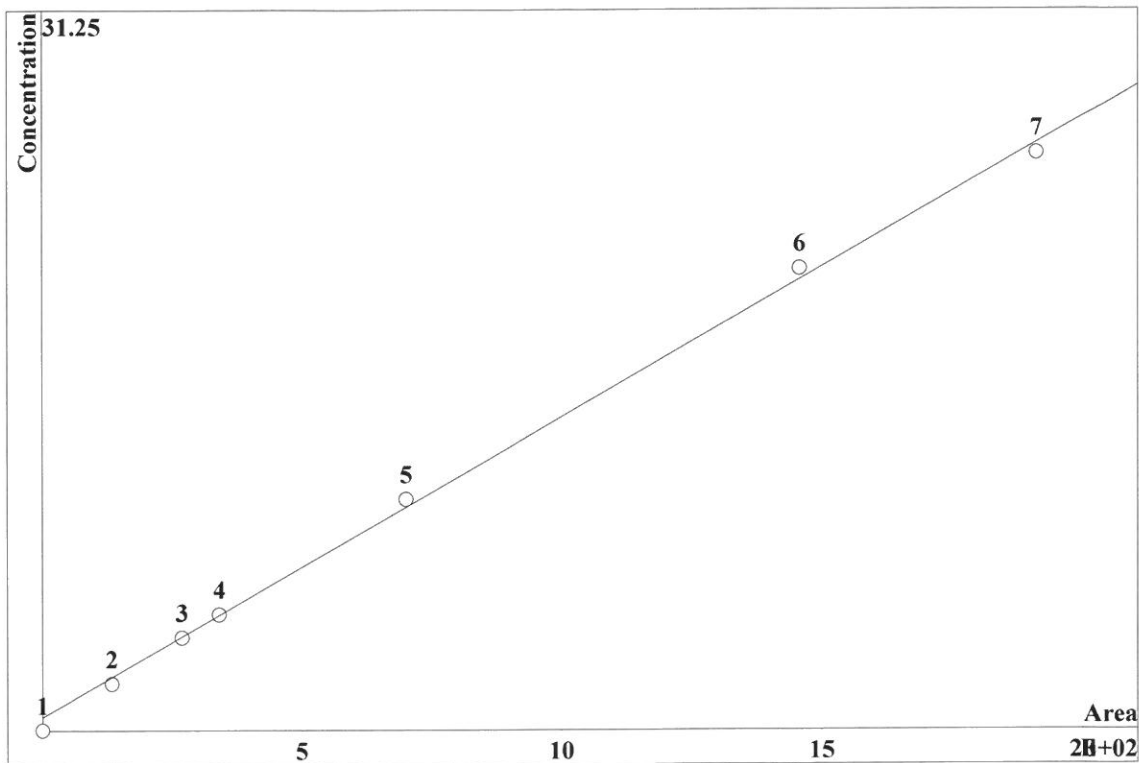


K3 = 0      K2 = 0      K1 = 0.260136      K0 = 11.2471  
 Base: Area  
 Ref.channel: chl  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File  |
|-------|--------|-------|-------|---------|-----------|------|-------|
| 1     | 0      | 0     | 0     | 0       | 0         |      | 0     |
| 2     | 6.102  | 134.2 | 134.2 | 2       | 20        |      | 13.53 |
| 3     | 12.67  | 268.8 | 268.8 | 4       | 20        |      | 13.53 |
| 4     | 16.26  | 340.2 | 340.2 | 5       | 20        |      | 13.53 |
| 5     | 33.77  | 699.7 | 699.7 | 10      | 20        |      | 13.53 |
| 6     | 71.87  | 1458  | 1458  | 20      | 20        |      | 13.53 |
| 7     | 95.82  | 1914  | 1914  | 25      | 20        |      | 13.53 |

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-022422.mtw  
 Equation:  $Q = 0.0453553 \cdot A + 3.00908$   
 RSD: 3.969 %  
 Correlation coefficient: 0.999141

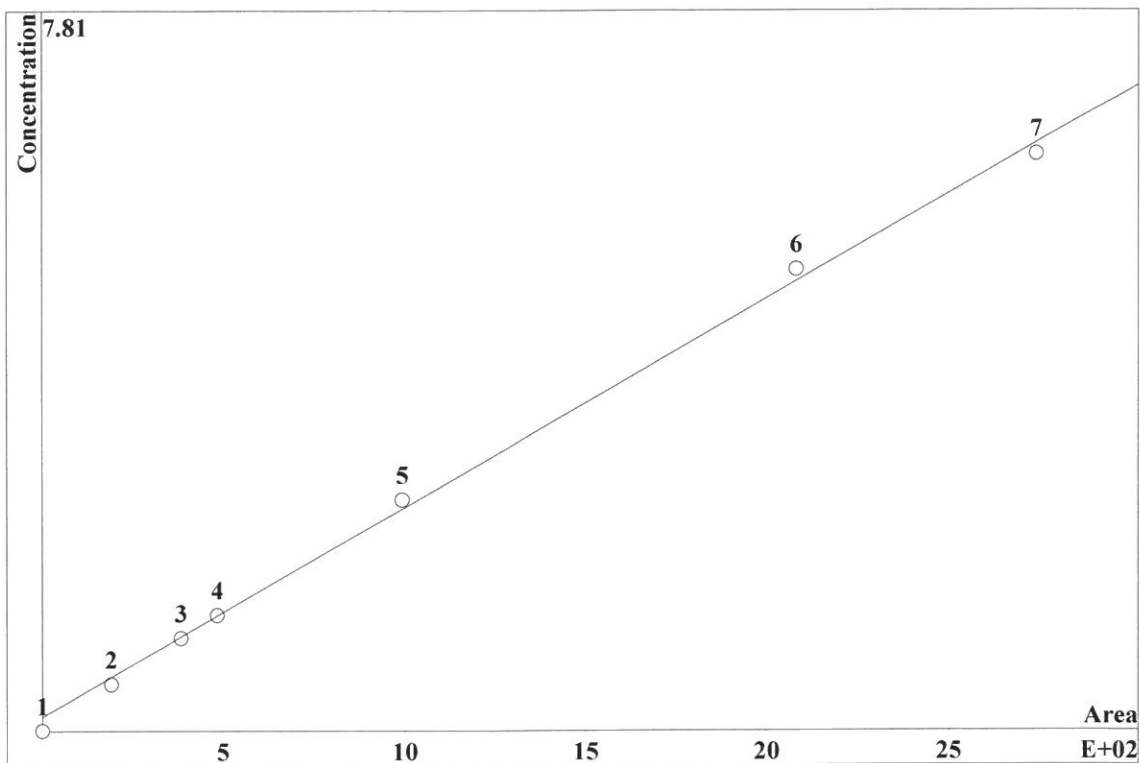


K3 = 0      K2 = 0      K1 = 0.0453553      K0 = 3.00908  
 Base: Area  
 Ref.channel: chl  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      | 0     | 0     | 0       | 0         |      | 0    |
| 2     | 7.344  | 190.7 | 0.5   | 20      | 15.58     |      |      |
| 3     | 15.14  | 383.8 | 1     | 20      | 15.58     |      |      |
| 4     | 19.39  | 483.7 | 1.25  | 20      | 15.58     |      |      |
| 5     | 39.92  | 992.6 | 2.5   | 20      | 15.58     |      |      |
| 6     | 84.9   | 2083  | 5     | 20      | 15.58     |      |      |
| 7     | 113.9  | 2744  | 6.25  | 20      | 15.58     |      |      |

## CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-022422.mtw  
 Equation:  $Q = 0.0861764 \cdot A - 2.37045$   
 RSD: 1.900 %  
 Correlation coefficient: 0.999803

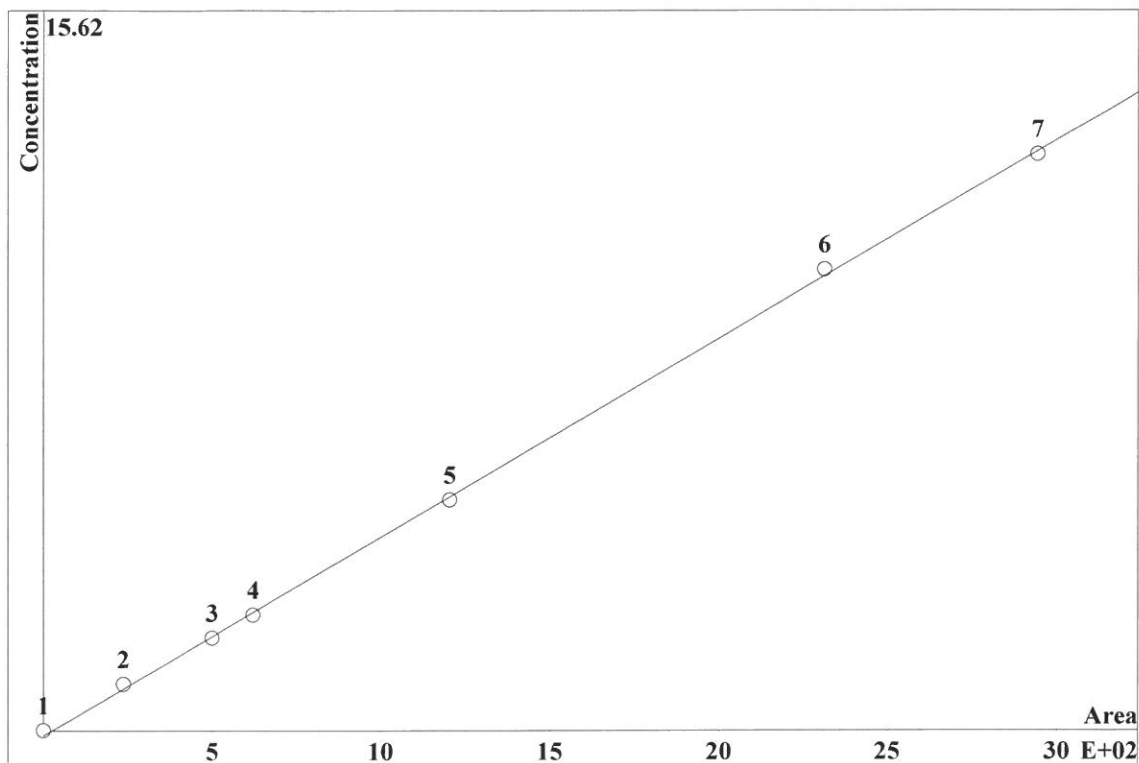


K3 = 0      K2 = 0      K1 = 0.0861764      K0 = -2.37045

Base: Area  
 Ref.channel: ch1  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      | 0     | 0     | 0       | 0         |      | 0    |
| 2     | 6.46   | 236.8 | 1     | 20      | 20.18     |      |      |
| 3     | 14.08  | 499.5 | 2     | 20      | 20.18     |      |      |
| 4     | 17.58  | 622.5 | 2.5   | 20      | 20.18     |      |      |
| 5     | 35.64  | 1204  | 5     | 20      | 20.18     |      |      |
| 6     | 72.25  | 2316  | 10    | 20      | 20.18     |      |      |
| 7     | 93.42  | 2945  | 12.5  | 20      | 20.18     |      |      |

## CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-022422.mtw  
 Equation:  $Q = 0.146407 \cdot A + 20.8785$   
 RSD: 4.370 %  
 Correlation coefficient: 0.998958

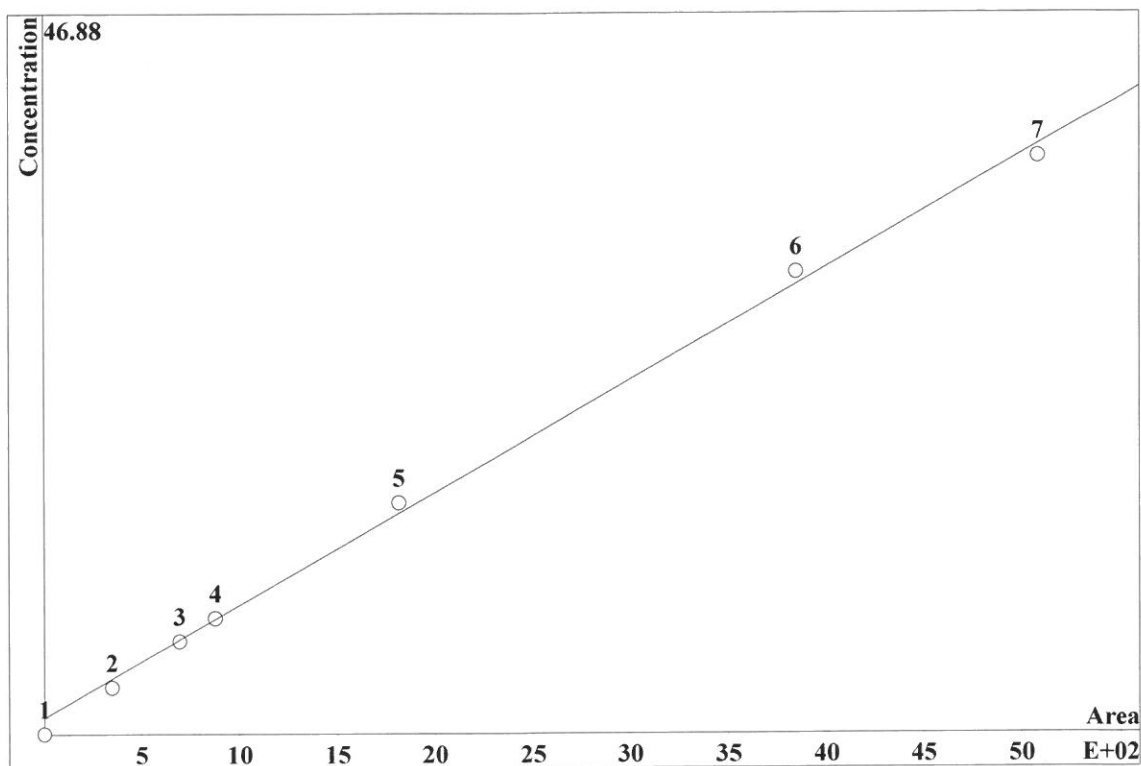

K3 = 0      K2 = 0      K1 = 0.146407      K0 = 20.8785  
 Base: Area  
 Ref.channel: ch1  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      | 0     | 0     | 0       | 0         |      | 0    |
| 2     | 11.49  | 348.3 | 3     | 20      | 23.09     |      |      |
| 3     | 23.49  | 694.2 | 6     | 20      | 23.09     |      |      |
| 4     | 29.89  | 875.7 | 7.5   | 20      | 23.09     |      |      |
| 5     | 62.29  | 1815  | 15    | 20      | 23.09     |      |      |
| 6     | 135.5  | 3846  | 30    | 20      | 23.09     |      |      |
| 7     | 180.8  | 5088  | 37.5  | 20      | 23.09     |      |      |

Report date: 2/24/2022 12:58:32 PM  
Printed by: wet


Ident: STD1  
Analysis from: 2/24/2022 9:19:04 AM  
File: \_2022-02-24\_

Last save: 2/24/2022 12:37:49 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30171

Last save: 2/24/2022 12:08

SAMPLE:  
: IZ/AP  
Vial number: 2  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

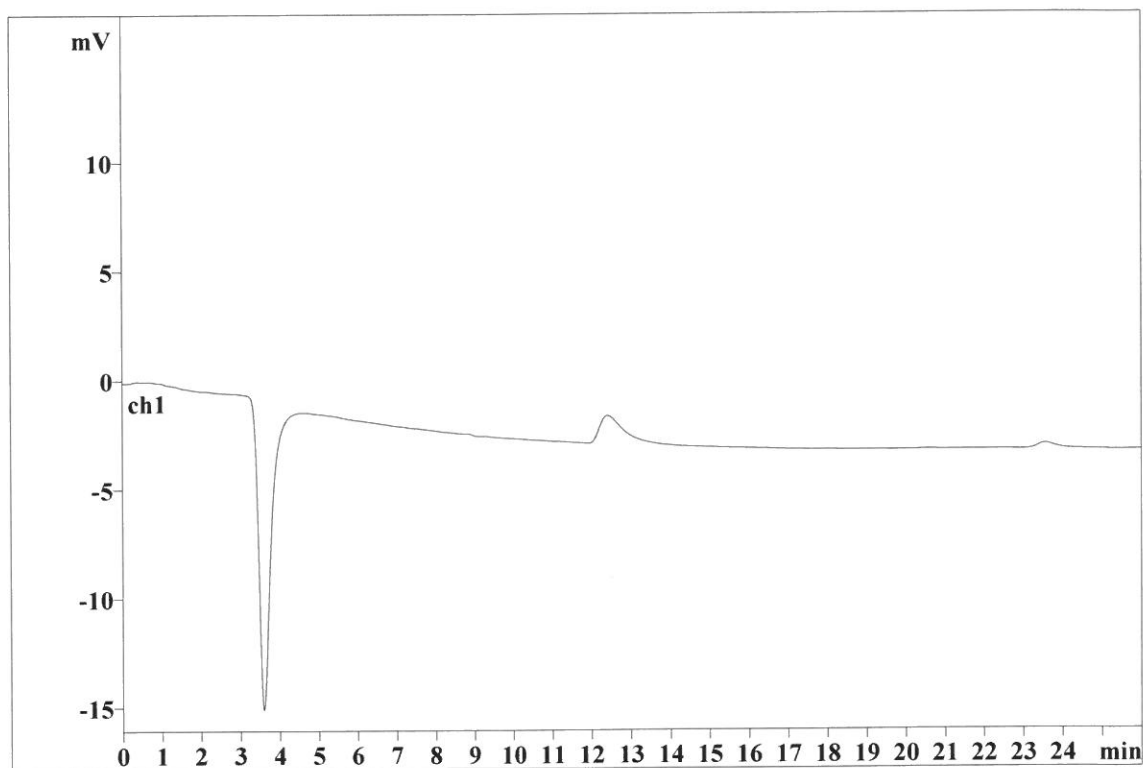

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 2/24/2022 12:58:40 PM  
Printed by: wet


Ident: STD2  
Analysis from: 2/24/2022 9:47:41 AM  
File: \_2022-02-24\_

Last save: 2/24/2022 12:37:49 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30172

Last save: 2/24/2022 12:08

SAMPLE:  
: IZ/AP  
Vial number: 3  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

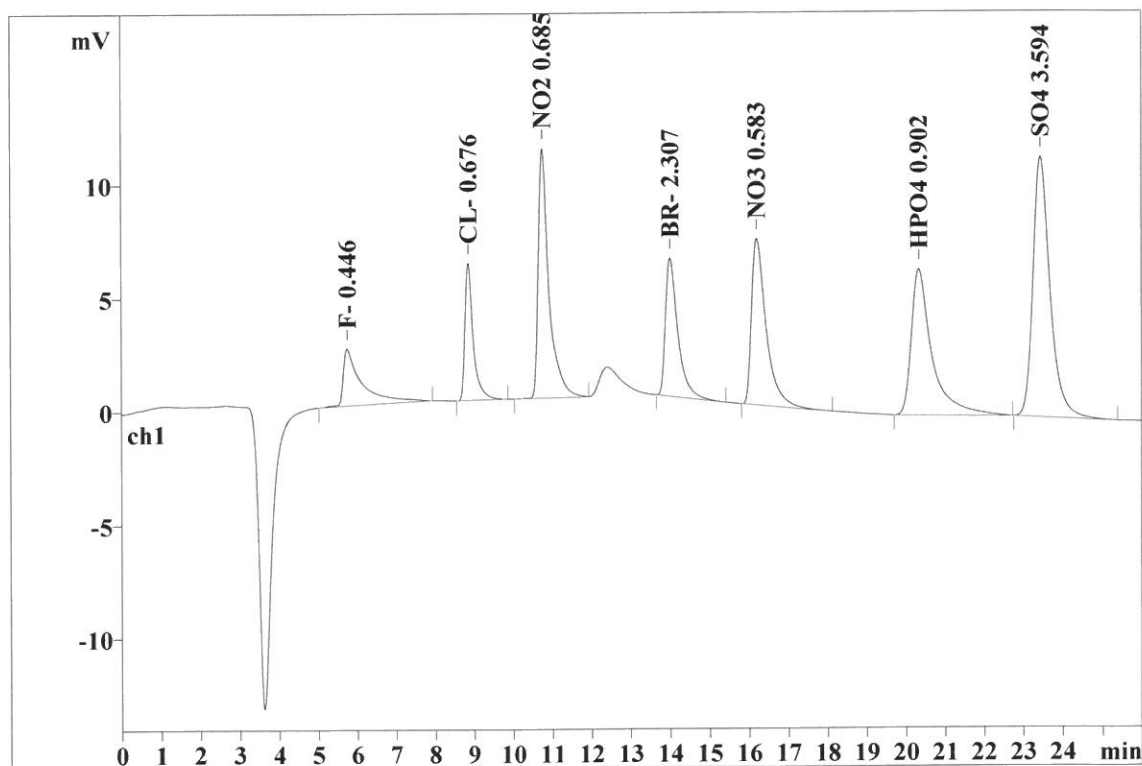

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.74             | 0.380          | 2.52         | 4.94        | 85.147         | 6.59      |
| 2  | 8.85             | 0.207          | 6.05         | 11.87       | 90.857         | 7.03      |
| 3  | 10.75            | 0.249          | 11.01        | 21.60       | 206.531        | 15.98     |
| 4  | 14.02            | 0.316          | 6.10         | 11.97       | 134.157        | 10.38     |
| 5  | 16.21            | 0.371          | 7.34         | 14.41       | 190.700        | 14.75     |
| 6  | 20.34            | 0.481          | 6.46         | 12.67       | 236.813        | 18.32     |
| 7  | 23.46            | 0.444          | 11.49        | 22.53       | 348.336        | 26.95     |
| 7  | 26.00            | 0.350          | 50.98        | 99.99       | 1292.541       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/24/2022 12:58:57 PM  
Printed by: wet


Ident: STD3  
Analysis from: 2/24/2022 10:16:20 AM  
File: \_2022-02-24\_

Last save: 2/24/2022 12:37:49 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30173

Last save: 2/24/2022 12:08

SAMPLE:  
: IZ/AP  
Vial number: 4  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

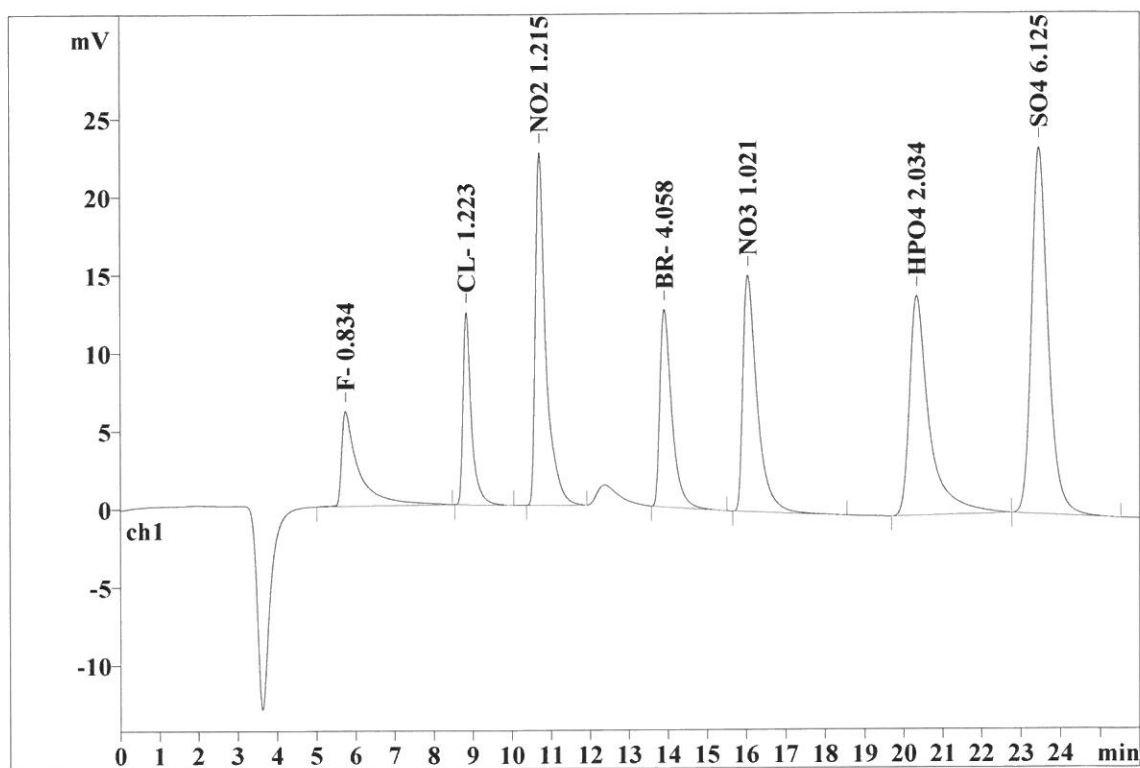

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.74             | 0.350          | 6.09         | 5.73        | 185.328        | 7.04      |
| 2  | 8.83             | 0.207          | 12.33        | 11.59       | 184.998        | 7.03      |
| 3  | 10.70            | 0.246          | 22.61        | 21.25       | 415.655        | 15.79     |
| 4  | 13.92            | 0.307          | 12.67        | 11.90       | 268.754        | 10.21     |
| 5  | 16.05            | 0.363          | 15.14        | 14.23       | 383.843        | 14.58     |
| 6  | 20.34            | 0.468          | 14.08        | 13.23       | 499.459        | 18.97     |
| 7  | 23.47            | 0.437          | 23.49        | 22.07       | 694.162        | 26.37     |
| 7  | 26.00            | 0.340          | 106.40       | 99.99       | 2632.199       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/24/2022 12:59:06 PM  
Printed by: wet


Ident: STD4  
Analysis from: 2/24/2022 10:44:59 AM  
File: \_2022-02-24\_

Last save: 2/24/2022 12:37:49 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30174

Last save: 2/24/2022 12:08

SAMPLE:  
: IZ/AP  
Vial number: 5  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

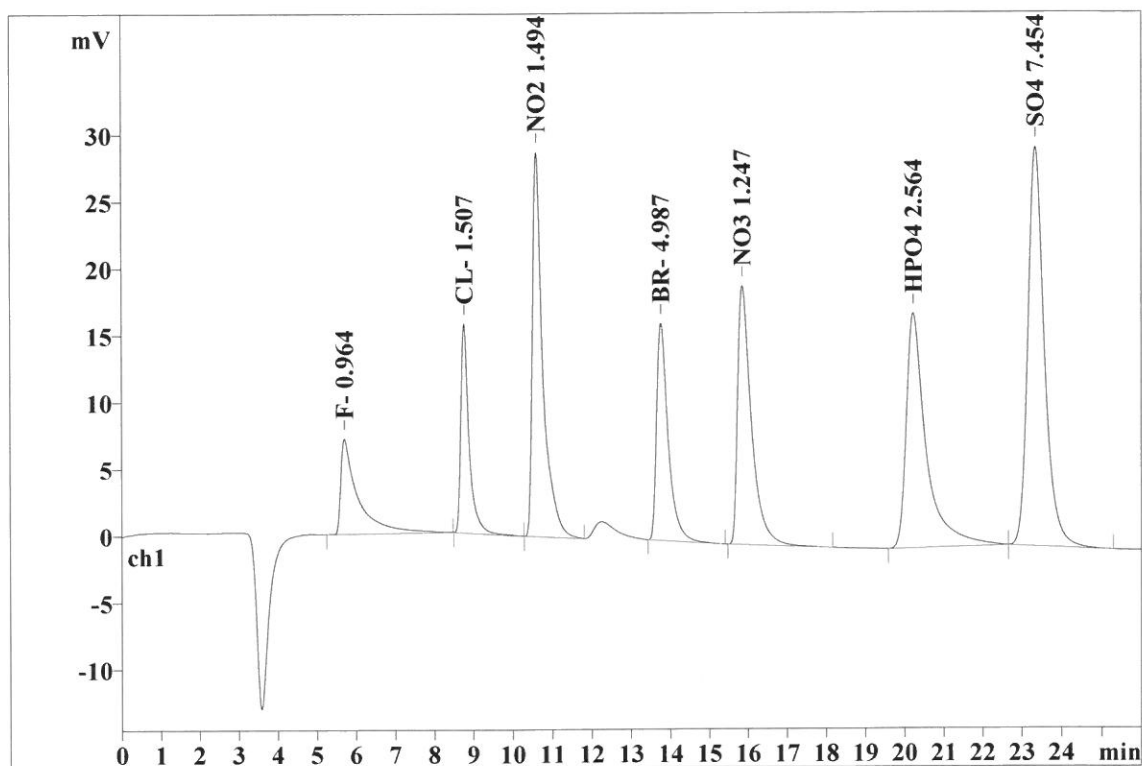

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.71             | 0.350          | 7.12         | 5.29        | 218.746        | 6.63      |
| 2  | 8.76             | 0.205          | 15.65        | 11.62       | 233.967        | 7.09      |
| 3  | 10.60            | 0.245          | 28.77        | 21.36       | 526.072        | 15.94     |
| 4  | 13.77            | 0.302          | 16.26        | 12.08       | 340.215        | 10.31     |
| 5  | 15.86            | 0.357          | 19.39        | 14.40       | 483.720        | 14.65     |
| 6  | 20.24            | 0.465          | 17.58        | 13.06       | 622.544        | 18.86     |
| 7  | 23.35            | 0.432          | 29.89        | 22.19       | 875.690        | 26.53     |
| 7  | 26.00            | 0.337          | 134.67       | 100.00      | 3300.954       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/24/2022 12:59:14 PM  
Printed by: wet


Ident: STD5  
Analysis from: 2/24/2022 11:13:37 AM  
File: \_2022-02-24\_

Last save: 2/24/2022 12:37:49 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30175

Last save: 2/24/2022 12:08

SAMPLE:  
: IZ/AP  
Vial number: 6  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

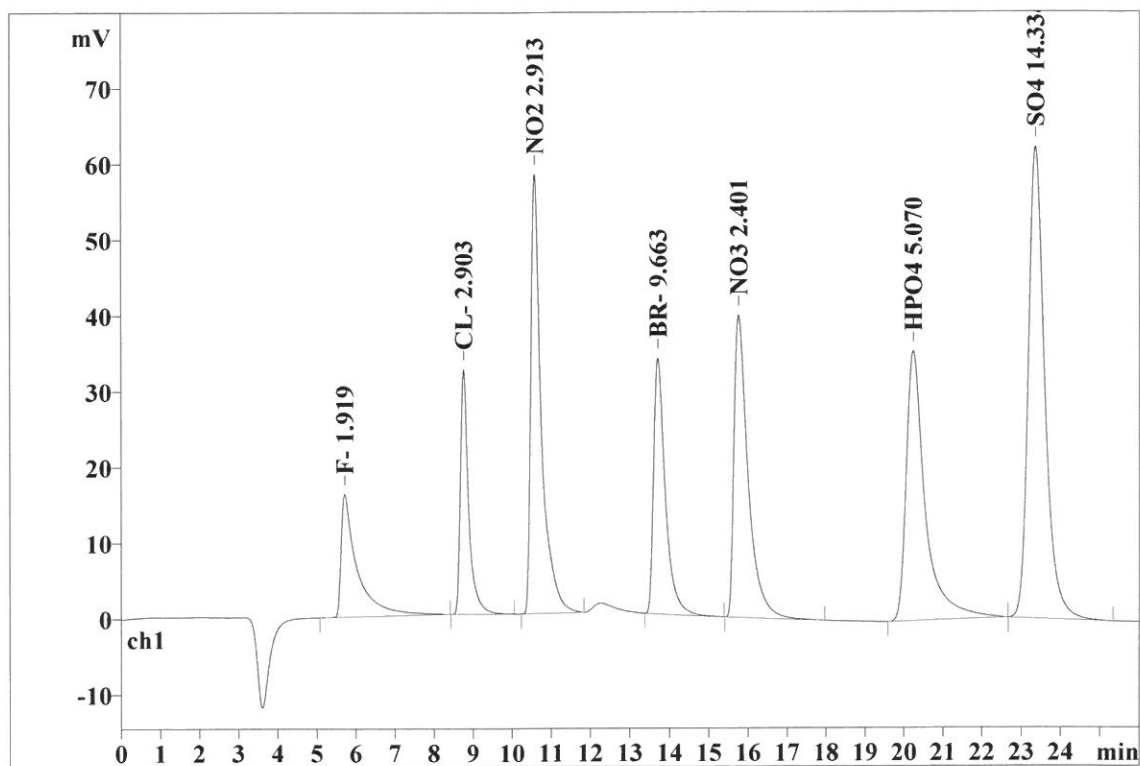

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.71             | 0.337          | 16.21        | 5.83        | 465.440        | 6.91      |
| 2  | 8.75             | 0.200          | 32.32        | 11.62       | 474.516        | 7.04      |
| 3  | 10.58            | 0.250          | 58.00        | 20.85       | 1086.780       | 16.13     |
| 4  | 13.71            | 0.297          | 33.77        | 12.14       | 699.665        | 10.38     |
| 5  | 15.77            | 0.354          | 39.92        | 14.35       | 992.591        | 14.73     |
| 6  | 20.25            | 0.448          | 35.64        | 12.81       | 1204.217       | 17.87     |
| 7  | 23.37            | 0.427          | 62.29        | 22.39       | 1815.436       | 26.94     |
| 7  | 26.00            | 0.330          | 278.15       | 100.00      | 6738.647       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/24/2022 12:59:21 PM  
Printed by: wet


Ident: STD6  
Analysis from: 2/24/2022 11:42:15 AM  
File: \_2022-02-24\_

Last save: 2/24/2022 12:37:49 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30176

Last save: 2/24/2022 12:08

SAMPLE:  
: IZ/AP  
Vial number: 7  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

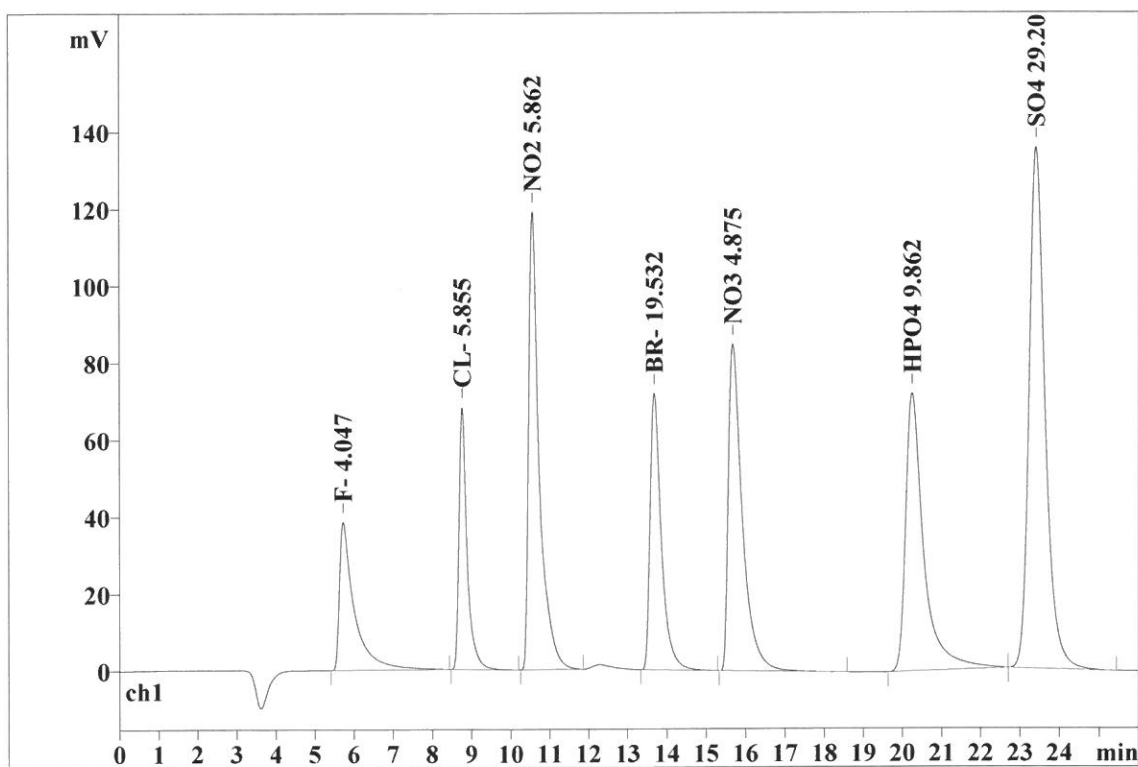

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.73             | 0.324          | 38.49        | 6.52        | 1015.017       | 7.27      |
| 2  | 8.75             | 0.199          | 68.10        | 11.54       | 983.311        | 7.05      |
| 3  | 10.56            | 0.255          | 118.99       | 20.16       | 2251.976       | 16.14     |
| 4  | 13.68            | 0.293          | 71.87        | 12.18       | 1458.432       | 10.45     |
| 5  | 15.69            | 0.350          | 84.90        | 14.39       | 2083.319       | 14.93     |
| 6  | 20.26            | 0.431          | 72.24        | 12.24       | 2316.210       | 16.60     |
| 7  | 23.41            | 0.419          | 135.48       | 22.96       | 3846.415       | 27.56     |
| 7  | 26.00            | 0.324          | 590.08       | 100.00      | 13954.680      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/24/2022 12:59:29 PM  
Printed by: wet


Ident: STD7  
Analysis from: 2/24/2022 12:10:54 PM  
File: \_2022-02-24\_

Last save: 2/24/2022 12:37:49 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30177

Last save: 2/24/2022 12:08

SAMPLE:  
: IZ/AP  
Vial number: 8  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

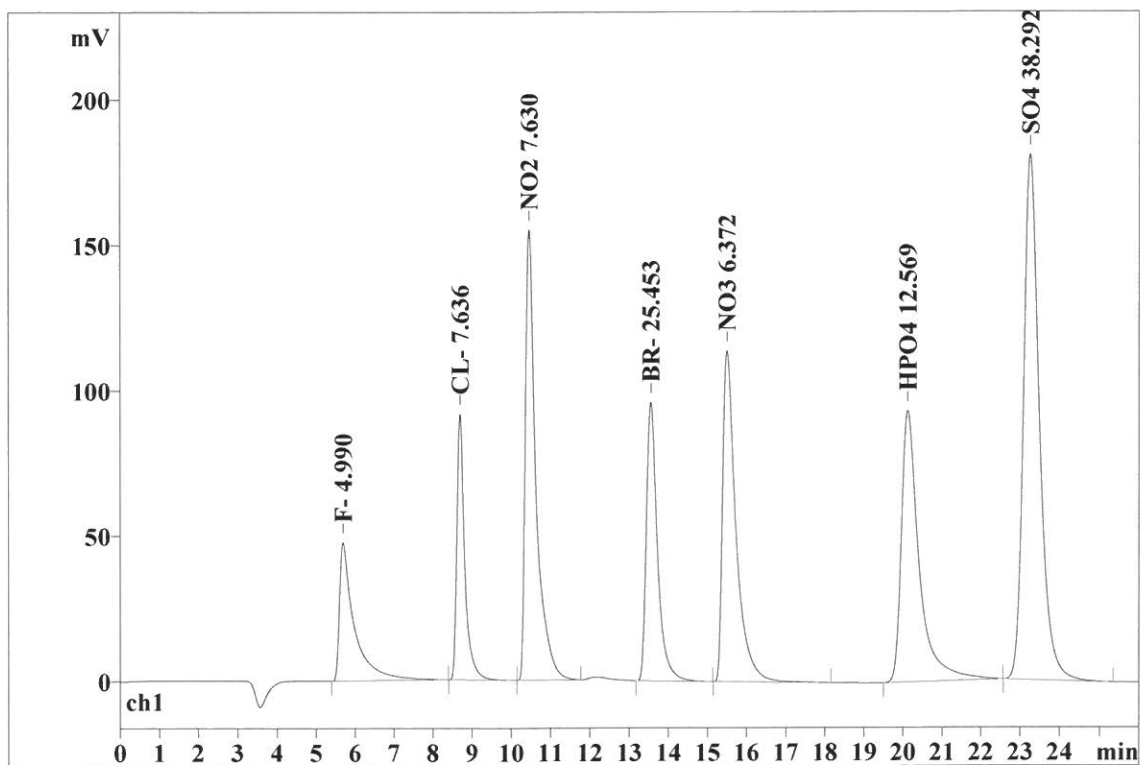

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.69             | 0.313          | 47.61        | 6.12        | 1258.404       | 6.92      |
| 2  | 8.68             | 0.193          | 91.47        | 11.76       | 1290.330       | 7.09      |
| 3  | 10.45            | 0.258          | 154.95       | 19.92       | 2950.434       | 16.22     |
| 4  | 13.54            | 0.288          | 95.82        | 12.32       | 1913.636       | 10.52     |
| 5  | 15.50            | 0.342          | 113.87       | 14.64       | 2743.646       | 15.08     |
| 6  | 20.13            | 0.424          | 93.42        | 12.01       | 2944.504       | 16.19     |
| 7  | 23.27            | 0.414          | 180.82       | 23.24       | 5088.277       | 27.97     |
| 7  | 26.00            | 0.319          | 777.95       | 100.00      | 18189.231      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/24/2022 2:05:54 PM  
Printed by: wet


Ident: ICV  
Analysis from: 2/24/2022 1:22:55 PM  
File: \_2022-02-24\_

Last save: 2/24/2022 1:48:55 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30179

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 9  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

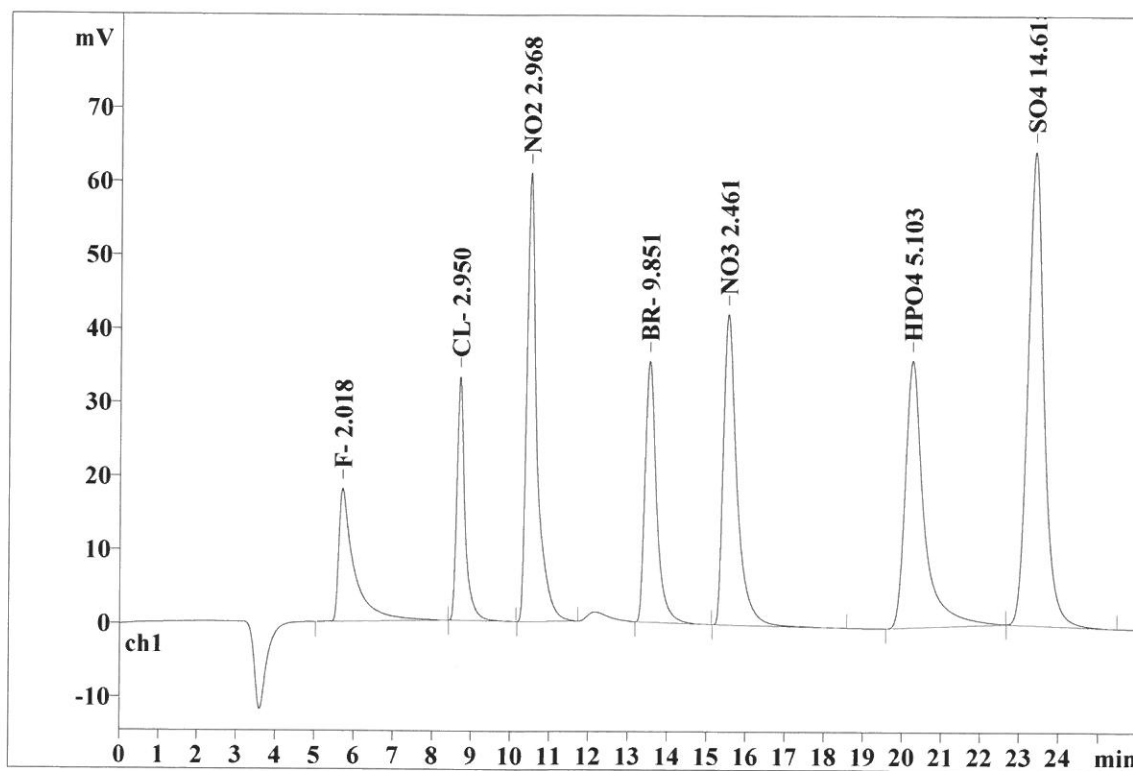

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.70             | 0.327          | 18.05        | 6.22        | 491.102        | 7.14      |
| 2  | 8.68             | 0.200          | 33.10        | 11.41       | 482.727        | 7.02      |
| 3  | 10.47            | 0.243          | 60.87        | 20.98       | 1108.208       | 16.11     |
| 4  | 13.52            | 0.291          | 35.44        | 12.21       | 714.120        | 10.38     |
| 5  | 15.52            | 0.345          | 42.16        | 14.53       | 1018.650       | 14.80     |
| 6  | 20.23            | 0.444          | 36.24        | 12.49       | 1211.847       | 17.61     |
| 7  | 23.36            | 0.424          | 64.29        | 22.16       | 1853.934       | 26.94     |
| 7  | 26.00            | 0.325          | 290.13       | 100.00      | 6880.588       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/24/2022 2:34:43 PM  
Printed by: wet


Ident: ICB  
Analysis from: 2/24/2022 1:52:06 PM  
File: \_2022-02-24\_

Last save: 2/24/2022 2:18:07 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30180

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 10  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

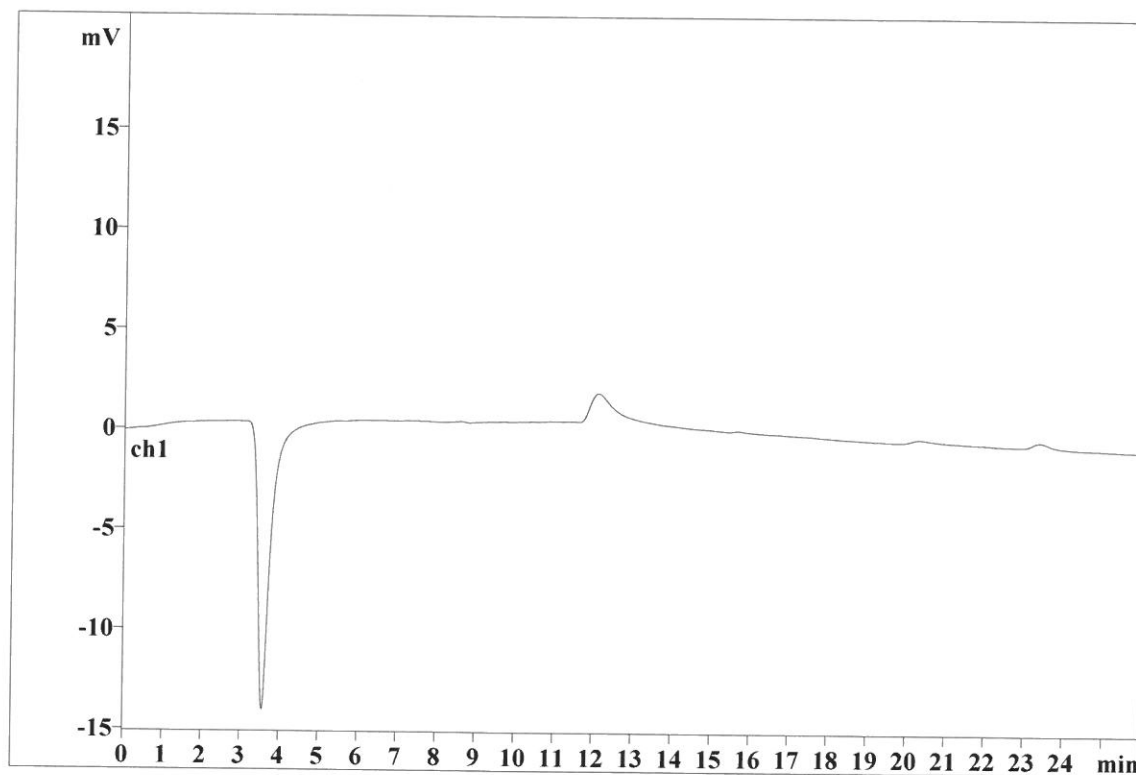

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 1:25:58 PM  
Printed by: wet


Ident: CCV  
Analysis from: 2/24/2022 11:28:18 PM  
File: \_2022-02-24\_

Last save: 2/24/2022 11:54:18 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30200

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 11  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

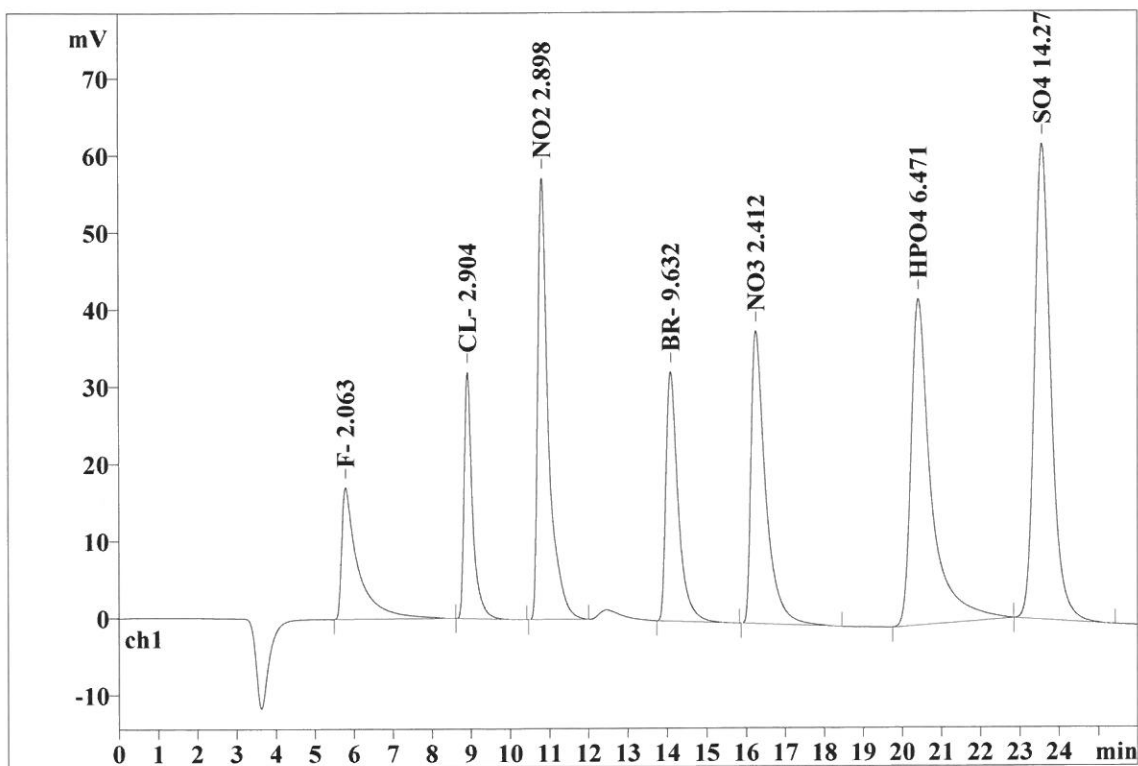

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.78             | 0.352          | 17.09        | 6.08        | 502.611        | 7.09      |
| 2  | 8.90             | 0.205          | 31.98        | 11.38       | 474.790        | 6.70      |
| 3  | 10.80            | 0.252          | 57.32        | 20.40       | 1080.662       | 15.24     |
| 4  | 14.09            | 0.310          | 32.38        | 11.53       | 697.282        | 9.84      |
| 5  | 16.25            | 0.372          | 38.02        | 13.53       | 997.176        | 14.07     |
| 6  | 20.41            | 0.469          | 42.36        | 15.08       | 1529.403       | 21.57     |
| 7  | 23.57            | 0.431          | 61.76        | 21.99       | 1807.595       | 25.50     |
| 7  | 26.00            | 0.342          | 280.90       | 100.00      | 7089.520       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 1:26:11 PM  
Printed by: wet


Ident: CCB  
Analysis from: 2/24/2022 11:56:56 PM  
File: \_2022-02-24\_

Last save: 2/25/2022 12:22:56 AM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30201

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 12  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

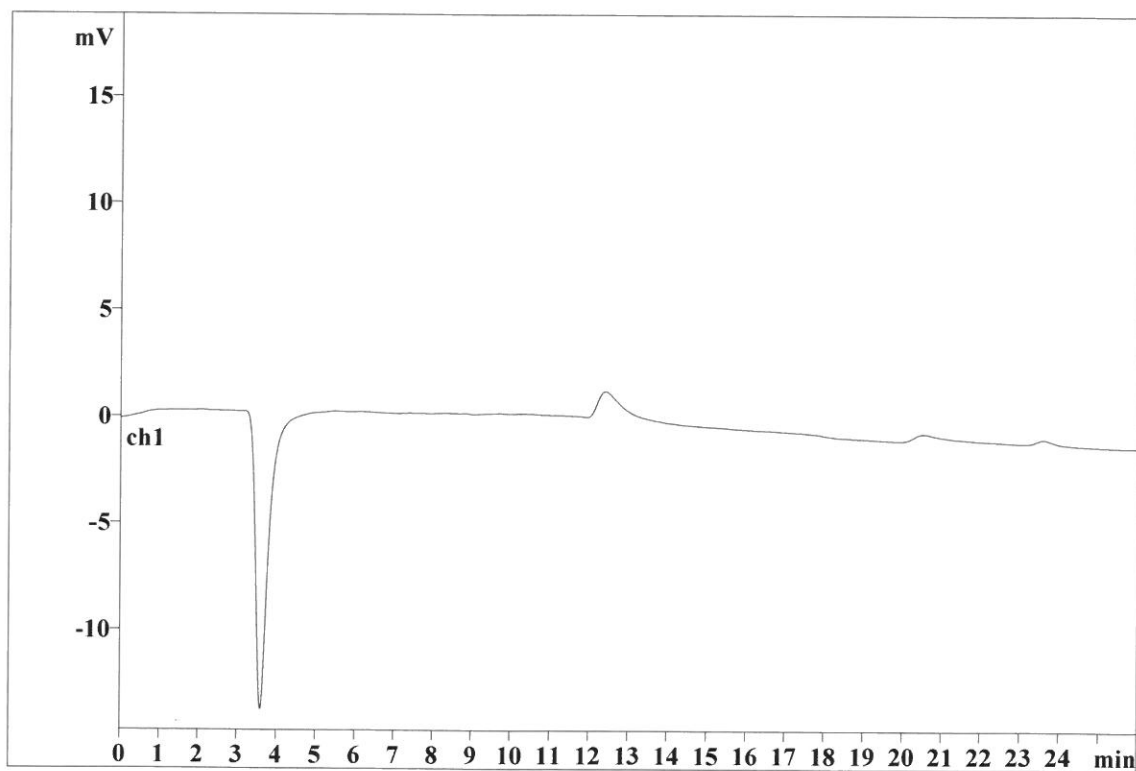

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 1:27:22 PM  
Printed by: wet


Ident: N1671-01  
Analysis from: 2/25/2022 9:05:39 AM  
File: \_2022-02-25\_

Last save: 2/25/2022 9:51:52 AM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30205

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 26  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

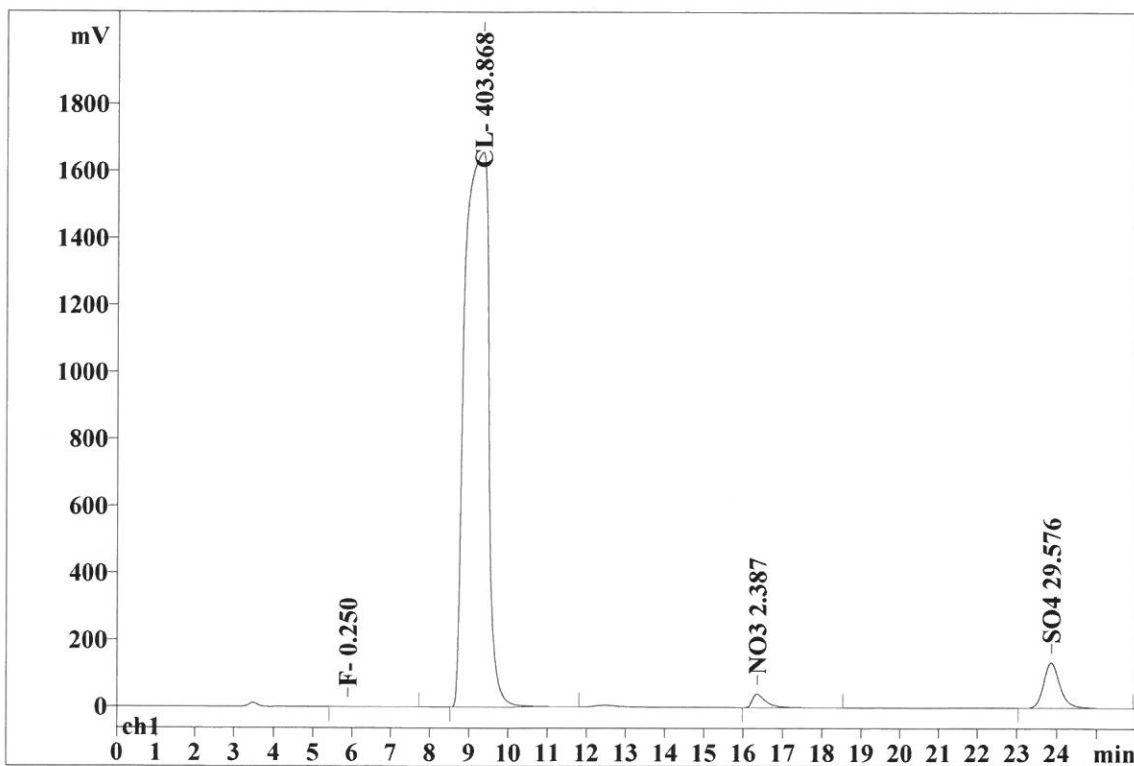

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.88             | 0.751          | 0.66         | 0.04        | 34.468         | 0.05      |
| 2  | 9.29             | 0.687          | 1656.89      | 90.34       | 69575.764      | 93.40     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 16.35            | 0.348          | 40.55        | 2.21        | 986.452        | 1.32      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 23.85            | 0.419          | 135.91       | 7.41        | 3897.651       | 5.23      |
| 7  | 26.00            | 0.315          | 1834.01      | 100.00      | 74494.335      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 1:27:36 PM  
Printed by: wet


Ident: N1671-03  
Analysis from: 2/25/2022 9:34:17 AM  
File: \_2022-02-25\_

Last save: 2/25/2022 10:19:53 AM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30206

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 27  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

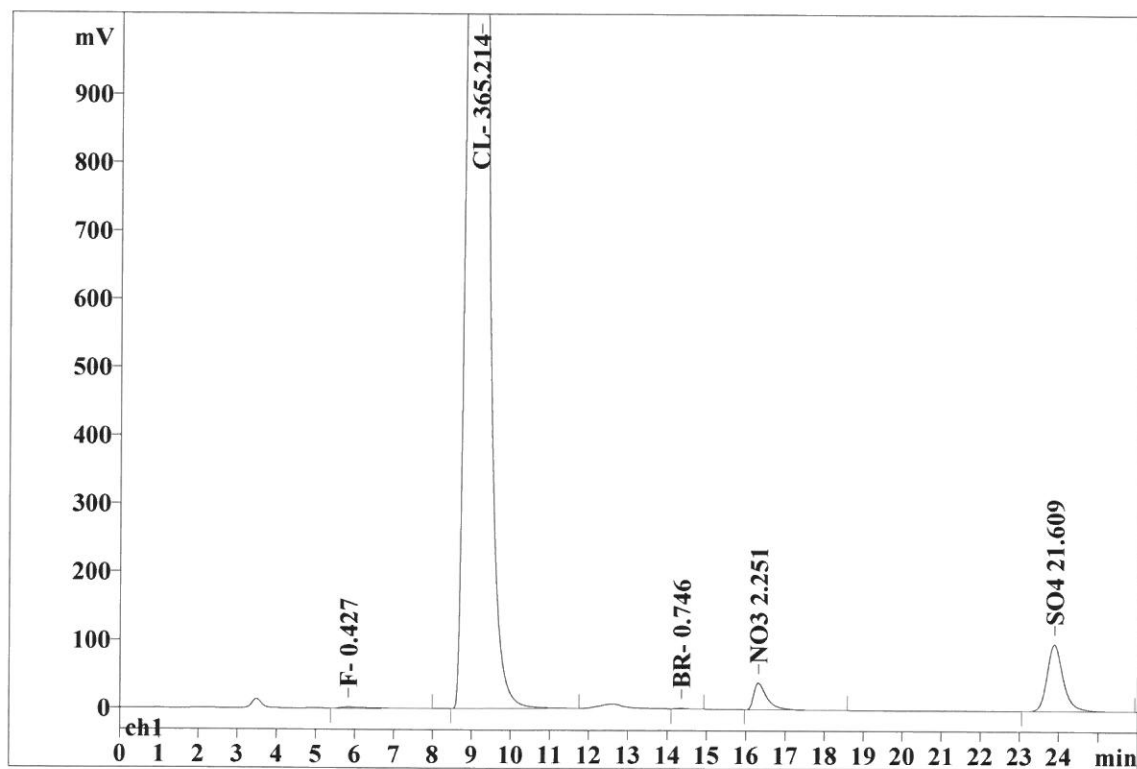

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.84             | 0.725          | 1.54         | 0.09        | 80.159         | 0.12      |
| 2  | 9.14             | 0.606          | 1627.21      | 92.10       | 62914.188      | 94.26     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 14.36            | 0.275          | 0.79         | 0.04        | 14.110         | 0.02      |
| 5  | 16.31            | 0.335          | 39.33        | 2.23        | 926.228        | 1.39      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 23.88            | 0.417          | 97.97        | 5.54        | 2809.294       | 4.21      |
| 7  | 26.00            | 0.337          | 1766.83      | 100.00      | 66743.979      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 1:28:33 PM  
Printed by: wet


Ident: N1671-05  
Analysis from: 2/25/2022 10:02:55 AM  
File: \_2022-02-25\_

Last save: 2/25/2022 10:28:56 AM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30207

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 28  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

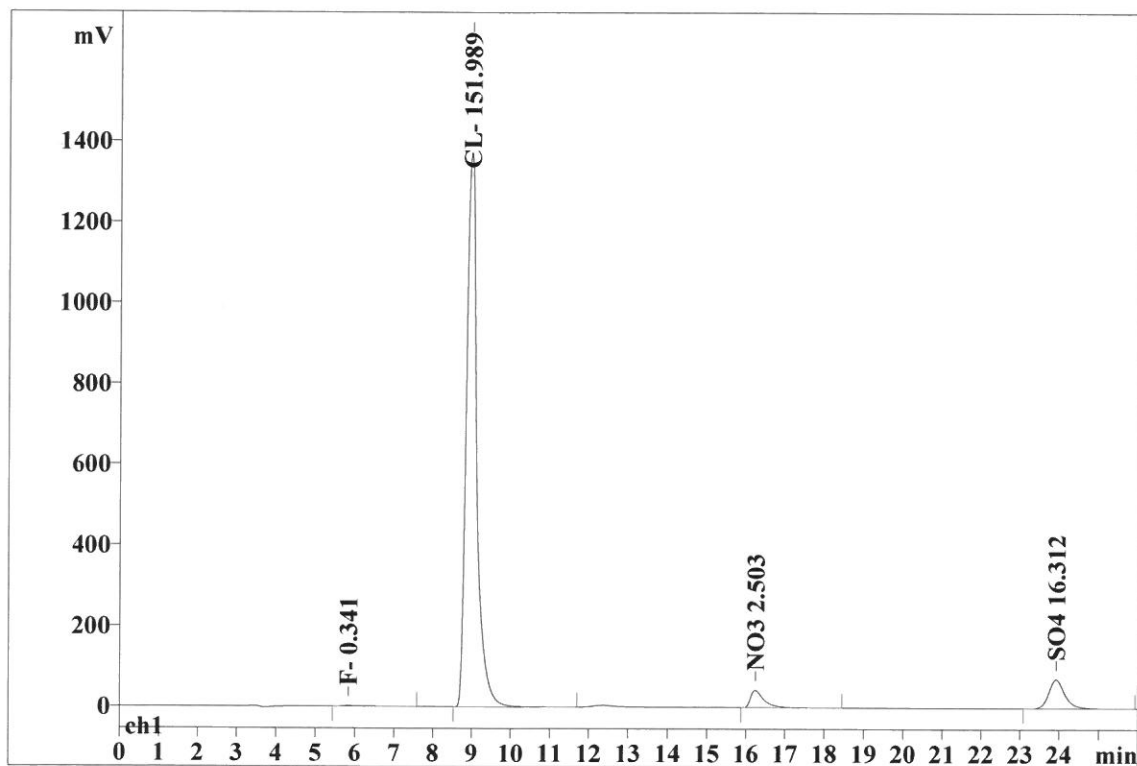

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.83             | 0.595          | 1.34         | 0.09        | 58.046         | 0.20      |
| 2  | 8.94             | 0.267          | 1372.93      | 92.23       | 26167.687      | 89.16     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 16.24            | 0.345          | 42.79        | 2.87        | 1037.254       | 3.53      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 23.92            | 0.426          | 71.61        | 4.81        | 2085.737       | 7.11      |
| 7  | 26.00            | 0.233          | 1488.67      | 100.00      | 29348.725      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 1:28:50 PM  
Printed by: wet


Ident: N1671-07  
Analysis from: 2/25/2022 10:31:34 AM  
File: \_2022-02-25\_

Last save: 2/25/2022 11:07:29 AM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30208

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 29  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

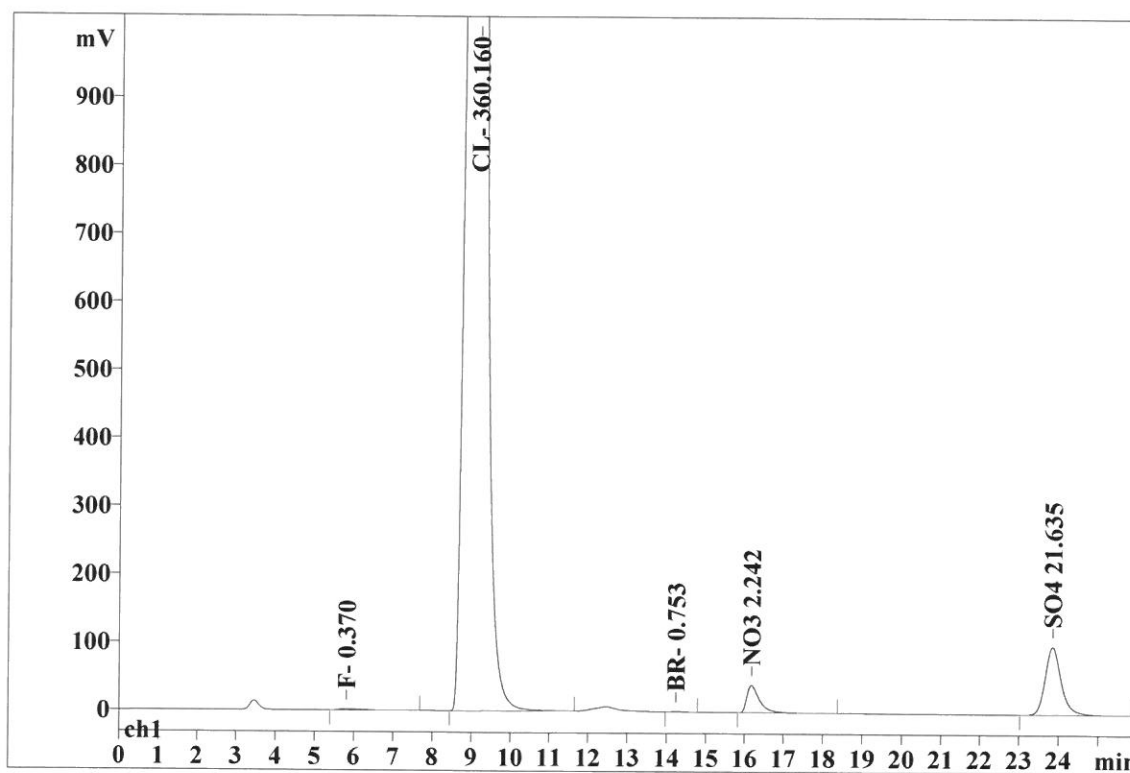

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.81             | 0.654          | 1.40         | 0.08        | 65.456         | 0.10      |
| 2  | 9.11             | 0.605          | 1630.09      | 91.98       | 62043.189      | 94.21     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 14.24            | 0.274          | 0.82         | 0.05        | 14.649         | 0.02      |
| 5  | 16.18            | 0.330          | 40.09        | 2.26        | 922.420        | 1.40      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 23.84            | 0.413          | 99.75        | 5.63        | 2812.885       | 4.27      |
| 7  | 26.00            | 0.325          | 1772.15      | 100.00      | 65858.599      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 1:29:06 PM  
Printed by: wet

Ident: N1671-07MS  
Analysis from: 2/25/2022 11:00:12 AM  
File: \_2022-02-25\_


Last save: 2/25/2022 12:32:15 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30209

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 30  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

*Refere*

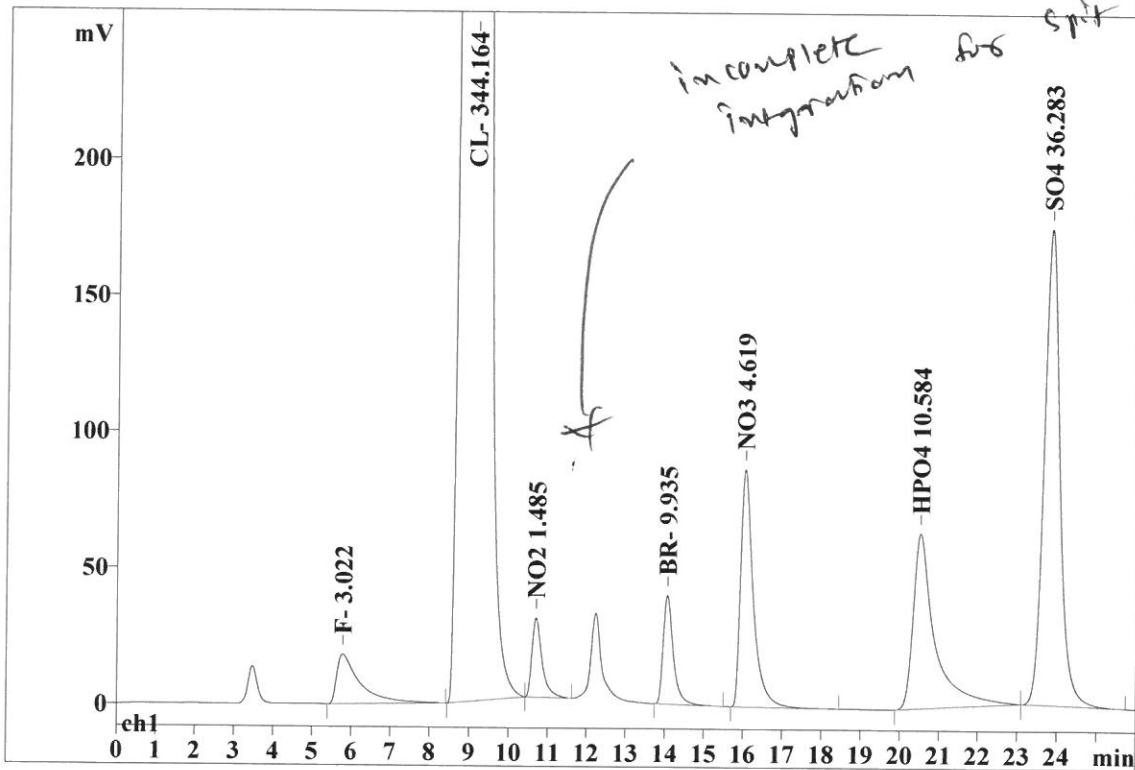

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.78             | 0.537          | 18.17        | 0.89        | 750.158        | 1.06      |
| 2  | 9.09             | 0.582          | 1626.66      | 79.75       | 59286.548      | 84.04     |
| 3  | 10.69            | 0.257          | 29.00        | 1.42        | 522.560        | 0.74      |
| 4  | 14.06            | 0.261          | 39.91        | 1.96        | 720.601        | 1.02      |
| 5  | 16.03            | 0.324          | 87.09        | 4.27        | 1970.608       | 2.79      |
| 6  | 20.50            | 0.474          | 64.22        | 3.15        | 2483.904       | 3.52      |
| 7  | 23.80            | 0.407          | 174.57       | 8.56        | 4813.802       | 6.82      |
| 7  | 26.00            | 0.406          | 2039.61      | 100.00      | 70548.181      | 100.00    |

This report has been created by IC Net  
METROHM LTD


Report date: 2/25/2022 1:29:26 PM  
Printed by: wet

Ident: N1671-07MS  
Analysis from: 2/25/2022 11:00:12 AM  
File: 2022-02-25\_  
Modified! Manual peaks!  
Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30209

Last save: 2/25/2022 12:32:15 PM

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 30  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

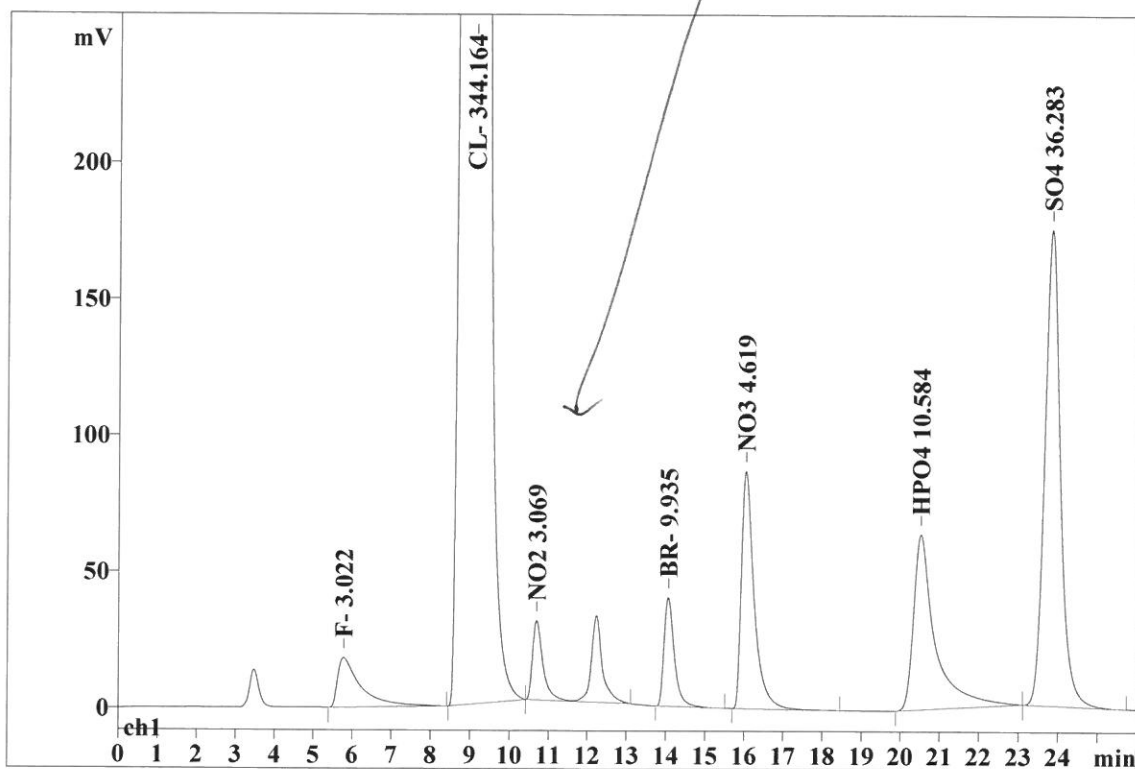

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.78             | 0.537          | 18.17        | 0.89        | 750.158        | 1.05      |
| 2  | 9.09             | 0.582          | 1626.66      | 79.75       | 59286.548      | 83.30     |
| 3  | 10.69            | 0.525          | 29.04        | 1.42        | 1148.161       | 1.61      |
| 4  | 14.06            | 0.261          | 39.91        | 1.96        | 720.601        | 1.01      |
| 5  | 16.03            | 0.324          | 87.09        | 4.27        | 1970.608       | 2.77      |
| 6  | 20.50            | 0.474          | 64.22        | 3.15        | 2483.904       | 3.49      |
| 7  | 23.80            | 0.407          | 174.57       | 8.56        | 4813.802       | 6.76      |
| 7  | 26.00            | 0.444          | 2039.65      | 100.00      | 71173.781      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 1:29:37 PM  
Printed by: wet


Ident: N1671-07MSD  
Analysis from: 2/25/2022 11:28:51 AM  
File: \_2022-02-25\_

Last save: 2/25/2022 12:31:53 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30210

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 31  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

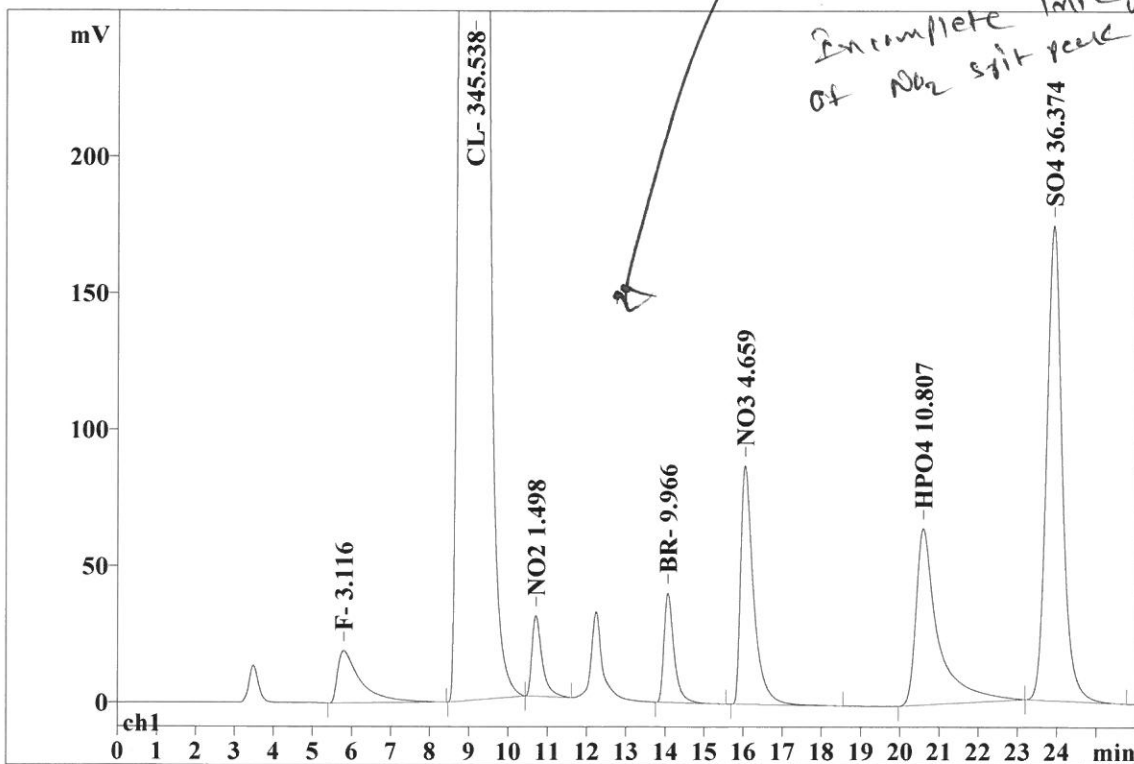

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.80             | 0.531          | 19.14        | 0.94        | 774.631        | 1.09      |
| 2  | 9.11             | 0.584          | 1625.03      | 79.66       | 59523.350      | 83.96     |
| 3  | 10.70            | 0.255          | 29.61        | 1.45        | 527.641        | 0.74      |
| 4  | 14.07            | 0.262          | 40.04        | 1.96        | 722.955        | 1.02      |
| 5  | 16.04            | 0.324          | 87.38        | 4.28        | 1988.072       | 2.80      |
| 6  | 20.58            | 0.480          | 64.65        | 3.17        | 2535.584       | 3.58      |
| 7  | 23.89            | 0.409          | 174.02       | 8.53        | 4826.292       | 6.81      |
| 7  | 26.00            | 0.406          | 2039.88      | 100.00      | 70898.525      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 1:29:50 PM  
Printed by: wet


Ident: N1671-07MSD  
Analysis from: 2/25/2022 11:28:51 AM  
File: 2022-02-25  
Modified! Manual peaks!  
Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30210

Last save: 2/25/2022 12:31:53 PM

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 31  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

*After*  
*2/25/22*

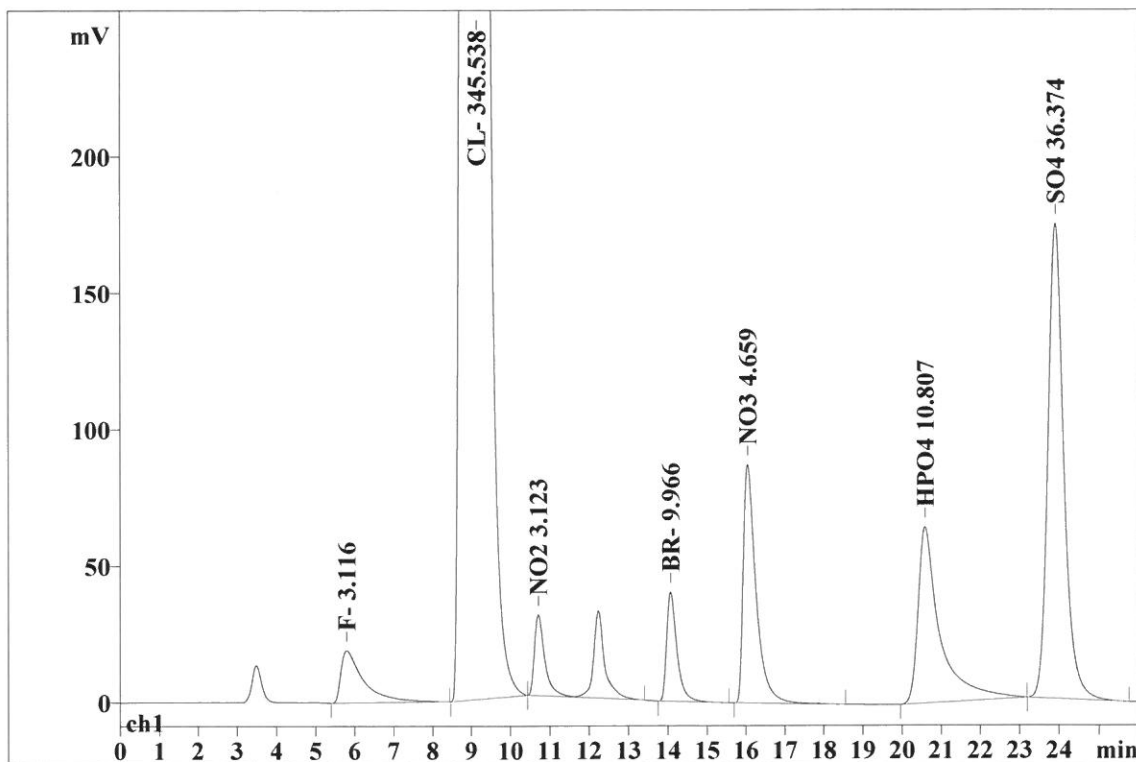

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.80             | 0.531          | 19.14        | 0.94        | 774.631        | 1.08      |
| 2  | 9.11             | 0.584          | 1625.03      | 79.66       | 59523.350      | 83.20     |
| 3  | 10.70            | 0.517          | 29.66        | 1.45        | 1169.786       | 1.64      |
| 4  | 14.07            | 0.262          | 40.04        | 1.96        | 722.955        | 1.01      |
| 5  | 16.04            | 0.324          | 87.38        | 4.28        | 1988.072       | 2.78      |
| 6  | 20.58            | 0.480          | 64.65        | 3.17        | 2535.584       | 3.54      |
| 7  | 23.89            | 0.409          | 174.02       | 8.53        | 4826.292       | 6.75      |
| 7  | 26.00            | 0.444          | 2039.93      | 100.00      | 71540.669      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/28/2022 10:21:54 AM  
Printed by: wet


Ident: LB118840BLW  
Analysis from: 2/25/2022 11:57:37 AM  
File: \_2022-02-25\_

Last save: 2/28/2022 10:21:42 AM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30211

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 13  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

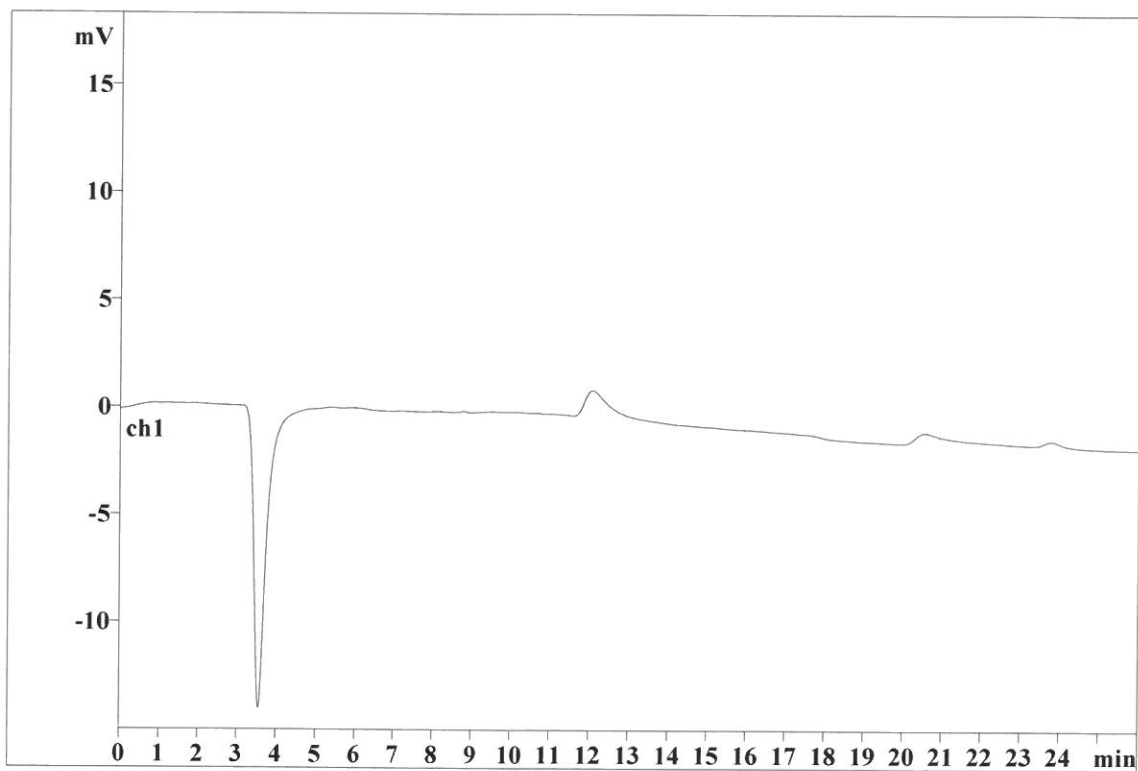

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 2/28/2022 10:22:03 AM  
Printed by: wet


Ident: LB118840BSW  
Analysis from: 2/25/2022 12:26:15 PM  
File: \_2022-02-25\_

Last save: 2/28/2022 10:21:42 AM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30212

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 14  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

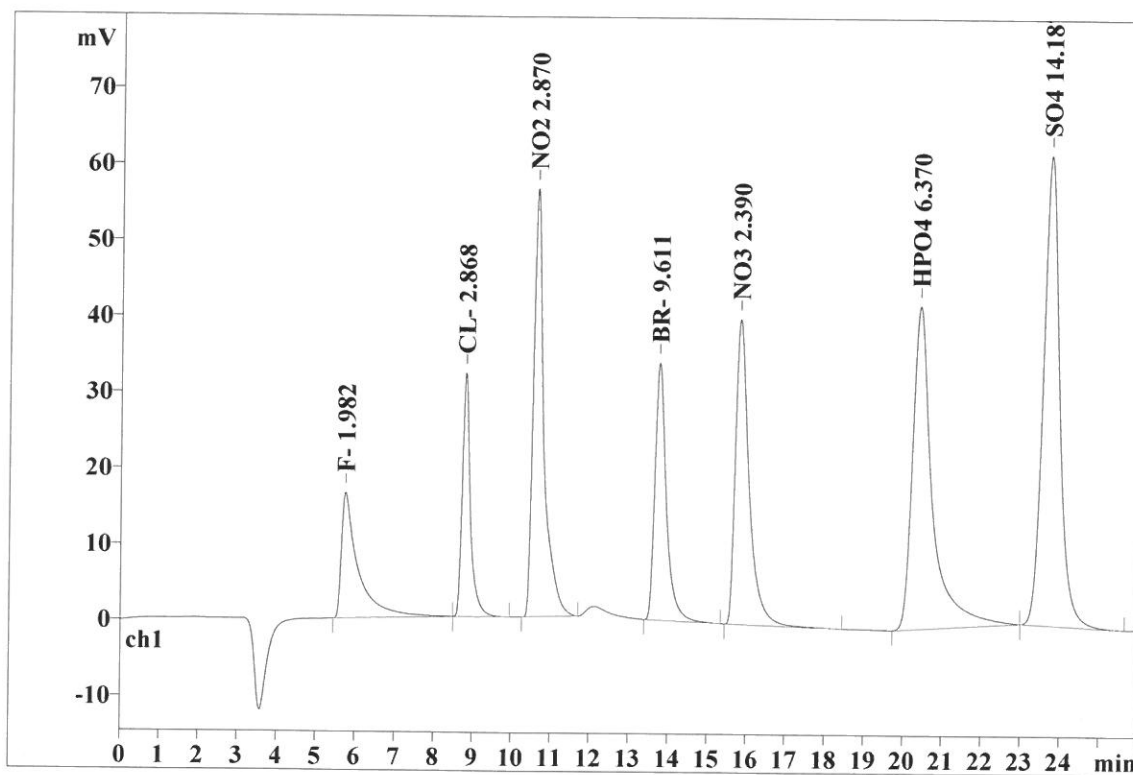

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.74             | 0.349          | 16.48        | 5.82        | 481.789        | 6.88      |
| 2  | 8.77             | 0.203          | 32.03        | 11.32       | 468.618        | 6.69      |
| 3  | 10.60            | 0.253          | 56.27        | 19.89       | 1069.667       | 15.27     |
| 4  | 13.74            | 0.297          | 33.82        | 11.95       | 695.678        | 9.93      |
| 5  | 15.81            | 0.352          | 40.14        | 14.19       | 987.462        | 14.10     |
| 6  | 20.39            | 0.458          | 42.43        | 14.99       | 1505.898       | 21.50     |
| 7  | 23.71            | 0.429          | 61.79        | 21.84       | 1795.454       | 25.63     |
| 7  | 26.00            | 0.334          | 282.96       | 100.00      | 7004.565       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 1:30:16 PM  
Printed by: wet


Ident: CCV  
Analysis from: 2/25/2022 12:54:56 PM  
File: \_2022-02-25\_

Last save: 2/25/2022 1:20:56 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30213

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 11  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

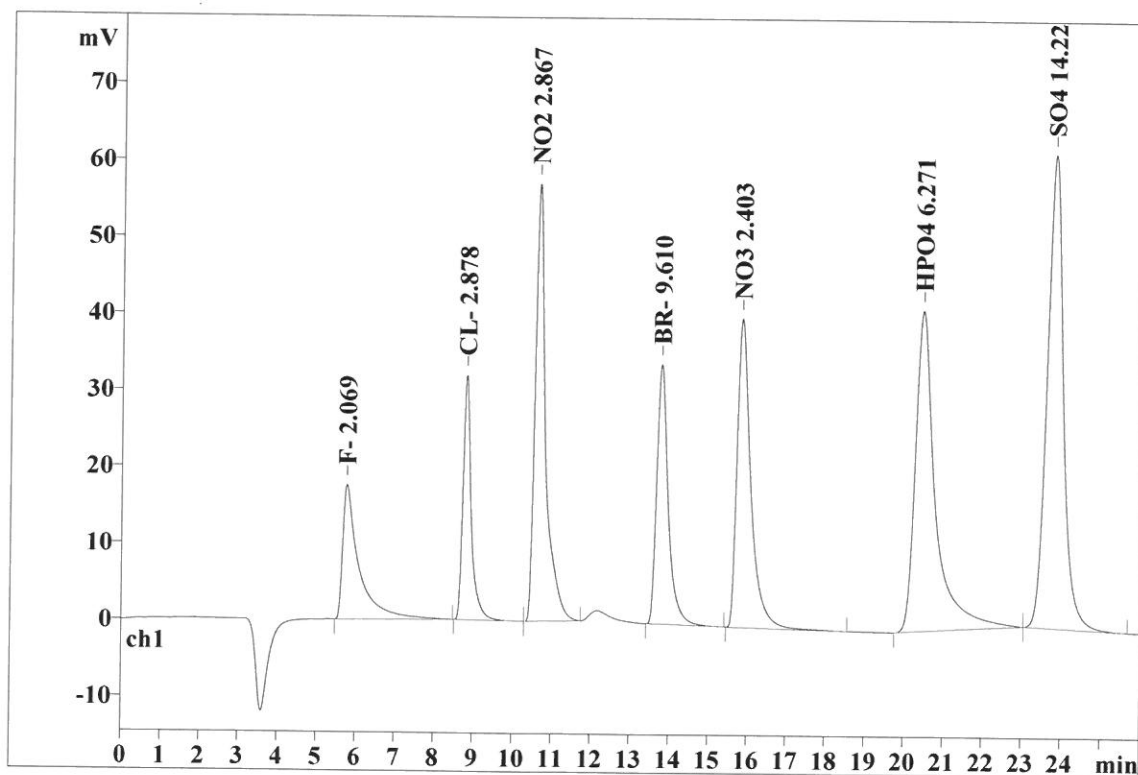

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.76             | 0.348          | 17.54        | 6.17        | 504.287        | 7.19      |
| 2  | 8.79             | 0.204          | 31.92        | 11.23       | 470.332        | 6.70      |
| 3  | 10.62            | 0.248          | 57.06        | 20.08       | 1068.407       | 15.23     |
| 4  | 13.77            | 0.297          | 33.89        | 11.92       | 695.631        | 9.92      |
| 5  | 15.82            | 0.352          | 40.26        | 14.16       | 993.506        | 14.16     |
| 6  | 20.44            | 0.458          | 41.80        | 14.71       | 1482.782       | 21.14     |
| 7  | 23.77            | 0.430          | 61.76        | 21.73       | 1800.025       | 25.66     |
| 7  | 26.00            | 0.334          | 284.23       | 100.00      | 7014.971       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 2:06:40 PM  
Printed by: wet


Ident: CCB  
Analysis from: 2/25/2022 1:23:35 PM  
File: \_2022-02-25\_

Last save: 2/25/2022 1:49:35 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30214

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 12  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

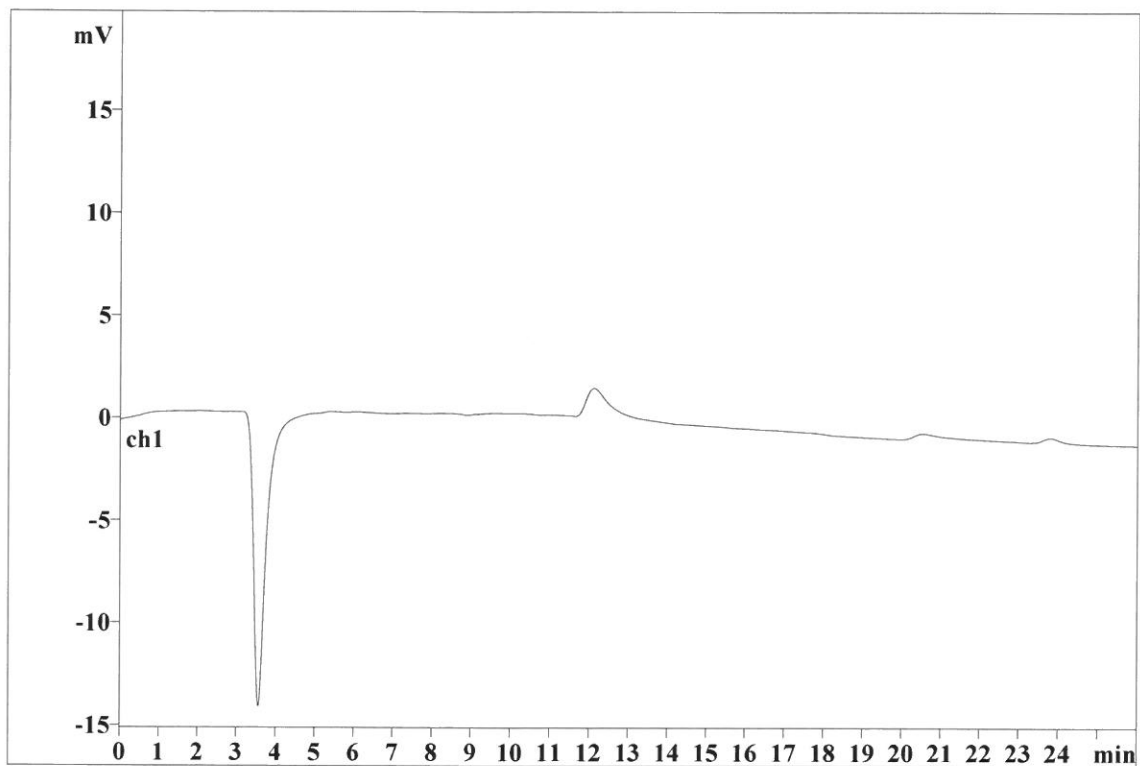

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 3:15:54 PM  
Printed by: wet


Ident: N1680-01  
Analysis from: 2/25/2022 1:52:23 PM  
File: \_2022-02-25\_

Last save: 2/25/2022 2:18:23 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30215

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 32  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

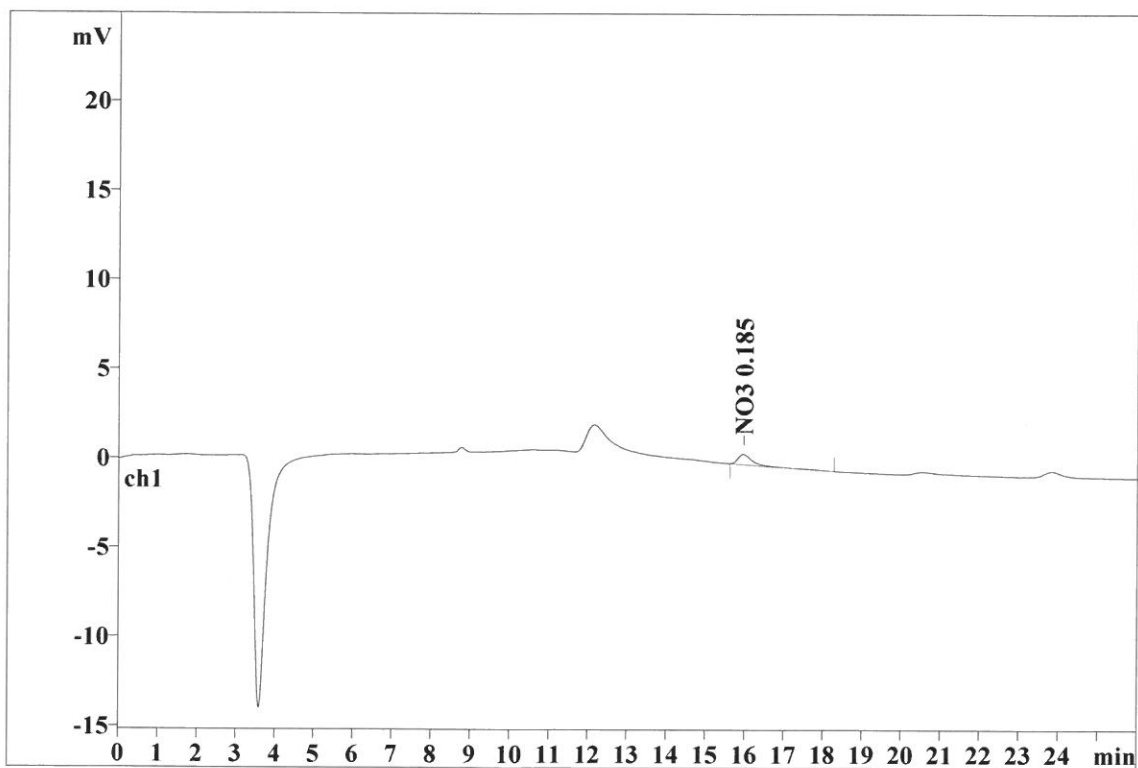

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.96            | 0.357          | 0.57         | 99.70       | 15.151         | 100.00    |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 26.00            | 0.051          | 0.57         | 99.70       | 15.151         | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 3:16:04 PM  
Printed by: wet


Ident: N1680-02  
Analysis from: 2/25/2022 2:21:01 PM  
File: \_2022-02-25\_

Last save: 2/25/2022 2:47:01 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30216

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 33  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

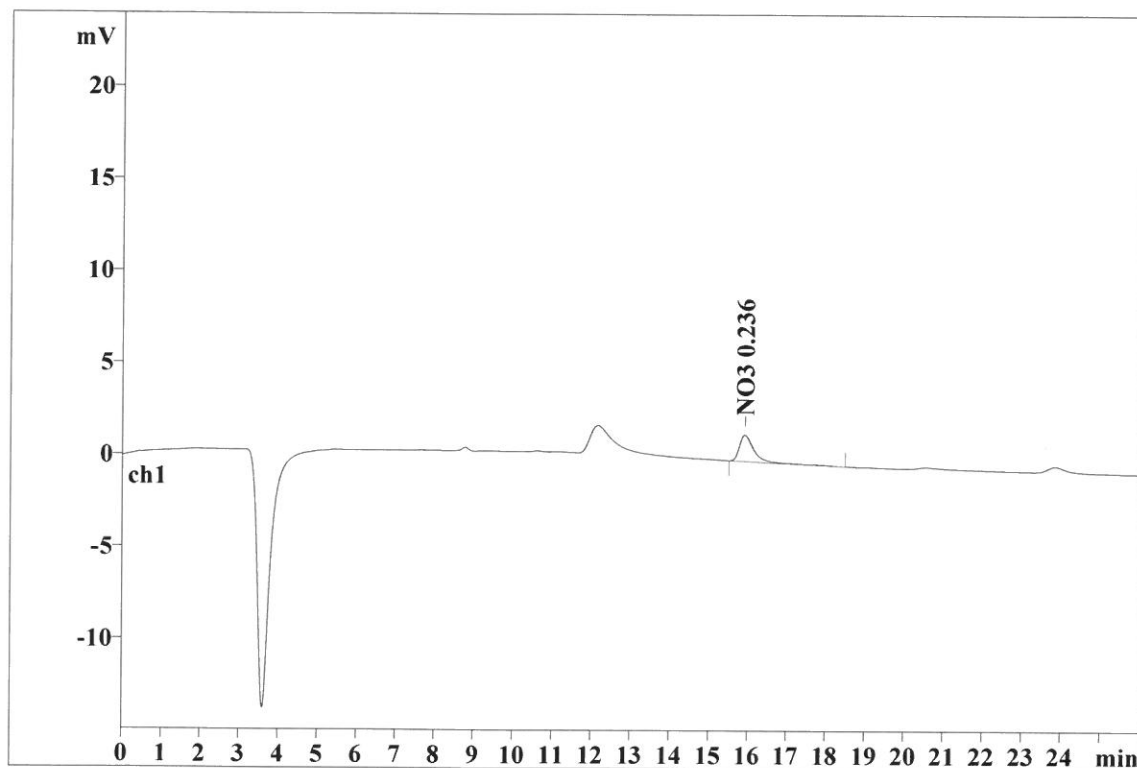

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.91            | 0.360          | 1.44         | 99.88       | 37.590         | 100.00    |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 26.00            | 0.051          | 1.44         | 99.88       | 37.590         | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 3:16:13 PM  
Printed by: wet


Ident: N1680-03  
Analysis from: 2/25/2022 2:49:38 PM  
File: \_2022-02-25\_

Last save: 2/25/2022 3:15:39 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30217

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 34  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

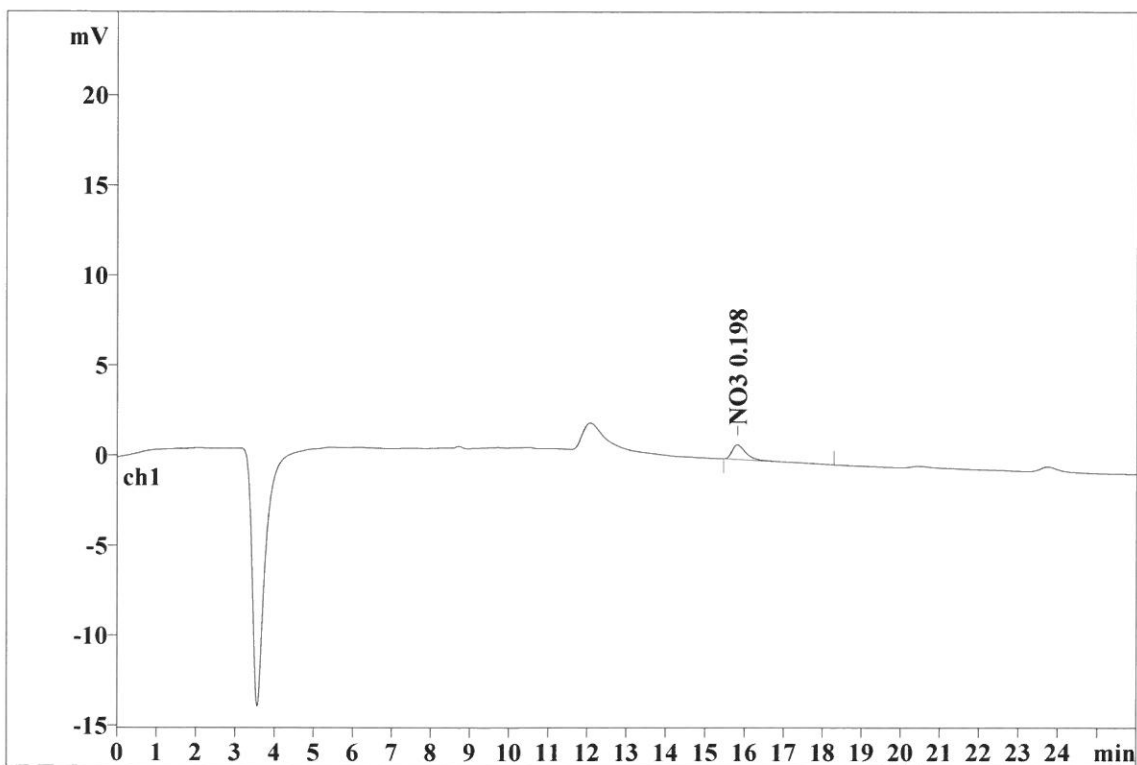

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.81            | 0.356          | 0.82         | 99.72       | 21.092         | 100.00    |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 26.00            | 0.051          | 0.82         | 99.72       | 21.092         | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 3:44:34 PM  
Printed by: wet


Ident: N1671-01DLX100  
Analysis from: 2/25/2022 3:18:17 PM  
File: \_2022-02-25\_

Last save: 2/25/2022 3:44:18 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30218

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 35  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

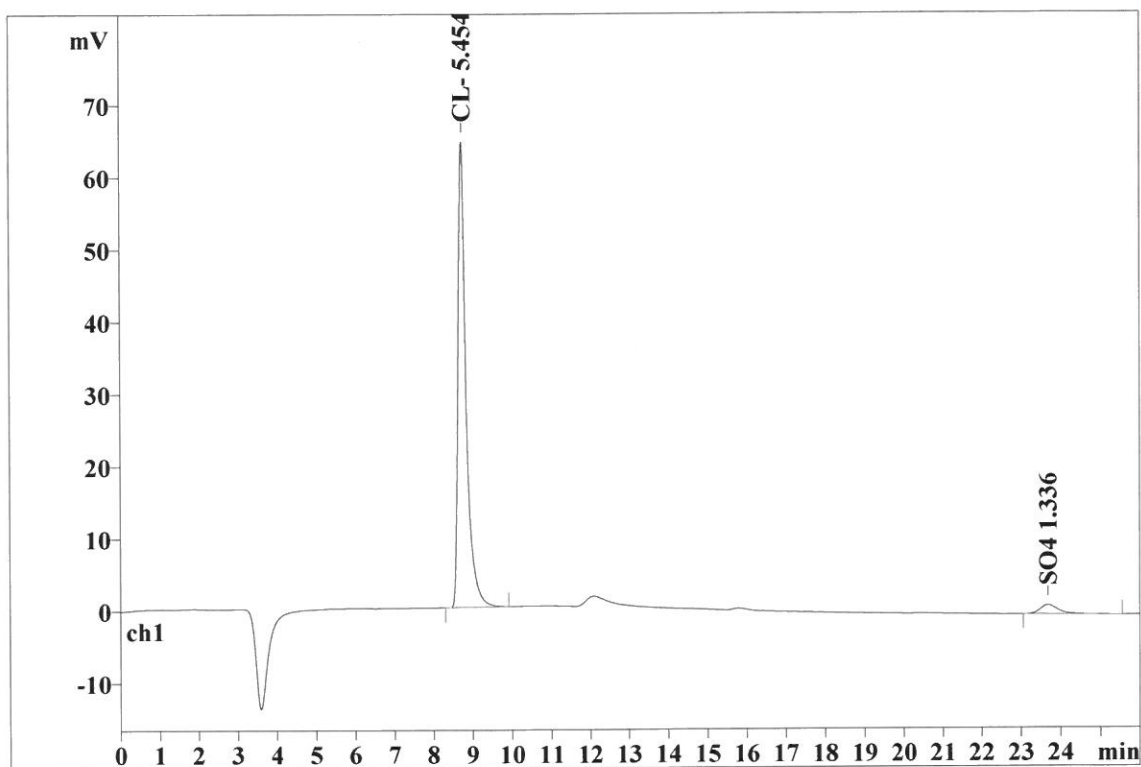

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.71             | 0.196          | 64.49        | 98.07       | 914.276        | 95.82     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 23.68            | 0.459          | 1.27         | 1.93        | 39.852         | 4.18      |
| 7  | 26.00            | 0.094          | 65.76        | 100.00      | 954.127        | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 4:26:41 PM  
Printed by: wet


Ident: N1671-03DLX100  
Analysis from: 2/25/2022 3:46:56 PM  
File: \_2022-02-25\_

Last save: 2/25/2022 4:12:57 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30219

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 36  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

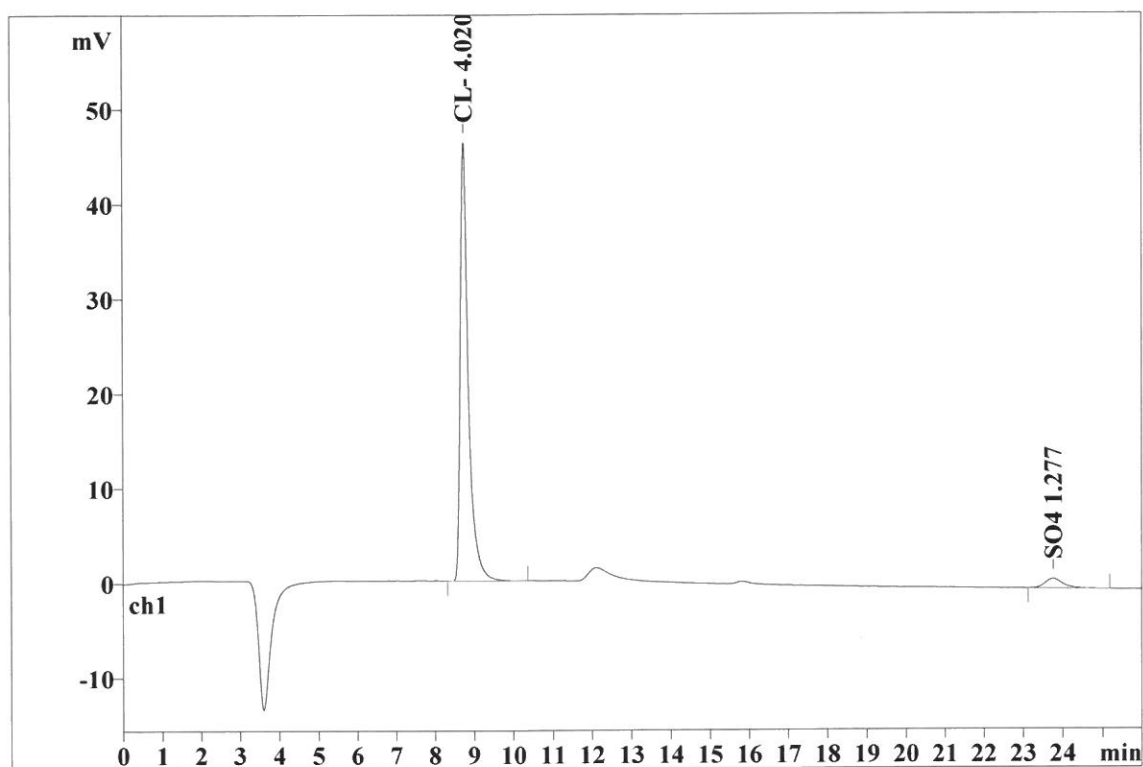

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.73             | 0.199          | 46.28        | 97.88       | 667.006        | 95.44     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 23.76            | 0.463          | 1.00         | 2.11        | 31.841         | 4.56      |
| 7  | 26.00            | 0.095          | 47.28        | 99.99       | 698.847        | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/25/2022 4:46:14 PM  
Printed by: wet


Ident: N1671-05DLX50  
Analysis from: 2/25/2022 4:15:34 PM  
File: \_2022-02-25\_

Last save: 2/25/2022 4:41:35 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30220

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 37  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

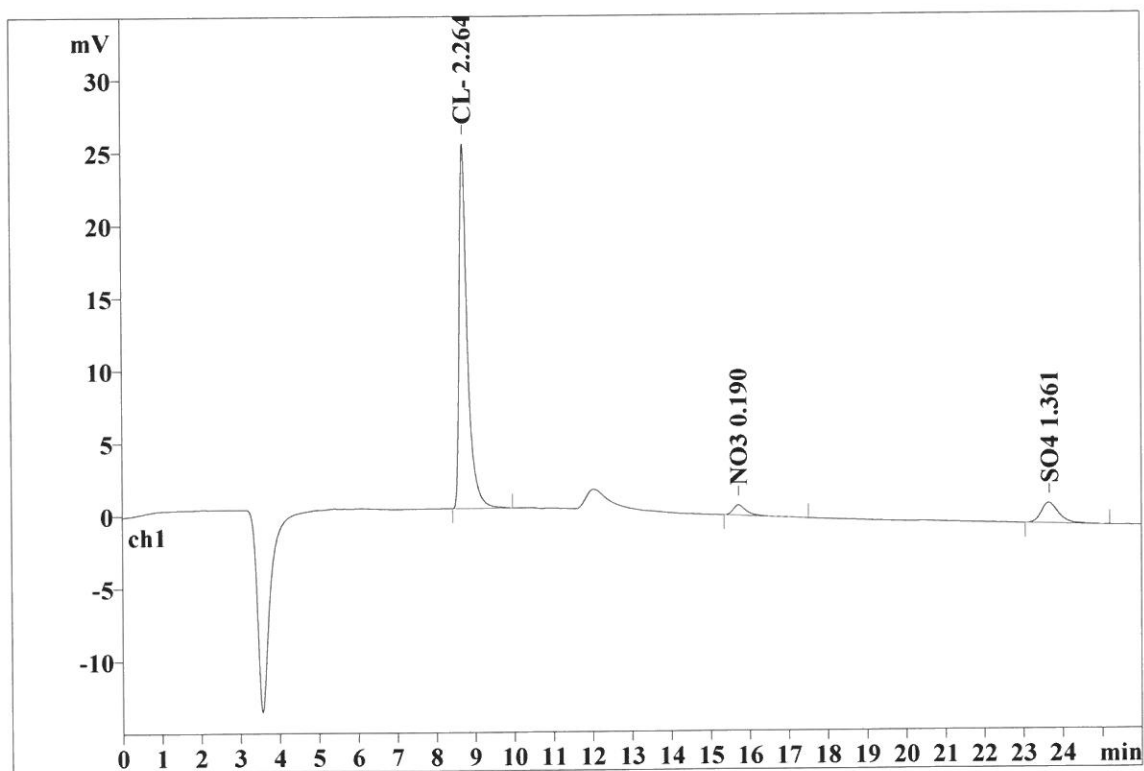

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.69             | 0.201          | 25.11        | 92.24       | 364.505        | 85.72     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.72            | 0.351          | 0.70         | 2.59        | 17.362         | 4.08      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 23.66            | 0.457          | 1.40         | 5.15        | 43.336         | 10.19     |
| 7  | 26.00            | 0.144          | 27.21        | 99.98       | 425.203        | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/28/2022 10:04:11 AM  
Printed by: wet


Ident: N1671-07DLX100  
Analysis from: 2/25/2022 4:44:12 PM  
File: \_2022-02-25\_

Last save: 2/25/2022 5:10:13 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30221

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 38  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

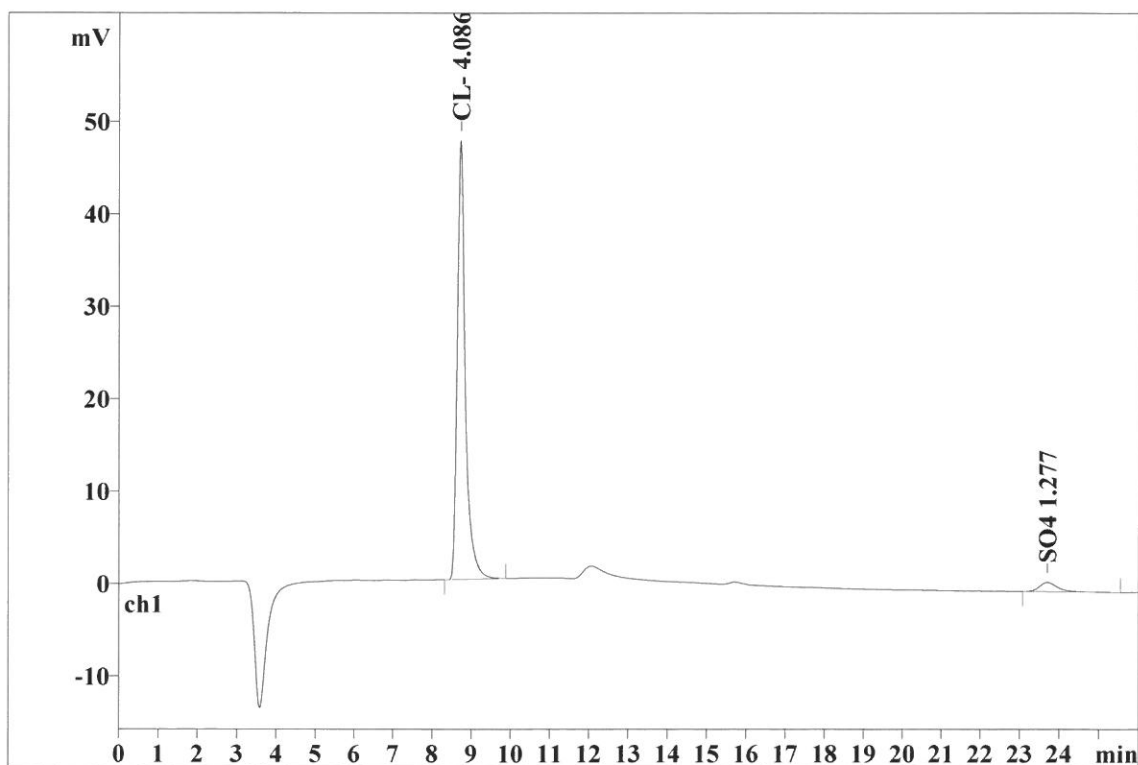

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.69             | 0.198          | 47.51        | 97.92       | 678.411        | 95.52     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 23.70            | 0.462          | 1.01         | 2.07        | 31.791         | 4.48      |
| 7  | 26.00            | 0.094          | 48.52        | 99.99       | 710.202        | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/28/2022 10:04:24 AM  
Printed by: wet


Ident: CCV  
Analysis from: 2/25/2022 5:13:01 PM  
File: \_2022-02-25\_

Last save: 2/25/2022 5:39:01 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30222

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 11  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

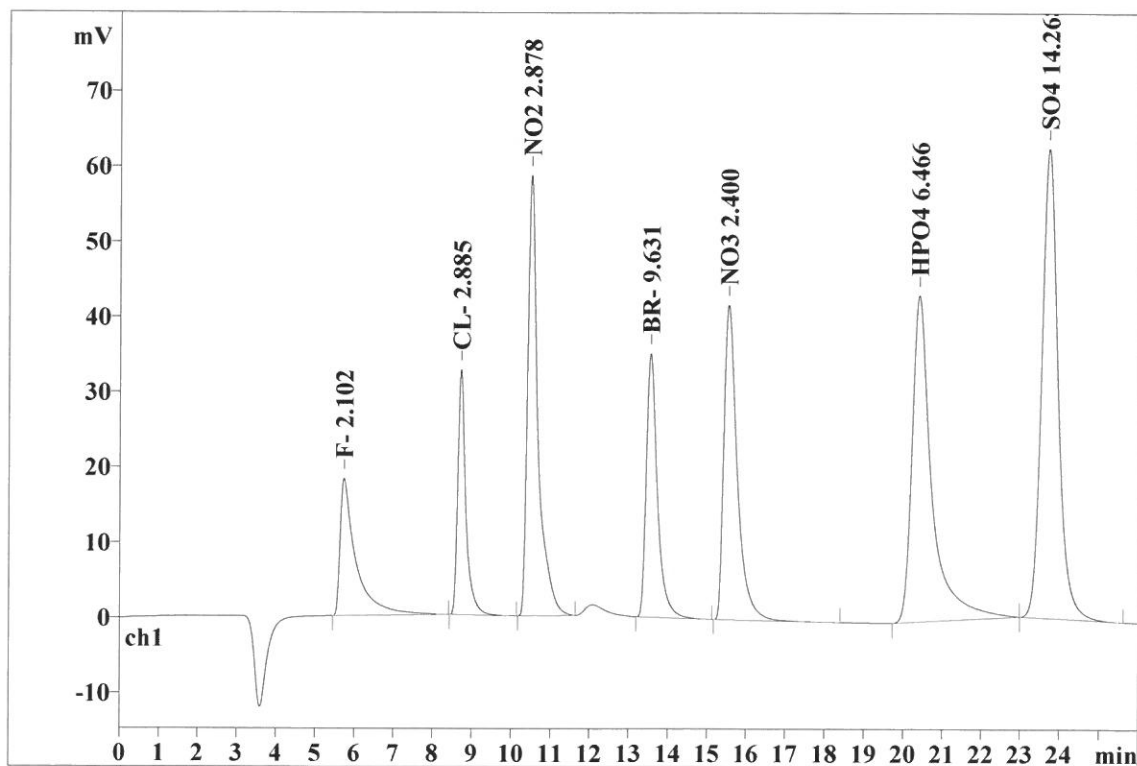

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.73             | 0.342          | 18.24        | 6.24        | 512.645        | 7.24      |
| 2  | 8.71             | 0.200          | 32.59        | 11.15       | 471.460        | 6.66      |
| 3  | 10.49            | 0.243          | 58.57        | 20.04       | 1072.808       | 15.15     |
| 4  | 13.54            | 0.288          | 35.09        | 12.01       | 697.195        | 9.85      |
| 5  | 15.54            | 0.340          | 41.88        | 14.33       | 992.075        | 14.01     |
| 6  | 20.39            | 0.455          | 43.41        | 14.86       | 1528.246       | 21.58     |
| 7  | 23.71            | 0.426          | 62.44        | 21.37       | 1806.453       | 25.51     |
| 7  | 26.00            | 0.328          | 292.22       | 100.00      | 7080.881       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 2/28/2022 10:04:33 AM  
Printed by: wet


Ident: CCB  
Analysis from: 2/25/2022 5:41:39 PM  
File: \_2022-02-25\_

Last save: 2/25/2022 6:07:39 PM

Method: AnionsIC2-022422.mtw  
Run operator: wet  
Analysis number: 30223

Last save: 2/24/2022 12:51

SAMPLE:  
: IZ/AP  
Vial number: 12  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

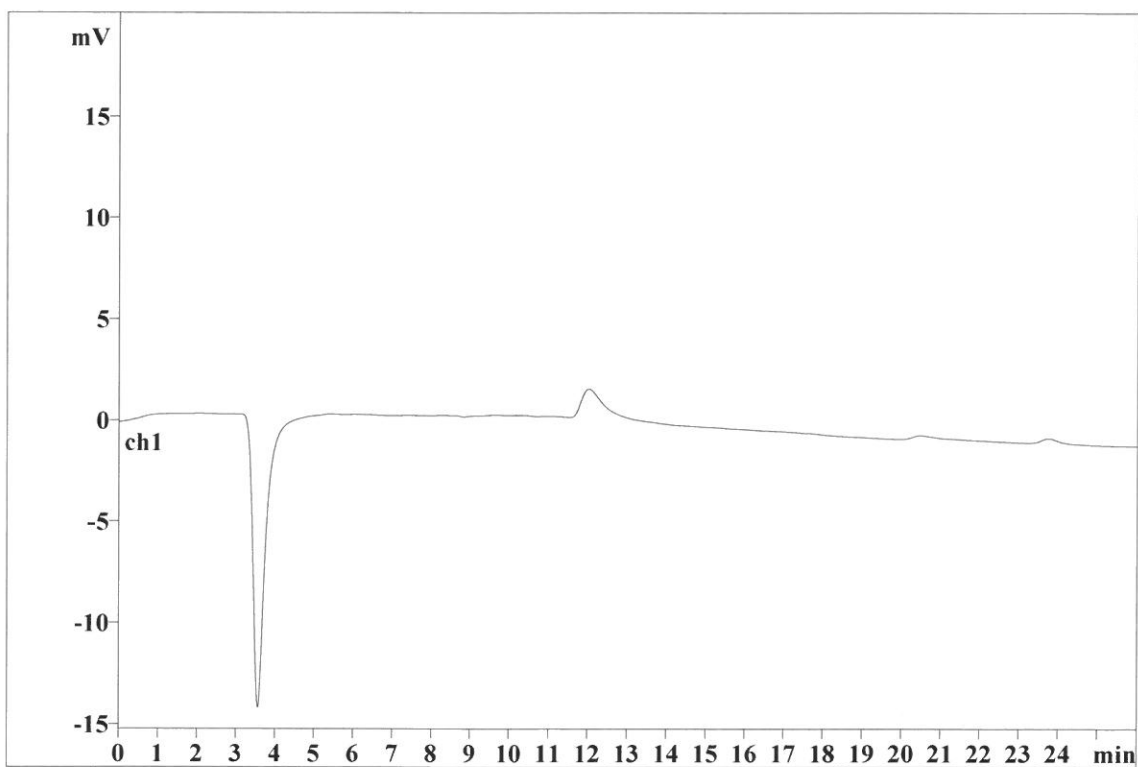

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD