

LB118 934

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

3/1/2022 14:46

Reviewed by : 16 Instrument ID : Konelab

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.984	0.0	0.104	
ICB1	0.001	0.0	0.005	
CCV1	0.987	0.0	0.104	
CCB1	0.003	0.0	0.005	
PB142994BL	0.002	0.0	0.005	
PB142994BS	1.003	0.0	0.106	
N1645-03	0.027	0.0	0.008	
PB142996BL	0.002	0.0	0.005	
PB142996BS	0.985	0.0	0.104	
N1645-09	0.026	0.0	0.008	
CCV2	0.987	0.0	0.104	
CCB2	0.000	0.0	0.005	

N	12
Mean	0.417
SD	0.5050
CV%	121.02

Aquakem v. 7.2AQ1

Results from time period:

Tue Mar 01 13:58:48 2022

Tue Mar 01 14:38:33 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0015	mg/l	3/1/2022 13:58:48	
0.05PPM	A	Phenolics-	P	0.0548	mg/l	3/1/2022 13:58:49	
0.1PPM	A	Phenolics-	P	0.1052	mg/l	3/1/2022 13:58:50	
0.25PPM	A	Phenolics-	P	0.2551	mg/l	3/1/2022 13:58:51	
0.50PPM	A	Phenolics-	P	0.4953	mg/l	3/1/2022 13:58:52	
1.0PPM	A	Phenolics-	P	0.976	mg/l	3/1/2022 13:58:53	
2.0PPM	A	Phenolics-	P	2.0121	mg/l	3/1/2022 13:58:54	
ICV1	S	Phenolics-	P	0.9841	mg/l	3/1/2022 14:28:21	
ICB1	S	Phenolics-	P	0.0007	mg/l	3/1/2022 14:28:22	
CCV1	S	Phenolics-	P	0.9872	mg/l	3/1/2022 14:28:24	
CCB1	S	Phenolics-	P	0.003	mg/l	3/1/2022 14:28:26	
PB142994BL	S	Phenolics-	P	0.0017	mg/l	3/1/2022 14:28:29	
PB142994BS	S	Phenolics-	P	1.0029	mg/l	3/1/2022 14:28:31	
N1645-03	S	Phenolics-	P	0.0271	mg/l	3/1/2022 14:38:22	
PB142996BL	S	Phenolics-	P	0.0021	mg/l	3/1/2022 14:38:24	
PB142996BS	S	Phenolics-	P	0.9852	mg/l	3/1/2022 14:38:27	
N1645-09	S	Phenolics-	P	0.0263	mg/l	3/1/2022 14:38:28	
CCV2	S	Phenolics-	P	0.9872	mg/l	3/1/2022 14:38:31	
CCB2	S	Phenolics-	P	0.0001	mg/l	3/1/2022 14:38:32	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

3/1/2022 14:06


Test Phenolics-

Accepted 3/1/2022 14:01

Factor 9.958
Bias 0.005

Coeff. of det. 0.999739

Errors

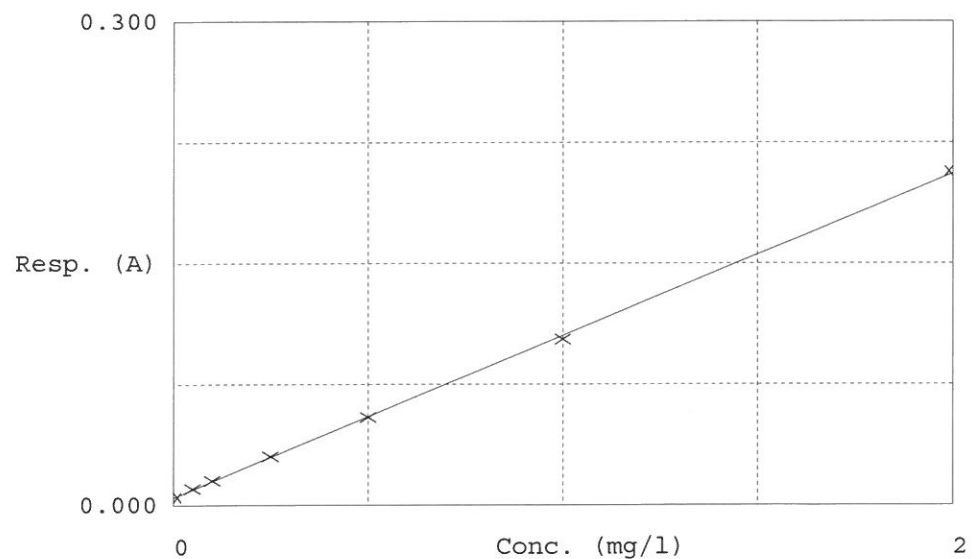

	Calibrator	Response	Calc. con.	Conc.	Re Errors
1	0.00PPM	0.005	0.0015	0.0000	-
2	Phenol-2	0.010	0.0548	0.0500	9.6
3	Phenol-2	0.015	0.1052	0.1000	5.2
4	Phenol-2	0.030	0.2551	0.2500	2.0
5	Phenol-2	0.055	0.4953	0.5000	-0.9
6	Phenol-2	0.103	0.9760	1.0000	-2.4
7	Phenol-2	0.207	2.0121	2.0000	0.6

12 3/1/22