

Clear table

Instrument ID: IC-2										Method:		300.0 / 9056A	
		Analyst :		IZ									
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-02-24_	2/24/22 9:19		IZ/AP		
STD2	0.4460	0.6760	0.6850	2.3070	0.5830	0.9020	3.5940	2022-02-24_	2/24/22 9:47		IZ/AP		
STD3	0.8340	1.2230	1.2150	4.0580	1.0210	2.0340	6.1250	2022-02-24_	2/24/22 10:16		IZ/AP		
STD4	0.9640	1.5070	1.4940	4.9870	1.2470	2.5640	7.4540	2022-02-24_	2/24/22 10:44		IZ/AP		
STD5	1.9190	2.9030	2.9130	9.6630	2.4010	5.0700	14.3340	2022-02-24_	2/24/22 11:13		IZ/AP		
STD6	4.0470	5.8550	5.8620	19.5320	4.8750	9.8620	29.2010	2022-02-24_	2/24/22 11:42		IZ/AP		
STD7	4.9900	7.6360	7.6300	25.4530	6.3720	12.5690	38.2920	2022-02-24_	2/24/22 12:10		IZ/AP		
ICV	2.0180	2.9500	2.9680	9.8510	2.4610	5.1030	14.6150	2022-02-24_	2/24/22 13:22		IZ/AP		
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-02-24_	2/24/22 13:52		IZ/AP		
CCV	1.9270	2.9070	2.9220	9.6260	2.3980	4.7890	14.3470	2022-03-01_	3/1/22 8:58		IZ/AP		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-03-01_	3/1/22 9:29		IZ/AP		
LB118939BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-03-01_	3/1/22 9:58		IZ/AP		
LB118939BSW	1.9500	2.9330	2.9480	9.6790	2.4110	5.1830	14.3980	2022-03-01_	3/1/22 10:26		IZ/AP		
N1710-01	0.0000	341.0840	0.0000	0.0000	1.5320	0.0000	32.9230	2022-03-01_	3/1/22 12:14		IZ/AP		
N1710-02	0.0000	512.8950	0.0000	0.0000	1.7710	0.0000	28.6100	2022-03-01_	3/1/22 12:42		IZ/AP		
N1710-02MS	2.9970	496.7430	2.3090	10.3110	4.2590	11.9900	43.7910	2022-03-01_	3/1/22 13:11		IZ/AP		
N1710-02MSD	2.9120	498.0600	2.2550	10.2360	4.2590	11.9470	43.5170	2022-03-01_	3/1/22 13:40		IZ/AP		
N1710-01DLX100	0.0000	4.1530	0.0000	0.0000	0.0000	0.0000	0.0000	2022-03-01_	3/1/22 14:08		IZ/AP		
N1710-02DLX200	0.0000	3.9180	0.0000	0.0000	0.0000	0.0000	0.0000	2022-03-01_	3/1/22 14:37		IZ/AP		
CCV	2.0920	2.8110	2.8280	9.3140	2.3390	6.0020	13.8510	2022-03-01_	3/1/22 16:55		IZ/AP		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-03-01_	3/1/22 17:23		IZ/AP		

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A


ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-02-24	2/24/22 9:19		IZ/AP
STD2	0.4460	0.6760	0.6850	2.3070	0.5830	0.9020	3.5940	2022-02-24	2/24/22 9:47		IZ/AP
STD3	0.8340	1.2230	1.2150	4.0580	1.0210	2.0340	6.1250	2022-02-24	2/24/22 10:16		IZ/AP
STD4	0.9640	1.5070	1.4940	4.9870	1.2470	2.5640	7.4540	2022-02-24	2/24/22 10:44		IZ/AP
STD5	1.9190	2.9030	2.9130	9.6630	2.4010	5.0700	14.3340	2022-02-24	2/24/22 11:13		IZ/AP
STD6	4.0470	5.8550	5.8620	19.5320	4.8750	9.8620	29.2010	2022-02-24	2/24/22 11:42		IZ/AP
STD7	4.9900	7.6360	7.6300	25.4530	6.3720	12.5690	38.2920	2022-02-24	2/24/22 12:10		IZ/AP

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1	11.5000	12.6667	14.1667	15.3500	16.6000	-9.8000	19.8000
STD2	4.2500	1.9167	1.2500	1.4500	2.1000	1.7000	2.0833
STD3	-3.6000	0.4667	-0.4000	-0.2600	-0.2400	2.5600	-0.6133
STD4	-4.0500	-3.2333	-2.9000	-3.3700	-3.9600	1.4000	-4.4400
STD5	1.1750	-2.4167	-2.3000	-2.3400	-2.5000	-1.3800	-2.6633
STD6	-0.2000	1.8133	1.7333	1.8120	1.9520	0.5520	3.4919
STD7							

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-022422.mtw
 Equation: $Q = 0.0774574 \cdot A + 2.3269$
 RSD: 2.644 %
 Correlation coefficient: 0.999619

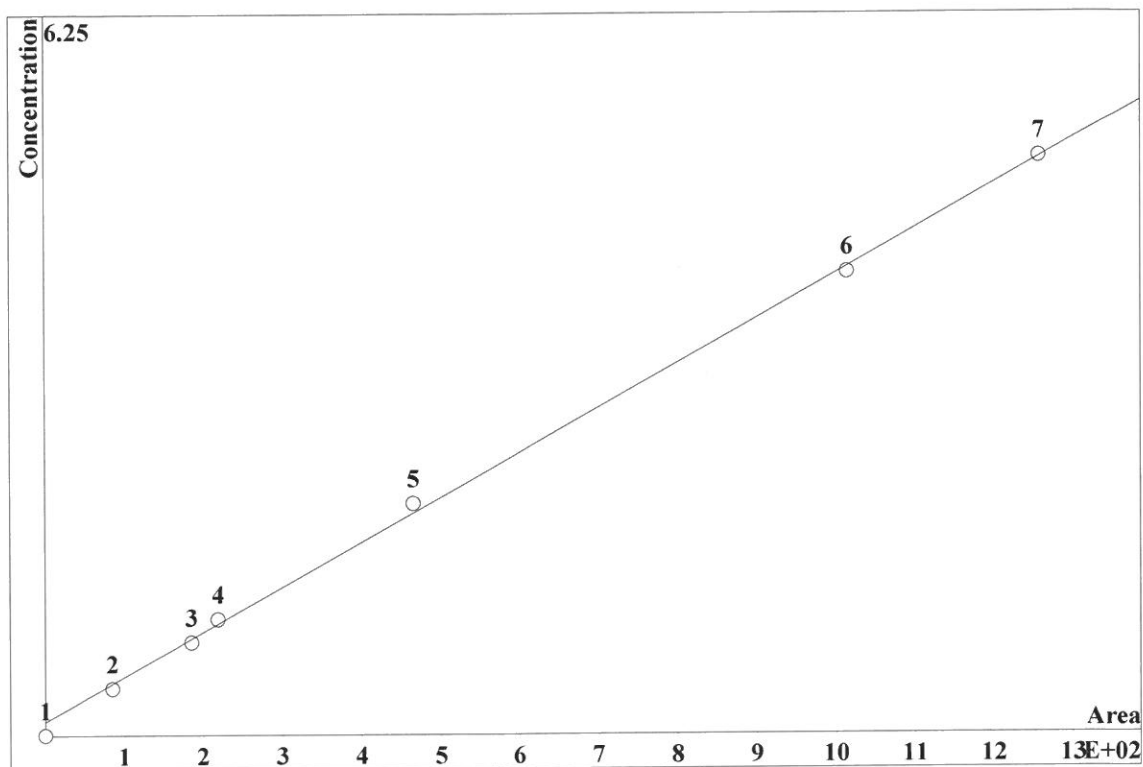


K3 = 0 K2 = 0 K1 = 0.0774574 K0 = 2.3269
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	2.522	85.15	0.4	20	5.653		
3	6.096	185.3	0.8	20	5.653		
4	7.125	218.7	1	20	5.653		
5	16.21	465.4	2	20	5.653		
6	38.5	1015	4	20	5.653		
7	47.61	1258	5	20	5.653		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-022422.mtw
 Equation: $Q = 0.116052 \cdot A + 2.98439$
 RSD: 3.571 %
 Correlation coefficient: 0.999305

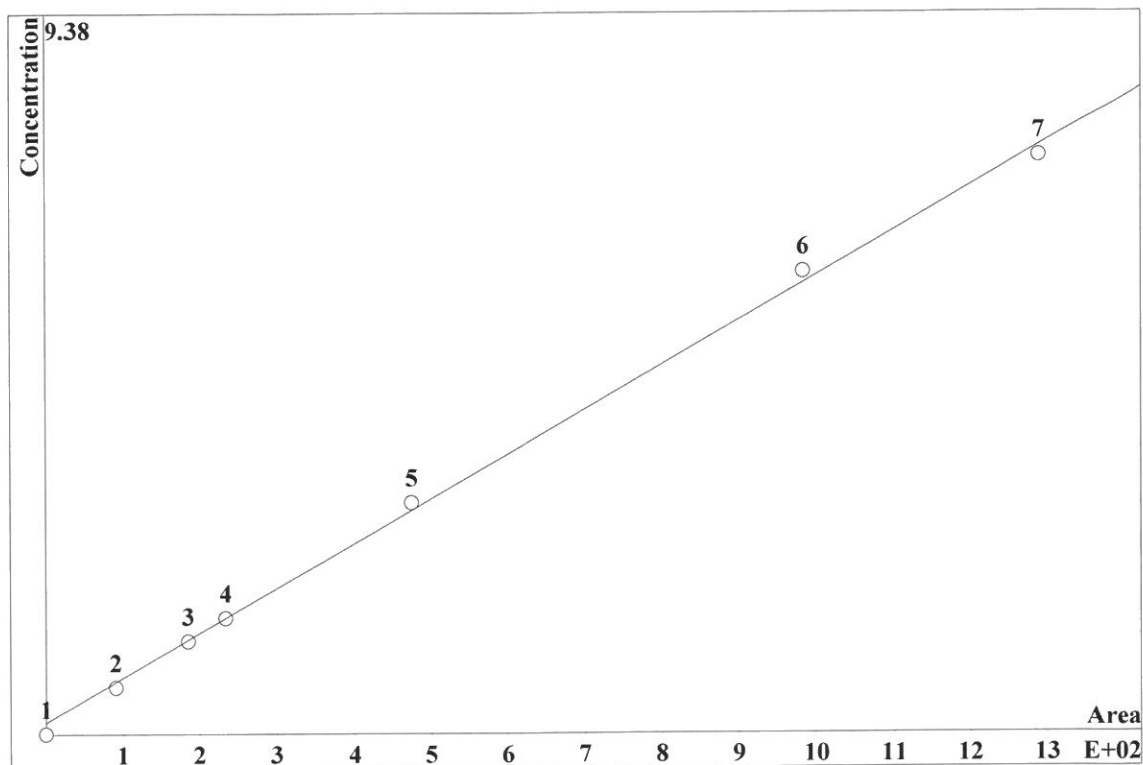


K3 = 0 K2 = 0 K1 = 0.116052 K0 = 2.98439
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.052	90.86	0.6	20	8.643		
3	12.33	185	1.2	20	8.643		
4	15.65	234	1.5	20	8.643		
5	32.32	474.5	3	20	8.643		
6	68.1	983.3	6	20	8.643		
7	91.47	1290	7.5	20	8.643		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-022422.mtw
 Equation: $Q = 0.0506181 \cdot A + 3.25506$
 RSD: 3.420 %
 Correlation coefficient: 0.999362

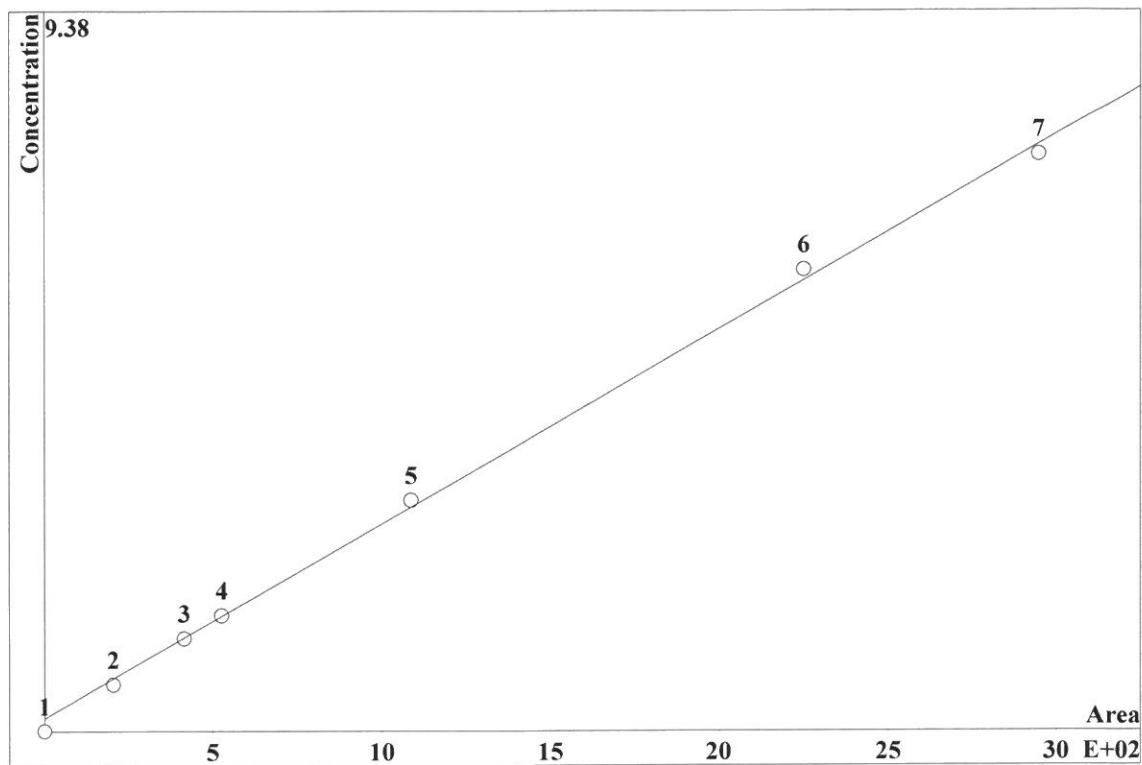


K3 = 0 K2 = 0 K1 = 0.0506181 K0 = 3.25506
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	11.01	206.5	0.6	20	11.04	
3	22.61	415.7	1.2	20	11.04	
4	28.77	526.1	1.5	20	11.04	
5	58	1087	3	20	11.04	
6	119	2252	6	20	11.04	
7	155	2950	7.5	20	10.45	

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-022422.mtw
 Equation: $Q = 0.260136 \cdot A + 11.2471$
 RSD: 3.624 %
 Correlation coefficient: 0.999284

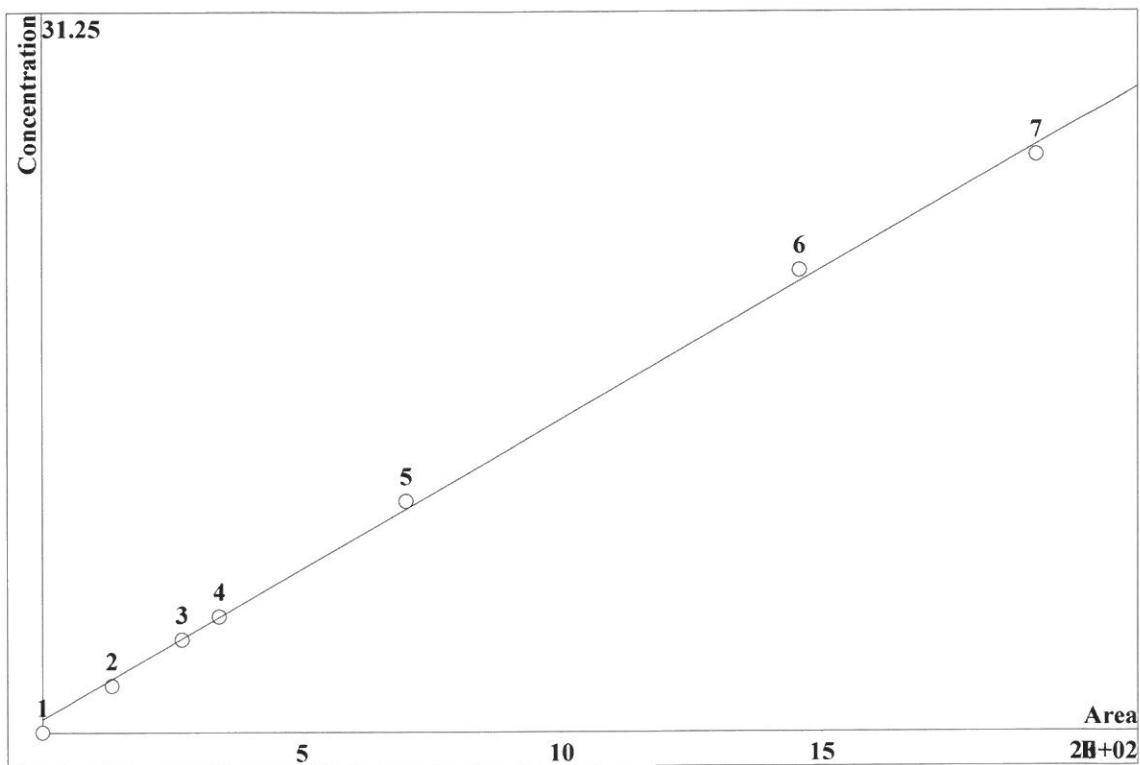


K3 = 0 K2 = 0 K1 = 0.260136 K0 = 11.2471
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.102	134.2	2	20			13.53
3	12.67	268.8	4	20			13.53
4	16.26	340.2	5	20			13.53
5	33.77	699.7	10	20			13.53
6	71.87	1458	20	20			13.53
7	95.82	1914	25	20			13.53

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-022422.mtw
 Equation: $Q = 0.0453553 \cdot A + 3.00908$
 RSD: 3.969 %
 Correlation coefficient: 0.999141

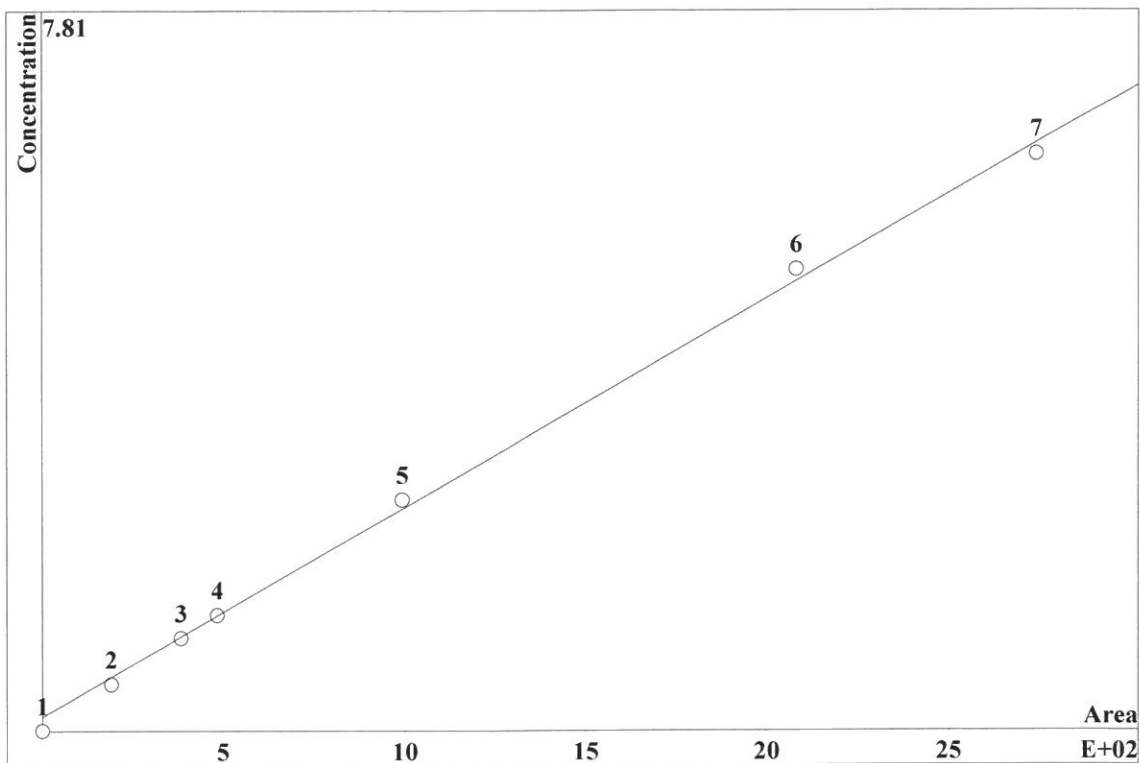


K3 = 0 K2 = 0 K1 = 0.0453553 K0 = 3.00908
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.344	190.7	0.5	20	15.58		
3	15.14	383.8	1	20	15.58		
4	19.39	483.7	1.25	20	15.58		
5	39.92	992.6	2.5	20	15.58		
6	84.9	2083	5	20	15.58		
7	113.9	2744	6.25	20	15.58		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-022422.mtw
 Equation: $Q = 0.0861764 \cdot A - 2.37045$
 RSD: 1.900 %
 Correlation coefficient: 0.999803

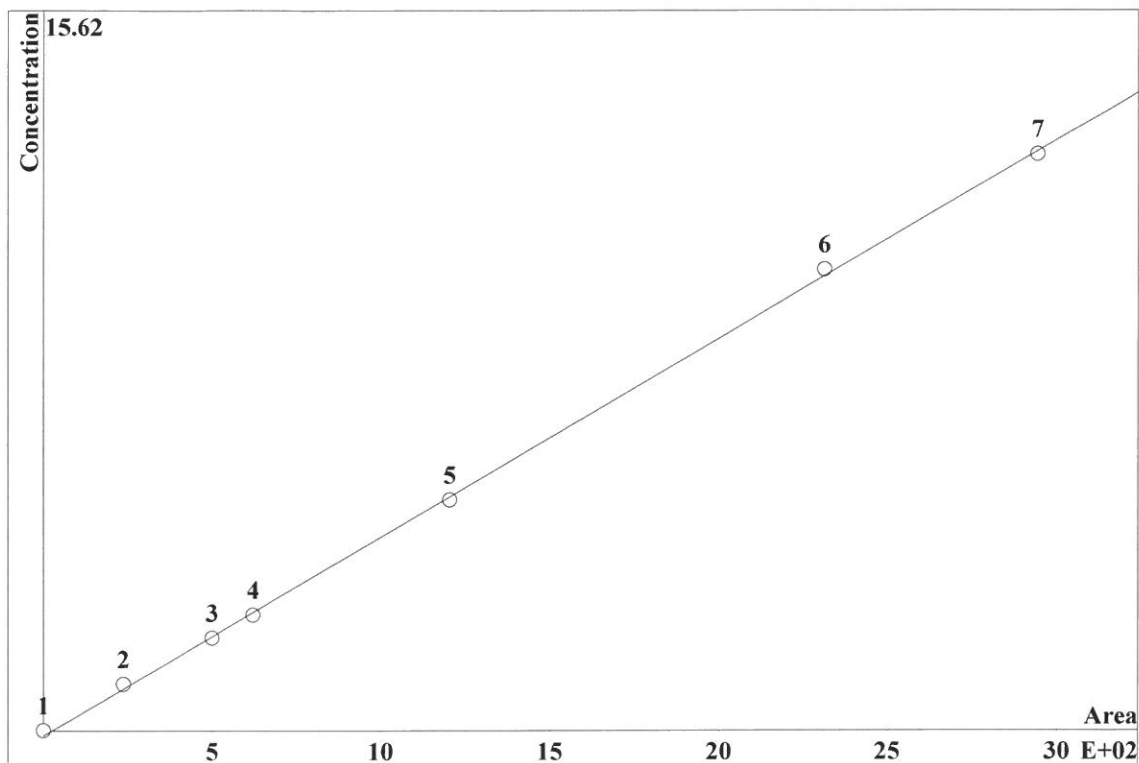


K3 = 0 K2 = 0 K1 = 0.0861764 K0 = -2.37045

Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0		0	0	0		0
2	6.46	236.8		1	20		20.18
3	14.08	499.5		2	20		20.18
4	17.58	622.5		2.5	20		20.18
5	35.64	1204		5	20		20.18
6	72.25	2316		10	20		20.18
7	93.42	2945		12.5	20		20.18

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-022422.mtw
 Equation: $Q = 0.146407 \cdot A + 20.8785$
 RSD: 4.370 %
 Correlation coefficient: 0.998958

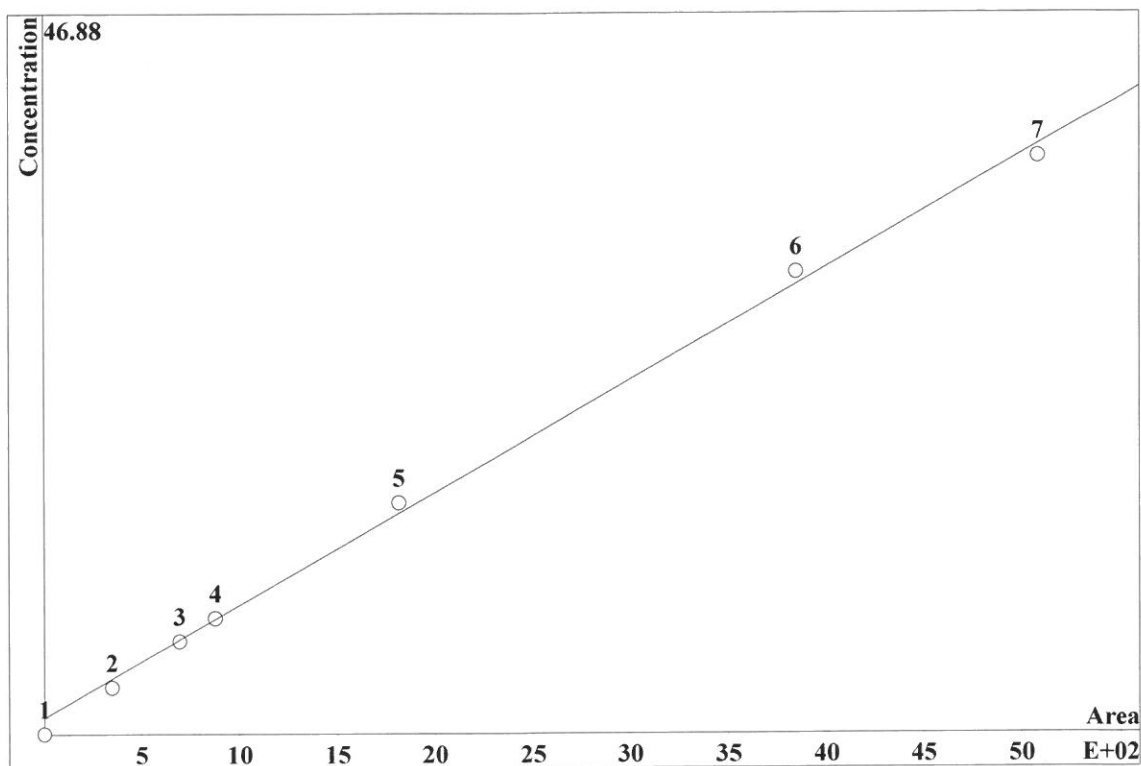

K3 = 0 K2 = 0 K1 = 0.146407 K0 = 20.8785
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	11.49	348.3	3	20	23.09		
3	23.49	694.2	6	20	23.09		
4	29.89	875.7	7.5	20	23.09		
5	62.29	1815	15	20	23.09		
6	135.5	3846	30	20	23.09		
7	180.8	5088	37.5	20	23.09		

Report date: 2/24/2022 12:58:32 PM
Printed by: wet


Ident: STD1
Analysis from: 2/24/2022 9:19:04 AM
File: _2022-02-24_

Last save: 2/24/2022 12:37:49 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30171

Last save: 2/24/2022 12:08

SAMPLE:
: IZ/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

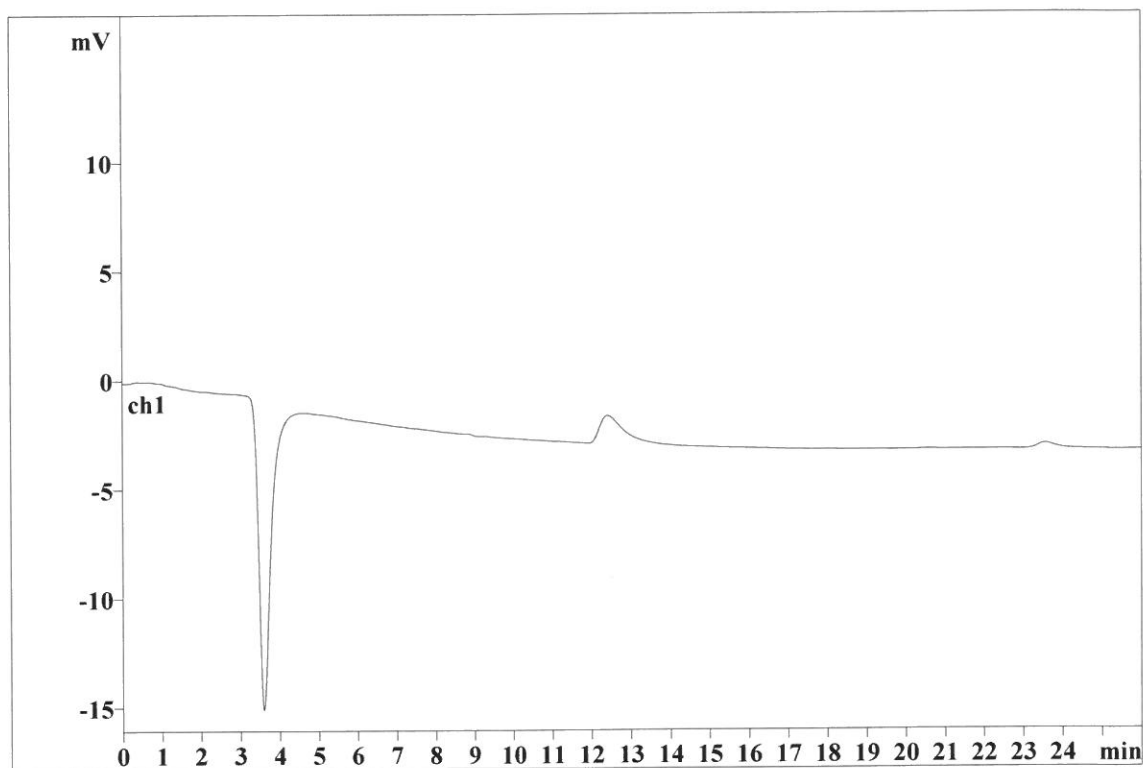

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 2/24/2022 12:58:40 PM
Printed by: wet


Ident: STD2
Analysis from: 2/24/2022 9:47:41 AM
File: _2022-02-24_

Last save: 2/24/2022 12:37:49 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30172

Last save: 2/24/2022 12:08

SAMPLE:
: IZ/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

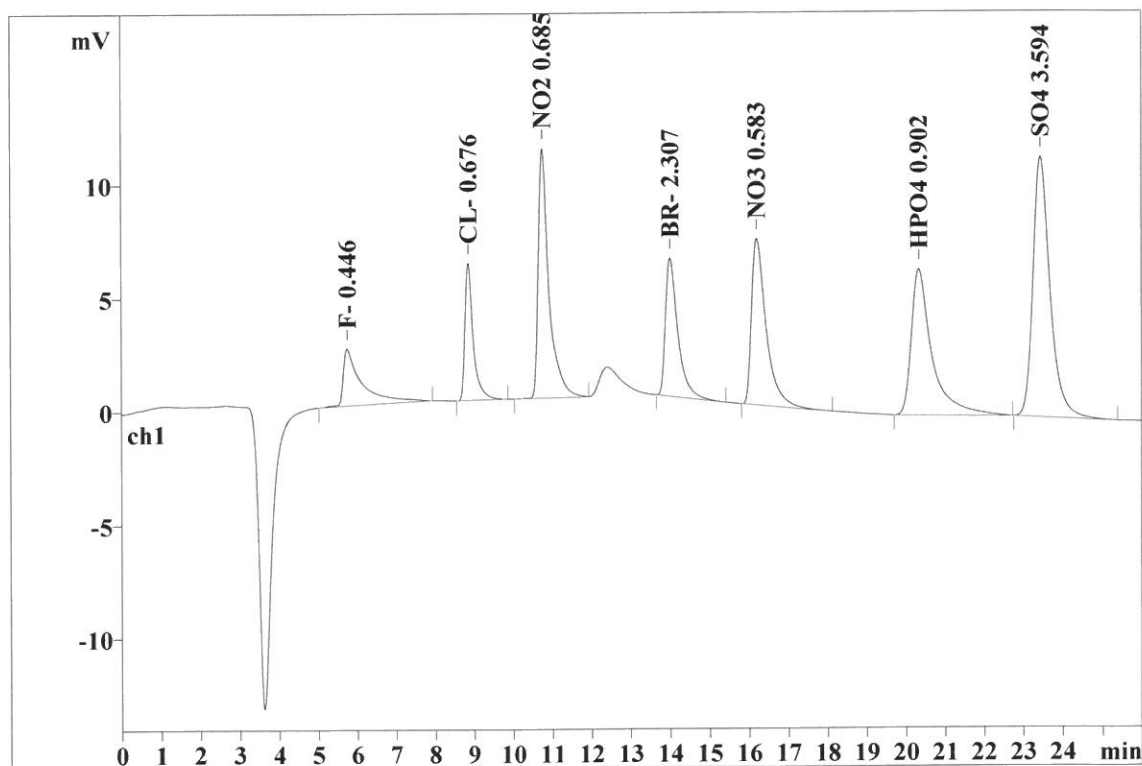

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.74	0.380	2.52	4.94	85.147	6.59
2	8.85	0.207	6.05	11.87	90.857	7.03
3	10.75	0.249	11.01	21.60	206.531	15.98
4	14.02	0.316	6.10	11.97	134.157	10.38
5	16.21	0.371	7.34	14.41	190.700	14.75
6	20.34	0.481	6.46	12.67	236.813	18.32
7	23.46	0.444	11.49	22.53	348.336	26.95
7	26.00	0.350	50.98	99.99	1292.541	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/24/2022 12:58:57 PM
Printed by: wet


Ident: STD3
Analysis from: 2/24/2022 10:16:20 AM
File: _2022-02-24_

Last save: 2/24/2022 12:37:49 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30173

Last save: 2/24/2022 12:08

SAMPLE:
: IZ/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

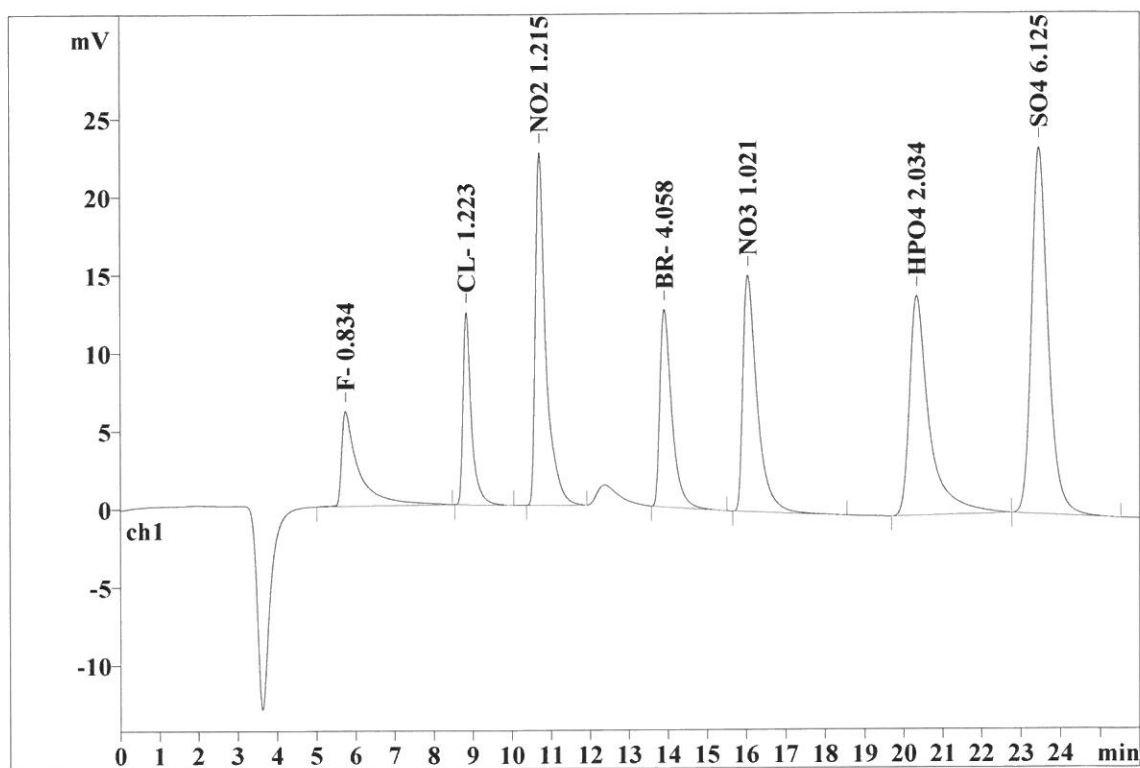

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.74	0.350	6.09	5.73	185.328	7.04
2	8.83	0.207	12.33	11.59	184.998	7.03
3	10.70	0.246	22.61	21.25	415.655	15.79
4	13.92	0.307	12.67	11.90	268.754	10.21
5	16.05	0.363	15.14	14.23	383.843	14.58
6	20.34	0.468	14.08	13.23	499.459	18.97
7	23.47	0.437	23.49	22.07	694.162	26.37
7	26.00	0.340	106.40	99.99	2632.199	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/24/2022 12:59:06 PM
Printed by: wet


Ident: STD4
Analysis from: 2/24/2022 10:44:59 AM
File: _2022-02-24_

Last save: 2/24/2022 12:37:49 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30174

Last save: 2/24/2022 12:08

SAMPLE:
: IZ/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

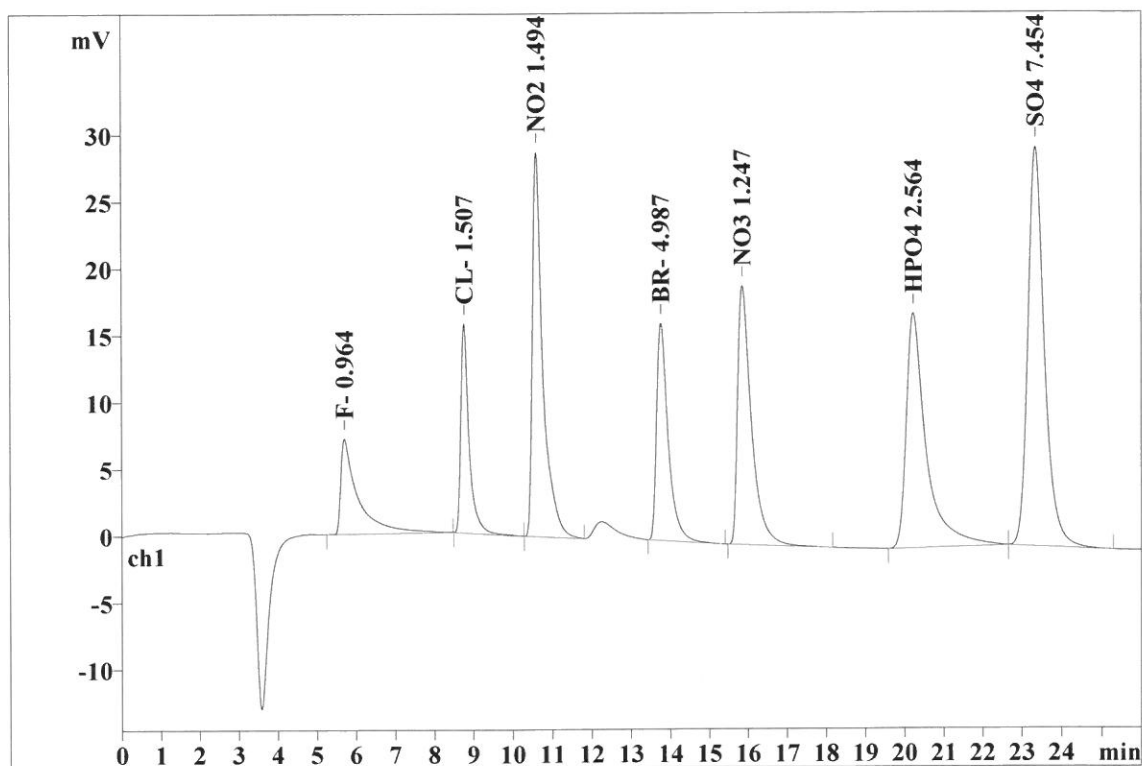

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.71	0.350	7.12	5.29	218.746	6.63
2	8.76	0.205	15.65	11.62	233.967	7.09
3	10.60	0.245	28.77	21.36	526.072	15.94
4	13.77	0.302	16.26	12.08	340.215	10.31
5	15.86	0.357	19.39	14.40	483.720	14.65
6	20.24	0.465	17.58	13.06	622.544	18.86
7	23.35	0.432	29.89	22.19	875.690	26.53
7	26.00	0.337	134.67	100.00	3300.954	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/24/2022 12:59:14 PM
Printed by: wet


Ident: STD5
Analysis from: 2/24/2022 11:13:37 AM
File: _2022-02-24_

Last save: 2/24/2022 12:37:49 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30175

Last save: 2/24/2022 12:08

SAMPLE:
: IZ/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

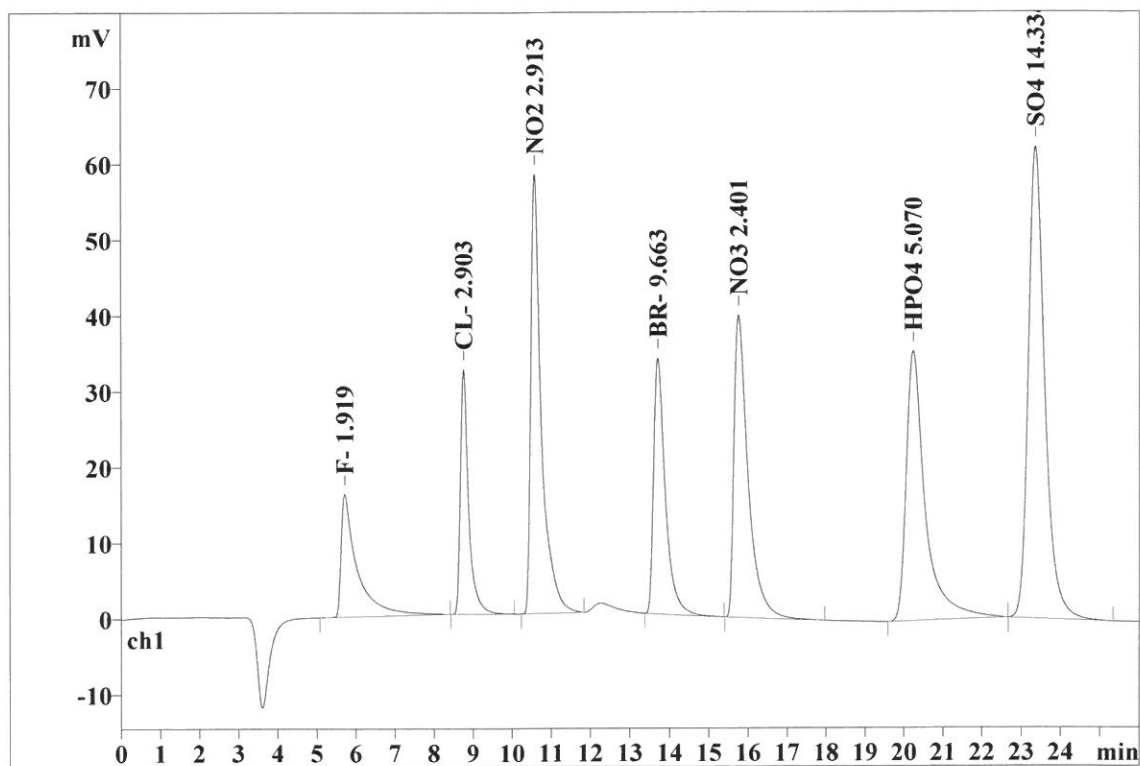

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.71	0.337	16.21	5.83	465.440	6.91
2	8.75	0.200	32.32	11.62	474.516	7.04
3	10.58	0.250	58.00	20.85	1086.780	16.13
4	13.71	0.297	33.77	12.14	699.665	10.38
5	15.77	0.354	39.92	14.35	992.591	14.73
6	20.25	0.448	35.64	12.81	1204.217	17.87
7	23.37	0.427	62.29	22.39	1815.436	26.94
7	26.00	0.330	278.15	100.00	6738.647	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/24/2022 12:59:21 PM
Printed by: wet


Ident: STD6
Analysis from: 2/24/2022 11:42:15 AM
File: _2022-02-24_

Last save: 2/24/2022 12:37:49 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30176

Last save: 2/24/2022 12:08

SAMPLE:
: IZ/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

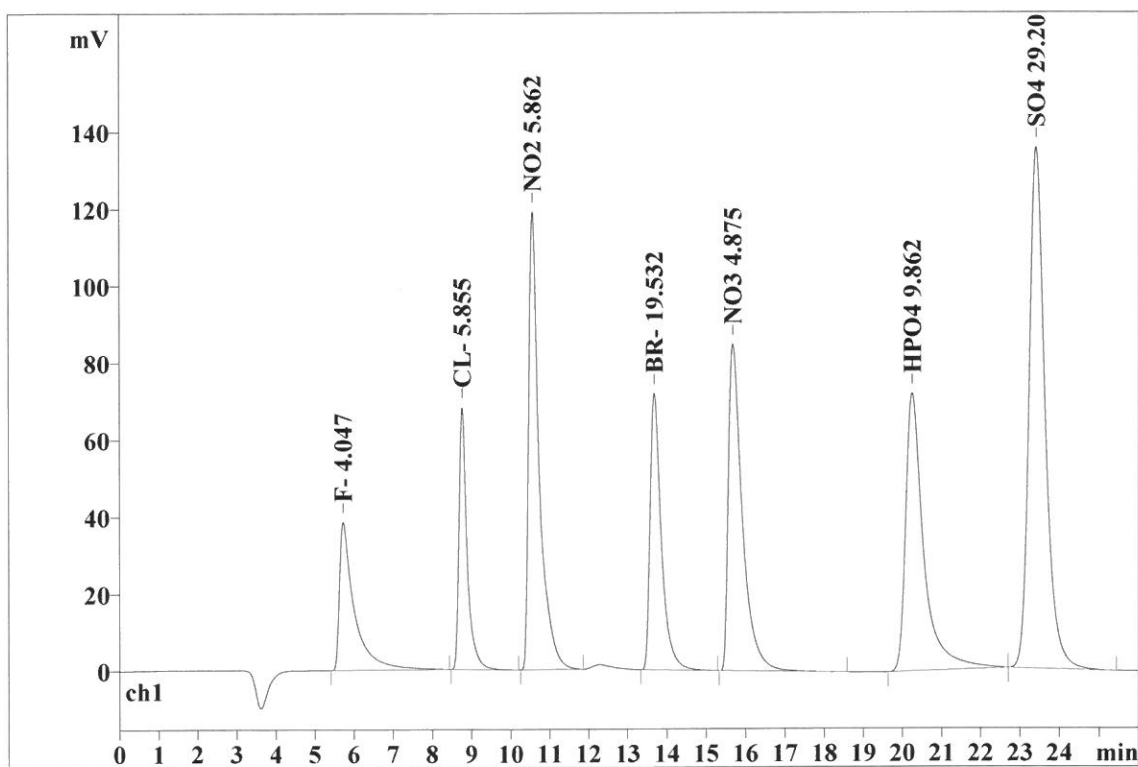

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.73	0.324	38.49	6.52	1015.017	7.27
2	8.75	0.199	68.10	11.54	983.311	7.05
3	10.56	0.255	118.99	20.16	2251.976	16.14
4	13.68	0.293	71.87	12.18	1458.432	10.45
5	15.69	0.350	84.90	14.39	2083.319	14.93
6	20.26	0.431	72.24	12.24	2316.210	16.60
7	23.41	0.419	135.48	22.96	3846.415	27.56
7	26.00	0.324	590.08	100.00	13954.680	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/24/2022 12:59:29 PM
Printed by: wet


Ident: STD7
Analysis from: 2/24/2022 12:10:54 PM
File: _2022-02-24_

Last save: 2/24/2022 12:37:49 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30177

Last save: 2/24/2022 12:08

SAMPLE:
: IZ/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

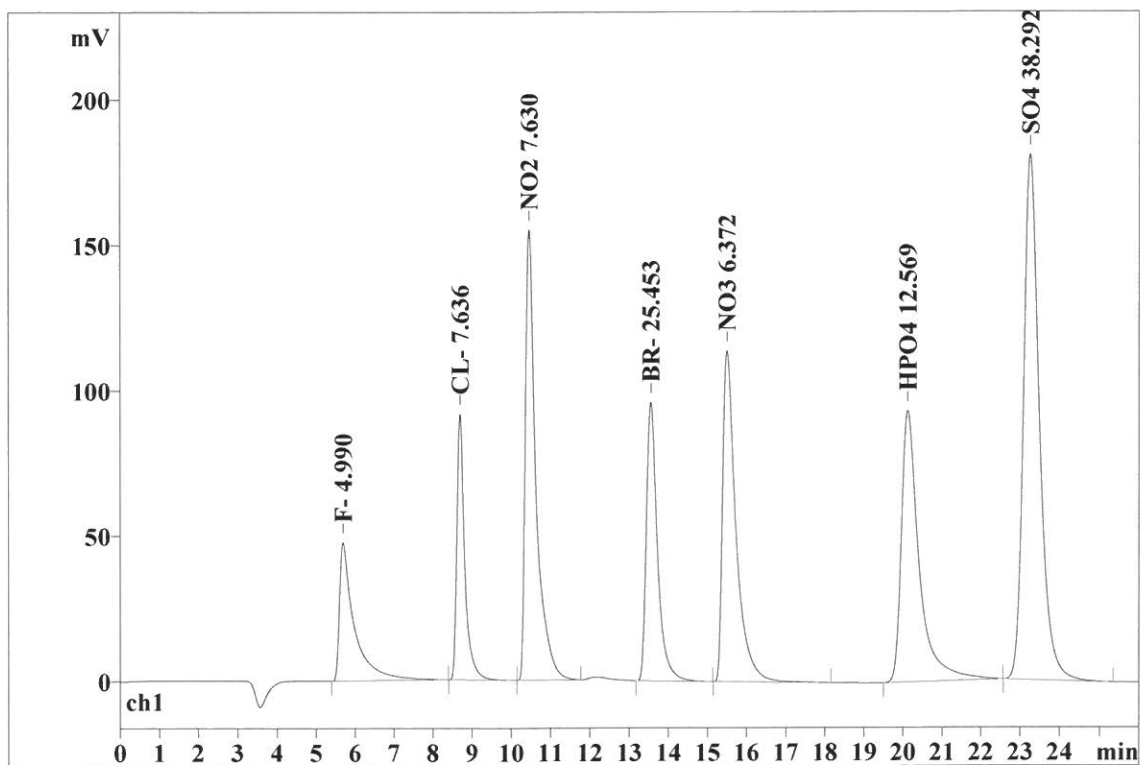

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.69	0.313	47.61	6.12	1258.404	6.92
2	8.68	0.193	91.47	11.76	1290.330	7.09
3	10.45	0.258	154.95	19.92	2950.434	16.22
4	13.54	0.288	95.82	12.32	1913.636	10.52
5	15.50	0.342	113.87	14.64	2743.646	15.08
6	20.13	0.424	93.42	12.01	2944.504	16.19
7	23.27	0.414	180.82	23.24	5088.277	27.97
7	26.00	0.319	777.95	100.00	18189.231	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/24/2022 2:05:54 PM
Printed by: wet


Ident: ICV
Analysis from: 2/24/2022 1:22:55 PM
File: _2022-02-24_

Last save: 2/24/2022 1:48:55 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30179

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

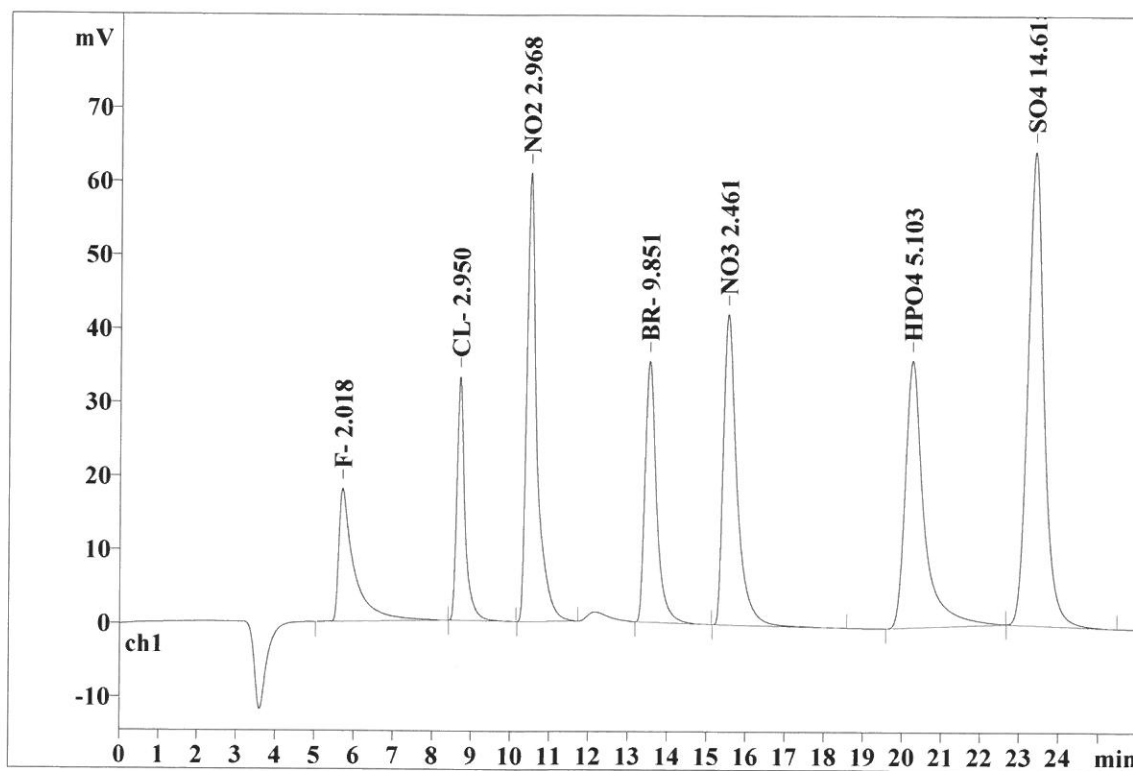

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.70	0.327	18.05	6.22	491.102	7.14
2	8.68	0.200	33.10	11.41	482.727	7.02
3	10.47	0.243	60.87	20.98	1108.208	16.11
4	13.52	0.291	35.44	12.21	714.120	10.38
5	15.52	0.345	42.16	14.53	1018.650	14.80
6	20.23	0.444	36.24	12.49	1211.847	17.61
7	23.36	0.424	64.29	22.16	1853.934	26.94
7	26.00	0.325	290.13	100.00	6880.588	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/24/2022 2:34:43 PM
Printed by: wet


Ident: ICB
Analysis from: 2/24/2022 1:52:06 PM
File: _2022-02-24_

Last save: 2/24/2022 2:18:07 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30180

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

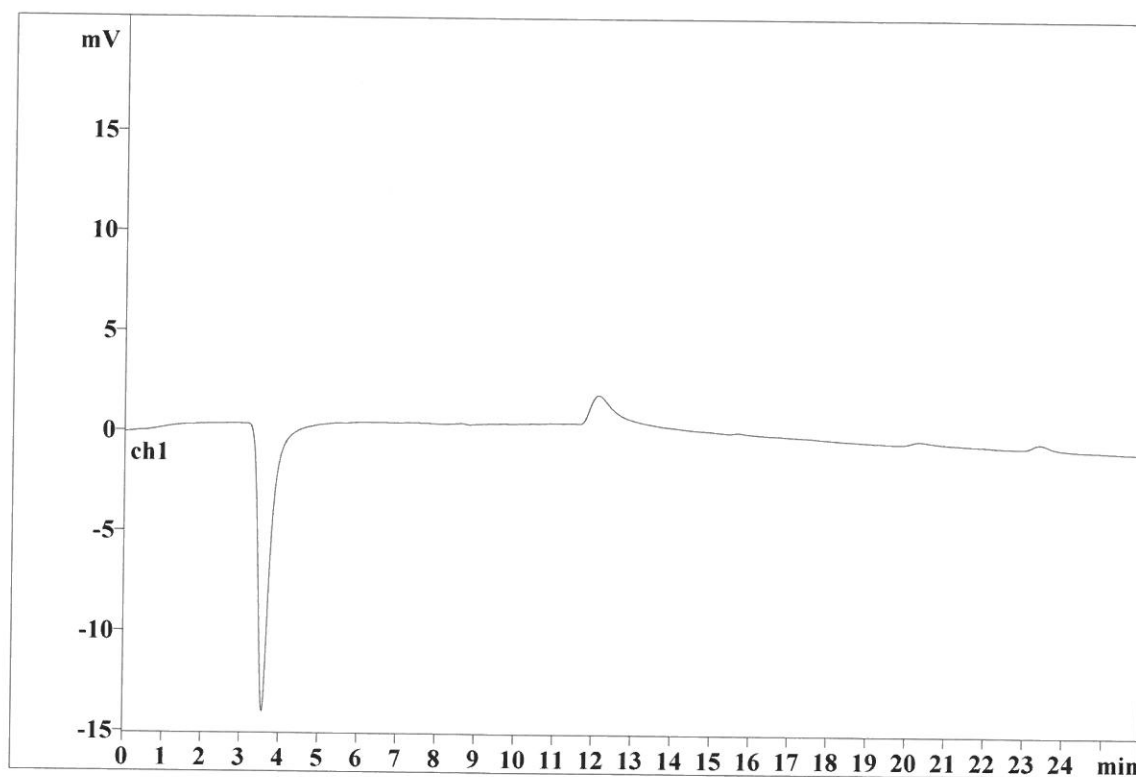

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/2/2022 11:40:54 AM
Printed by: wet


Ident: CCV
Analysis from: 3/1/2022 8:58:00 AM
File: _2022-03-01_

Last save: 3/1/2022 9:24:01 AM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30245

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

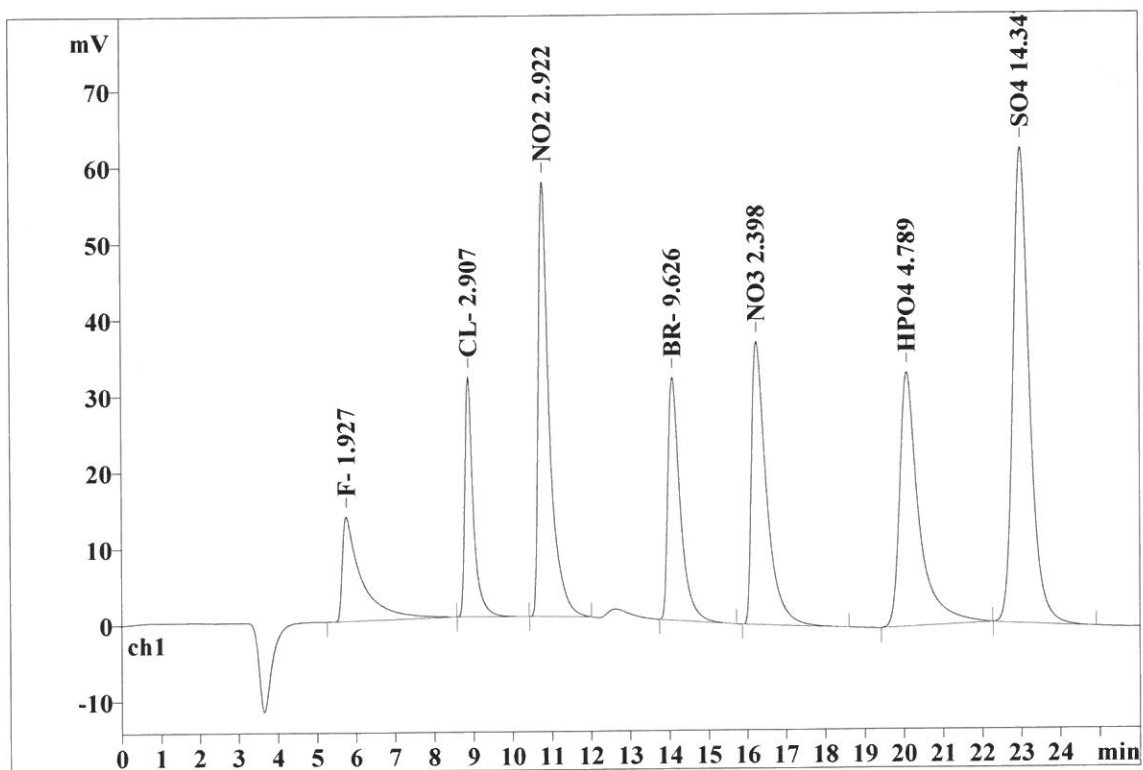

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.76	0.404	13.71	5.14	467.601	7.00
2	8.87	0.208	31.49	11.80	475.348	7.12
3	10.78	0.259	57.01	21.36	1090.133	16.33
4	14.09	0.314	31.87	11.94	696.804	10.44
5	16.25	0.379	37.12	13.91	991.255	14.85
6	20.10	0.457	33.33	12.49	1138.920	17.06
7	23.00	0.427	62.38	23.37	1817.254	27.22
7	26.00	0.350	266.90	100.00	6677.315	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/2/2022 11:41:05 AM
Printed by: wet


Ident: CCB
Analysis from: 3/1/2022 9:29:34 AM
File: _2022-03-01_

Last save: 3/1/2022 9:55:34 AM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30246

Last save: 2/24/2022 12:51

SAMPLE:
:
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

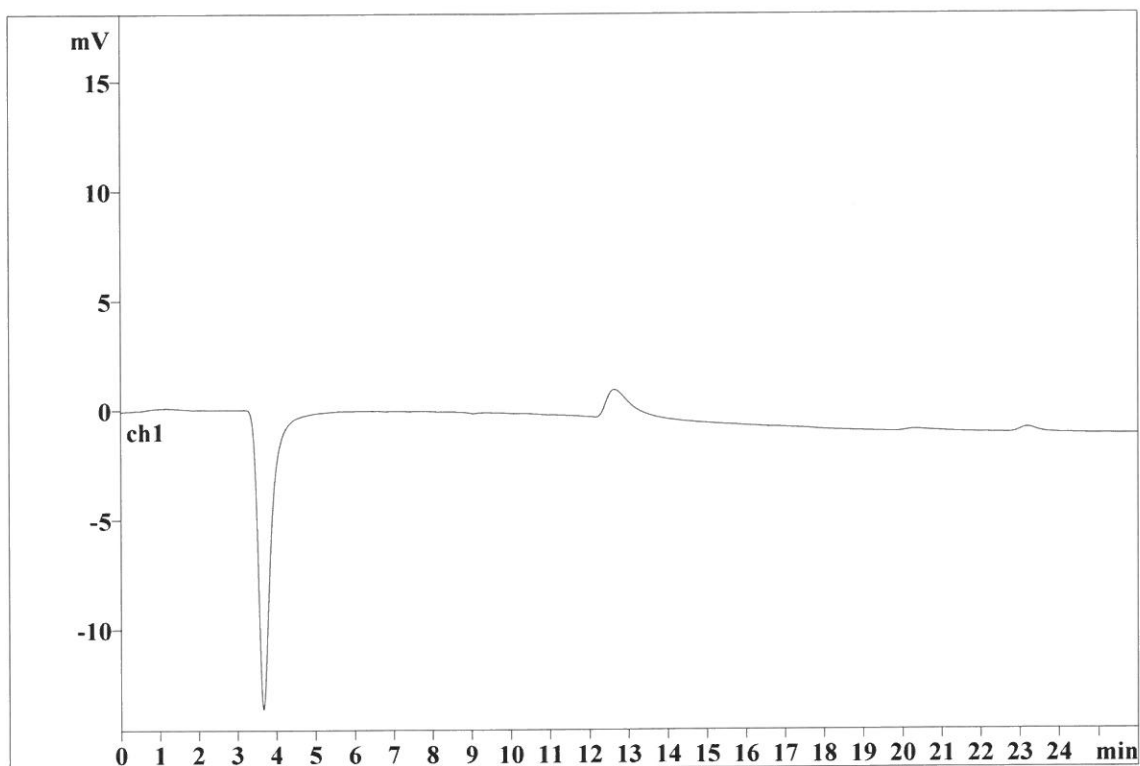

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/2/2022 11:41:14 AM
Printed by: wet


Ident: LB118939BLW
Analysis from: 3/1/2022 9:58:12 AM
File: _2022-03-01_

Last save: 3/2/2022 9:03:40 AM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30247

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

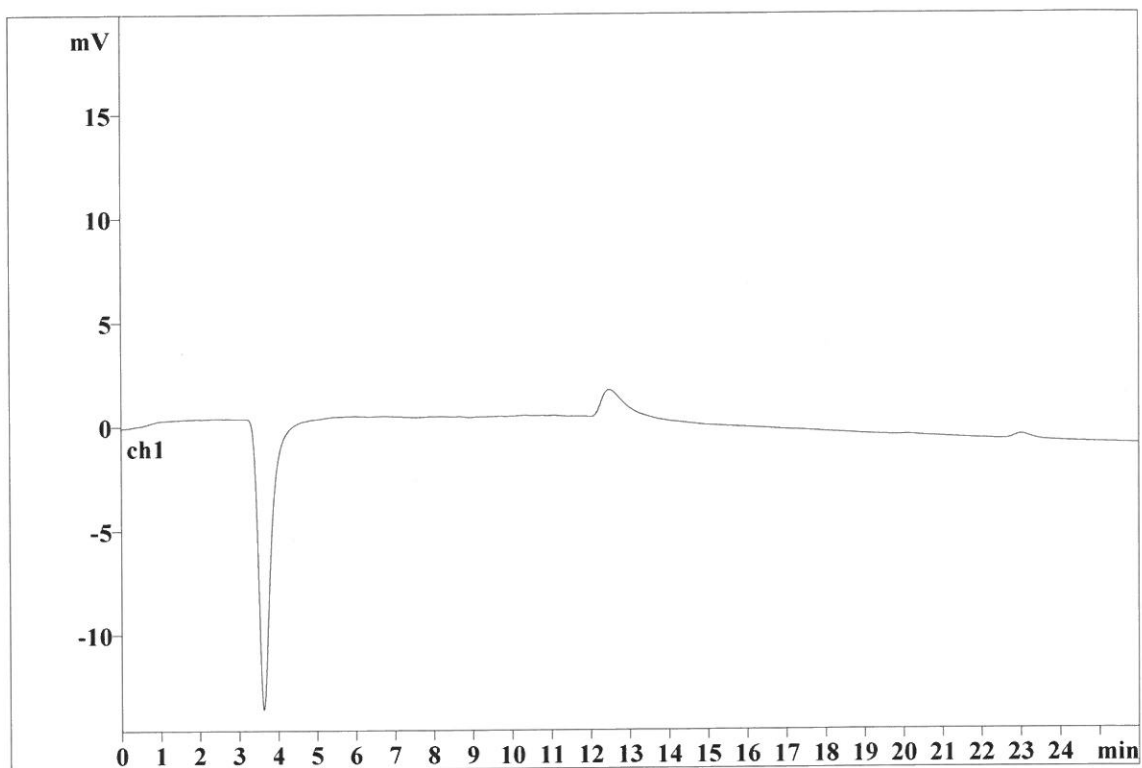

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/2/2022 11:41:25 AM
Printed by: wet


Ident: LB118939BSW
Analysis from: 3/1/2022 10:26:50 AM
File: _2022-03-01_

Last save: 3/2/2022 9:03:41 AM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30248

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

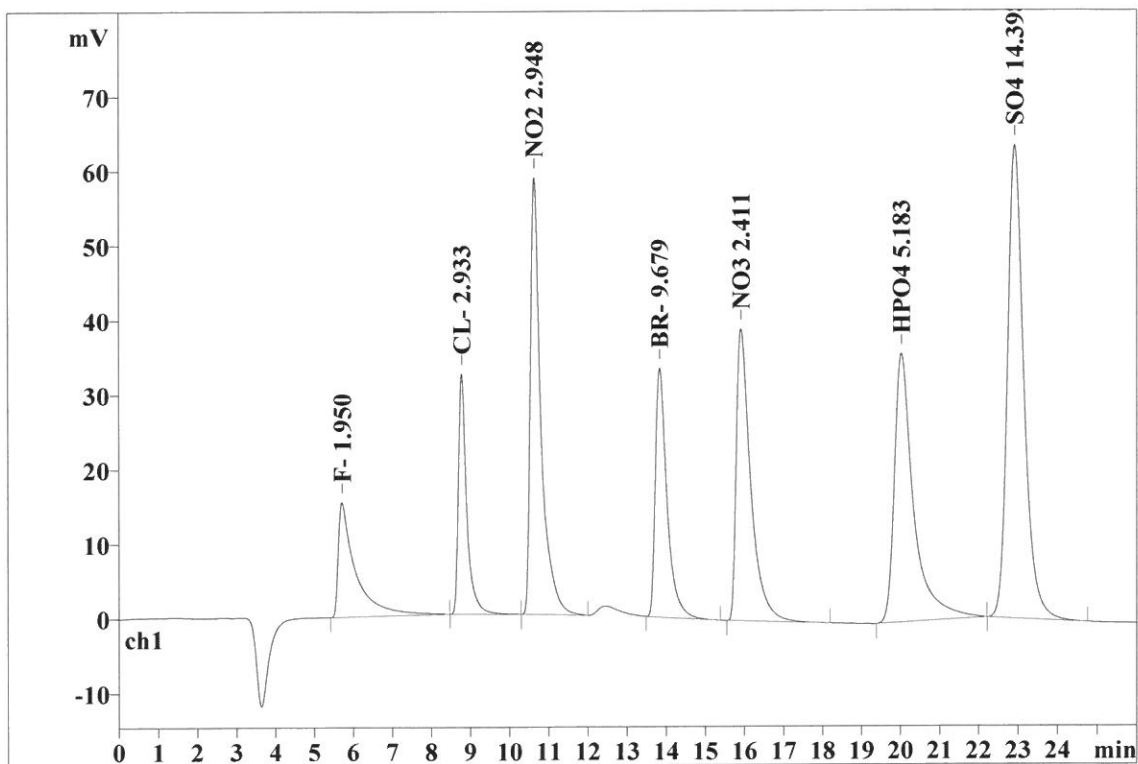

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.363	15.37	5.52	473.537	6.96
2	8.77	0.205	32.21	11.58	479.778	7.05
3	10.64	0.254	58.58	21.06	1100.520	16.17
4	13.84	0.303	33.38	12.00	700.896	10.30
5	15.93	0.364	39.15	14.07	997.025	14.65
6	20.04	0.454	36.03	12.95	1230.377	18.08
7	22.93	0.423	63.48	22.82	1824.286	26.80
7	26.00	0.338	278.20	100.00	6806.418	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/2/2022 11:41:47 AM
Printed by: wet


Ident: N1710-01
Analysis from: 3/1/2022 12:14:12 PM
File: _2022-03-01_

Last save: 3/1/2022 12:51:46 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30251

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

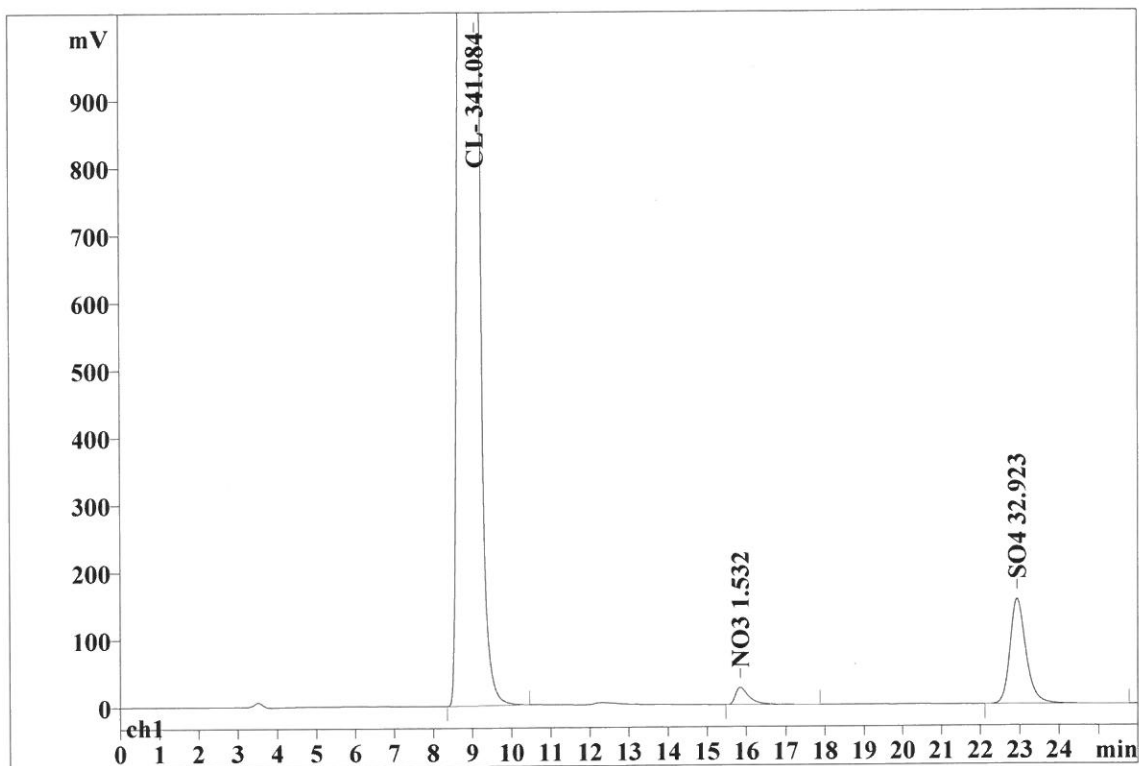

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.08	0.593	1634.77	90.03	58755.734	92.21
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.85	0.348	25.28	1.39	609.070	0.96
6	0.00	0.000	0.00	0.00	0.000	0.00
7	22.94	0.410	155.72	8.58	4354.874	6.83
7	26.00	0.193	1815.77	100.00	63719.678	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/2/2022 11:41:59 AM
Printed by: wet


Ident: N1710-02
Analysis from: 3/1/2022 12:42:50 PM
File: _2022-03-01_

Last save: 3/1/2022 1:11:36 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30252

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 19
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

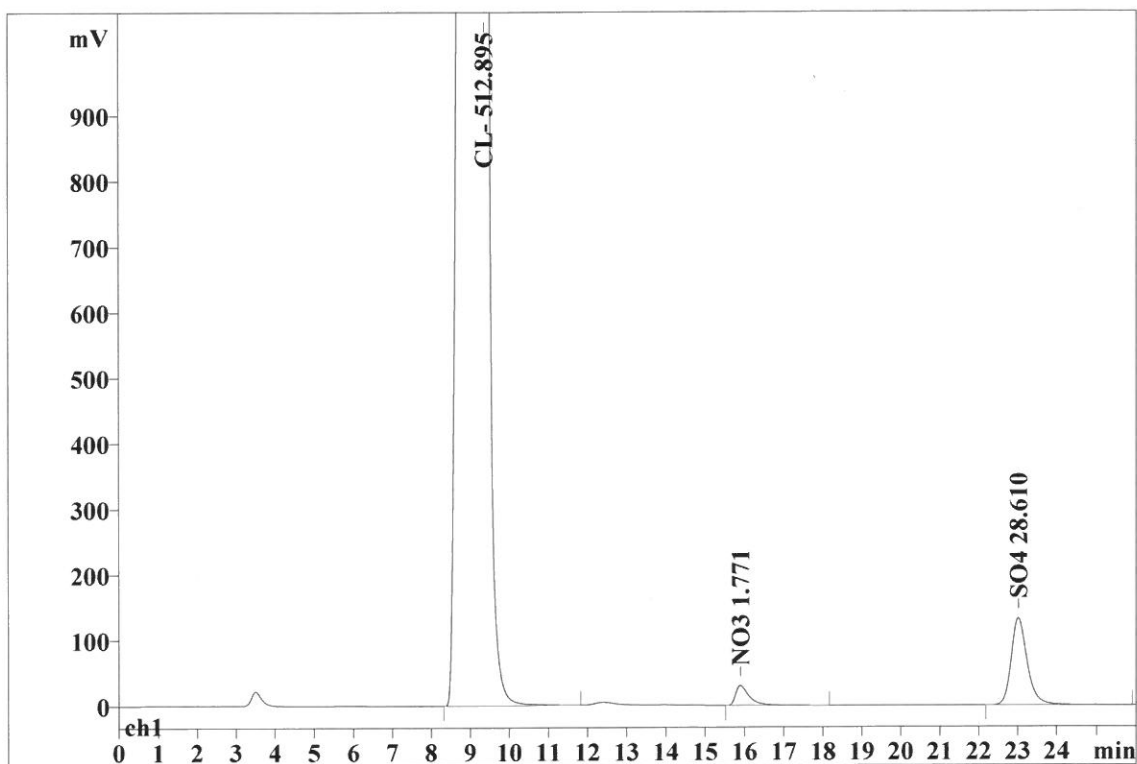

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.33	0.881	1680.77	91.16	88365.168	95.17
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.90	0.341	30.11	1.63	714.669	0.77
6	0.00	0.000	0.00	0.00	0.000	0.00
7	23.02	0.415	132.78	7.20	3765.668	4.06
7	26.00	0.234	1843.66	100.00	92845.506	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/2/2022 11:42:54 AM
Printed by: wet


Ident: N1710-02MS
Analysis from: 3/1/2022 1:11:28 PM
File: _2022-03-01_

Last save: 3/1/2022 1:47:17 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30253

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 20
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

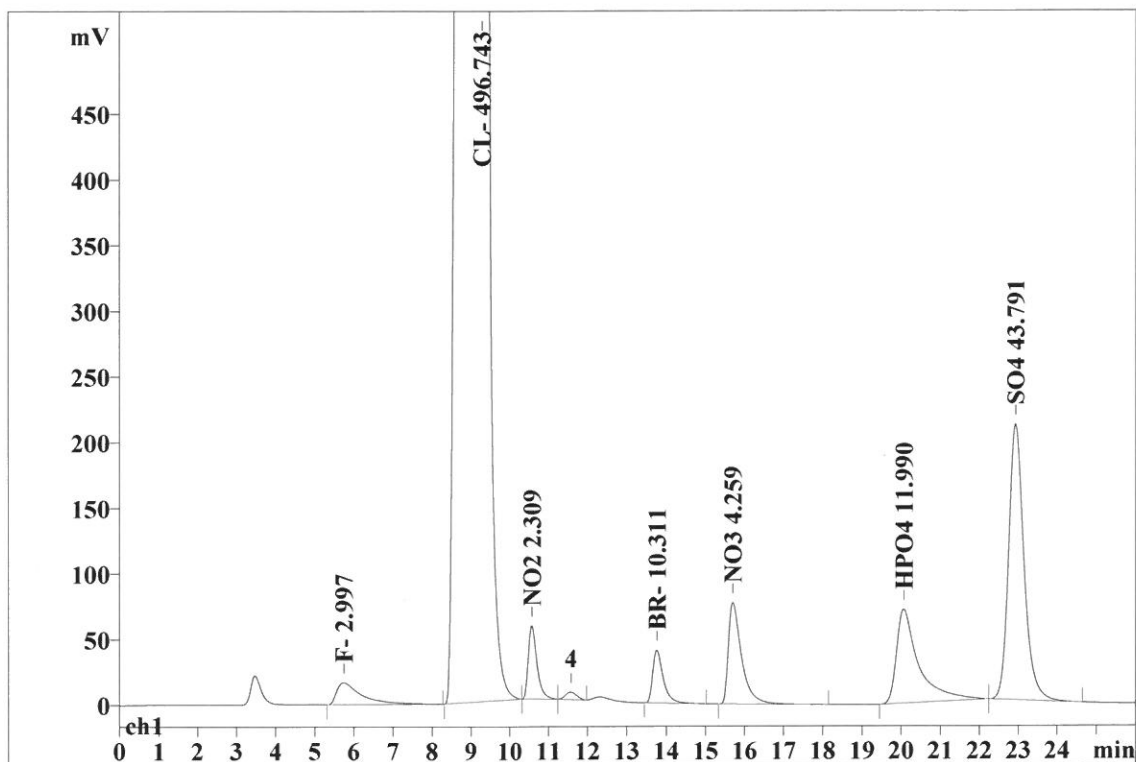

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.74	0.600	16.70	0.78	743.835	0.76
2	9.26	0.856	1676.73	77.84	85581.607	86.89
3	10.57	0.224	55.83	2.59	848.003	0.86
4	13.76	0.271	40.25	1.87	749.509	0.76
5	15.70	0.336	77.16	3.58	1811.841	1.84
6	20.06	0.496	71.71	3.33	2810.151	2.85
7	22.92	0.411	209.92	9.75	5839.541	5.93
7	26.00	0.456	2148.31	99.74	98384.485	99.88

This report has been created by IC Net
METROHM LTD

Report date: 3/2/2022 11:43:15 AM
Printed by: wet


Ident: N1710-02MSD
Analysis from: 3/1/2022 1:40:11 PM
File: _2022-03-01_

Last save: 3/1/2022 2:19:48 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30254

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 21
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

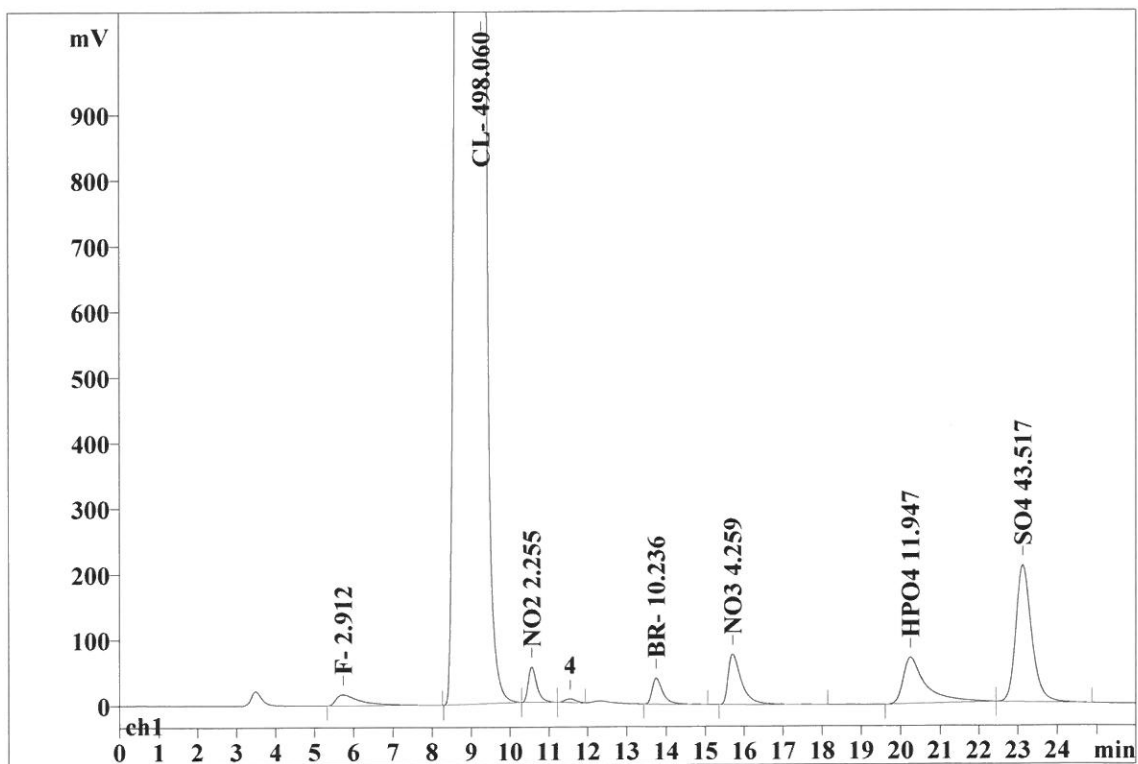

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.73	0.585	16.69	0.78	721.758	0.73
2	9.25	0.859	1677.66	78.06	85808.556	87.00
3	10.56	0.227	54.02	2.51	826.552	0.84
4	13.75	0.275	39.35	1.83	743.735	0.75
5	15.71	0.336	76.69	3.57	1811.545	1.84
6	20.25	0.503	70.62	3.29	2800.269	2.84
7	23.12	0.411	208.65	9.71	5801.999	5.88
7	26.00	0.456	2143.68	99.74	98514.414	99.89

This report has been created by IC Net
METROHM LTD

Report date: 3/2/2022 11:43:26 AM
Printed by: wet


Ident: N1710-01DLX100
Analysis from: 3/1/2022 2:08:50 PM
File: _2022-03-01_

Last save: 3/1/2022 3:12:20 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30255

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 22
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

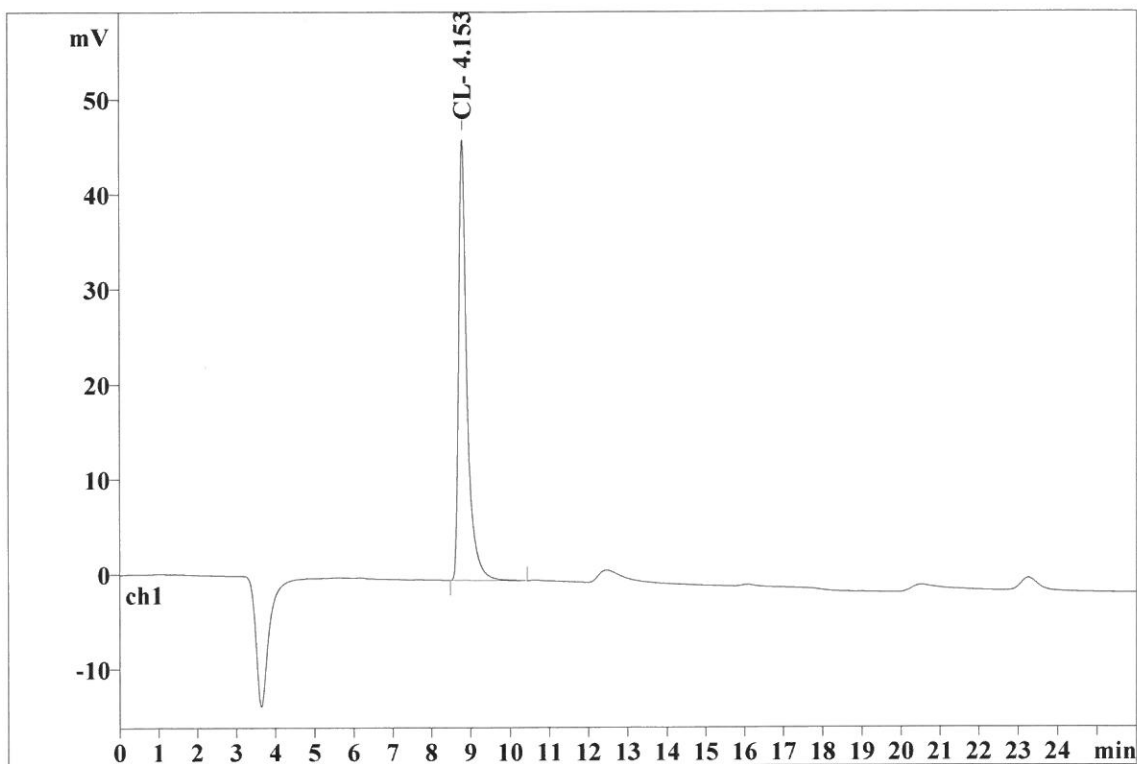

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.78	0.204	46.45	100.01	690.070	100.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	26.00	0.029	46.45	100.01	690.070	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/2/2022 11:43:35 AM
Printed by: wet


Ident: N1710-02DLX200
Analysis from: 3/1/2022 2:37:28 PM
File: _2022-03-01_

Last save: 3/1/2022 3:11:40 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30256

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 23
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

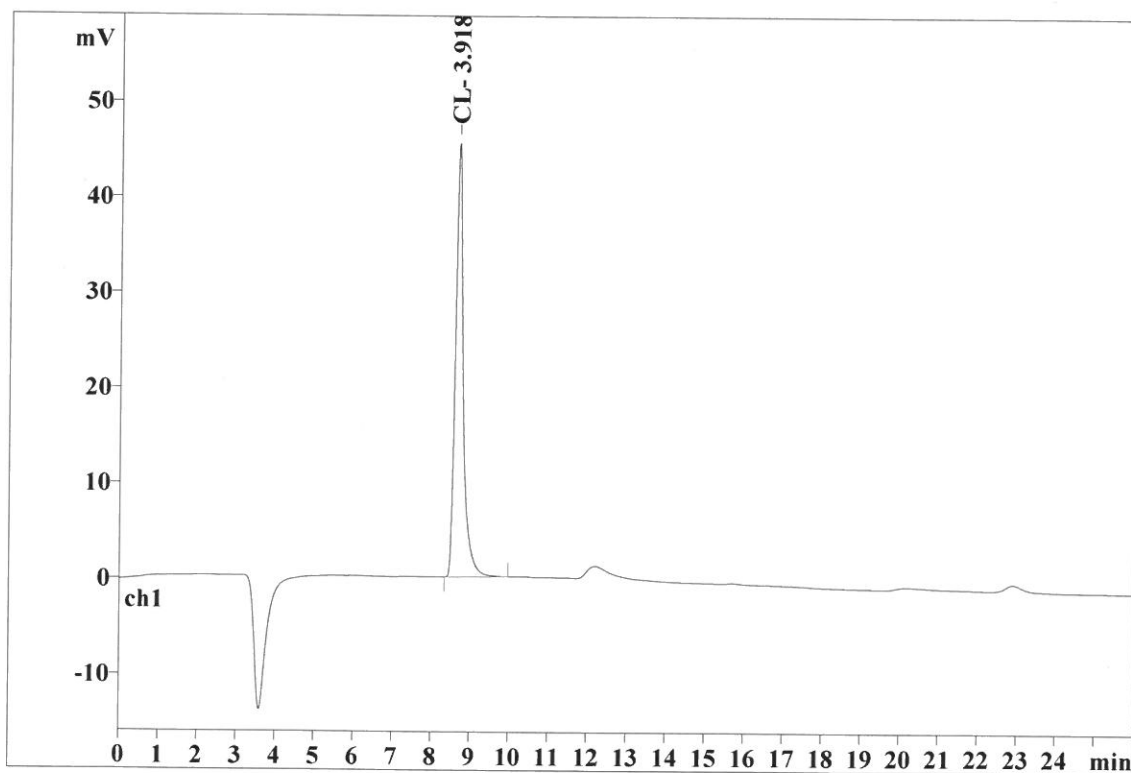

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.64	0.198	45.41	100.00	649.492	100.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	26.00	0.028	45.41	100.00	649.492	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/2/2022 11:43:47 AM
Printed by: wet


Ident: CCV
Analysis from: 3/1/2022 4:55:16 PM
File: _2022-03-01_

Last save: 3/1/2022 5:21:16 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30260

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

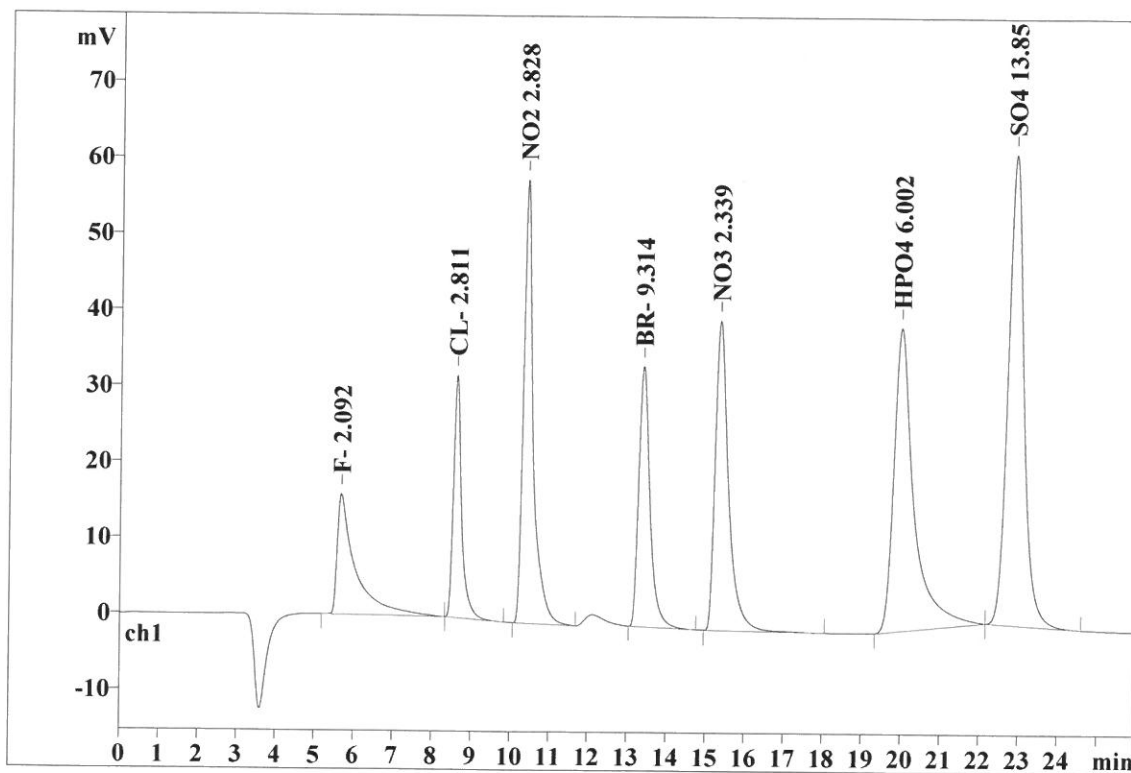

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.66	0.370	15.82	5.59	510.012	7.47
2	8.60	0.199	31.91	11.28	458.720	6.72
3	10.37	0.243	58.35	20.62	1053.156	15.42
4	13.38	0.285	34.29	12.12	672.822	9.85
5	15.33	0.339	40.73	14.40	965.008	14.13
6	19.97	0.465	39.88	14.09	1420.543	20.80
7	22.85	0.417	61.96	21.90	1749.480	25.62
7	26.00	0.331	282.95	100.00	6829.741	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/2/2022 11:43:57 AM
Printed by: wet


Ident: CCB
Analysis from: 3/1/2022 5:23:55 PM
File: _2022-03-01_

Last save: 3/1/2022 5:49:55 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30261

Last save: 2/24/2022 12:51

SAMPLE:
:
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

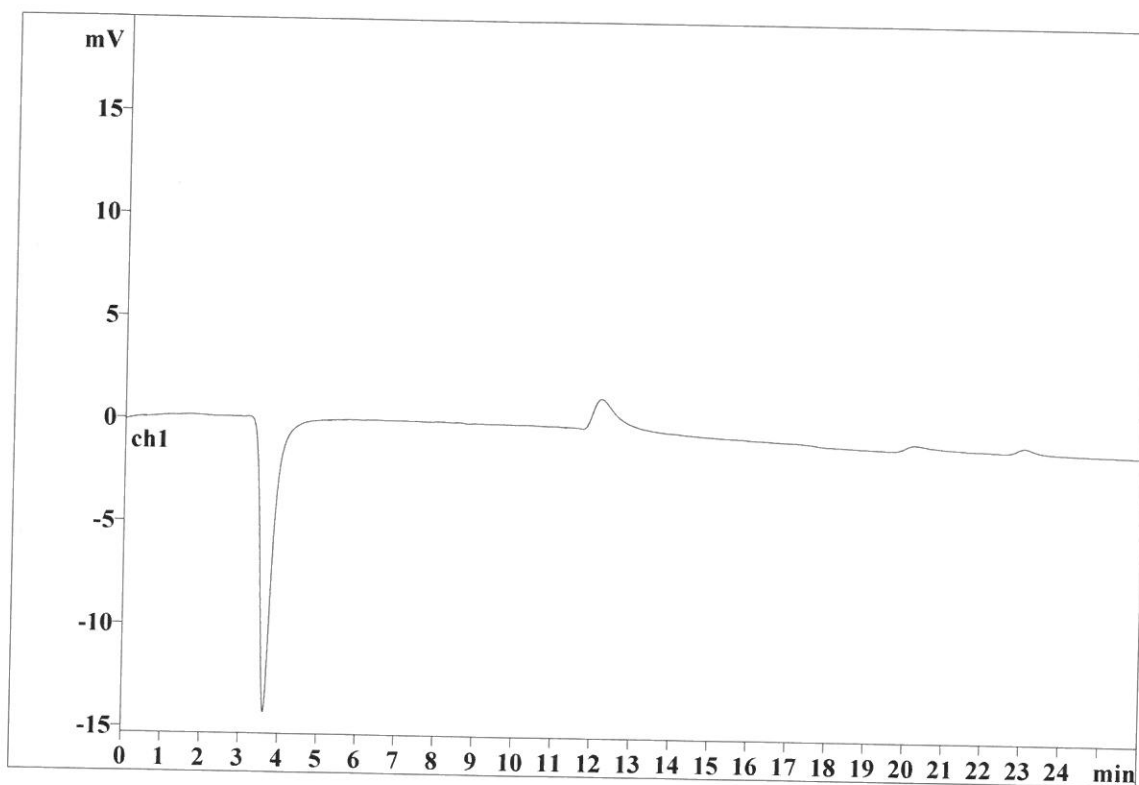

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD