

LB118945

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

3/2/2022 13:26

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.999	0.0	0.080	
ICB1	0.204	0.0	0.001	
CCV1	243.021	0.0	0.206	
CCB1	0.144	0.0	0.001	
PB143013BL	0.064	0.0	0.001	
N1703-01	-0.024	0.0	0.001	
N1703-01DUP	0.022	0.0	0.001	
N1713-01	0.234	0.0	0.001	
N1713-04	0.079	0.0	0.001	
N1717-02	-0.052	0.0	0.001	
12 CCV12	253.860	0.0	0.215	
3/4/22 CCB12	0.056	0.0	0.001	

N	12
Mean	49.301
SD	96.8474
CV%	196.44

Aquakem v. 7.2AQ1

Results from time period:

Wed Mar 02 13:16:00 2022

Wed Mar 02 13:21:49 2022

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.099	µg/l	3/2/2022 10:49:27	
5.OPPBCN	A	Total CN	P	4.4533	µg/l	3/2/2022 10:49:28	
10PPBCN	A	Total CN	P	9.6235	µg/l	3/2/2022 10:49:29	
50PPBCN	A	Total CN	P	48.7535	µg/l	3/2/2022 10:49:30	
100PPBCN	A	Total CN	P	99.3055	µg/l	3/2/2022 10:49:31	
250PPBCN	A	Total CN	P	254.9773	µg/l	3/2/2022 10:49:32	
500PPBCN	A	Total CN	P	497.7879	µg/l	3/2/2022 10:49:33	
ICV1	S	Total CN	P	93.9993	µg/l	3/2/2022 13:16:00	
ICB1	S	Total CN	P	0.2044	µg/l	3/2/2022 13:16:01	
CCV1	S	Total CN	P	243.0207	µg/l	3/2/2022 13:16:02	
CCB1	S	Total CN	P	0.1437	µg/l	3/2/2022 13:16:03	
PB143013BL	S	Total CN	P	0.0636	µg/l	3/2/2022 13:16:04	
N1703-01	S	Total CN	P	-0.0243	µg/l	3/2/2022 13:16:05	
N1703-01DUP	S	Total CN	P	0.0222	µg/l	3/2/2022 13:16:06	
N1713-01	S	Total CN	P	0.2342	µg/l	3/2/2022 13:16:07	
N1713-04	S	Total CN	P	0.0794	µg/l	3/2/2022 13:16:08	
N1717-02	S	Total CN	P	-0.052	µg/l	3/2/2022 13:16:09	
CCV2	S	Total CN	P	253.8604	µg/l	3/2/2022 13:21:45	
CCB2	S	Total CN	P	0.0557	µg/l	3/2/2022 13:21:46	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

3/2/2022 10:50


Test Total CN

Accepted 3/2/2022 10:50

Factor 1184
Bias 0.001

Coeff. of det. 0.999844

Errors

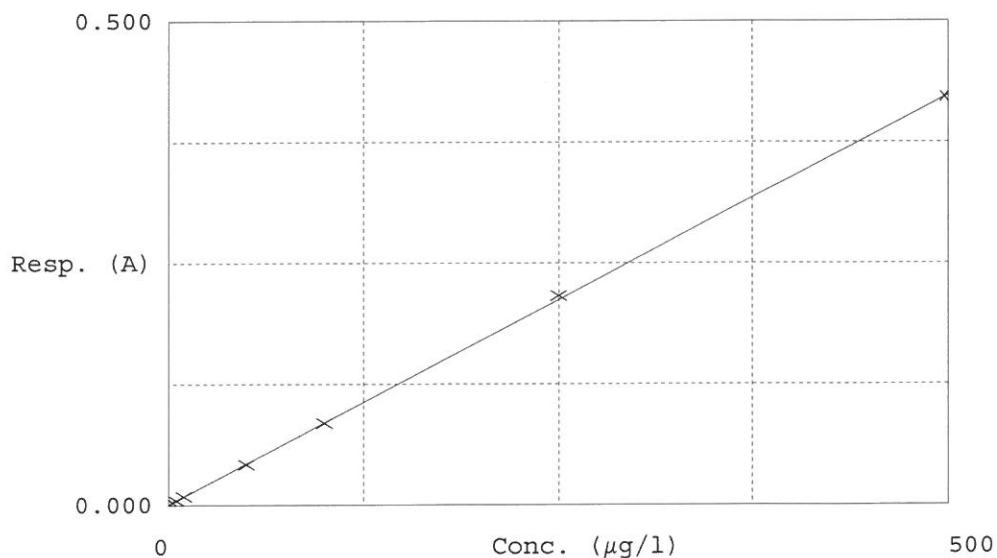

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.0990	0.0000	-
2	5.0PPBCN	0.005	4.4533	5.0000	-10.9
3	10PPBCN	0.009	9.6235	10.0000	-3.8
4	50PPBCN	0.042	48.7535	50.0000	-2.5
5	100PPBCN	0.085	99.3055	100.0000	-0.7
6	250PPBCN	0.216	254.9773	250.0000	2.0
7	500PPBCN	0.422	497.7879	500.0000	-0.4

12 3/2/22