

Clear table

Instrument ID: IC-2										Method:		300.0 / 9056A	
Analyst :										IZ			
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2022-02-24_	2/24/22 9:19		IZ/AP		
STD2	0.4460	0.6760	0.6850	2.3070	0.5830	0.9020	3.5940	0.0000_2022-02-24_	2/24/22 9:47		IZ/AP		
STD3	0.8340	1.2230	1.2150	4.0580	1.0210	2.0340	6.1250	0.0000_2022-02-24_	2/24/22 10:16		IZ/AP		
STD4	0.9640	1.5070	1.4940	4.9870	1.2470	2.5640	7.4540	0.0000_2022-02-24_	2/24/22 10:44		IZ/AP		
STD5	1.9190	2.9030	2.9130	9.6630	2.4010	5.0700	14.3340	0.0000_2022-02-24_	2/24/22 11:13		IZ/AP		
STD6	4.0470	5.8550	5.8620	19.5320	4.8750	9.8620	29.2010	0.0000_2022-02-24_	2/24/22 11:42		IZ/AP		
STD7	4.9900	7.6360	7.6300	25.4530	6.3720	12.5690	38.2920	0.0000_2022-02-24_	2/24/22 12:10		IZ/AP		
ICV	2.0180	2.9500	2.9680	9.8510	2.4610	5.1030	14.6150	0.0000_2022-02-24_	2/24/22 13:22		IZ/AP		
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2022-02-24_	2/24/22 13:52		IZ/AP		
CCV	1.9830	2.8890	2.9000	9.6140	2.3910	5.4020	14.2260	0.0000_2022-03-02_	3/2/22 9:15		IZ/AP		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2022-03-02_	3/2/22 9:46		IZ/AP		
LB118966BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2022-03-02_	3/2/22 10:15		IZ/AP		
LB118966BSW	1.8210	2.8050	2.8240	9.2960	2.3320	5.4990	14.0640	0.0000_2022-03-02_	3/2/22 11:14		IZ/AP		
N1645-09	0.2740	0.4320	0.4590	1.4490	0.3890	0.6400	2.4780	0.0000_2022-03-02_	3/2/22 11:43		IZ/AP		
N1645-09RE 0.25M	0.2000	0.2880	0.3100	1.0100	0.2750	0.2740	1.7950	0.0000_2022-03-02_	3/2/22 12:41		IZ/AP		
N1752-01	0.0000	0.0000	0.0000	0.0000	0.2840	0.0000	1.1750	0.0000_2022-03-02_	3/2/22 14:26		IZ/AP		
N1752-01MS	2.1730	3.0430	2.9870	9.9580	2.6260	6.7630	14.7690	0.0000_2022-03-02_	3/2/22 14:55		IZ/AP		
N1752-01MSD	2.2110	2.9280	2.9060	9.6070	2.5520	6.3960	14.3460	0.0000_2022-03-02_	3/2/22 15:23		IZ/AP		
CCV	1.9200	2.9010	2.9450	9.6720	2.4140	5.4980	14.3280	0.0000_2022-03-02_	3/2/22 16:26		IZ/AP		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2022-03-02_	3/2/22 16:54		IZ/AP		

Report date: 3/3/2022 10:09:43 AM
Printed by: wet


Ident: CCV
Analysis from: 3/2/2022 9:15:02 AM
File: _2022-03-02_

Last save: 3/2/2022 9:41:03 AM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30271

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

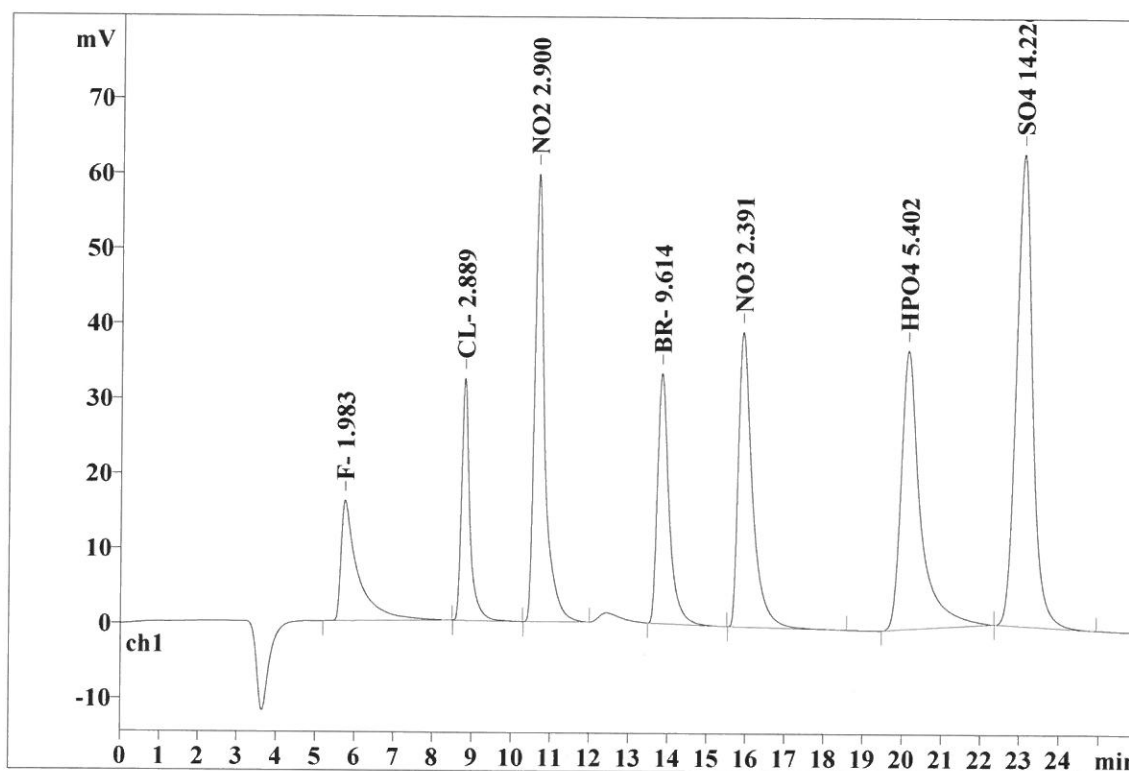

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.74	0.360	16.08	5.72	482.081	7.09
2	8.79	0.202	32.30	11.50	472.184	6.94
3	10.64	0.245	59.71	21.26	1081.702	15.90
4	13.82	0.300	33.37	11.88	695.944	10.23
5	15.90	0.357	39.32	14.00	988.209	14.53
6	20.13	0.454	37.16	13.23	1281.133	18.83
7	23.05	0.420	62.95	22.41	1800.786	26.47
7	26.00	0.334	280.89	100.00	6802.039	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/3/2022 10:10:16 AM
Printed by: wet


Ident: CCB
Analysis from: 3/2/2022 9:46:40 AM
File: _2022-03-02_

Last save: 3/2/2022 10:12:41 AM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30272

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

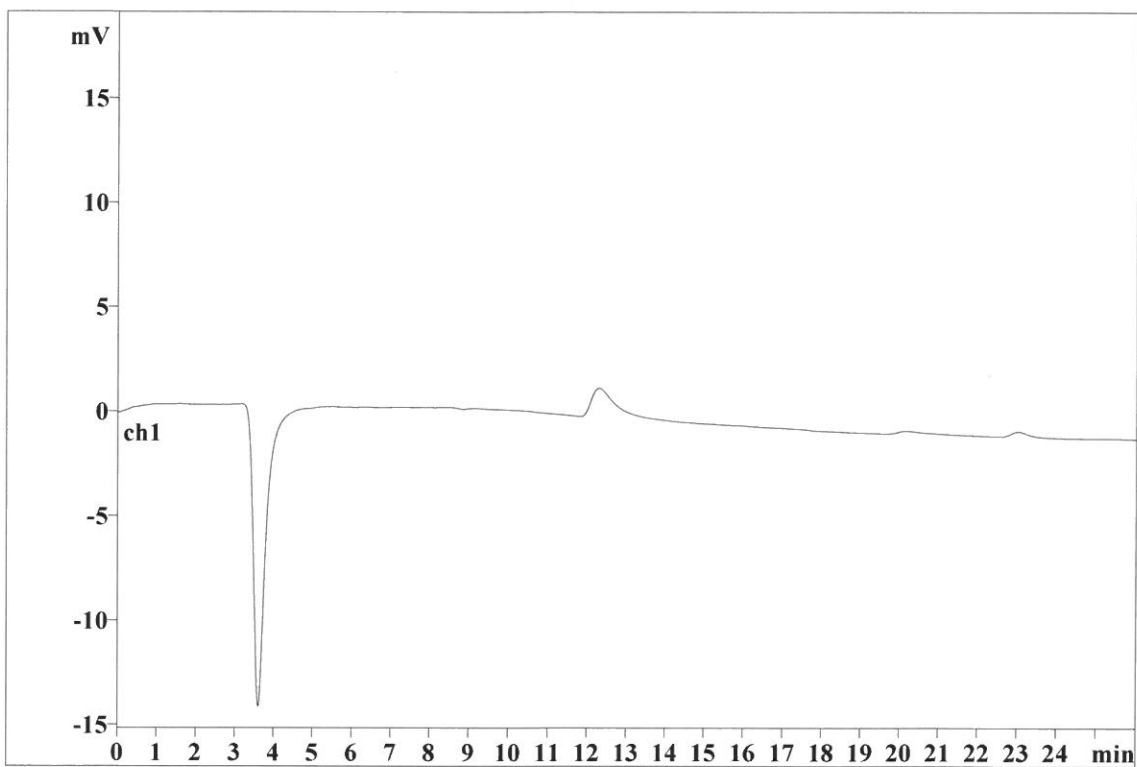

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/3/2022 10:10:23 AM

Printed by:

wet

LB118919BLW sb 3/3/22

Ident: LB118919BLW

Analysis from: 3/2/2022 10:15:23 AM

File: _2022-03-02_

Last save: 3/2/2022 10:41:24 AM

Method: AnionsIC2-022422.mtw

Last save: 2/24/2022 12:51

Run operator: wet

Analysis number: 30273

SAMPLE:

:

IZ/AP

Vial number:

13

Volume:


20.0 µL

Dilution:

1.00

Amount:

1.0000

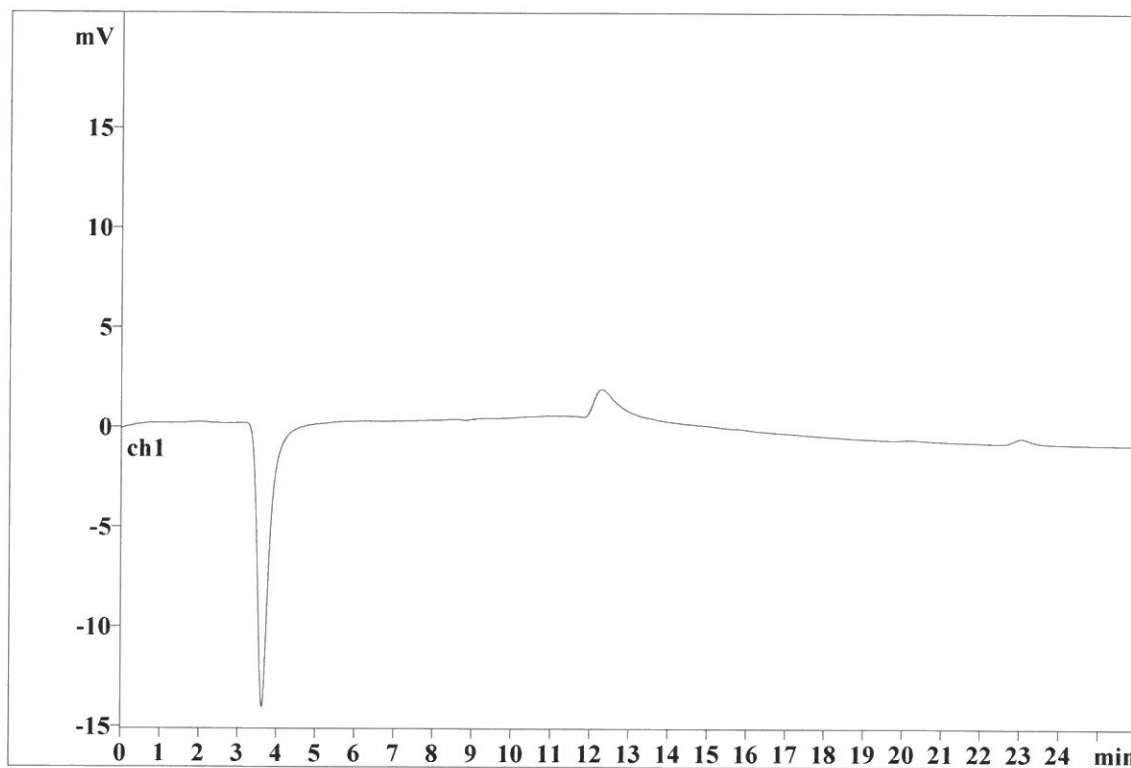

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/3/2022 10:10:48 AM
Printed by: wet


Ident: LB118966BSW
Analysis from: 3/2/2022 11:14:51 AM
File: _2022-03-02_

Last save: 3/3/2022 10:05:03 AM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30275

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

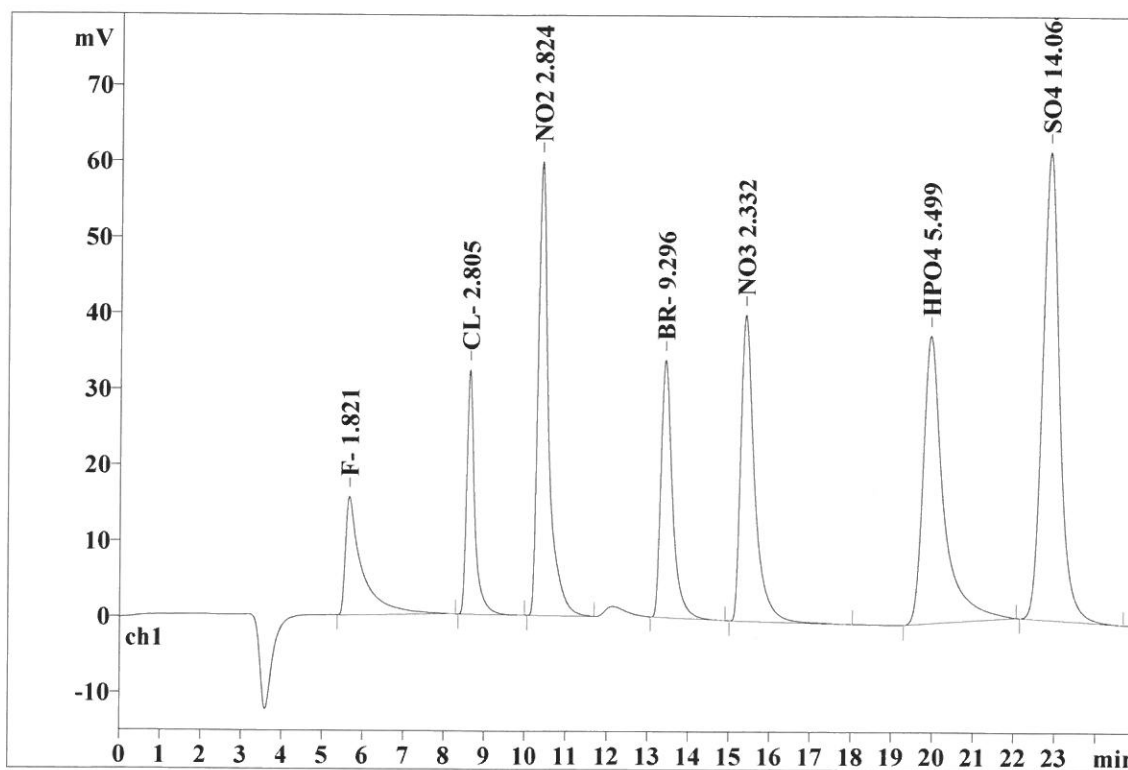

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.66	0.327	15.58	5.53	440.088	6.60
2	8.61	0.195	32.23	11.45	457.685	6.87
3	10.38	0.237	59.81	21.25	1051.641	15.78
4	13.41	0.285	33.94	12.06	671.430	10.07
5	15.38	0.339	40.33	14.33	961.898	14.43
6	19.93	0.452	37.91	13.47	1303.751	19.56
7	22.85	0.424	61.65	21.91	1778.671	26.69
7	25.00	0.323	281.44	100.00	6665.165	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/3/2022 10:10:56 AM
Printed by: wet


Ident: N1645-09
Analysis from: 3/2/2022 11:43:25 AM
File: _2022-03-02_

Last save: 3/2/2022 12:09:26 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30276

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 16
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

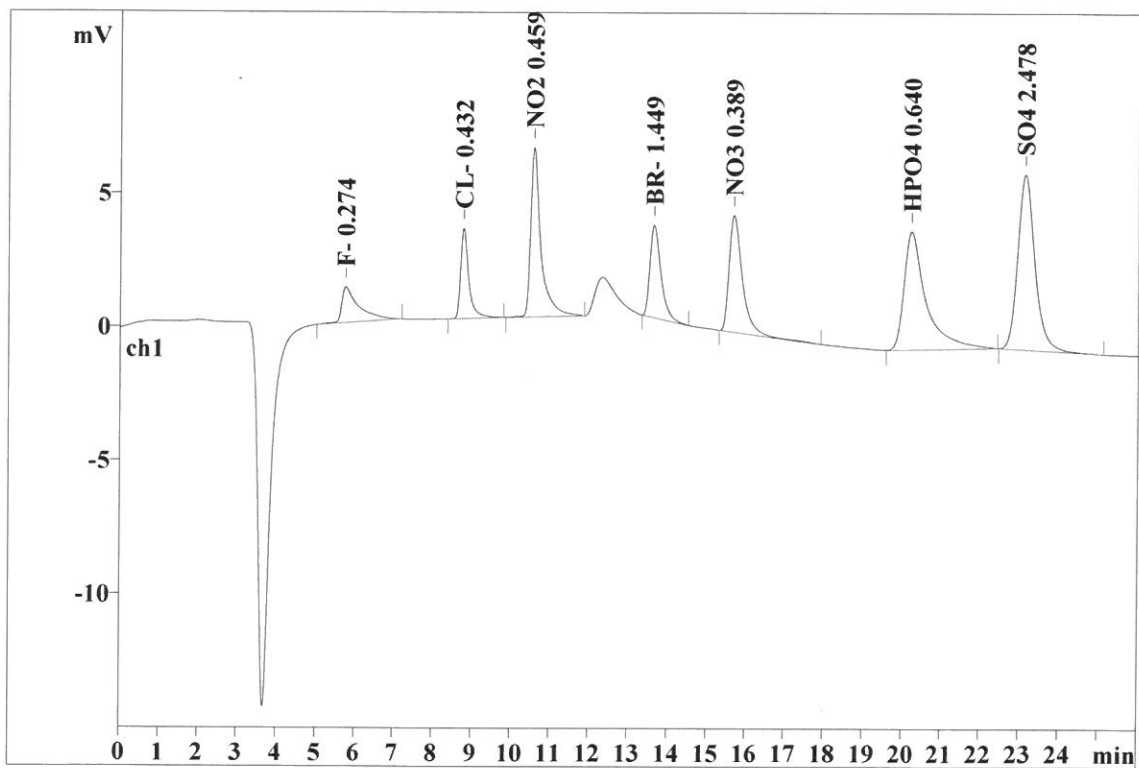

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.76	0.378	1.34	4.47	40.707	5.42
2	8.77	0.199	3.38	11.31	48.775	6.49
3	10.58	0.240	6.33	21.21	116.921	15.56
4	13.64	0.292	3.47	11.60	68.191	9.07
5	15.68	0.343	4.37	14.64	105.016	13.98
6	20.23	0.515	4.42	14.80	175.954	23.42
7	23.14	0.439	6.55	21.94	195.889	26.07
7	26.00	0.344	29.85	99.97	751.454	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/3/2022 10:11:11 AM
Printed by: wet


Ident: N1645-09RE 0.25ML
Analysis from: 3/2/2022 12:41:41 PM
File: _2022-03-02_

Last save: 3/2/2022 1:07:41 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30278

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 17
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

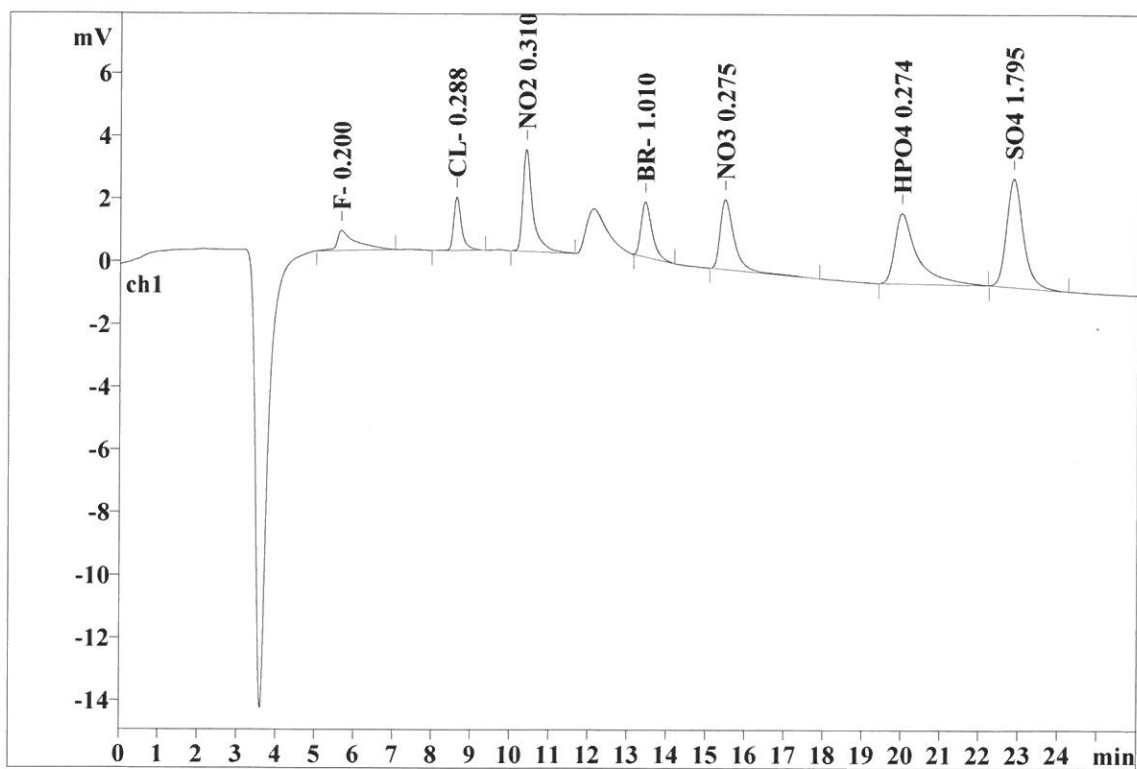

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.65	0.396	0.64	4.18	21.472	5.55
2	8.59	0.196	1.70	11.14	23.993	6.20
3	10.38	0.237	3.26	21.30	58.163	15.03
4	13.42	0.292	1.75	11.44	34.431	8.90
5	15.46	0.344	2.23	14.59	55.141	14.25
6	19.99	0.521	2.25	14.68	91.050	23.53
7	22.85	0.436	3.46	22.63	102.664	26.53
7	26.00	0.346	15.30	99.95	386.914	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/3/2022 10:11:28 AM
Printed by: wet


Ident: N1752-01
Analysis from: 3/2/2022 2:26:26 PM
File: _2022-03-02_

Last save: 3/2/2022 2:52:26 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30281

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

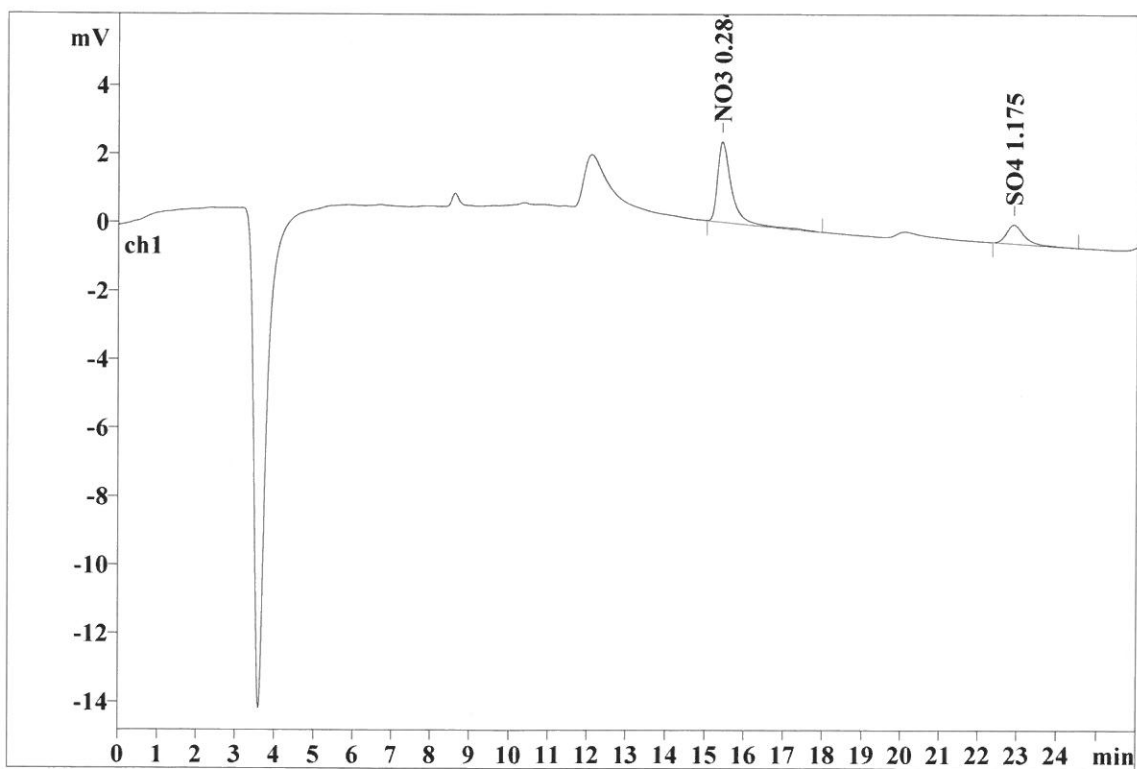

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.41	0.343	2.34	80.61	58.871	76.71
6	0.00	0.000	0.00	0.00	0.000	0.00
7	22.90	0.460	0.56	19.19	17.871	23.29
7	26.00	0.115	2.90	99.80	76.743	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/3/2022 10:11:43 AM
Printed by: wet


Ident: N1752-01MS
Analysis from: 3/2/2022 2:55:05 PM
File: _2022-03-02_

Last save: 3/2/2022 3:21:05 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30282

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 19
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

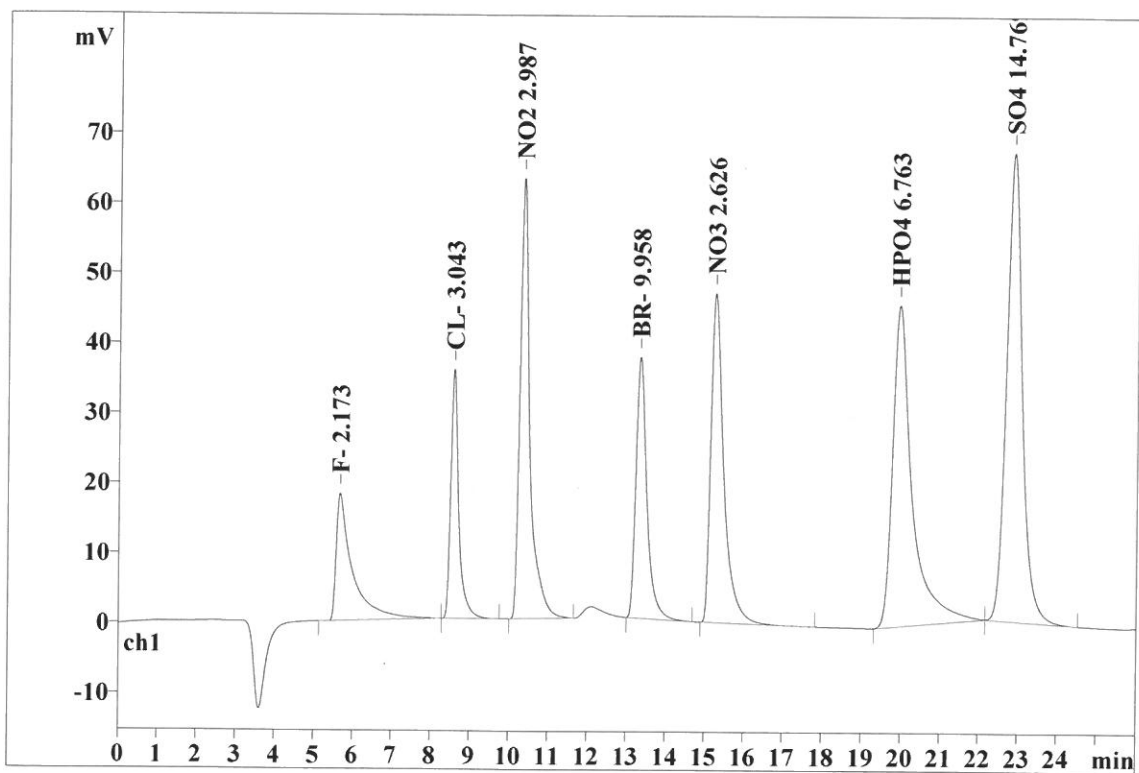

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.66	0.347	18.13	5.78	531.056	7.15
2	8.58	0.193	35.58	11.34	498.782	6.71
3	10.34	0.238	62.89	20.04	1115.959	15.02
4	13.33	0.280	37.29	11.89	722.336	9.72
5	15.26	0.331	47.03	14.99	1091.757	14.69
6	19.95	0.453	45.86	14.62	1597.097	21.49
7	22.85	0.412	66.95	21.34	1874.918	25.23
7	26.00	0.322	313.74	100.00	7431.905	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/3/2022 10:11:51 AM
Printed by: wet


Ident: N1752-01MSD
Analysis from: 3/2/2022 3:23:43 PM
File: _2022-03-02_

Last save: 3/2/2022 3:49:43 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30283

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 20
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

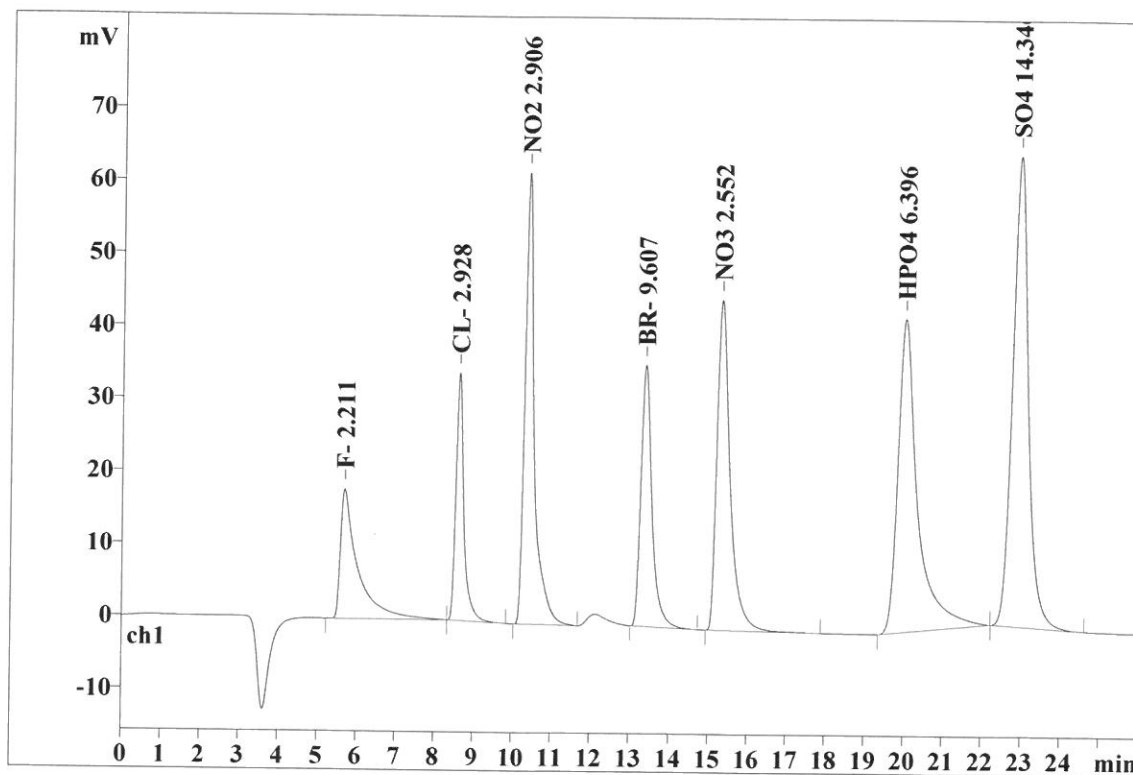

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.68	0.362	17.82	5.87	540.890	7.53
2	8.60	0.194	34.10	11.24	478.966	6.66
3	10.36	0.233	62.15	20.49	1083.740	15.08
4	13.36	0.280	35.97	11.86	695.417	9.68
5	15.29	0.332	45.45	14.98	1059.172	14.74
6	20.00	0.456	43.10	14.21	1511.993	21.04
7	22.91	0.413	64.76	21.35	1817.192	25.28
7	26.00	0.324	303.36	99.99	7187.369	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/3/2022 10:12:02 AM
Printed by: wet


Ident: CCV
Analysis from: 3/2/2022 4:26:03 PM
File: _2022-03-02_

Last save: 3/2/2022 4:52:03 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30285

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

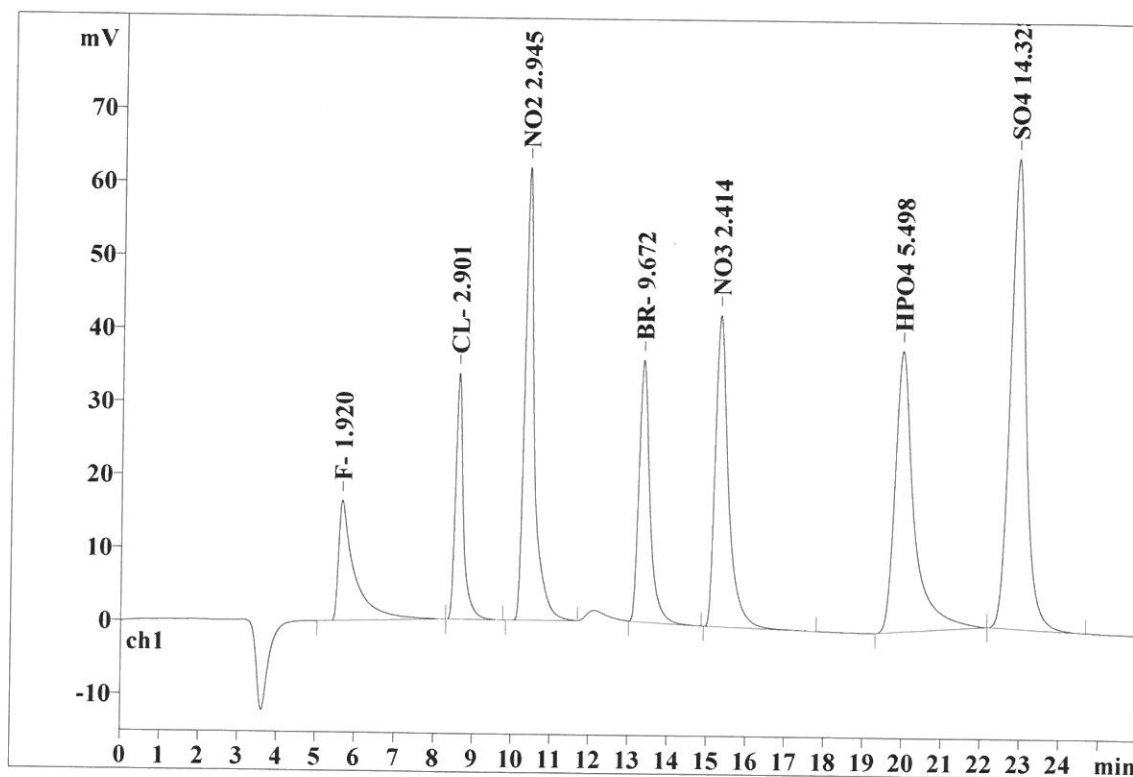

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.66	0.335	16.39	5.60	465.641	6.79
2	8.58	0.194	33.61	11.48	474.165	6.92
3	10.35	0.239	61.84	21.13	1099.460	16.04
4	13.33	0.283	35.75	12.21	700.373	10.22
5	15.28	0.334	42.53	14.53	998.196	14.56
6	19.94	0.447	38.36	13.11	1303.545	19.01
7	22.85	0.415	64.24	21.94	1814.614	26.47
7	26.00	0.321	292.72	100.00	6855.994	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/3/2022 10:12:11 AM
Printed by: wet


Ident: CCB
Analysis from: 3/2/2022 4:54:46 PM
File: _2022-03-02_

Last save: 3/2/2022 5:20:46 PM

Method: AnionsIC2-022422.mtw
Run operator: wet
Analysis number: 30286

Last save: 2/24/2022 12:51

SAMPLE:
: IZ/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

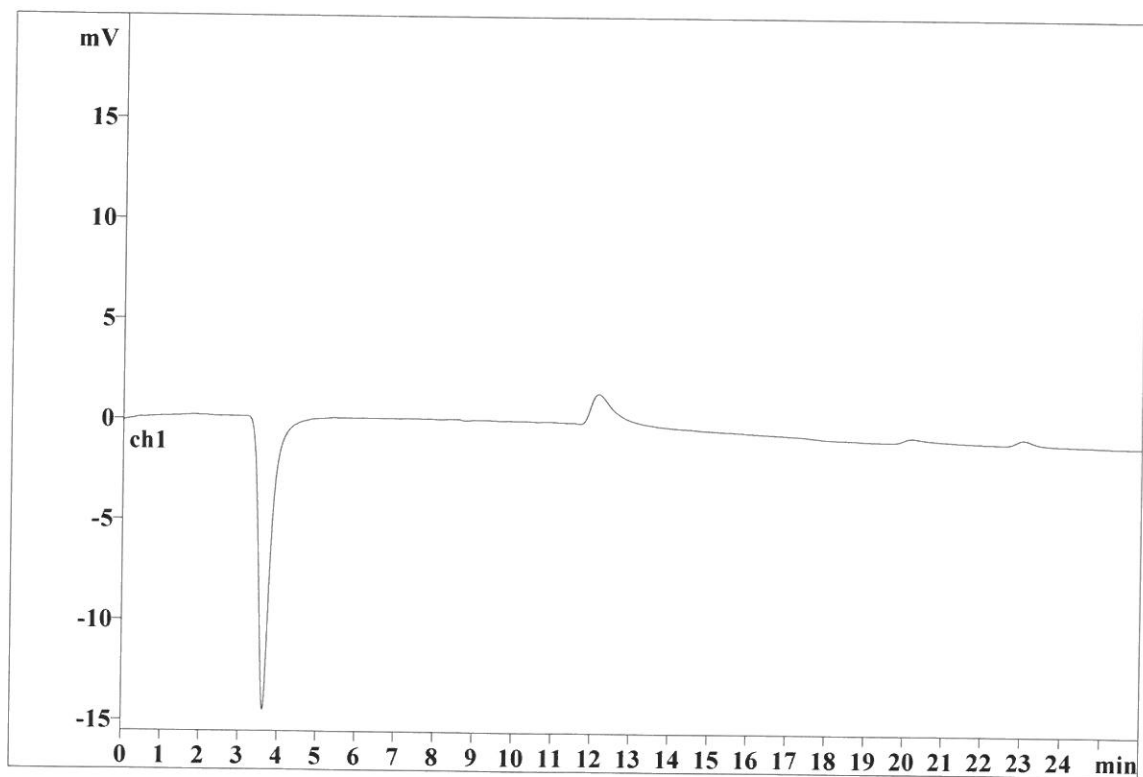

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD