


LB118971

7470A INSTRUMENT ID: CV1

Linear

 μ Abs.:

39469

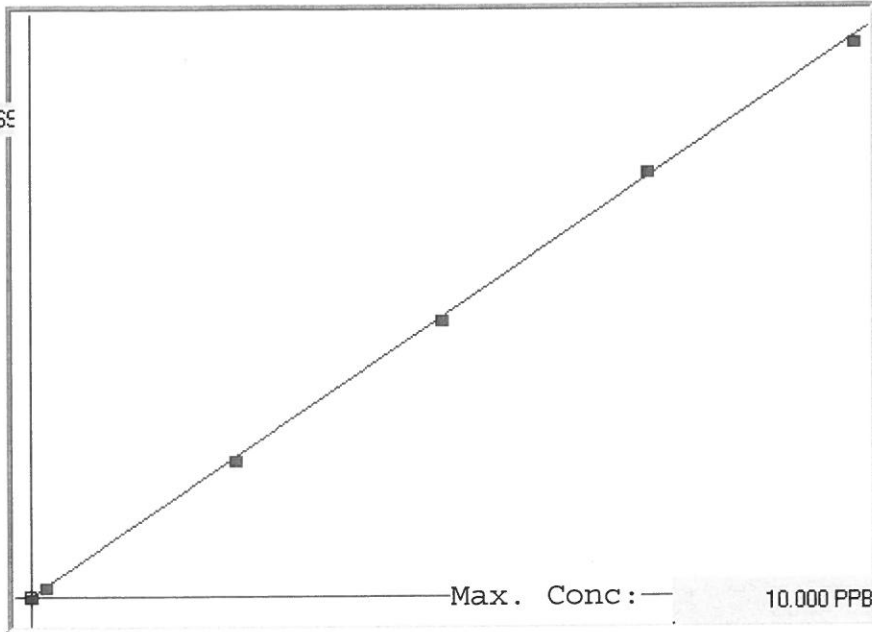

A= 0.0000e+000

B= 2.5145e-004

C= 9.5931e-003

Rho= 0.9999038

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	Q/D
0.0	0.000	0.009	0.009	-4	0.000	-4					-5
0.2	0.200	0.191	-0.009	720	0.0 %	720					-1
2.5	2.500	2.478	-0.022	9815	0.0 %	9815					0
5.0	5.000	4.987	-0.013	19794	0.0 %	19794					1
7.5	7.500	7.603	0.103	30197	0.0 %	30197					-1
10.0	10.000	9.934	-0.066	39469	0.0 %	39469					

LB118971 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 03 Mar 2022 12:09:36				
Sample ID	Extended ID	µ Abs.	Conc.	Std. Conc.	Method	Units	Date	Type
0.0 - 1	50	-4	-	0.0000	7470A	PPB	03 Mar 2022 12:14:54	S Std
0.2 - 1	02	720	-	0.2000	7470A	PPB	03 Mar 2022 12:17:11	S Std
2.5 - 1	52.5	9815	-	2.5000	7470A	PPB	03 Mar 2022 12:19:28	S Std
5.0 - 1	55	19794	-	5.0000	7470A	PPB	03 Mar 2022 12:21:45	S Std
7.5 - 1	57.5	30197	-	7.5000	7470A	PPB	03 Mar 2022 12:24:02	S Std
10.0 - 1	511	39469	-	10.0000	7470A	PPB	03 Mar 2022 12:26:18	S Std
ICV17 - 1	ICV17	15206	3.8331	-	7470A	PPB	03 Mar 2022 12:28:59	U SMPL
ICB17 - 1	ICB17	-35	0.0008	-	7470A	PPB	03 Mar 2022 12:31:14	U SMPL
CCV89 - 1	CCV89	18680	4.7066	-	7470A	PPB	03 Mar 2022 12:33:30	U SMPL
CCB89 - 1	CCB89	-36	0.0005	-	7470A	PPB	03 Mar 2022 12:35:45	U SMPL
CRA - 1	CRA	738	0.1952	-	7470A	PPB	03 Mar 2022 12:38:00	U SMPL
HighStd - 1	HighStd	39751	10.0049	-	7470A	PPB	03 Mar 2022 12:40:16	U SMPL
ChkStd - 1	ChkStd	27216	6.8530	-	7470A	PPB	03 Mar 2022 12:42:31	U SMPL
PB143047BL - 1	PBW	-54	-0.0040	-	7470A	PPB	03 Mar 2022 12:44:47	U SMPL
PB143047BS - 1	LCSW	15344	3.8678	-	7470A	PPB	03 Mar 2022 12:47:03	U SMPL
N1717-02 - 1	ETGI-359	-19	0.0048	-	7470A	PPB	03 Mar 2022 12:49:20	U SMPL
N1717-02DUP - 1	ETGI-359DUP	29	0.0169	-	7470A	PPB	03 Mar 2022 12:51:37	U SMPL
N1717-02MS - 1	ETGI-359MS	14985	3.7775	-	7470A	PPB	03 Mar 2022 12:53:54	U SMPL
N1717-02MSD - 1	ETGI-359MSD	16071	4.0506	-	7470A	PPB	03 Mar 2022 12:56:11	U SMPL
PB143080BL - 1	PBW	-26	0.0031	-	7470A	PPB	03 Mar 2022 12:58:26	U SMPL
CCV90 - 1	CCV90	19404	4.8887	-	7470A	PPB	03 Mar 2022 13:00:42	U SMPL
CCB90 - 1	CCB90	-42	-0.0010	-	7470A	PPB	03 Mar 2022 13:02:57	U SMPL
PB143080BS - 1	LCSW	15956	4.0217	-	7470A	PPB	03 Mar 2022 13:05:13	U SMPL
N1727-01 - 1	20220215-096-21-03-ELUTRIATE	30	0.0171	-	7470A	PPB	03 Mar 2022 13:07:28	U SMPL
N1727-01DUP - 1	20220215-096-21-03-ELUTRIATEDUP	81	0.0300	-	7470A	PPB	03 Mar 2022 13:09:44	U SMPL
N1727-01MS - 1	20220215-096-21-03-ELUTRIATEMS	17333	4.3679	-	7470A	PPB	03 Mar 2022 13:12:00	U SMPL
N1727-01MSD - 1	20220215-096-21-03-ELUTRIATEMSD	16219	4.0878	-	7470A	PPB	03 Mar 2022 13:14:16	U SMPL
N1727-02 - 1	20220216-098-21-01-ELUTRIATE	3	0.0103	-	7470A	PPB	03 Mar 2022 13:16:32	U SMPL
PB143039TB - 1	PB143039TB	-35	0.0008	-	7470A	PPB	03 Mar 2022 13:18:49	U SMPL
CCV91 - 1	CCV91	19087	4.8090	-	7470A	PPB	03 Mar 2022 13:21:06	U SMPL
CCB91 - 1	CCB91	-51	-0.0032	-	7470A	PPB	03 Mar 2022 13:23:23	U SMPL
N1717-02LX5 - 1		4	0.0106	-	7470A	PPB	03 Mar 2022 13:25:40	U SMPL
N1717-02A - 1		15600	3.9322	-	7470A	PPB	03 Mar 2022 13:27:55	U SMPL
N1727-01LX5 - 1		-3	0.0088	-	7470A	PPB	03 Mar 2022 13:30:11	U SMPL
N1727-01A - 1		16971	4.2769	-	7470A	PPB	03 Mar 2022 13:32:27	U SMPL
CCV92 - 1	CCV92	18767	4.7285	-	7470A	PPB	03 Mar 2022 13:34:43	U SMPL
CCB92 - 1	CCB92	-42	-0.0010	-	7470A	PPB	03 Mar 2022 13:36:58	U SMPL