

LB11P236

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

3/18/2022 13:12

Test: ~~total~~ ^{Relative} CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.988	0.0	0.087	
ICB1	0.365	0.0	0.001	
CCV1	249.056	0.0	0.227	
CCB1	-0.260	0.0	0.001	
PB143458BL	-0.209	0.0	0.001	
N1994-03	-0.509	0.0	0.001	
N1994-03DUP	0.005	0.0	0.001	
N1994-06	-0.502	0.0	0.001	
N1994-09	-0.310	0.0	0.001	
N1994-12	-0.544	0.0	0.000	
N1994-15	-0.302	0.0	0.001	
N1995-03	-0.547	0.0	0.000	
N1995-06	-0.310	0.0	0.001	
N1995-09	-0.474	0.0	0.001	
CCV2	244.964	0.0	0.223	
CCB2	0.053	0.0	0.001	

N	16
Mean	36.591
SD	85.4939
CV%	233.64

Aquakem v. 7.2AQ1

Results from time period:

Fri Mar 18 10:39:24 2022

Fri Mar 18 13:09:48 2022

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.1393	µg/l	3/18/2022 10:39:24	
5.OPPBCN	A	Reactive CN	P	4.5499	µg/l	3/18/2022 10:39:25	
10PPBCN	A	Reactive CN	P	9.2959	µg/l	3/18/2022 10:39:26	
50PPBCN	A	Reactive CN	P	48.5447	µg/l	3/18/2022 10:39:27	
100PPBCN	A	Reactive CN	P	99.6606	µg/l	3/18/2022 10:39:28	
250PPBCN	A	Reactive CN	P	255.1553	µg/l	3/18/2022 10:39:29	
500PPBCN	A	Reactive CN	P	497.6543	µg/l	3/18/2022 10:39:30	
ICV1	S	Reactive CN	P	94.9884	µg/l	3/18/2022 12:44:15	
ICB1	S	Reactive CN	P	0.3654	µg/l	3/18/2022 12:44:18	
CCV1	S	Reactive CN	P	249.0558	µg/l	3/18/2022 12:44:19	
CCB1	S	Reactive CN	P	-0.2597	µg/l	3/18/2022 12:44:22	
PB143458BL	S	Reactive CN	P	-0.2092	µg/l	3/18/2022 12:44:24	
N1994-03	S	Reactive CN	P	-0.5091	µg/l	3/18/2022 12:44:25	
N1994-03DUP	S	Reactive CN	P	0.0053	µg/l	3/18/2022 12:51:50	
N1994-06	S	Reactive CN	P	-0.5023	µg/l	3/18/2022 12:51:51	
N1994-09	S	Reactive CN	P	-0.3103	µg/l	3/18/2022 12:51:52	
N1994-12	S	Reactive CN	P	-0.544	µg/l	3/18/2022 12:51:53	
N1994-15	S	Reactive CN	P	-0.3019	µg/l	3/18/2022 12:51:54	
N1995-03	S	Reactive CN	P	-0.547	µg/l	3/18/2022 12:51:55	
N1995-06	S	Reactive CN	P	-0.3101	µg/l	3/18/2022 12:51:56	
N1995-09	S	Reactive CN	P	-0.4744	µg/l	3/18/2022 12:51:57	
CCV2	S	Reactive CN	P	244.9643	µg/l	3/18/2022 12:52:00	
CCB2	S	Reactive CN	P	0.0528	µg/l	3/18/2022 13:09:48	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

3/18/2022 10:47


Test Total CN

Accepted 3/18/2022 10:47

Factor 1102
Bias 0.001

Coeff. of det. 0.999830

Errors

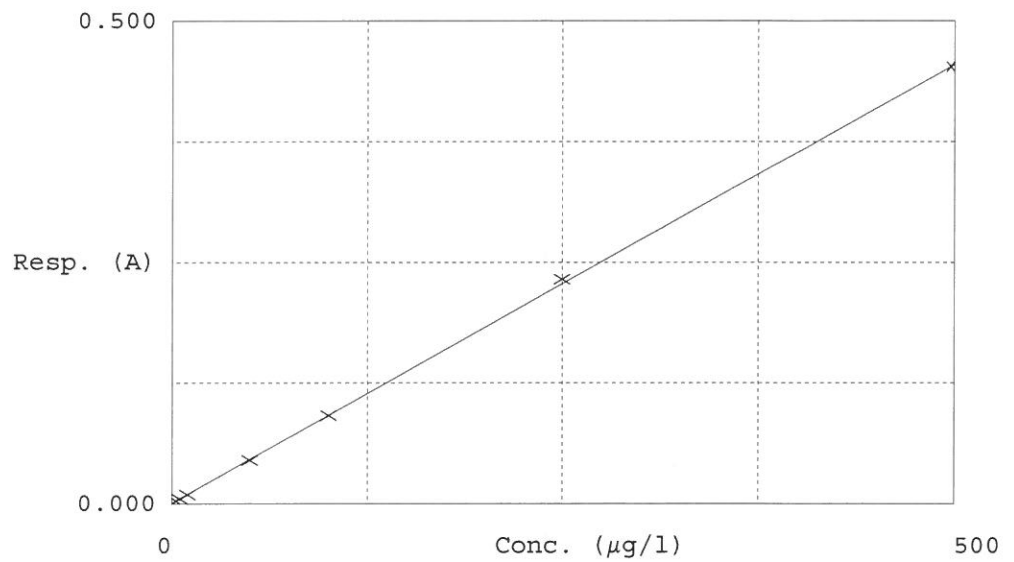

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.1393	0.0000	-
2	5.0PPBCN	0.005	4.5499	5.0000	-9.0
3	10PPBCN	0.009	9.2959	10.0000	-7.0
4	50PPBCN	0.045	48.5447	50.0000	-2.9
5	100PPBCN	0.091	99.6606	100.0000	-0.3
6	250PPBCN	0.233	255.1553	250.0000	2.1
7	500PPBCN	0.453	497.6543	500.0000	-0.5

12 3/18/22