


LB119255

7470A

INSTRUMENT ID: CV1

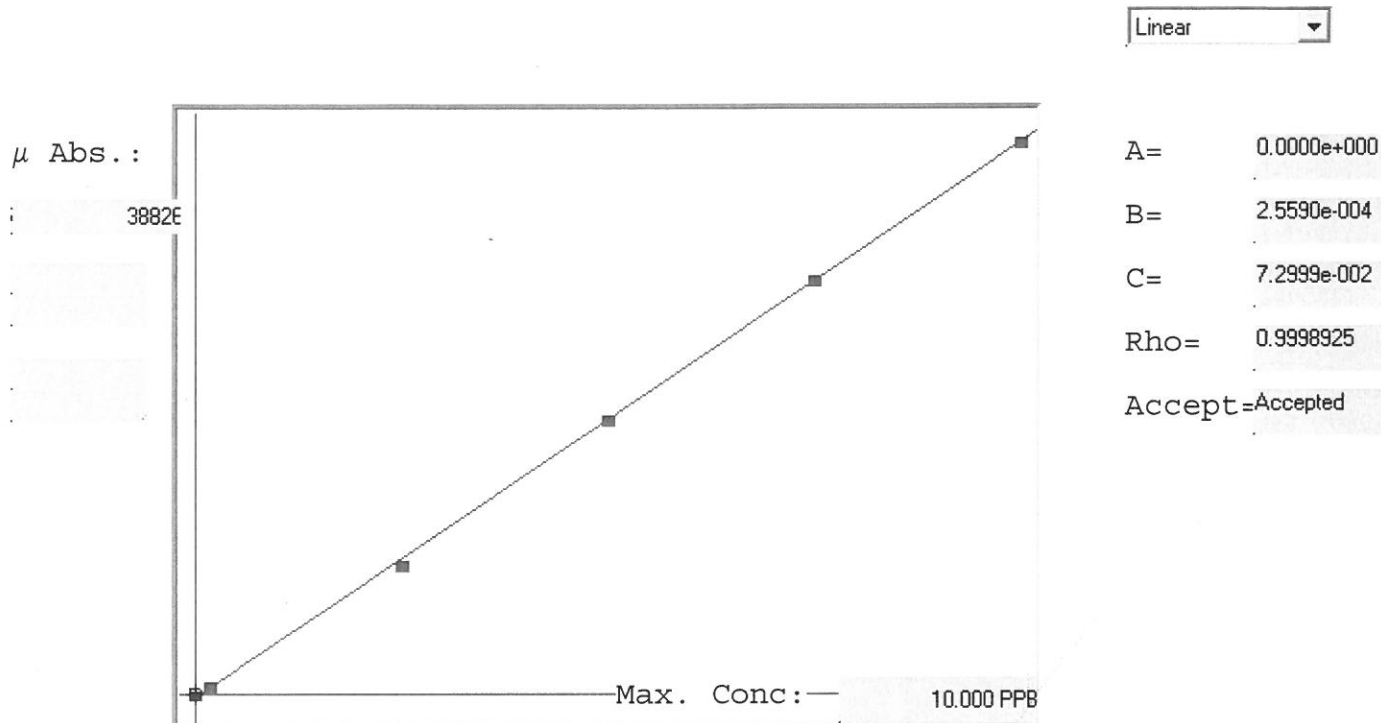

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	g/100
0.0	0.000	0.049	0.049	-93	0.000	-93					5
0.2	0.200	0.232	0.032	621	0.0 %	621					16
2.5	2.500	2.383	-0.117	9028	0.0 %	9028					5
5.0	5.000	5.008	0.008	19286	0.0 %	19286					0
7.5	7.500	7.519	0.019	29097	0.0 %	29097					0
10.0	10.000	10.009	0.009	38826	0.0 %	38826					0

LB119255 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 21 Mar 2022 08:43:18				
Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	-93	-	0.00007470A	PPB	21 Mar 2022 08:57:20	S	Std
0.2 - 1	50.2	621	-	0.20007470A	PPB	21 Mar 2022 08:59:38	S	Std
2.5 - 1	52.5	9028	-	2.50007470A	PPB	21 Mar 2022 09:01:55	S	Std
5.0 - 1	55	19286	-	5.00007470A	PPB	21 Mar 2022 09:04:12	S	Std
7.5 - 1	57.5	29097	-	7.50007470A	PPB	21 Mar 2022 09:06:30	S	Std
10.0 - 1	510	38826	-	10.00007470A	PPB	21 Mar 2022 09:08:47	S	Std
ICV38 - 1	ICV38	14572	3.8020	-7470A	PPB	21 Mar 2022 09:16:49	U	SMPL
ICB38 - 1	ICB38	-85	0.0512	-7470A	PPB	21 Mar 2022 09:19:04	U	SMPL
CCV84 - 1	CCV84	19807	5.1416	-7470A	PPB	21 Mar 2022 09:21:20	U	SMPL
CCB84 - 1	CCB84	-74	0.0541	-7470A	PPB	21 Mar 2022 09:23:35	U	SMPL
HighStd - 1	HighStd	40042	10.3197	-7470A	PPB	21 Mar 2022 09:28:07	U	SMPL
ChkStd - 1	ChkStd	28382	7.3359	-7470A	PPB	21 Mar 2022 09:30:23	U	SMPL
PB143461BL - 1	PBW	-89	0.0502	-7470A	PPB	21 Mar 2022 09:32:41	U	SMPL
PB143461BS - 1	LCSW	16235	4.2275	-7470A	PPB	21 Mar 2022 09:34:59	U	SMPL
N1947-01 - 1	NWB-1728	-57	0.0584	-7470A	PPB	21 Mar 2022 09:37:16	U	SMPL
N1982-02 - 1	CONCRETE-A	-8	0.0710	-7470A	PPB	21 Mar 2022 09:39:33	U	SMPL
N1982-04 - 1	CONCRETE-B	13	0.0763	-7470A	PPB	21 Mar 2022 09:41:50	U	SMPL
N1983-02 - 1	124035	-12	0.0699	-7470A	PPB	21 Mar 2022 09:44:07	U	SMPL
N1983-04 - 1	124042	6	0.0745	-7470A	PPB	21 Mar 2022 09:46:23	U	SMPL
CCV85 - 1	CCV85	19347	5.0239	-7470A	PPB	21 Mar 2022 09:48:38	U	SMPL
CCB85 - 1	CCB85	-57	0.0584	-7470A	PPB	21 Mar 2022 09:50:54	U	SMPL
N1983-06 - 1	124019	0	0.0730	-7470A	PPB	21 Mar 2022 09:53:10	U	SMPL
N1983-08 - 1	124055	1	0.0733	-7470A	PPB	21 Mar 2022 09:55:26	U	SMPL
N1985-02 - 1	VACLOT-SOIL-1	57	0.0876	-7470A	PPB	21 Mar 2022 09:57:41	U	SMPL
N1985-05 - 1	VACLOT-SOIL-2	30	0.0807	-7470A	PPB	21 Mar 2022 09:59:57	U	SMPL
N1994-03 - 1	SB-01-COMP	10	0.0756	-7470A	PPB	21 Mar 2022 10:02:19	U	SMPL
N1994-06 - 1	SB-02-COMP	33	0.0814	-7470A	PPB	21 Mar 2022 10:04:37	U	SMPL
N1994-09 - 1	SB-03-COMP	7	0.0748	-7470A	PPB	21 Mar 2022 10:06:55	U	SMPL
N1994-12 - 1	SB-04-COMP	6	0.0745	-7470A	PPB	21 Mar 2022 10:09:13	U	SMPL
N1994-15 - 1	SB-05-COMP	18	0.0776	-7470A	PPB	21 Mar 2022 10:11:30	U	SMPL
N1995-03 - 1	SB-06-COMP	15	0.0768	-7470A	PPB	21 Mar 2022 10:13:46	U	SMPL
CCV86 - 1	CCV86	20138	5.2263	-7470A	PPB	21 Mar 2022 10:16:02	U	SMPL
CCB86 - 1	CCB86	-57	0.0584	-7470A	PPB	21 Mar 2022 10:18:17	U	SMPL
N1995-06 - 1	SB-07-COMP	-13	0.0697	-7470A	PPB	21 Mar 2022 10:20:34	U	SMPL
N1995-09 - 1	SB-06-COMP	26	0.0797	-7470A	PPB	21 Mar 2022 10:22:50	U	SMPL
N1995-09DUP - 1	SB-06-COMPDUP	23	0.0789	-7470A	PPB	21 Mar 2022 10:25:06	U	SMPL
N1995-09MS - 1	SB-06-COMPMS	15303	3.9890	-7470A	PPB	21 Mar 2022 10:27:22	U	SMPL
N1995-09MSD - 1	SB-06-COMPMSD	14461	3.7735	-7470A	PPB	21 Mar 2022 10:29:37	U	SMPL
PB143462BL - 1	PBW	-72	0.0546	-7470A	PPB	21 Mar 2022 10:31:55	U	SMPL
PB143462BS - 1	LCSW	16122	4.1986	-7470A	PPB	21 Mar 2022 10:34:12	U	SMPL
N1974-13 - 1	B-3	-21	0.0676	-7470A	PPB	21 Mar 2022 10:36:29	U	SMPL
N1974-13DUP - 1	B-3DUP	43	0.0840	-7470A	PPB	21 Mar 2022 10:38:48	U	SMPL
N1974-13MS - 1	B-3MS	16859	4.3872	-7470A	PPB	21 Mar 2022 10:41:04	U	SMPL
CCV87 - 1	CCV87	20101	5.2168	-7470A	PPB	21 Mar 2022 10:43:20	U	SMPL
CCB87 - 1	CCB87	-45	0.0615	-7470A	PPB	21 Mar 2022 10:45:36	U	SMPL
N1974-13MSD - 1	B-3MSD	14869	3.8780	-7470A	PPB	21 Mar 2022 10:47:53	U	SMPL
PB143463BL - 1	PBW	-49	0.0605	-7470A	PPB	21 Mar 2022 10:50:09	U	SMPL
PB143463BS - 1	LCSW	15968	4.1592	-7470A	PPB	21 Mar 2022 10:52:26	U	SMPL
N1960-17 - 1	EB-20220316	-52	0.0597	-7470A	PPB	21 Mar 2022 10:54:41	U	SMPL
N1977-08 - 1	EB-20220315	-2	0.0725	-7470A	PPB	21 Mar 2022 10:56:59	U	SMPL
N1986-01 - 1	PW-410	269	0.1418	-7470A	PPB	21 Mar 2022 10:59:15	U	SMPL
N1986-01DUP - 1	PW-410DUP	263	0.1403	-7470A	PPB	21 Mar 2022 11:01:32	U	SMPL
N1986-01MS - 1	PW-410MS	13556	3.5420	-7470A	PPB	21 Mar 2022 11:03:49	U	SMPL
N1986-01MSD - 1	PW-410MSD	15403	4.0146	-7470A	PPB	21 Mar 2022 11:06:06	U	SMPL
N1992-01 - 1	N-37853	146	0.1104	-7470A	PPB	21 Mar 2022 11:08:23	U	SMPL
CCV88 - 1	CCV88	19814	5.1434	-7470A	PPB	21 Mar 2022 12:14:57	U	SMPL
CCB88 - 1	CCB88	-55	0.0589	-7470A	PPB	21 Mar 2022 12:17:12	U	SMPL
N2009-03 - 1	31722	1469	0.4489	-7470A	PPB	21 Mar 2022 12:19:28	U	SMPL
N2009-06 - 1	40453	137	0.1081	-7470A	PPB	21 Mar 2022 12:21:44	U	SMPL
PB143434TB - 1	PB143434TB	27	0.0799	-7470A	PPB	21 Mar 2022 12:24:00	U	SMPL
PB143437TB - 1	PB143437TB	-1	0.0727	-7470A	PPB	21 Mar 2022 12:26:16	U	SMPL
N1995-09LX5 - 1		0	0.0730	-7470A	PPB	21 Mar 2022 12:28:32	U	SMPL
N1995-09A - 1		16429	4.2772	-7470A	PPB	21 Mar 2022 12:33:37	U	SMPL
N1974-13LX5 - 1		-48	0.0607	-7470A	PPB	21 Mar 2022 12:35:53	U	SMPL
N1974-13A - 1		16529	4.3027	-7470A	PPB	21 Mar 2022 12:38:11	U	SMPL
N1986-01LX5 - 1		-27	0.0661	-7470A	PPB	21 Mar 2022 12:40:28	U	SMPL
N1986-01A - 1		15816	4.1203	-7470A	PPB	21 Mar 2022 12:42:45	U	SMPL
CCV89 - 1	CCV89	20002	5.1915	-7470A	PPB	21 Mar 2022 12:45:02	U	SMPL
CCB89 - 1	CCB89	-67	0.0559	-7470A	PPB	21 Mar 2022 12:47:19	U	SMPL
CRA - 1	CRA	265	0.1408	-7470A	PPB	21 Mar 2022 12:49:37	U	SMPL
CCV90 - 1	CCV90	20106	5.2181	-7470A	PPB	21 Mar 2022 12:57:12	U	SMPL
CCB90 - 1	CCB90	-46	0.0612	-7470A	PPB	21 Mar 2022 12:59:29	U	SMPL