

LB119265

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

3/21/2022 12:54

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.974	0.0	0.106	
ICB1	-0.020	0.0	0.005	
CCV1	1.001	0.0	0.109	
CCB1	-0.019	0.0	0.006	
PB143492BL	-0.018	0.0	0.006	
PB143492BS	0.993	0.0	0.108	
N2007-01	-0.001	0.0	0.007	
N2007-01DUP	0.002	0.0	0.008	
N2007-01MS	1.060	0.0	0.115	
N2007-01MSD	1.066	0.0	0.115	
N2007-02	-0.002	0.0	0.007	
N2007-03	0.009	0.0	0.008	
CCV2	0.991	0.0	0.108	
CCB2	-0.015	0.0	0.006	

N 14
Mean 0.430
SD 0.5254
CV% 122.17

Aquakem v. 7.2AQ1

Results from time period:

Mon Mar 21 10:15:16 2022

Mon Mar 21 12:37:25 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0	mg/l	3/21/2022 10:15:16	
0.05PPM	A	Phenolics-	P	0.0575	mg/l	3/21/2022 10:15:17	
0.1PPM	A	Phenolics-	P	0.1093	mg/l	3/21/2022 10:15:18	
0.25PPM	A	Phenolics-	P	0.2522	mg/l	3/21/2022 10:15:19	
0.50PPM	A	Phenolics-	P	0.4969	mg/l	3/21/2022 10:15:20	
1.0PPM	A	Phenolics-	P	0.9706	mg/l	3/21/2022 10:15:21	
2.0PPM	A	Phenolics-	P	2.0146	mg/l	3/21/2022 10:15:22	
ICV1	S	Phenolics-	P	0.974	mg/l	3/21/2022 12:27:28	
ICB1	S	Phenolics-	P	-0.0199	mg/l	3/21/2022 12:27:29	
CCV1	S	Phenolics-	P	1.0006	mg/l	3/21/2022 12:27:30	
CCB1	S	Phenolics-	P	-0.0188	mg/l	3/21/2022 12:27:31	
PB143492BL	S	Phenolics-	P	-0.0178	mg/l	3/21/2022 12:27:32	
PB143492BS	S	Phenolics-	P	0.9928	mg/l	3/21/2022 12:27:33	
N2007-01	S	Phenolics-	P	-0.0014	mg/l	3/21/2022 12:27:34	
N2007-01DUP	S	Phenolics-	P	0.0018	mg/l	3/21/2022 12:27:35	
N2007-01MS	S	Phenolics-	P	1.0595	mg/l	3/21/2022 12:27:36	
N2007-01MSD	S	Phenolics-	P	1.066	mg/l	3/21/2022 12:27:37	
N2007-02	S	Phenolics-	P	-0.0017	mg/l	3/21/2022 12:27:38	
N2007-03	S	Phenolics-	P	0.0094	mg/l	3/21/2022 12:27:39	
CCV2	S	Phenolics-	P	0.9906	mg/l	3/21/2022 12:37:24	
CCB2	S	Phenolics-	P	-0.0147	mg/l	3/21/2022 12:37:25	

CHEMTECH CONSULTING GROUP INC
 284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

3/21/2022 10:18


Test Phenolics-

Accepted 3/21/2022 10:18

Factor 9.891
 Bias 0.007

Coeff. of det. 0.999608

Errors

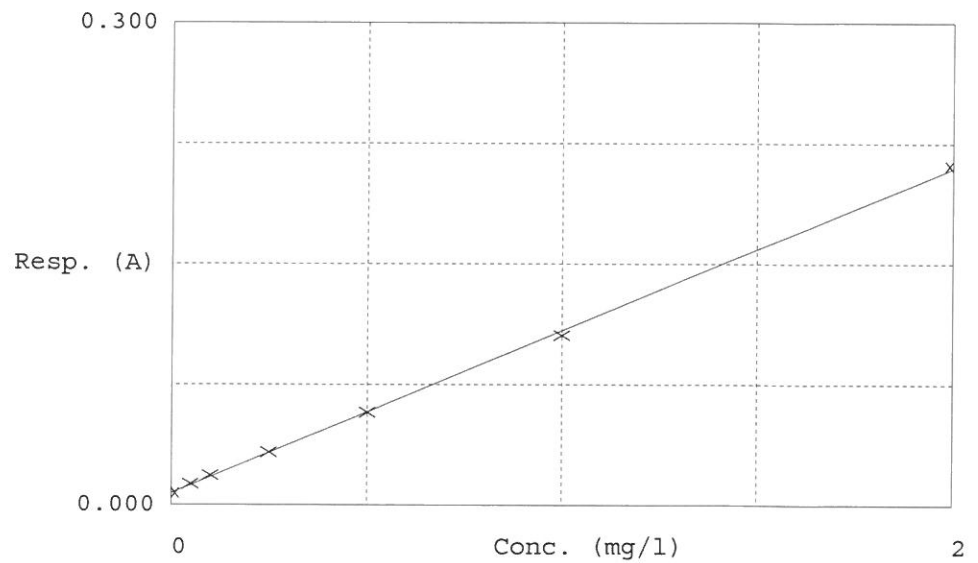

Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	-0.0010	0.0000	-
2	Phenol-2	0.0575	0.0500	15.0
3	Phenol-2	0.1093	0.1000	9.3
4	Phenol-2	0.2522	0.2500	0.9
5	Phenol-2	0.4969	0.5000	-0.6
6	Phenol-2	0.9706	1.0000	-2.9
7	Phenol-2	2.0146	2.0000	0.7

12 3/21/22