

L13119266

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

3/21/2022 13:42

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.978	0.0	0.106	
ICB1	-0.020	0.0	0.005	
CCV1	0.996	0.0	0.108	
CCB1	-0.017	0.0	0.006	
PB143493BL	-0.016	0.0	0.006	
PB143493BS	0.991	0.0	0.108	
N1996-01	0.038	0.0	0.011	
N1996-01DUP	0.038	0.0	0.011	
N1996-01MS	1.102	0.0	0.119	
N1996-01MSD	1.115	0.0	0.120	
CCV2	0.990	0.0	0.108	
CCB2	-0.019	0.0	0.005	

N	12
Mean	0.515
SD	0.5388
CV%	104.71

Aquakem v. 7.2AQ1

Results from time period:

Mon Mar 21 13:18:20 2022

Mon Mar 21 13:39:20 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0	mg/l	3/21/2022 10:15:16	
0.05PPM	A	Phenolics-	P	0.0575	mg/l	3/21/2022 10:15:17	
0.1PPM	A	Phenolics-	P	0.1093	mg/l	3/21/2022 10:15:18	
0.25PPM	A	Phenolics-	P	0.2522	mg/l	3/21/2022 10:15:19	
0.50PPM	A	Phenolics-	P	0.4969	mg/l	3/21/2022 10:15:20	
1.0PPM	A	Phenolics-	P	0.9706	mg/l	3/21/2022 10:15:21	
2.0PPM	A	Phenolics-	P	2.0146	mg/l	3/21/2022 10:15:22	
ICV1	S	Phenolics-	P	0.978	mg/l	3/21/2022 13:18:21	
ICB1	S	Phenolics-	P	-0.02	mg/l	3/21/2022 13:18:23	
CCV1	S	Phenolics-	P	0.9956	mg/l	3/21/2022 13:18:25	
CCB1	S	Phenolics-	P	-0.017	mg/l	3/21/2022 13:18:26	
PB143493BL	S	Phenolics-	P	-0.0164	mg/l	3/21/2022 13:18:29	
PB143493BS	S	Phenolics-	P	0.9912	mg/l	3/21/2022 13:18:30	
N1996-01	S	Phenolics-	P	0.0384	mg/l	3/21/2022 13:39:13	
N1996-01DUP	S	Phenolics-	P	0.0379	mg/l	3/21/2022 13:39:14	
N1996-01MS	S	Phenolics-	P	1.1016	mg/l	3/21/2022 13:39:15	
N1996-01MSD	S	Phenolics-	P	1.1153	mg/l	3/21/2022 13:39:16	
CCV2	S	Phenolics-	P	0.9897	mg/l	3/21/2022 13:39:17	
CCB2	S	Phenolics-	P	-0.0193	mg/l	3/21/2022 13:39:19	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

3/21/2022 10:18

Test Phenolics-


Accepted 3/21/2022 10:18

Factor 9.891

Bias 0.007

Coeff. of det. 0.999608

Errors

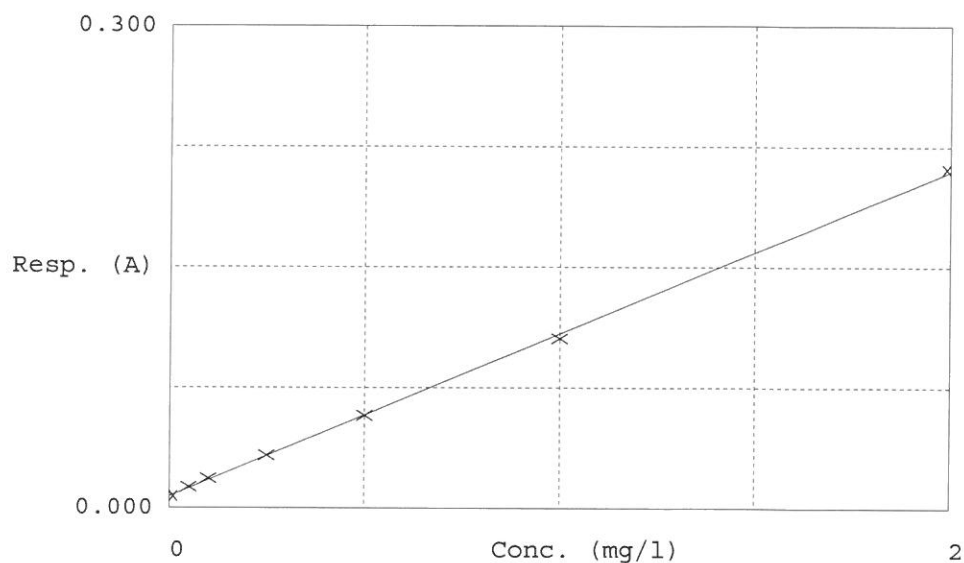

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.007	-0.0010	0.0000	-
2	Phenol-2	0.013	0.0575	0.0500	15.0
3	Phenol-2	0.018	0.1093	0.1000	9.3
4	Phenol-2	0.033	0.2522	0.2500	0.9
5	Phenol-2	0.058	0.4969	0.5000	-0.6
6	Phenol-2	0.106	0.9706	1.0000	-2.9
7	Phenol-2	0.211	2.0146	2.0000	0.7

12 3/21/22