


LB119289

7471B

INSTRUMENT ID: CV4

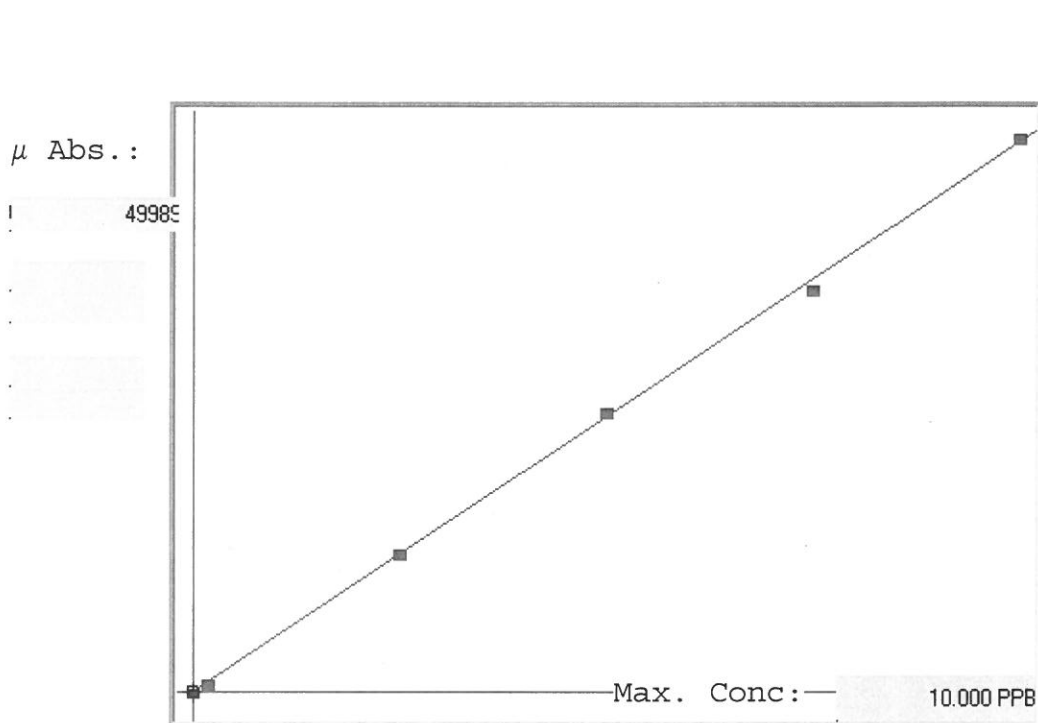

Linear

A= 0.0000e+000

B= 2.0126e-004

C= 1.2126e-003

Rho= 0.9997256

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.007	0.007	28	0.000	28					
0.2	0.200	0.172	-0.028	849	0.0 %	849					-14
2.5	2.500	2.515	0.015	12492	0.0 %	12492					1
5.0	5.000	5.110	0.110	25385	0.0 %	25385					2
7.5	7.500	7.333	-0.167	36431	0.0 %	36431					-2
10.0	10.000	10.062	0.062	49989	0.0 %	49989					1

LB119289 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 22 Mar 2022 15:29:42

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	28	-	0.0000	7471B	PPB	22 Mar 2022 15:31:59	S	Std
0.2 - 1	50.2	849	-	0.2000	7471B	PPB	22 Mar 2022 15:34:16	S	Std
2.5 - 1	52.5	12492	-	2.5000	7471B	PPB	22 Mar 2022 15:36:33	S	Std
5.0 - 1	55	25385	-	5.0000	7471B	PPB	22 Mar 2022 15:38:50	S	Std
7.5 - 1	57.5	36431	-	7.5000	7471B	PPB	22 Mar 2022 15:41:09	S	Std
10.0 - 1	510	49989	-	10.0000	7471B	PPB	22 Mar 2022 15:46:13	S	Std
ICV40 - 1	ICV40	20327	4.0923	-	7471B	PPB	22 Mar 2022 15:48:52	U	SMPL
ICB40 - 1	ICB40	-99	-0.0187	-	7471B	PPB	22 Mar 2022 15:51:08	U	SMPL
CCV97 - 1	CCV97	25597	5.1529	-	7471B	PPB	22 Mar 2022 15:53:26	U	SMPL
CCB97 - 1	CCB97	-131	-0.0252	-	7471B	PPB	22 Mar 2022 15:55:41	U	SMPL
CRA - 1	CRA	874	0.1771	-	7471B	PPB	22 Mar 2022 15:58:00	U	SMPL
HighStd - 1	HighStd	50636	10.1923	-	7471B	PPB	22 Mar 2022 16:00:15	U	SMPL
ChkStd - 1	ChkStd	34311	6.9067	-	7471B	PPB	22 Mar 2022 16:02:31	U	SMPL
PB143506BL - 1	PBS	-184	-0.0358	-	7471B	PPB	22 Mar 2022 16:04:53	U	SMPL
PB143506BS - 1	LCSS	20339	4.0947	-	7471B	PPB	22 Mar 2022 16:10:06	U	SMPL
N2021-03 - 1	MHQ-SP	4087	0.8238	-	7471B	PPB	22 Mar 2022 16:12:22	U	SMPL
N2027-01 - 1	NB-08-031822	391	0.0799	-	7471B	PPB	22 Mar 2022 16:14:41	U	SMPL
N2027-01DUP - 1	NB-08-031822DUP	454	0.0926	-	7471B	PPB	22 Mar 2022 16:19:42	U	SMPL
N2027-01MS - 1	NB-08-031822MS	21316	4.2913	-	7471B	PPB	22 Mar 2022 16:21:59	U	SMPL
N2027-01MSD - 1	NB-08-031822MSD	20172	4.0611	-	7471B	PPB	22 Mar 2022 16:24:15	U	SMPL
CCV98 - 1	CCV98	25678	5.1692	-	7471B	PPB	22 Mar 2022 16:26:34	U	SMPL
CCB98 - 1	CCB98	-169	-0.0328	-	7471B	PPB	22 Mar 2022 16:28:53	U	SMPL
N2030-01 - 1	MR-1	846	0.1715	-	7471B	PPB	22 Mar 2022 16:31:11	U	SMPL
N2031-02 - 1	CMP-B1-031822-0-2	2380	0.4802	-	7471B	PPB	22 Mar 2022 16:33:27	U	SMPL
N2031-04 - 1	CMP-B1-031822-2-5	1944	0.3925	-	7471B	PPB	22 Mar 2022 16:35:43	U	SMPL
N2031-06 - 1	CMP-B1-031822-0-2-BD	3082	0.6215	-	7471B	PPB	22 Mar 2022 16:37:59	U	SMPL
N2031-10 - 1	CMP-B3-031822-0-6	28866	5.8108	-	7471B	PPB	22 Mar 2022 16:40:15	U	SMPL
N2031-12 - 1	CMP-B2-031822-0-2	8192	1.6499	-	7471B	PPB	22 Mar 2022 16:42:32	U	SMPL
N2031-14 - 1	CMP-B2-031822-2-5	5684	1.1452	-	7471B	PPB	22 Mar 2022 16:44:51	U	SMPL
N2033-03 - 1	VNJ-237	4337	0.8741	-	7471B	PPB	22 Mar 2022 16:47:10	U	SMPL
N2039-01 - 1	OK-03-031822	1280	0.2588	-	7471B	PPB	22 Mar 2022 16:49:29	U	SMPL
N2053-01 - 1	AUD-1285	2932	0.5913	-	7471B	PPB	22 Mar 2022 16:51:45	U	SMPL
CCV99 - 1	CCV99	25892	5.2123	-	7471B	PPB	22 Mar 2022 16:54:01	U	SMPL
CCB99 - 1	CCB99	-124	-0.0237	-	7471B	PPB	22 Mar 2022 16:56:17	U	SMPL
N2053-02 - 1	AUD-1286	2937	0.5923	-	7471B	PPB	22 Mar 2022 16:58:36	U	SMPL
N2058-01 - 1	VR-TP1	331	0.0678	-	7471B	PPB	22 Mar 2022 17:00:52	U	SMPL
N2027-01LX5 - 1		117	0.0248	-	7471B	PPB	22 Mar 2022 17:03:08	U	SMPL
N2027-01A - 1		20967	4.2211	-	7471B	PPB	22 Mar 2022 17:05:24	U	SMPL
CCV01 - 1	CCV01	25785	5.1907	-	7471B	PPB	22 Mar 2022 17:07:40	U	SMPL
CCB01 - 1	CCB01	-123	-0.0235	-	7471B	PPB	22 Mar 2022 17:09:59	U	SMPL