

LB119301

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

3/23/2022 10:19

Test: ^{Positive}~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.233	0.0	0.082	
ICB1	-0.830	0.0	0.001	
CCV1	240.540	0.0	0.200	
CCB1	-0.558	0.0	0.001	
PB143526BL	-0.974	0.0	0.001	
N2010-02	-0.931	0.0	0.001	
N2010-02DUP	-0.600	0.0	0.001	
N2025-01	-0.846	0.0	0.001	
N2058-02	-0.814	0.0	0.001	
N2060-01	-0.807	0.0	0.001	
CCV2	249.470	0.0	0.208	
CCB2	-0.604	0.0	0.001	

N	12
Mean	48.357
SD	96.0561
CV%	198.64

Aquakem v. 7.2AQ1

Results from time period:

Wed Mar 23 09:09:50 2022

Wed Mar 23 10:18:12 2022

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	Reactive CN	P	-0.6988	µg/l	3/23/2022 9:48:34
5.OPPBCN	A	Reactive CN	P	4.0722	µg/l	3/23/2022 9:48:35
10PPBCN	A	Reactive CN	P	9.2803	µg/l	3/23/2022 9:48:36
50PPBCN	A	Reactive CN	P	49.9541	µg/l	3/23/2022 9:48:37
100PPBCN	A	Reactive CN	P	102.6058	µg/l	3/23/2022 9:48:38
250PPBCN	A	Reactive CN	P	250.5587	µg/l	3/23/2022 9:48:39
500PPBCN	A	Reactive CN	P	499.2278	µg/l	3/23/2022 9:48:40
ICV1	S	Reactive CN	P	97.2327	µg/l	3/23/2022 10:12:24
ICB1	S	Reactive CN	P	-0.8304	µg/l	3/23/2022 10:12:26
CCV1	S	Reactive CN	P	240.5403	µg/l	3/23/2022 10:12:28
CCB1	S	Reactive CN	P	-0.5576	µg/l	3/23/2022 10:12:29
PB143526BL	S	Reactive CN	P	-0.974	µg/l	3/23/2022 10:12:31
N2010-02	S	Reactive CN	P	-0.9314	µg/l	3/23/2022 10:12:33
N2010-02DUP	S	Reactive CN	P	-0.5998	µg/l	3/23/2022 10:18:06
N2025-01	S	Reactive CN	P	-0.846	µg/l	3/23/2022 10:18:07
N2058-02	S	Reactive CN	P	-0.8138	µg/l	3/23/2022 10:18:08
N2060-01	S	Reactive CN	P	-0.8068	µg/l	3/23/2022 10:18:09
CCV2	S	Reactive CN	P	249.4704	µg/l	3/23/2022 10:18:11
CCB2	S	Reactive CN	P	-0.6042	µg/l	3/23/2022 10:18:12

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

3/23/2022 9:49


Test Total CN

Accepted 3/23/2022 9:49

Factor 1211
Bias 0.001

Coeff. of det. 0.999953

Errors

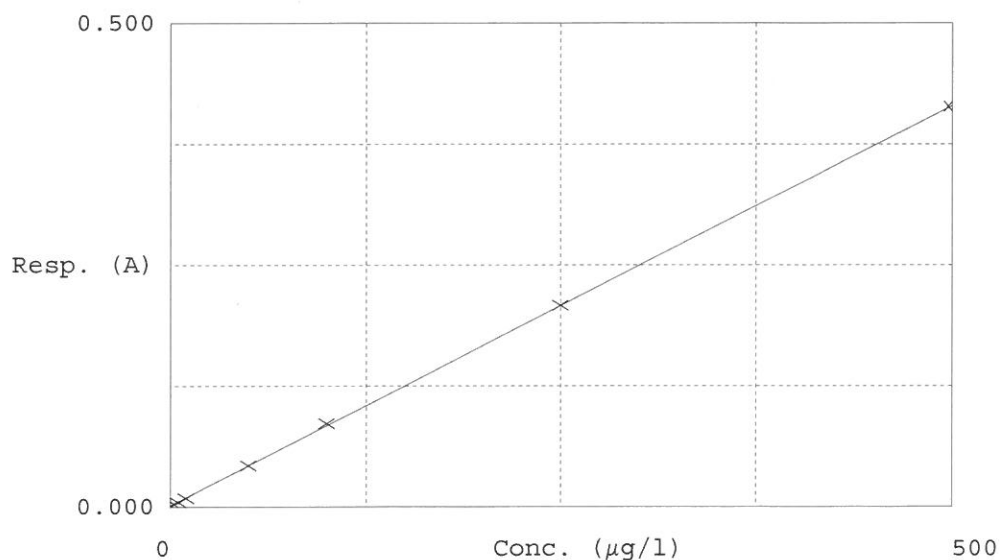

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.6988	0.0000	-
2	5.0PPBCN	0.005	4.0722	5.0000	-18.6
3	10PPBCN	0.009	9.2803	10.0000	-7.2
4	50PPBCN	0.043	49.9541	50.0000	-0.1
5	100PPBCN	0.086	102.6058	100.0000	2.6
6	250PPBCN	0.208	250.5587	250.0000	0.2
7	500PPBCN	0.414	499.2278	500.0000	-0.2

12 3/23/22