


LAB 119323

7470A

INSTRUMENT ID: CV1

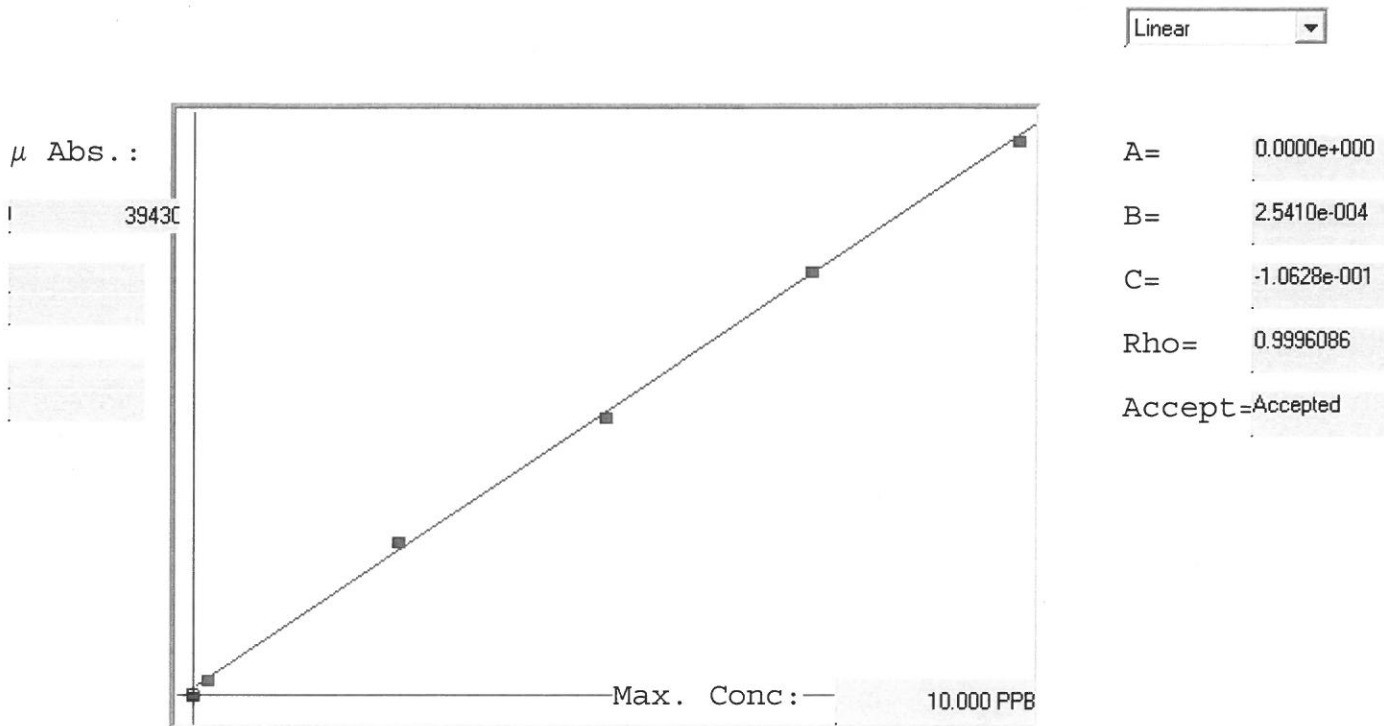

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.102	-0.102	17	0.000	17					
0.2	0.200	0.177	-0.023	1116	0.0 %	1116					-12
2.5	2.500	2.685	0.185	10986	0.0 %	10986					7
5.0	5.000	4.940	-0.060	19860	0.0 %	19860					-1
7.5	7.500	7.587	0.087	30276	0.0 %	30276					1
10.0	10.000	9.913	-0.087	39430	0.0 %	39430					-1

LB119323 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 24 Mar 2022 10:20:11					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SP	17	-	0.0000	7470A	PPB	24 Mar 2022 10:23:42	S	Std
0.2 - 1	SP-2	1116	-	0.2000	7470A	PPB	24 Mar 2022 10:25:59	S	Std
2.5 - 1	SP-5	10986	-	2.5000	7470A	PPB	24 Mar 2022 10:31:02	S	Std
5.0 - 1	SP	19860	-	5.0000	7470A	PPB	24 Mar 2022 10:33:19	S	Std
7.5 - 1	SP-5	30276	-	7.5000	7470A	PPB	24 Mar 2022 10:38:07	S	Std
10.0 - 1	SP	39430	-	10.0000	7470A	PPB	24 Mar 2022 10:40:23	S	Std
ICV43 - 1	ICV43	15087	3.7273	-7470A	PPB	PPB	24 Mar 2022 10:43:11	U	SMPL
ICB43 - 1	ICB43	527	0.0276	-7470A	PPB	PPB	24 Mar 2022 10:47:55	U	SMPL
CCV09 - 1	CCV09	19916	4.9543	-7470A	PPB	PPB	24 Mar 2022 10:50:10	U	SMPL
CCB09 - 1	CCB09	153	-0.0674	-7470A	PPB	PPB	24 Mar 2022 10:52:26	U	SMPL
CRA - 1	CRA	1100	0.1732	-7470A	PPB	PPB	24 Mar 2022 10:54:42	U	SMPL
HighStd - 1	HighStd	39166	9.8456	-7470A	PPB	PPB	24 Mar 2022 10:56:57	U	SMPL
ChkStd - 1	ChkStd	27909	6.9853	-7470A	PPB	PPB	24 Mar 2022 11:01:43	U	SMPL
PB143547BL - 1	PBW	605	0.0474	-7470A	PPB	PPB	24 Mar 2022 11:03:59	U	SMPL
PB143547BS - 1	LCSW	15037	3.7146	-7470A	PPB	PPB	24 Mar 2022 11:08:49	U	SMPL
N2058-02 - 1	MHA	408	-0.0026	-7470A	PPB	PPB	24 Mar 2022 11:11:05	U	SMPL
N2058-02DUP - 1	MHADUP	494	0.0192	-7470A	PPB	PPB	24 Mar 2022 11:13:23	U	SMPL
N2058-02MS - 1	MHAMS	16623	4.1175	-7470A	PPB	PPB	24 Mar 2022 11:15:40	U	SMPL
N2058-02MSD - 1	MHAMSD	16738	4.1468	-7470A	PPB	PPB	24 Mar 2022 11:17:57	U	SMPL
PB143575BL - 1	PBW	248	-0.0433	-7470A	PPB	PPB	24 Mar 2022 11:20:13	U	SMPL
CCV10 - 1	CCV10	19679	4.8941	-7470A	PPB	PPB	24 Mar 2022 11:22:28	U	SMPL
CCB10 - 1	CCB10	209	-0.0532	-7470A	PPB	PPB	24 Mar 2022 11:24:44	U	SMPL
PB143575BS - 1	LCSW	15703	3.8838	-7470A	PPB	PPB	24 Mar 2022 11:29:29	U	SMPL
N2076-01 - 1	WC-20220322	490	0.0182	-7470A	PPB	PPB	24 Mar 2022 11:31:44	U	SMPL
N2076-01DUP - 1	WC-20220322DUP	536	0.0299	-7470A	PPB	PPB	24 Mar 2022 11:34:00	U	SMPL
N2076-01MS - 1	WC-20220322MS	16490	4.0838	-7470A	PPB	PPB	24 Mar 2022 11:36:16	U	SMPL
N2076-01MSD - 1	WC-20220322MSD	16454	4.0746	-7470A	PPB	PPB	24 Mar 2022 11:38:31	U	SMPL
PB143528TB - 1	PB143528TB	668	0.0635	-7470A	PPB	PPB	24 Mar 2022 11:40:48	U	SMPL
PB143554TB - 1	PB143554TB	298	-0.0306	-7470A	PPB	PPB	24 Mar 2022 11:47:41	U	SMPL
CCV11 - 1	CCV11	19771	4.9174	-7470A	PPB	PPB	24 Mar 2022 11:49:58	U	SMPL
CCB11 - 1	CCB11	198	-0.0560	-7470A	PPB	PPB	24 Mar 2022 11:52:15	U	SMPL
N2058-02LX5 - 1		76	-0.0870	-7470A	PPB	PPB	24 Mar 2022 11:54:32	U	SMPL
N2058-02A - 1		15046	3.7168	-7470A	PPB	PPB	24 Mar 2022 11:56:48	U	SMPL
N2076-01LX5 - 1		34	-0.0976	-7470A	PPB	PPB	24 Mar 2022 11:59:04	U	SMPL
N2076-01A - 1		15085	3.7267	-7470A	PPB	PPB	24 Mar 2022 12:01:21	U	SMPL
CCV12 - 1	CCV12	19713	4.9027	-7470A	PPB	PPB	24 Mar 2022 12:03:37	U	SMPL
CCB12 - 1	CCB12	206	-0.0539	-7470A	PPB	PPB	24 Mar 2022 12:05:53	U	SMPL