

215 112 328

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

3/24/2022 13:35

Test: Residue
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.480	0.0	0.084	
ICB1	0.449	0.0	0.001	
CCV1	240.343	0.0	0.207	
CCB1	0.455	0.0	0.001	
PB143579BL	0.234	0.0	0.001	
N2077-04	0.184	0.0	0.001	
N2077-04DUP	0.331	0.0	0.001	
N2077-08	0.111	0.0	0.001	
N2077-12	0.247	0.0	0.001	
N2077-16	0.107	0.0	0.001	
N2084-02	0.151	0.0	0.001	
N2091-02	0.091	0.0	0.001	
PB143580BL	0.474	0.0	0.001	
CCV2	240.283	0.0	0.207	
CCB2	0.626	0.0	0.001	
N2076-01	-0.045	0.0	0.001	
N2076-01DUP	0.068	0.0	0.001	
N2085-01	0.276	0.0	0.001	
CCV3	251.426	0.0	0.217	
CCB3	0.193	0.0	0.001	

N	20
Mean	41.624
SD	89.8462
CV%	215.85

Aquakem v. 7.2AQ1

Results from time period:

Thu Mar 24 13:17:59 2022

Thu Mar 24 13:30:25 2022

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.4039	µg/l	3/24/2022 10:24:15	
5.OPPBCN	A	Reactive CN	P	4.7229	µg/l	3/24/2022 10:24:16	
10PPBCN	A	Reactive CN	P	9.6605	µg/l	3/24/2022 10:24:17	
50PPBCN	A	Reactive CN	P	49.7405	µg/l	3/24/2022 10:24:18	
100PPBCN	A	Reactive CN	P	101.698	µg/l	3/24/2022 10:24:19	
250PPBCN	A	Reactive CN	P	248.1566	µg/l	3/24/2022 10:24:20	
500PPBCN	A	Reactive CN	P	500.6176	µg/l	3/24/2022 10:24:21	
ICV1	S	Reactive CN	P	96.4805	µg/l	3/24/2022 13:18:00	
ICB1	S	Reactive CN	P	0.4488	µg/l	3/24/2022 13:18:01	
CCV1	S	Reactive CN	P	240.3431	µg/l	3/24/2022 13:18:04	
CCB1	S	Reactive CN	P	0.4548	µg/l	3/24/2022 13:18:05	
PB143579BL	S	Reactive CN	P	0.2344	µg/l	3/24/2022 13:18:07	
N2077-04	S	Reactive CN	P	0.1844	µg/l	3/24/2022 13:18:09	
N2077-04DUP	S	Reactive CN	P	0.3308	µg/l	3/24/2022 13:25:34	
N2077-08	S	Reactive CN	P	0.1113	µg/l	3/24/2022 13:25:35	
N2077-12	S	Reactive CN	P	0.2471	µg/l	3/24/2022 13:25:36	
N2077-16	S	Reactive CN	P	0.1073	µg/l	3/24/2022 13:25:37	
N2084-02	S	Reactive CN	P	0.1506	µg/l	3/24/2022 13:25:38	
N2091-02	S	Reactive CN	P	0.0914	µg/l	3/24/2022 13:25:39	
PB143580BL	S	Reactive CN	P	0.474	µg/l	3/24/2022 13:25:40	
CCV2	S	Reactive CN	P	240.283	µg/l	3/24/2022 13:25:43	
CCB2	S	Reactive CN	P	0.6256	µg/l	3/24/2022 13:25:44	
N2076-01	S	Reactive CN	P	-0.0451	µg/l	3/24/2022 13:30:21	
N2076-01DUP	S	Reactive CN	P	0.0676	µg/l	3/24/2022 13:30:22	
N2085-01	S	Reactive CN	P	0.2755	µg/l	3/24/2022 13:30:23	
CCV3	S	Reactive CN	P	251.4262	µg/l	3/24/2022 13:30:24	
CCB3	S	Reactive CN	P	0.1928	µg/l	3/24/2022 13:30:25	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

3/24/2022 10:26


Test Total CN

Accepted 3/24/2022 10:26

Factor 1164
Bias 0.001

Coeff. of det. 0.999966

Errors

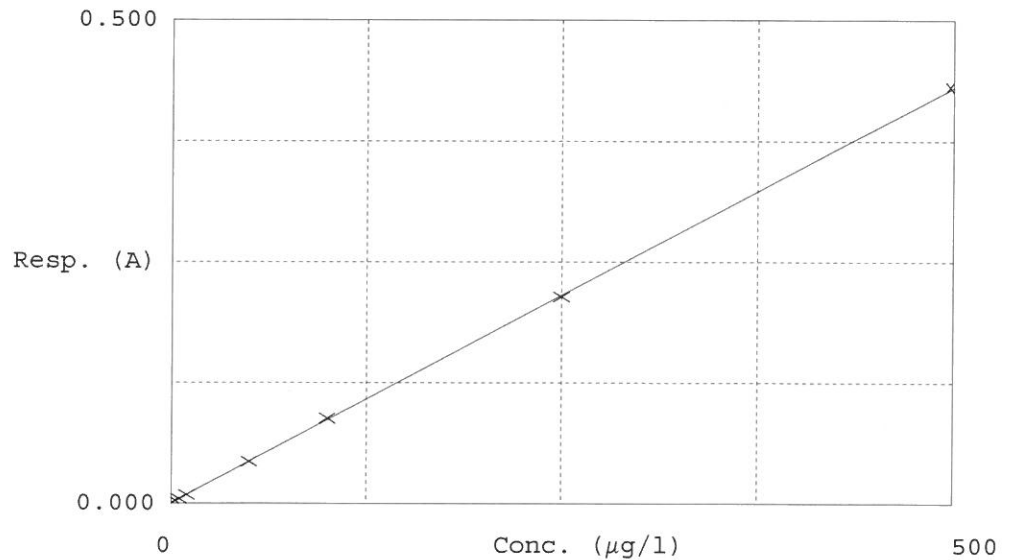

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.4039	0.0000	-
2	5.0PPBCN	0.005	4.7229	5.0000	-5.5
3	10PPBCN	0.009	9.6605	10.0000	-3.6
4	50PPBCN	0.044	49.7405	50.0000	-0.5
5	100PPBCN	0.088	101.6980	100.0000	1.7
6	250PPBCN	0.214	248.1566	250.0000	-0.7
7	500PPBCN	0.431	500.6176	500.0000	0.1

12 3/24/22