

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

3/31/2022 13:50

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.001	0.0	0.105	
ICB1	-0.001	0.0	0.007	
CCV1	1.036	0.0	0.108	
CCB1	-0.005	0.0	0.006	
PB143769BL	-0.007	0.0	0.006	
PB143769BS	1.008	0.0	0.106	
N1873-27	1.997	0.0	0.203	
DOC-1	1.018	0.0	0.107	
DOC-2	1.010	0.0	0.106	
DOC-3	1.009	0.0	0.106	
DOC-4	1.012	0.0	0.106	
CCV2	1.037	0.0	0.108	
CCB2	-0.005	0.0	0.006	

N	13
Mean	0.778
SD	0.6049
CV%	77.77

Aquakem v. 7.2AQ1

Results from time period:

Thu Mar 31 12:38:28 2022

Thu Mar 31 13:47:45 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.008	mg/l	3/31/2022 12:38:28	
0.05PPM	A	Phenolics-	P	0.0543	mg/l	3/31/2022 12:38:29	
0.1PPM	A	Phenolics-	P	0.1049	mg/l	3/31/2022 12:38:30	
0.25PPM	A	Phenolics-	P	0.2488	mg/l	3/31/2022 12:38:31	
0.50PPM	A	Phenolics-	P	0.5099	mg/l	3/31/2022 12:38:32	
1.0PPM	A	Phenolics-	P	0.9853	mg/l	3/31/2022 12:38:33	
2.0PPM	A	Phenolics-	P	2.0047	mg/l	3/31/2022 12:38:34	
ICV1	S	Phenolics-	P	1.0011	mg/l	3/31/2022 13:14:47	
ICB1	S	Phenolics-	P	-0.0014	mg/l	3/31/2022 13:14:49	
CCV1	S	Phenolics-	P	1.0359	mg/l	3/31/2022 13:14:51	
CCB1	S	Phenolics-	P	-0.0049	mg/l	3/31/2022 13:14:53	
PB143769BL	S	Phenolics-	P	-0.0066	mg/l	3/31/2022 13:14:54	
PB143769BS	S	Phenolics-	P	1.0078	mg/l	3/31/2022 13:14:56	
N1873-27	S	Phenolics-	P	1.9973	mg/l	3/31/2022 13:24:50	
DOC-1	S	Phenolics-	P	1.0181	mg/l	3/31/2022 13:24:58	
DOC-2	S	Phenolics-	P	1.0102	mg/l	3/31/2022 13:41:51	
DOC-3	S	Phenolics-	P	1.0092	mg/l	3/31/2022 13:41:52	
DOC-4	S	Phenolics-	P	1.0122	mg/l	3/31/2022 13:47:40	
CCV2	S	Phenolics-	P	1.0375	mg/l	3/31/2022 13:47:43	
CCB2	S	Phenolics-	P	-0.0046	mg/l	3/31/2022 13:47:44	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

3/31/2022 12:43


Test Phenolics-

Accepted 3/31/2022 12:43

Factor 10.2
Bias 0.007

Coeff. of det. 0.999859

Errors

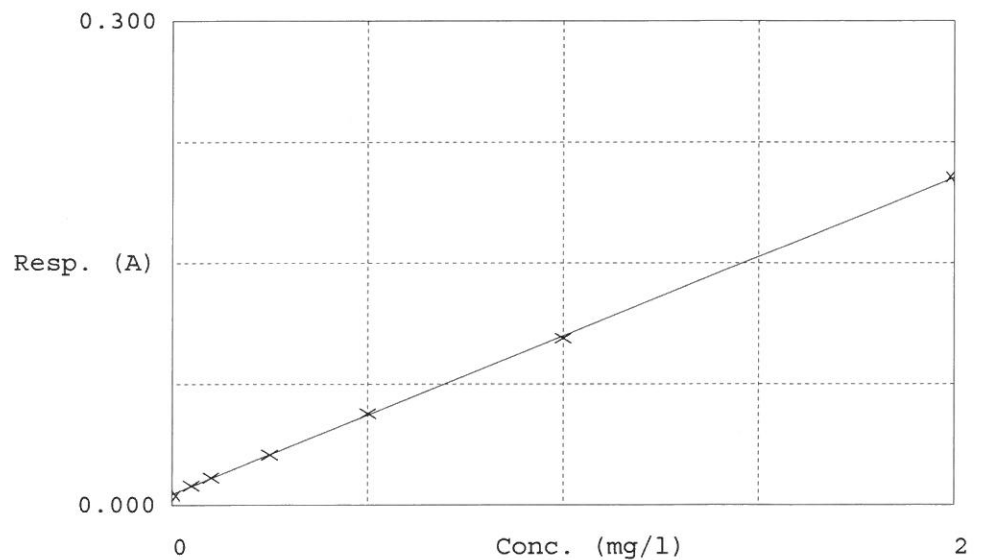

	Calibrator	Response	Calc. con.	Conc.	<u>Errors</u>
1	0.00PPM	0.006	-0.0080	0.0000	-
2	Phenol-2	0.012	0.0543	0.0500	8.6
3	Phenol-2	0.017	0.1049	0.1000	4.9
4	Phenol-2	0.031	0.2488	0.2500	-0.5
5	Phenol-2	0.057	0.5099	0.5000	2.0
6	Phenol-2	0.103	0.9853	1.0000	-1.5
7	Phenol-2	0.203	2.0047	2.0000	0.2

12 3/31/22