


LB11951A (LB119511)

7471B

INSTRUMENT ID: CV1

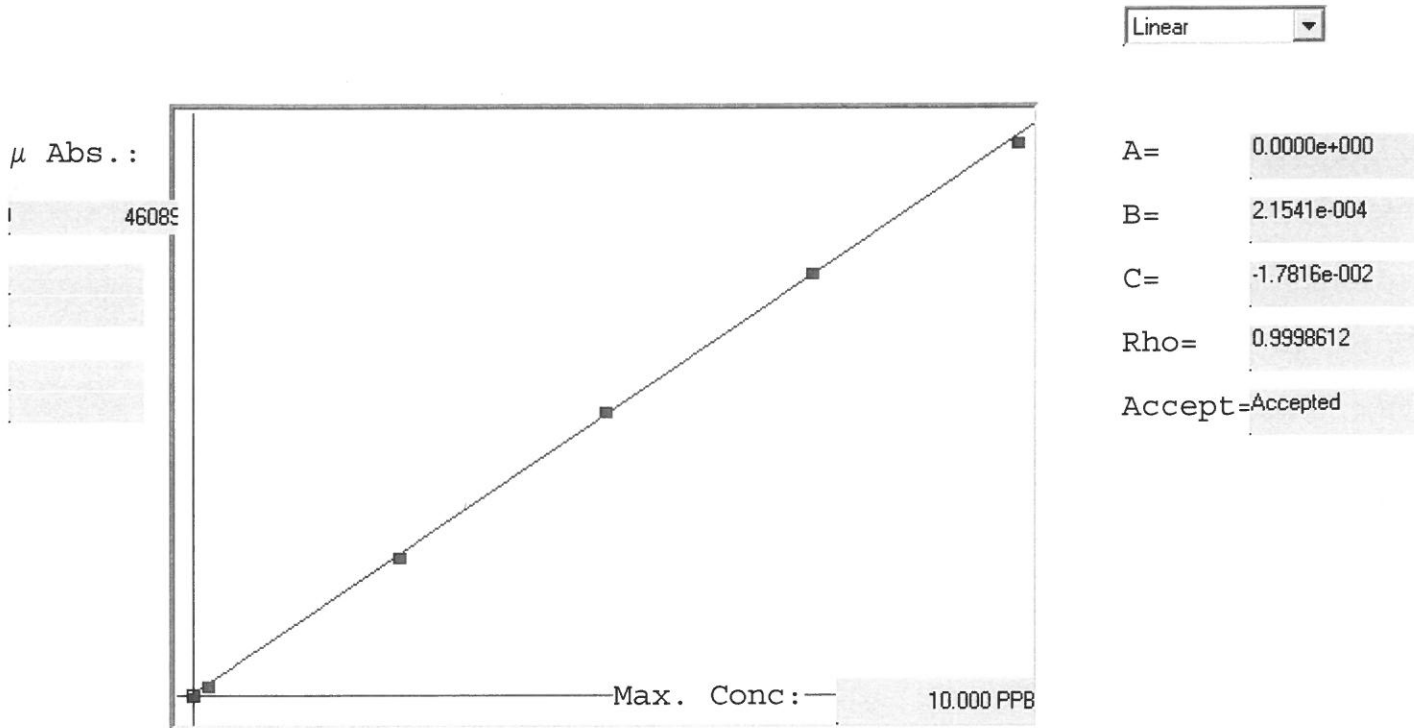

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.020	-0.020	-11	0.000	-11					-10
0.2	0.200	0.181	-0.019	922	0.0 %	922					-1
2.5	2.500	2.471	-0.029	11553	0.0 %	11553					2
5.0	5.000	5.094	0.094	23732	0.0 %	23732					1
7.5	7.500	7.564	0.064	35197	0.0 %	35197					-1
10.0	10.000	9.910	-0.090	46089	0.0 %	46089					

LB119511 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 04 Apr 2022 13:29:49					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-11	-	0.00007471B	PPB		04 Apr 2022 13:36:37	S	Std
0.2 - 1	50.2	922	-	0.20007471B	PPB		04 Apr 2022 13:38:54	S	Std
2.5 - 1	52.1	11553	-	2.50007471B	PPB		04 Apr 2022 13:41:11	S	Std
5.0 - 1	55	23732	-	5.00007471B	PPB		04 Apr 2022 13:43:28	S	Std
7.5 - 1	57.5	35197	-	7.50007471B	PPB		04 Apr 2022 13:45:46	S	Std
10.0 - 1	510	46089	-	10.00007471B	PPB		04 Apr 2022 13:50:52	S	Std
ICV59 - 1	ICV59	17773	3.8107	-7471B	PPB		04 Apr 2022 13:53:35	U	SMPL
ICB59 - 1	ICB59	84	0.0003	-7471B	PPB		04 Apr 2022 14:09:20	U	SMPL
CCV79 - 1	CCV79	23769	5.1023	-7471B	PPB		04 Apr 2022 14:11:35	U	SMPL
CCB79 - 1	CCB79	-257	-0.0732	-7471B	PPB		04 Apr 2022 14:13:51	U	SMPL
CRA - 1	CRA	852	0.1657	-7471B	PPB		04 Apr 2022 14:16:08	U	SMPL
HighStd - 1	HighStd	44839	9.6410	-7471B	PPB		04 Apr 2022 14:18:23	U	SMPL
ChkStd - 1	ChkStd	35190	7.5625	-7471B	PPB		04 Apr 2022 14:20:39	U	SMPL
PB143849BL - 1	PBS	-36	-0.0256	-7471B	PPB		04 Apr 2022 14:25:49	U	SMPL
PB143849BS - 1	LCSS	17000	3.6442	-7471B	PPB		04 Apr 2022 14:28:04	U	SMPL
N2207-01 - 1	20220340-096-21-01	1857	0.3822	-7471B	PPB		04 Apr 2022 14:30:21	U	SMPL
N2207-02 - 1	20220341-096-21-02	15572	3.3366	-7471B	PPB		04 Apr 2022 14:32:40	U	SMPL
N2207-03 - 1	20220342-096-21-03	16627	3.5638	-7471B	PPB		04 Apr 2022 14:34:58	U	SMPL
N2207-04 - 1	20220343-098-21-01	4200	0.8869	-7471B	PPB		04 Apr 2022 14:37:18	U	SMPL
N2207-05 - 1	20220349-AMENDED-096-21-01	883	0.1724	-7471B	PPB		04 Apr 2022 14:39:37	U	SMPL
CCV80 - 1	CCV80	23655	5.0777	-7471B	PPB		04 Apr 2022 14:41:53	U	SMPL
CCB80 - 1	CCB80	-105	-0.0404	-7471B	PPB		04 Apr 2022 14:44:09	U	SMPL
N2207-06 - 1	20220350-AMENDED-096-21-02	12065	2.5811	-7471B	PPB		04 Apr 2022 14:46:27	U	SMPL
N2207-07 - 1	20220351-AMENDED-096-21-03	9713	2.0745	-7471B	PPB		04 Apr 2022 14:48:42	U	SMPL
N2207-08 - 1	20220352-AMENDED-098-21-01	3593	0.7562	-7471B	PPB		04 Apr 2022 14:50:59	U	SMPL
N2215-01 - 1	COMP-1	604	0.1123	-7471B	PPB		04 Apr 2022 14:53:17	U	SMPL
N2215-02 - 1	COMP-2	1102	0.2196	-7471B	PPB		04 Apr 2022 14:55:35	U	SMPL
N2219-01 - 1	TP-3	900	0.1761	-7471B	PPB		04 Apr 2022 14:57:52	U	SMPL
N2219-01DUP - 1	TP-3DUP	832	0.1614	-7471B	PPB		04 Apr 2022 15:00:08	U	SMPL
N2219-01MS - 1	TP-3MS	18256	3.9147	-7471B	PPB		04 Apr 2022 15:02:25	U	SMPL
N2219-01MSD - 1	TP-3MSD	17404	3.7312	-7471B	PPB		04 Apr 2022 15:07:18	U	SMPL
PB143853BL - 1	PBS	6	-0.0165	-7471B	PPB		04 Apr 2022 15:09:33	U	SMPL
CCV81 - 1	CCV81	21894	4.6984	-7471B	PPB		04 Apr 2022 15:11:52	U	SMPL
CCB81 - 1	CCB81	-131	-0.0460	-7471B	PPB		04 Apr 2022 15:14:07	U	SMPL
PB143853BS - 1	LCSS	15962	3.4206	-7471B	PPB		04 Apr 2022 15:16:26	U	SMPL
N2220-01 - 1	A10015	12343	2.6410	-7471B	PPB		04 Apr 2022 15:18:42	U	SMPL
N2220-02 - 1	A10095	-64	-0.0316	-7471B	PPB		04 Apr 2022 15:21:00	U	SMPL
N2220-03 - 1	A11015	1872	0.3854	-7471B	PPB		04 Apr 2022 15:23:22	U	SMPL
N2220-04 - 1	A11105	4547	0.9617	-7471B	PPB		04 Apr 2022 15:25:52	U	SMPL
N2220-05 - 1	A03015	1262	0.2540	-7471B	PPB		04 Apr 2022 15:28:08	U	SMPL
N2220-06 - 1	A03140	1771	0.3637	-7471B	PPB		04 Apr 2022 15:29:25	U	SMPL
N2220-07 - 1	A02015	722	0.1377	-7471B	PPB		04 Apr 2022 15:29:42	U	SMPL
N2220-08 - 1	DUP0331	12550	2.6856	-7471B	PPB		04 Apr 2022 16:01:59	U	SMPL
N2220-09 - 1	A02145	1247	0.2508	-7471B	PPB		04 Apr 2022 16:04:14	U	SMPL
CCV82 - 1	CCV82	22961	4.9282	-7471B	PPB		04 Apr 2022 16:09:16	U	SMPL
CCB82 - 1	CCB82	-242	-0.0699	-7471B	PPB		04 Apr 2022 16:11:31	U	SMPL
N2220-10 - 1	A04015	1603	0.3275	-7471B	PPB		04 Apr 2022 16:13:49	U	SMPL
N2220-11 - 1	A04100	770	0.1481	-7471B	PPB		04 Apr 2022 16:16:06	U	SMPL
N2220-11DUP - 1	A04100DUP	836	0.1623	-7471B	PPB		04 Apr 2022 16:18:22	U	SMPL
N2220-11MS - 1	A04100MS	21549	4.6241	-7471B	PPB		04 Apr 2022 16:31:01	U	SMPL
N2220-11MSD - 1	A04100MSD	20367	4.3695	-7471B	PPB		04 Apr 2022 16:33:16	U	SMPL
N2220-12 - 1	A05015	31079	6.6769	-7471B	PPB		04 Apr 2022 16:35:36	U	SMPL
N2220-13 - 1	A05140	17744	3.8044	-7471B	PPB		04 Apr 2022 16:37:57	U	SMPL
N2220-14 - 1	A06015	19589	4.2019	-7471B	PPB		04 Apr 2022 16:40:20	U	SMPL
N2220-15 - 1	A06135	4272	0.9024	-7471B	PPB		04 Apr 2022 16:42:41	U	SMPL
N2220-16 - 1	A09015	6804	1.4478	-7471B	PPB		04 Apr 2022 16:44:59	U	SMPL
CCV83 - 1	CCV83	23057	4.9489	-7471B	PPB		04 Apr 2022 16:49:57	U	SMPL
CCB83 - 1	CCB83	-271	-0.0762	-7471B	PPB		04 Apr 2022 16:52:14	U	SMPL
N2220-17 - 1	A09145	5852	1.2428	-7471B	PPB		04 Apr 2022 16:54:32	U	SMPL
N2219-01LX5 - 1		8	-0.0161	-7471B	PPB		04 Apr 2022 16:56:48	U	SMPL
N2219-01A - 1		21171	4.5426	-7471B	PPB		04 Apr 2022 16:59:05	U	SMPL
N2220-11LX5 - 1		126	0.0093	-7471B	PPB		04 Apr 2022 17:01:21	U	SMPL
N2220-11A - 1		22168	4.7574	-7471B	PPB		04 Apr 2022 17:03:39	U	SMPL
CCV84 - 1	CCV84	25167	5.4034	-7471B	PPB		04 Apr 2022 17:05:56	U	SMPL
CCB84 - 1	CCB84	-244	-0.0704	-7471B	PPB		04 Apr 2022 17:08:15	U	SMPL