


LB119538

7471B

INSTRUMENT ID: EVA

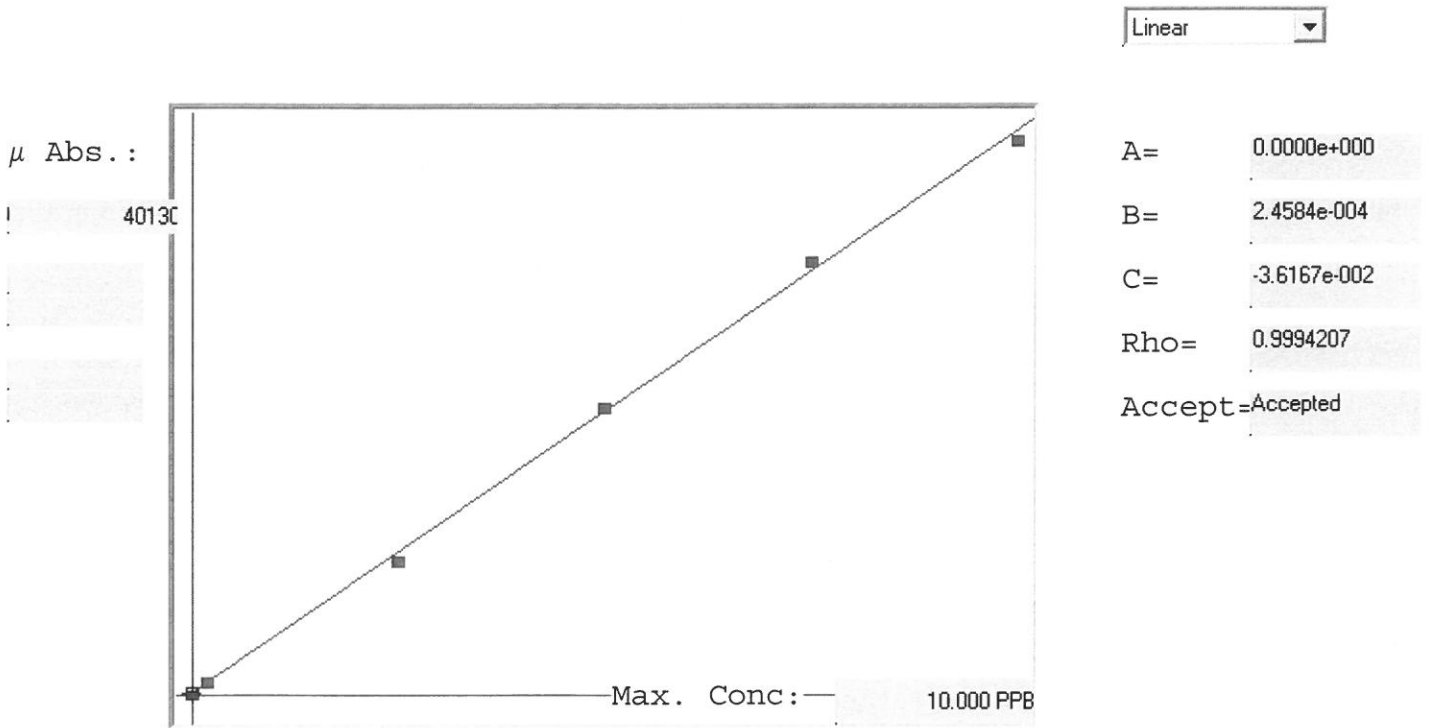

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.001	0.001	153	0.000	153					1
0.2	0.200	0.214	0.014	1017	0.0 %	1017					7
2.5	2.500	2.367	-0.133	9777	0.0 %	9777					-5
5.0	5.000	5.088	0.088	20842	0.0 %	20842					2
7.5	7.500	7.700	0.200	31469	0.0 %	31469					3
10.0	10.000	9.829	-0.171	40130	0.0 %	40130					-2

LB119538 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 05 Apr 2022 16:19:42

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	153	-	0.0000	7471B	PPB	06 Apr 2022 09:36:11	S	Std
0.2 - 1	51.2	1017	-	0.2000	7471B	PPB	06 Apr 2022 09:38:28	S	Std
2.5 - 1	52.5	9777	-	2.5000	7471B	PPB	06 Apr 2022 09:40:45	S	Std
5.0 - 1	55	20842	-	5.0000	7471B	PPB	06 Apr 2022 09:43:02	S	Std
7.5 - 1	59.5	31469	-	7.5000	7471B	PPB	06 Apr 2022 09:45:20	S	Std
10.0 - 1	510	40130	-	10.0000	7471B	PPB	06 Apr 2022 09:52:57	S	Std
ICV64 - 1	ICV64	16486	4.0168	-	7471B	PPB	06 Apr 2022 09:55:45	U	SMPL
ICB64 - 1	ICB64	16	-0.0322	-	7471B	PPB	06 Apr 2022 10:00:58	U	SMPL
CCV92 - 1	CCV92	21974	5.3659	-	7471B	PPB	06 Apr 2022 10:03:12	U	SMPL
CCB92 - 1	CCB92	27	-0.0295	-	7471B	PPB	06 Apr 2022 10:08:04	U	SMPL
CRA - 1	CRA	1193	0.2571	-	7471B	PPB	06 Apr 2022 10:12:50	U	SMPL
HighStd - 1	HighStd	39434	9.6583	-	7471B	PPB	06 Apr 2022 10:15:05	U	SMPL
ChkStd - 1	ChkStd	30912	7.5633	-	7471B	PPB	06 Apr 2022 10:17:20	U	SMPL
N2226-01 - 1	PFS-TP	15289	3.7225	-	7471B	PPB	06 Apr 2022 10:24:23	U	SMPL
N2227-01 - 1	124055	4530	1.0775	-	7471B	PPB	06 Apr 2022 10:26:42	U	SMPL
N2227-03 - 1	124035	2418	0.5583	-	7471B	PPB	06 Apr 2022 10:29:02	U	SMPL
N2229-01 - 1	SOIL-DRUM	2814	0.6556	-	7471B	PPB	06 Apr 2022 10:31:20	U	SMPL
N2237-01 - 1	A08015	2219	0.5094	-	7471B	PPB	06 Apr 2022 10:33:36	U	SMPL
CCV93 - 1	CCV93	21117	5.1553	-	7471B	PPB	06 Apr 2022 10:35:53	U	SMPL
CCB93 - 1	CCB93	223	0.0187	-	7471B	PPB	06 Apr 2022 10:40:47	U	SMPL
N2237-02 - 1	A13015	11093	2.6909	-	7471B	PPB	06 Apr 2022 10:43:02	U	SMPL
N2237-03 - 1	A13145	7437	1.7922	-	7471B	PPB	06 Apr 2022 10:45:17	U	SMPL
N2237-04 - 1	A12015	9795	2.3718	-	7471B	PPB	06 Apr 2022 10:47:34	U	SMPL
N2237-05 - 1	A12040	17294	4.2154	-	7471B	PPB	06 Apr 2022 10:49:52	U	SMPL
N2237-06 - 1	A01015	4026	0.9536	-	7471B	PPB	06 Apr 2022 10:52:09	U	SMPL
N2237-07 - 1	A01040	22628	5.5267	-	7471B	PPB	06 Apr 2022 10:54:28	U	SMPL
N2237-10 - 1	DUP-0401	3965	0.9386	-	7471B	PPB	06 Apr 2022 10:56:45	U	SMPL
N2238-01 - 1	72-11966	948	0.1969	-	7471B	PPB	06 Apr 2022 10:59:04	U	SMPL
N2238-01DUP - 1	72-11966DUP	911	0.1878	-	7471B	PPB	06 Apr 2022 11:01:21	U	SMPL
N2238-01MS - 1	72-11966MS	18367	4.4792	-	7471B	PPB	06 Apr 2022 11:06:17	U	SMPL
CCV94 - 1	CCV94	22346	5.4574	-	7471B	PPB	06 Apr 2022 11:08:32	U	SMPL
CCB94 - 1	CCB94	-208	-0.0873	-	7471B	PPB	06 Apr 2022 11:10:51	U	SMPL
N2238-01MSD - 1	72-11966MSD	16747	4.0809	-	7471B	PPB	06 Apr 2022 11:13:10	U	SMPL
N2239-01 - 1	TP-4	4214	0.9998	-	7471B	PPB	06 Apr 2022 11:15:25	U	SMPL
N2241-01 - 1	CL-02-040122	2880	0.6719	-	7471B	PPB	06 Apr 2022 11:17:44	U	SMPL
N2238-01LX5 - 1		90	-0.0140	-	7471B	PPB	06 Apr 2022 11:20:01	U	SMPL
N2238-01A - 1		17231	4.1999	-	7471B	PPB	06 Apr 2022 11:22:17	U	SMPL
PB143910BL - 1	PBS	-124	-0.0667	-	7471B	PPB	06 Apr 2022 11:26:38	U	SMPL
PB143910BS - 1	LCSS	17396	4.2405	-	7471B	PPB	06 Apr 2022 11:28:57	U	SMPL
CCV95 - 1	CCV95	21931	5.3554	-	7471B	PPB	06 Apr 2022 11:31:15	U	SMPL
CCB95 - 1	CCB95	-121	-0.0659	-	7471B	PPB	06 Apr 2022 11:33:33	U	SMPL