

LB 119568

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

4/7/2022 12:45 Reviewed by : 12 Instrument ID : Konelab

Test: Total CN

Sample Id	^{up/L} Result	Dil. 1 +	Response	Errors
ICV1	94.711	0.0	0.083	
ICB1	1.098	0.0	0.002	
CCV1	248.906	0.0	0.217	
CCB1	0.893	0.0	0.002	
PB143946BL	1.054	0.0	0.002	
PB143946BS	94.501	0.0	0.083	
LOWPB143946	10.523	0.0	0.010	105% (90-110)
HIGHPB143946	495.082	0.0	0.431	99% (90-110)
N2282-01	1.885	0.0	0.003	
N2282-01DUP	1.346	0.0	0.002	
N2282-01MS	41.259	0.0	0.037	12
N2282-01MSD	41.455	0.0	0.037	04/07/22
N2277-01	0.892	0.0	0.002	
CCV2	252.294	0.0	0.220	
CCB2	1.294	0.0	0.002	

N 15
Mean 85.813
SD 141.8495
CV% 165.30

Aquakem v. 7.2AQ1

Results from time period:

Thu Apr 07 11:51:37 2022

Thu Apr 07 12:31:01 2022

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.8747	µg/l	4/7/2022 11:51:37	
5.OPPBCN	A	Total CN	P	4.6965	µg/l	4/7/2022 11:51:38	
10PPBCN	A	Total CN	P	10.6085	µg/l	4/7/2022 11:51:39	
50PPBCN	A	Total CN	P	49.3671	µg/l	4/7/2022 11:51:40	
100PPBCN	A	Total CN	P	98.3328	µg/l	4/7/2022 11:51:41	
250PPBCN	A	Total CN	P	251.4655	µg/l	4/7/2022 11:51:42	
500PPBCN	A	Total CN	P	499.6548	µg/l	4/7/2022 11:51:43	
ICV1	S	Total CN	P	94.7109	µg/l	4/7/2022 12:18:35	
ICB1	S	Total CN	P	1.0979	µg/l	4/7/2022 12:18:37	
CCV1	S	Total CN	P	248.9056	µg/l	4/7/2022 12:18:41	
CCB1	S	Total CN	P	0.8935	µg/l	4/7/2022 12:18:43	
PB143946BL	S	Total CN	P	1.054	µg/l	4/7/2022 12:18:45	
PB143946BS	S	Total CN	P	94.5009	µg/l	4/7/2022 12:26:10	
LOWPB143946	S	Total CN	P	10.5232	µg/l	4/7/2022 12:26:12	
HIGHPB143946	S	Total CN	P	495.0818	µg/l	4/7/2022 12:26:15	
N2282-01	S	Total CN	P	1.8848	µg/l	4/7/2022 12:26:16	
N2282-01DUP	S	Total CN	P	1.3464	µg/l	4/7/2022 12:26:17	
N2282-01MS	S	Total CN	P	41.2588	µg/l	4/7/2022 12:26:18	
N2282-01MSD	S	Total CN	P	41.455	µg/l	4/7/2022 12:26:19	
N2277-01	S	Total CN	P	0.8919	µg/l	4/7/2022 12:30:58	
CCV2	S	Total CN	P	252.2944	µg/l	4/7/2022 12:30:59	
CCB2	S	Total CN	P	1.2943	µg/l	4/7/2022 12:31:00	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

4/7/2022 11:53


Test Total CN

Accepted 4/7/2022 11:53

Factor 1152
Bias 0.001

Coeff. of det. 0.999968

Errors

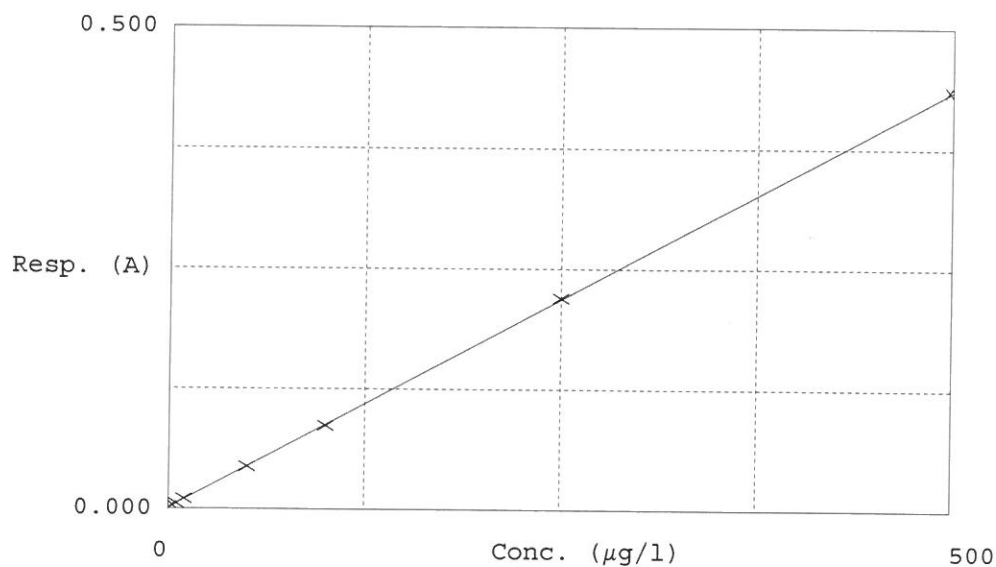

	Calibrator	Response	Calc. con.	Conc.	^{Re} Errors
1	0.0PPBCN	0.002	0.8747	0.0000	-
2	5.0PPBCN	0.005	4.6965	5.0000	-6.1
3	10PPBCN	0.010	10.6085	10.0000	6.1
4	50PPBCN	0.044	49.3671	50.0000	-1.3
5	100PPBCN	0.087	98.3328	100.0000	-1.7
6	250PPBCN	0.220	251.4655	250.0000	0.6
7	500PPBCN	0.435	499.6548	500.0000	-0.1

12
4/7/22