


LB119610

7471B

INSTRUMENT ID: CV1

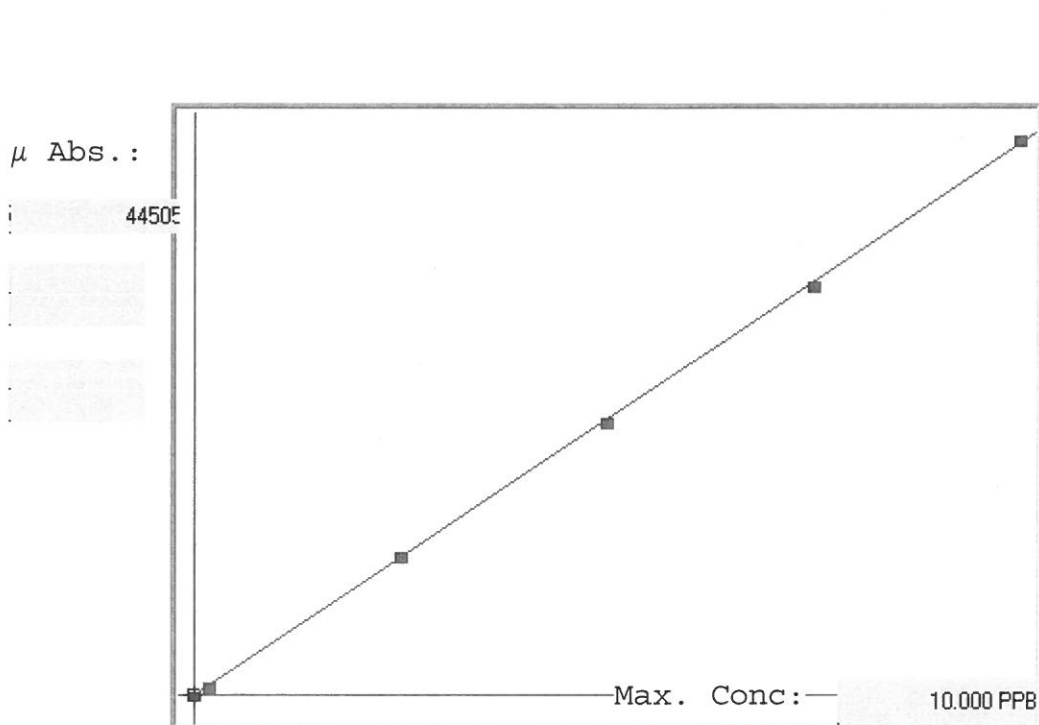

A= 0.0000e+000

B= 2.2567e-004

C= 1.7921e-002

Rho= 0.9999134

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.040	0.040	96	0.000	96					=
0.2	0.200	0.170	-0.030	675	0.0 %	675					-15
2.5	2.500	2.539	0.039	11173	0.0 %	11173					2
5.0	5.000	4.956	-0.044	21884	0.0 %	21884					-1
7.5	7.500	7.433	-0.067	32858	0.0 %	32858					-1
10.0	10.000	10.061	0.061	44505	0.0 %	44505					1

LB119610 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 10 Apr 2022 11:30:33

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	96	-	0.0000	7471B	PPB	10 Apr 2022 11:32:34	S	Std
0.2 - 1	50.2	675	-	0.2000	7471B	PPB	10 Apr 2022 11:34:50	S	Std
2.5 - 1	52.5	11173	-	2.5000	7471B	PPB	10 Apr 2022 11:37:08	S	Std
5.0 - 1	55	21884	-	5.0000	7471B	PPB	10 Apr 2022 11:39:25	S	Std
7.5 - 1	57.5	32858	-	7.5000	7471B	PPB	10 Apr 2022 11:41:41	S	Std
10.0 - 1	58	44505	-	10.0000	7471B	PPB	10 Apr 2022 11:49:06	S	Std
ICV71 - 1	ICV71	16865	3.8238	-	7471B	PPB	10 Apr 2022 11:51:43	U	SMPL
ICB71 - 1	ICB71	-92	-0.0028	-	7471B	PPB	10 Apr 2022 11:53:58	U	SMPL
CCV26 - 1	CCV26	21903	4.9608	-	7471B	PPB	10 Apr 2022 11:56:13	U	SMPL
CCB26 - 1	CCB26	-90	-0.0024	-	7471B	PPB	10 Apr 2022 11:58:28	U	SMPL
CRA - 1	CRA	660	0.1669	-	7471B	PPB	10 Apr 2022 12:00:44	U	SMPL
HighStd - 1	HighStd	44029	9.9539	-	7471B	PPB	10 Apr 2022 12:02:59	U	SMPL
ChkStd - 1	ChkStd	31968	7.2321	-	7471B	PPB	10 Apr 2022 12:05:14	U	SMPL
PB144008BL - 1	PBS	-83	-0.0008	-	7471B	PPB	10 Apr 2022 12:07:31	U	SMPL
PB144008BS - 1	LCSS	16345	3.7065	-	7471B	PPB	10 Apr 2022 12:09:49	U	SMPL
N2281-01 - 1	TR-05-040622	5186	1.1882	-	7471B	PPB	10 Apr 2022 12:12:05	U	SMPL
N2282-01 - 1	LA-1	1173	0.2826	-	7471B	PPB	10 Apr 2022 12:14:21	U	SMPL
N2282-01DUP - 1	LA-1DUP	1138	0.2747	-	7471B	PPB	10 Apr 2022 12:16:38	U	SMPL
N2282-01MS - 1	LA-1MS	17637	3.9981	-	7471B	PPB	10 Apr 2022 12:18:55	U	SMPL
N2282-01MSD - 1	LA-1MSD	17037	3.8627	-	7471B	PPB	10 Apr 2022 12:21:09	U	SMPL
CCV27 - 1	CCV27	21606	4.8937	-	7471B	PPB	10 Apr 2022 12:23:25	U	SMPL
CCB27 - 1	CCB27	-40	0.0089	-	7471B	PPB	10 Apr 2022 12:25:40	U	SMPL
N2298-01 - 1	RB21139	19	0.0222	-	7471B	PPB	10 Apr 2022 12:27:56	U	SMPL
N2306-01 - 1	2404-2405	195	0.0619	-	7471B	PPB	10 Apr 2022 12:30:11	U	SMPL
N2317-01 - 1	WEST-1	1506	0.3578	-	7471B	PPB	10 Apr 2022 12:32:27	U	SMPL
N2317-03 - 1	WEST-2	1623	0.3842	-	7471B	PPB	10 Apr 2022 12:34:42	U	SMPL
N2317-05 - 1	NORTH-1	185	0.0597	-	7471B	PPB	10 Apr 2022 13:05:06	U	SMPL
N2317-07 - 1	NORTH-2	1504	0.3573	-	7471B	PPB	10 Apr 2022 13:07:21	U	SMPL
N2317-09 - 1	NORTH-3	1633	0.3864	-	7471B	PPB	10 Apr 2022 13:09:37	U	SMPL
N2317-11 - 1	NORTH-4	2278	0.5320	-	7471B	PPB	10 Apr 2022 13:11:54	U	SMPL
N2317-13 - 1	NORTH-5	849	0.2095	-	7471B	PPB	10 Apr 2022 13:14:11	U	SMPL
N2317-15 - 1	NORTH-6	1266	0.3036	-	7471B	PPB	10 Apr 2022 13:16:26	U	SMPL
CCV28 - 1	CCV28	21713	4.9179	-	7471B	PPB	10 Apr 2022 13:21:12	U	SMPL
CCB28 - 1	CCB28	-151	-0.0162	-	7471B	PPB	10 Apr 2022 13:23:28	U	SMPL
N2317-17 - 1	TP1-A	1234	0.2964	-	7471B	PPB	10 Apr 2022 13:25:45	U	SMPL
N2317-19 - 1	TP1-B	263	0.0773	-	7471B	PPB	10 Apr 2022 13:28:00	U	SMPL
N2317-21 - 1	TP2-A	685	0.1725	-	7471B	PPB	10 Apr 2022 13:30:16	U	SMPL
N2317-23 - 1	TP2-B	1120	0.2707	-	7471B	PPB	10 Apr 2022 13:32:31	U	SMPL
N2329-01 - 1	285	1642	0.3885	-	7471B	PPB	10 Apr 2022 13:34:46	U	SMPL
N2329-03 - 1	RBR-346	223	0.0682	-	7471B	PPB	10 Apr 2022 13:37:02	U	SMPL
N2330-01 - 1	RBR-253	693	0.1743	-	7471B	PPB	10 Apr 2022 13:39:18	U	SMPL
N2282-01LX5 - 1		162	0.0545	-	7471B	PPB	10 Apr 2022 13:41:35	U	SMPL
N2282-01A - 1		16876	3.8263	-	7471B	PPB	10 Apr 2022 13:48:59	U	SMPL
CCV29 - 1	CCV29	23407	5.3002	-	7471B	PPB	10 Apr 2022 13:51:16	U	SMPL
CCB29 - 1	CCB29	-127	-0.0107	-	7471B	PPB	10 Apr 2022 13:53:33	U	SMPL