

LB 119640

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

4/12/2022 11:17

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.988	0.0	0.112	
ICB1	0.002	0.0	0.007	
CCV1	0.994	0.0	0.112	
CCB1	0.001	0.0	0.007	
PB144056BL	0.000	0.0	0.007	
PB144056BS	0.999	0.0	0.113	
N2340-11	-0.002	0.0	0.006	
N2340-11DUP	-0.002	0.0	0.006	
N2340-11MS	1.048	0.0	0.118	
N2340-11MSD	1.047	0.0	0.118	
CCV2	0.997	0.0	0.112	
CCB2	-0.000	0.0	0.006	

N	12
Mean	0.506
SD	0.5291
CV%	104.55

Aquakem v. 7.2AQ1

Results from time period:

Tue Apr 12 09:48:34 2022

Tue Apr 12 11:04:39 2022

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time
0.00PPM	A	Phenolics-	P	-0.0013	mg/l	4/12/2022 9:48:34
0.05PPM	A	Phenolics-	P	0.0544	mg/l	4/12/2022 9:48:35
0.1PPM	A	Phenolics-	P	0.1084	mg/l	4/12/2022 9:48:36
0.25PPM	A	Phenolics-	P	0.2587	mg/l	4/12/2022 9:48:37
0.50PPM	A	Phenolics-	P	0.5006	mg/l	4/12/2022 9:48:38
1.0PPM	A	Phenolics-	P	0.962	mg/l	4/12/2022 9:48:39
2.0PPM	A	Phenolics-	P	2.0172	mg/l	4/12/2022 9:48:40
ICV1	S	Phenolics-	P	0.9883	mg/l	4/12/2022 10:57:47
ICB1	S	Phenolics-	P	0.0022	mg/l	4/12/2022 10:57:49
CCV1	S	Phenolics-	P	0.9944	mg/l	4/12/2022 10:57:51
CCB1	S	Phenolics-	P	0.0008	mg/l	4/12/2022 10:57:52
PB144056BL	S	Phenolics-	P	0	mg/l	4/12/2022 10:57:54
PB144056BS	S	Phenolics-	P	0.999	mg/l	4/12/2022 10:57:56
N2340-11	S	Phenolics-	P	-0.0019	mg/l	4/12/2022 11:04:32
N2340-11DUP	S	Phenolics-	P	-0.0023	mg/l	4/12/2022 11:04:33
N2340-11MS	S	Phenolics-	P	1.0476	mg/l	4/12/2022 11:04:34
N2340-11MSD	S	Phenolics-	P	1.0471	mg/l	4/12/2022 11:04:35
CCV2	S	Phenolics-	P	0.9972	mg/l	4/12/2022 11:04:36
CCB2	S	Phenolics-	P	-0.0001	mg/l	4/12/2022 11:04:38

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

4/12/2022 9:50 Reviewed by : 12 Instrument ID : Konelab


Test Phenolics-

Accepted 4/12/2022 9:50

Factor 9.411
Bias 0.006

Coeff. of det. 0.999394

Errors

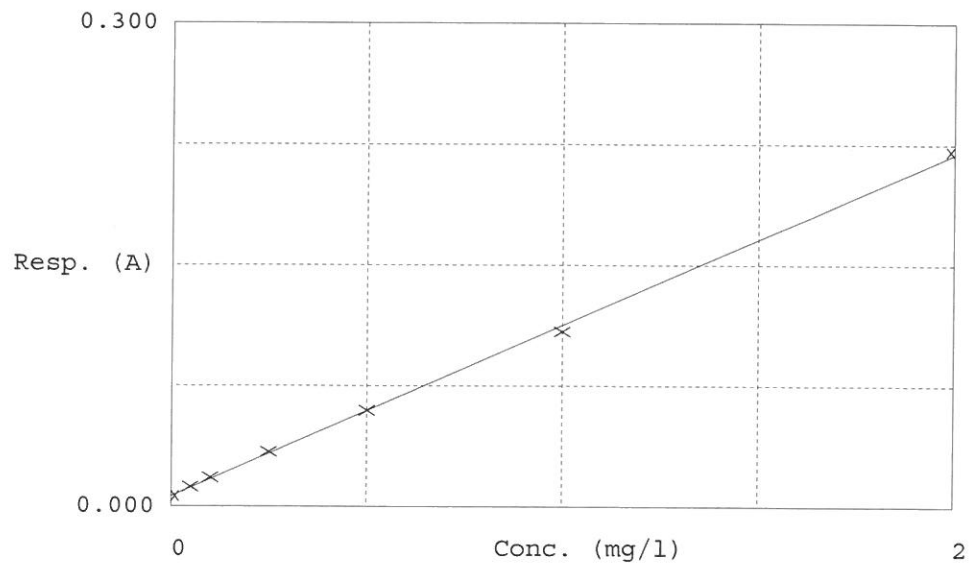

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.006	-0.0013	0.0000	-
2	Phenol-2	0.012	0.0544	0.0500	8.8
3	Phenol-2	0.018	0.1084	0.1000	8.4
4	Phenol-2	0.034	0.2587	0.2500	3.5
5	Phenol-2	0.060	0.5006	0.5000	0.1
6	Phenol-2	0.109	0.9620	1.0000	-3.8
7	Phenol-2	0.221	2.0172	2.0000	0.9

12 4/12/22