

LB 119653

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

4/13/2022 10:28

Test: Total CN

Sample Id	^{14/L} Result	Dil. 1 +	Response	Errors
ICV1	94.156	0.0	0.085	
ICB1	0.062	0.0	0.003	
CCV1	245.653	0.0	0.217	
CCB1	-0.087	0.0	0.003	
PB144078BL	-0.061	0.0	0.003	
N2364-02	-0.217	0.0	0.002	
N2364-02DUP	-0.192	0.0	0.002	
N2364-04	-0.175	0.0	0.002	
N2364-06	-0.221	0.0	0.002	
N2364-08	-0.176	0.0	0.002	
CCV2	254.938	0.0	0.225	
CCB2	-0.115	0.0	0.003	

N	12
Mean	49.464
SD	97.6285
CV%	197.37

Aquakem v. 7.2AQ1

Results from time period:

Wed Apr 13 09:51:22 2022

Wed Apr 13 10:23:20 2022

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.411	µg/l	4/13/2022 9:51:22	
5.OPPBCN	A	Reactive CN	P	3.6329	µg/l	4/13/2022 9:51:23	
10PPBCN	A	Reactive CN	P	9.6746	µg/l	4/13/2022 9:51:24	
50PPBCN	A	Reactive CN	P	48.9363	µg/l	4/13/2022 9:51:25	
100PPBCN	A	Reactive CN	P	101.6942	µg/l	4/13/2022 9:51:26	
250PPBCN	A	Reactive CN	P	253.3705	µg/l	4/13/2022 9:51:27	
500PPBCN	A	Reactive CN	P	498.1024	µg/l	4/13/2022 9:51:28	
ICV1	S	Reactive CN	P	94.1556	µg/l	4/13/2022 10:17:32	
ICB1	S	Reactive CN	P	0.062	µg/l	4/13/2022 10:17:34	
CCV1	S	Reactive CN	P	245.6535	µg/l	4/13/2022 10:17:36	
CCB1	S	Reactive CN	P	-0.0869	µg/l	4/13/2022 10:17:38	
PB144078BL	S	Reactive CN	P	-0.0614	µg/l	4/13/2022 10:17:39	
N2364-02	S	Reactive CN	P	-0.2173	µg/l	4/13/2022 10:17:41	
N2364-02DUP	S	Reactive CN	P	-0.1917	µg/l	4/13/2022 10:23:14	
N2364-04	S	Reactive CN	P	-0.1745	µg/l	4/13/2022 10:23:15	
N2364-06	S	Reactive CN	P	-0.221	µg/l	4/13/2022 10:23:16	
N2364-08	S	Reactive CN	P	-0.1764	µg/l	4/13/2022 10:23:17	
CCV2	S	Reactive CN	P	254.938	µg/l	4/13/2022 10:23:19	
CCB2	S	Reactive CN	P	-0.115	µg/l	4/13/2022 10:23:20	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

4/13/2022 9:54


Test Total CN

Accepted 4/13/2022 9:54

Factor 1148
Bias 0.003

Coeff. of det. 0.999897

Errors

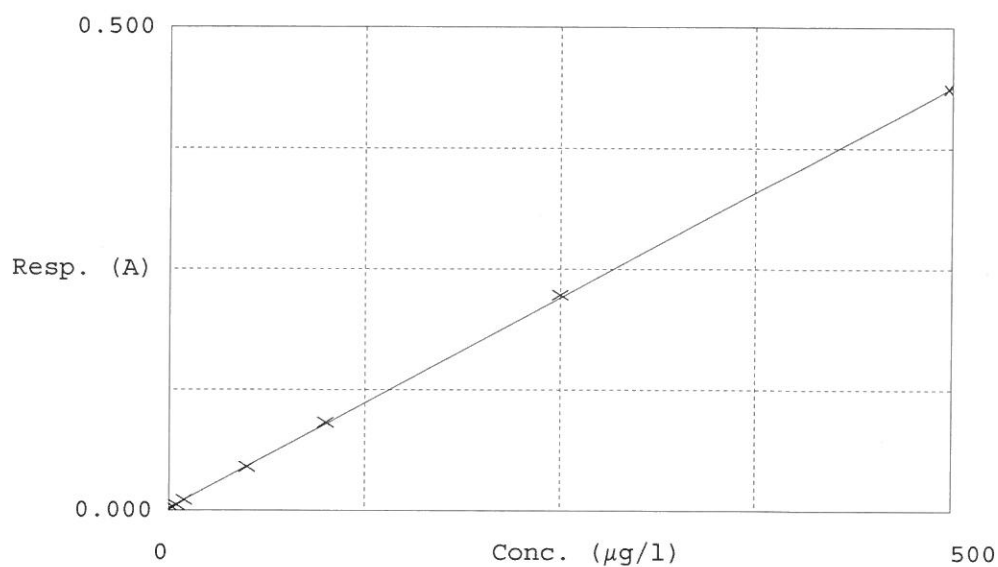

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.4110	0.0000	
2	5.0PPBCN	0.006	3.6329	5.0000	-27.3
3	10PPBCN	0.011	9.6746	10.0000	-3.3
4	50PPBCN	0.045	48.9363	50.0000	-2.1
5	100PPBCN	0.091	101.6942	100.0000	1.7
6	250PPBCN	0.223	253.3705	250.0000	1.3
7	500PPBCN	0.436	498.1024	500.0000	-0.4

12
4/13/22