


LB119794

7470A

INSTRUMENT ID: CX1

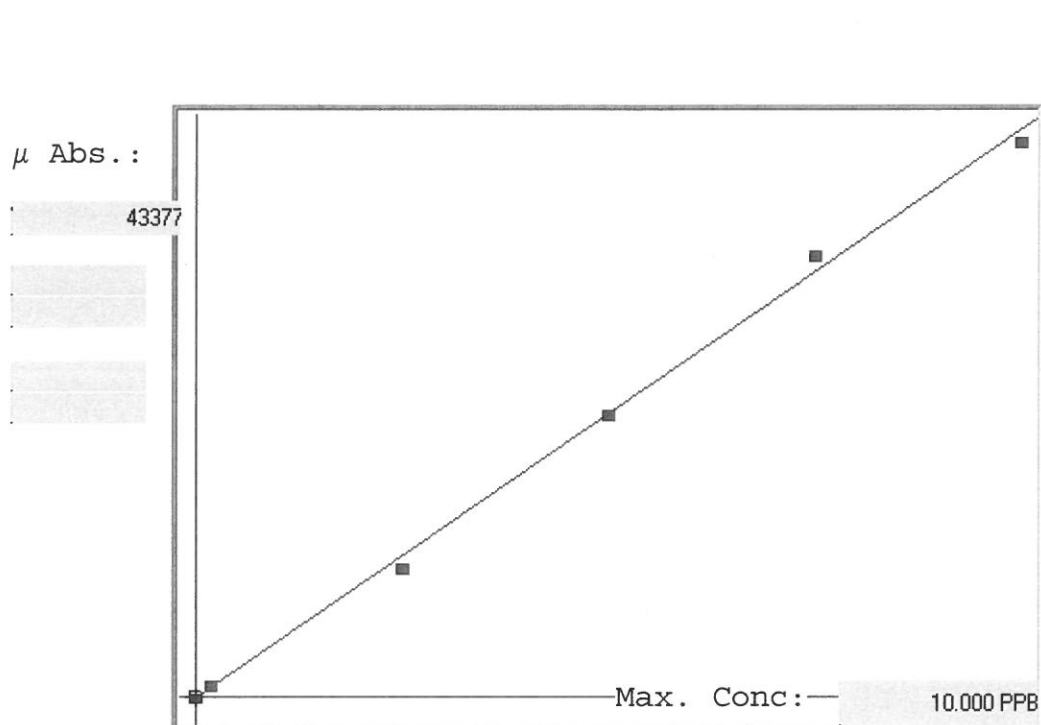

Linear

A= 0.0000e+000

B= 2.2502e-004

C= 3.1543e-002

Rho= 0.9989521

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.035	0.035	16	0.000	16					-
0.2	0.200	0.236	0.036	908	0.0 %	908					18
2.5	2.500	2.315	-0.185	10146	0.0 %	10146					-7
5.0	5.000	5.021	0.021	22175	0.0 %	22175					0
7.5	7.500	7.801	0.301	34528	0.0 %	34528					4
10.0	10.000	9.792	-0.208	43377	0.0 %	43377					-2

LB119794 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 22 Apr 2022 10:26:03

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	16	-	0.0000	7470A	PPB	22 Apr 2022 10:31:44	S	Std
0.2 - 1	50.2	908	-	0.2000	7470A	PPB	22 Apr 2022 10:41:18	S	Std
2.5 - 1	52.5	10146	-	2.5000	7470A	PPB	22 Apr 2022 10:43:35	S	Std
5.0 - 1	55	22175	-	5.0000	7470A	PPB	22 Apr 2022 10:45:52	S	Std
7.5 - 1	57.5	34528	-	7.5000	7470A	PPB	22 Apr 2022 10:48:08	S	Std
10.0 - 1	510	43377	-	10.0000	7470A	PPB	22 Apr 2022 10:50:24	S	Std
ICV90 - 1	ICV90	18260	4.1404	-	7470A	PPB	22 Apr 2022 11:00:19	U	SMPL
ICB90 - 1	ICB90	-53	0.0196	-	7470A	PPB	22 Apr 2022 11:02:33	U	SMPL
CCV19 - 1	CCV19	21813	4.9399	-	7470A	PPB	22 Apr 2022 11:04:48	U	SMPL
CCB19 - 1	CCB19	-47	0.0210	-	7470A	PPB	22 Apr 2022 11:07:04	U	SMPL
CRA - 1	CRA	953	0.2460	-	7470A	PPB	22 Apr 2022 11:09:19	U	SMPL
HighStd - 1	HighStd	41207	9.3039	-	7470A	PPB	22 Apr 2022 11:11:34	U	SMPL
ChkStd - 1	ChkStd	30062	6.7960	-	7470A	PPB	22 Apr 2022 11:13:49	U	SMPL
PB144312BL - 1	PBW	-94	0.0104	-	7470A	PPB	22 Apr 2022 11:16:05	U	SMPL
PB144312BS - 1	LCSW	18094	4.1030	-	7470A	PPB	22 Apr 2022 11:20:53	U	SMPL
N2511-06 - 1	1530	290	0.0968	-	7470A	PPB	22 Apr 2022 11:28:05	U	SMPL
N2511-06DUP - 1	1530DUP	233	0.0840	-	7470A	PPB	22 Apr 2022 11:30:22	U	SMPL
N2511-06MS - 1	1530MS	15562	3.5333	-	7470A	PPB	22 Apr 2022 11:37:11	U	SMPL
N2511-06MSD - 1	1530MSD	16776	3.8064	-	7470A	PPB	22 Apr 2022 11:39:30	U	SMPL
N2511-09 - 1	1590	150	0.0653	-	7470A	PPB	22 Apr 2022 11:41:48	U	SMPL
CCV20 - 1	CCV20	22070	4.9977	-	7470A	PPB	22 Apr 2022 11:44:05	U	SMPL
CCB20 - 1	CCB20	-21	0.0268	-	7470A	PPB	22 Apr 2022 11:46:20	U	SMPL
N2511-10 - 1	1593	1392	0.3448	-	7470A	PPB	22 Apr 2022 11:48:35	U	SMPL
N2511-11 - 1	1592	2962	0.6980	-	7470A	PPB	22 Apr 2022 11:50:50	U	SMPL
N2511-06LX5 - 1		33	0.0390	-	7470A	PPB	22 Apr 2022 11:53:06	U	SMPL
N2511-06A - 1		17769	4.0299	-	7470A	PPB	22 Apr 2022 11:55:21	U	SMPL
CCV21 - 1	CCV21	21478	4.8645	-	7470A	PPB	22 Apr 2022 11:59:39	U	SMPL
CCB21 - 1	CCB21	-27	0.0255	-	7470A	PPB	22 Apr 2022 12:01:54	U	SMPL