

===== LB119884 =====
Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092Reviewed by : 12 Instrument ID : Konelab4/29/2022 14:23

Test: Total CN

Sample Id	<i>ex/L</i> Result	Dil. 1 +	Response	Errors
ICV1	93.953	0.0	0.078	
ICB1	0.356	0.0	0.001	
CCV1	241.945	0.0	0.201	
CCB1	0.636	0.0	0.001	
PB144399BL	0.619	0.0	0.001	
PB144399BS	94.225	0.0	0.078	
MIDPB144399	244.395	0.0	0.203	98% (90-110)
N2571-01	1.679	0.0	0.002	
N2571-01DUP	4.693	0.0	0.004	
N2571-01MS	18.019	0.0	0.015	12
N2571-01MSD	17.607	0.0	0.015	4/29/22
CCV2	252.176	0.0	0.209	
CCB2	0.791	0.0	0.001	

N	13
Mean	74.699
SD	103.1526
CV%	138.09

Aquakem v. 7.2AQ1

Results from time period:

Fri Apr 29 13:50:11 2022

Fri Apr 29 14:18:47 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	Total CN	P	0.5229	µg/l	4/29/2022 13:50:11
5.OPPBCN	A	Total CN	P	5.2533	µg/l	4/29/2022 13:50:12
10PPBCN	A	Total CN	P	10.2447	µg/l	4/29/2022 13:50:13
50PPBCN	A	Total CN	P	48.9039	µg/l	4/29/2022 13:50:14
100PPBCN	A	Total CN	P	99.3241	µg/l	4/29/2022 13:50:15
250PPBCN	A	Total CN	P	251.0275	µg/l	4/29/2022 13:50:16
500PPBCN	A	Total CN	P	499.7236	µg/l	4/29/2022 13:50:17
ICV1	S	Total CN	P	93.9534	µg/l	4/29/2022 14:12:30
ICB1	S	Total CN	P	0.3555	µg/l	4/29/2022 14:12:32
CCV1	S	Total CN	P	241.9455	µg/l	4/29/2022 14:12:33
CCB1	S	Total CN	P	0.6363	µg/l	4/29/2022 14:12:36
PB144399BL	S	Total CN	P	0.6192	µg/l	4/29/2022 14:12:38
PB144399BS	S	Total CN	P	94.2246	µg/l	4/29/2022 14:12:39
MIDPB144399	S	Total CN	P	244.3949	µg/l	4/29/2022 14:18:41
N2571-01	S	Total CN	P	1.6785	µg/l	4/29/2022 14:18:42
N2571-01DUP	S	Total CN	P	4.6929	µg/l	4/29/2022 14:18:43
N2571-01MS	S	Total CN	P	18.0188	µg/l	4/29/2022 14:18:44
N2571-01MSD	S	Total CN	P	17.6071	µg/l	4/29/2022 14:18:45
CCV2	S	Total CN	P	252.1755	µg/l	4/29/2022 14:18:46
CCB2	S	Total CN	P	0.7907	µg/l	4/29/2022 14:18:47

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

4/29/2022 13:50


Test Total CN

Accepted 4/29/2022 13:50

Factor 1207
Bias 0

Coeff. of det. 0.999985

Errors

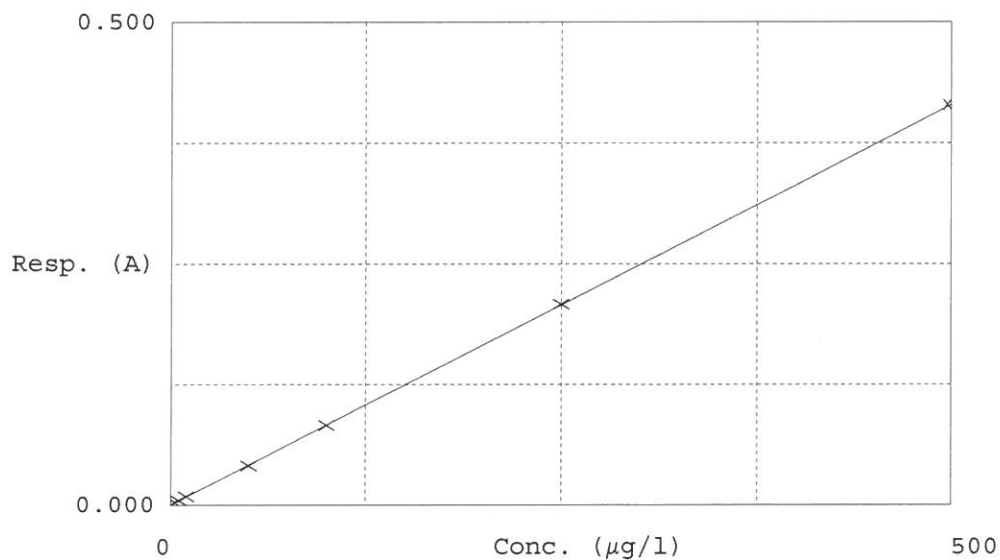

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.5229	0.0000	-
2	5.0PPBCN	0.005	5.2533	5.0000	5.1
3	10PPBCN	0.009	10.2447	10.0000	2.4
4	50PPBCN	0.041	48.9039	50.0000	-2.2
5	100PPBCN	0.083	99.3241	100.0000	-0.7
6	250PPBCN	0.208	251.0275	250.0000	0.4
7	500PPBCN	0.414	499.7236	500.0000	-0.1

12
4/29/22