

L B 119897


SFAM01.1

INSTRUMENT ID: CV2

Linear

μ Abs.:

43778

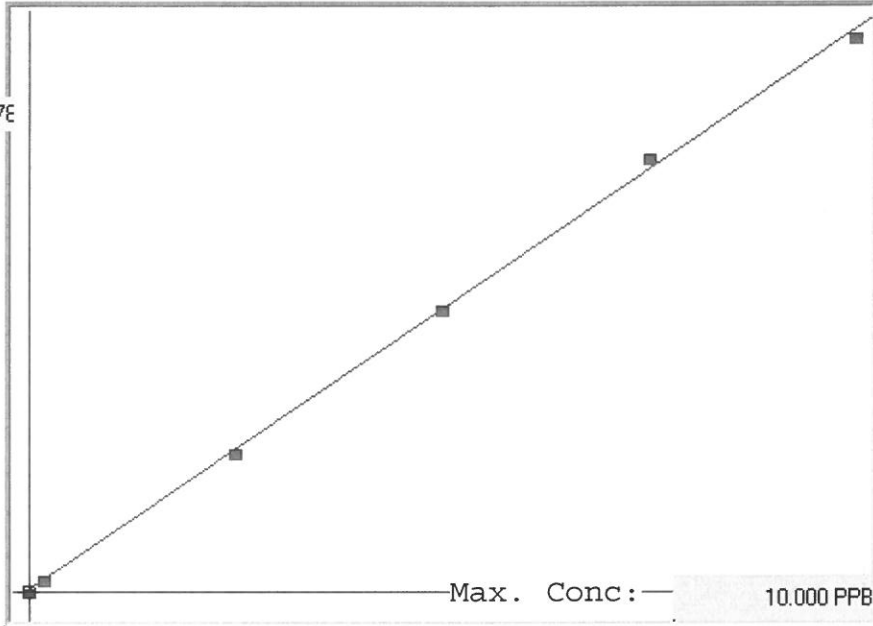

A= 0.0000e+000

B= 2.2569e-004 slope

C= -3.3511e-002 y-intercept

Rho= 0.9996041

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	-0.004	-0.004	130	0.000	130					=
0.05	0.050					185	0				-9
0.20	0.200	0.183	-0.017	959	0.0 %	959					-2
2.50	2.500	2.456	-0.044	11032	0.0 %	11032					0
5.00	5.000	5.022	0.022	22402	0.0 %	22402					3
7.50	7.500	7.696	0.196	34249	0.0 %	34249					-2
10.0	10.000	9.847	-0.153	43778	0.0 %	43778					

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	130	-		0 SFAM01.1	PPB	4/29/2022 11:48	Std
	0.2 S01	959	-		0.2 SFAM01.1	PPB	4/29/2022 11:50	Std
	2.5 S02	11032	-		2.5 SFAM01.1	PPB	4/29/2022 11:52	Std
	5 S03	22402	-		5 SFAM01.1	PPB	4/29/2022 11:54	Std
	7.5 S04	34249	-		7.5 SFAM01.1	PPB	4/29/2022 11:57	Std
	10 S05	43778	-		10 SFAM01.1	PPB	4/29/2022 11:59	Std
ICV001	ICV001	17453	3.9054 -		SFAM01.1	PPB	4/29/2022 12:02	SMPL
ICB001	ICB001	61	-0.0197 -		SFAM01.1	PPB	4/29/2022 12:04	SMPL
CCV053	CCV053	22184	4.9731 -		SFAM01.1	PPB	4/29/2022 12:06	SMPL
CCB053	CCB053	36	-0.0254 -		SFAM01.1	PPB	4/29/2022 12:09	SMPL
PB144467BL	PBW467	101	-0.0107 -		SFAM01.1	PPB	4/29/2022 12:13	SMPL
N2417-07	X3A20	19861	4.4489 -		SFAM01.1	PPB	4/29/2022 12:18	SMPL
N2417-08	X3A20D	20034	4.4879 -		SFAM01.1	PPB	4/29/2022 12:20	SMPL
N2417-09	X3A20S	24487	5.4929 -		SFAM01.1	PPB	4/29/2022 12:25	SMPL
CCV054	CCV054	21805	4.8876 -		SFAM01.1	PPB	4/29/2022 12:29	SMPL
CCB054	CCB054	15	-0.0301 -		SFAM01.1	PPB	4/29/2022 12:31	SMPL