

LB118905

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

4/29/2022 12:51

Test: Phenolics-

Sample Id	Result ^{µg/L}	Dil. 1 +	Response	Errors
ICV1	0.938	0.0	0.089	
ICB1	0.013	0.0	0.007	
CCV1	0.914	0.0	0.087	
CCB1	0.018	0.0	0.008	
PB144348BL	0.023	0.0	0.008	
PB144348BS	0.946	0.0	0.089	
N2550-01	0.009	0.0	0.007	
N2550-01DUP	-0.002	0.0	0.006	
N2550-02	0.022	0.0	0.008	
N2550-01MS	0.916	0.0	0.087	
N2550-01MSD	0.916	0.0	0.087	
CCV2	0.922	0.0	0.087	
CCB2	0.004	0.0	0.006	

N	13
Mean	0.434
SD	0.4737
CV%	109.21

Aquakem v. 7.2AQ1

Results from time period:

Fri Apr 29 10:40:50 2022

Fri Apr 29 12:37:35 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0033	mg/l	4/29/2022 10:40:50	
0.05PPM	A	Phenolics-	P	0.0546	mg/l	4/29/2022 10:40:51	
0.1PPM	A	Phenolics-	P	0.1043	mg/l	4/29/2022 10:40:52	
0.25PPM	A	Phenolics-	P	0.2532	mg/l	4/29/2022 10:40:53	
0.50PPM	A	Phenolics-	P	0.4989	mg/l	4/29/2022 10:40:54	
1.0PPM	A	Phenolics-	P	0.9724	mg/l	4/29/2022 10:40:55	
2.0PPM	A	Phenolics-	P	2.0134	mg/l	4/29/2022 10:40:56	
ICV1	S	Phenolics-	P	0.9376	mg/l	4/29/2022 12:13:22	
ICB1	S	Phenolics-	P	0.0132	mg/l	4/29/2022 12:13:23	
CCV1	S	Phenolics-	P	0.914	mg/l	4/29/2022 12:13:24	
CCB1	S	Phenolics-	P	0.0181	mg/l	4/29/2022 12:13:25	
PB144348BL	S	Phenolics-	P	0.0232	mg/l	4/29/2022 12:13:26	
PB144348BS	S	Phenolics-	P	0.9458	mg/l	4/29/2022 12:13:27	
N2550-01	S	Phenolics-	P	0.0086	mg/l	4/29/2022 12:13:28	
N2550-01DUP	S	Phenolics-	P	-0.0021	mg/l	4/29/2022 12:13:29	
N2550-02	S	Phenolics-	P	0.0223	mg/l	4/29/2022 12:13:32	
N2550-01MS	S	Phenolics-	P	0.9161	mg/l	4/29/2022 12:37:32	
N2550-01MSD	S	Phenolics-	P	0.9162	mg/l	4/29/2022 12:37:33	
CCV2	S	Phenolics-	P	0.9216	mg/l	4/29/2022 12:37:34	
CCB2	S	Phenolics-	P	0.0043	mg/l	4/29/2022 12:37:35	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

4/29/2022 10:42


Test Phenolics-

Accepted 4/29/2022 10:42

Factor 11.35
Bias 0.006

Coeff. of det. 0.999683

Errors

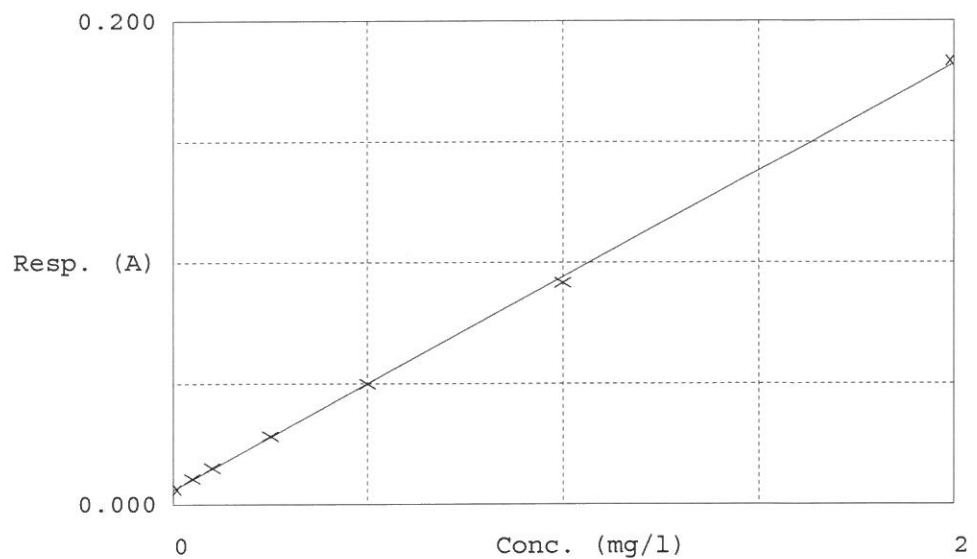

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.006	0.0033	0.0000	-
2	Phenol-2	0.011	0.0546	0.0500	9.2
3	Phenol-2	0.015	0.1043	0.1000	4.3
4	Phenol-2	0.028	0.2532	0.2500	1.3
5	Phenol-2	0.050	0.4989	0.5000	-0.2
6	Phenol-2	0.092	0.9724	1.0000	-2.8
7	Phenol-2	0.183	2.0134	2.0000	0.7

12
4/29/22