


LB119908

7471B

INSTRUMENT ID: CV2

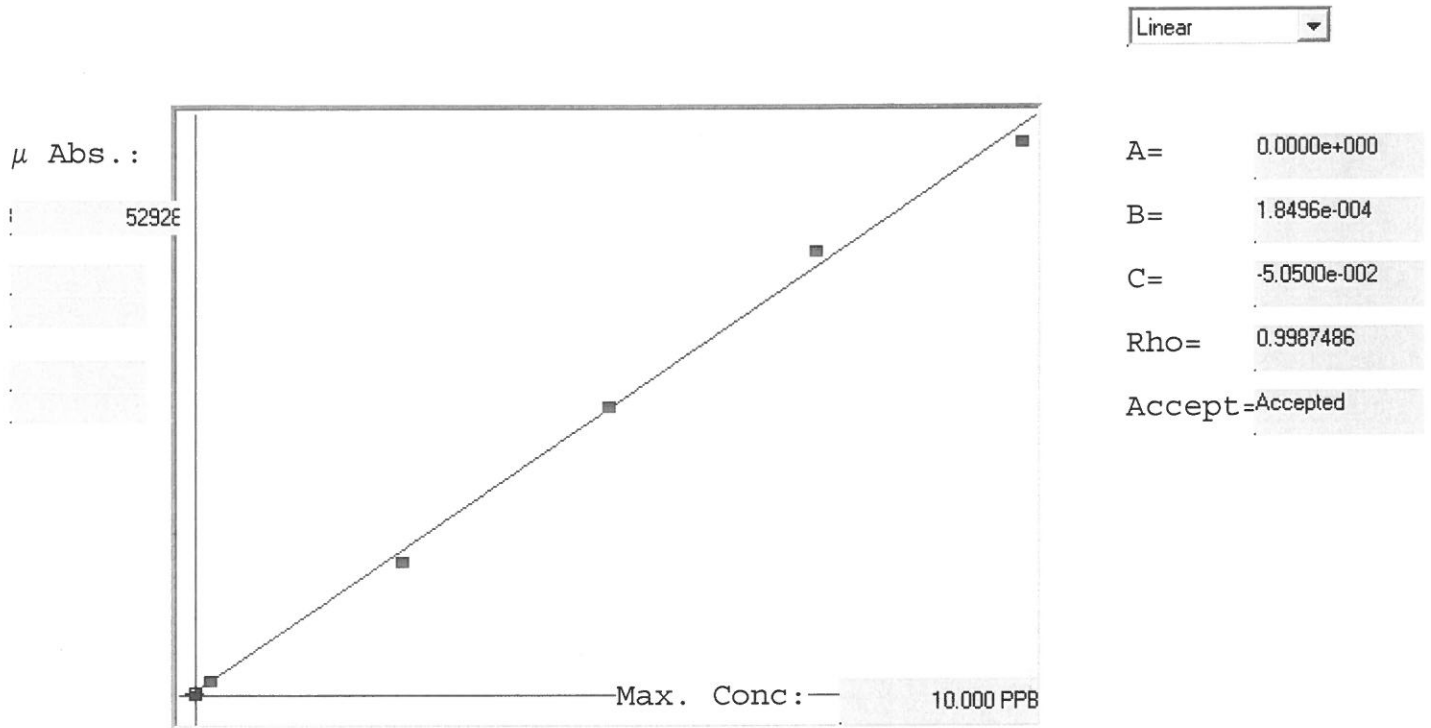

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.006	-0.006	243	0.000	243					-
0.2	0.200	0.227	0.027	1503	0.0 %	1503					14
2.5	2.500	2.330	-0.170	12870	0.0 %	12870					-7
5.0	5.000	5.097	0.097	27832	0.0 %	27832					2
7.5	7.500	7.812	0.312	42507	0.0 %	42507					4
10.0	10.000	9.739	-0.261	52928	0.0 %	52928					-3

LB119908 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 29 Apr 2022 15:12:43

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	5.2	243	-	0.0000	7471B	PPB	29 Apr 2022 15:15:12	S	Std
0.2 - 1	56.2	1503	-	0.2000	7471B	PPB	29 Apr 2022 15:17:29	S	Std
2.5 - 1	57.5	12870	-	2.5000	7471B	PPB	29 Apr 2022 15:19:45	S	Std
5.0 - 1	55	27832	-	5.0000	7471B	PPB	29 Apr 2022 15:22:02	S	Std
7.5 - 1	57.5	42507	-	7.5000	7471B	PPB	29 Apr 2022 15:24:18	S	Std
10.0 - 1	51.8	52928	-	10.0000	7471B	PPB	29 Apr 2022 15:29:09	S	Std
ICV03 - 1	ICV03	21867	3.9940	-	7471B	PPB	29 Apr 2022 15:31:55	U	SMPL
ICB03 - 1	ICB03	164	-0.0202	-	7471B	PPB	29 Apr 2022 15:34:10	U	SMPL
CCV58 - 1	CCV58	27463	5.0291	-	7471B	PPB	29 Apr 2022 15:36:25	U	SMPL
CCB58 - 1	CCB58	167	-0.0196	-	7471B	PPB	29 Apr 2022 15:38:40	U	SMPL
CRA - 1	CRA	1472	0.2218	-	7471B	PPB	29 Apr 2022 15:40:55	U	SMPL
HighStd - 1	HighStd	53633	9.8695	-	7471B	PPB	29 Apr 2022 15:43:10	U	SMPL
ChkStd - 1	ChkStd	39188	7.1978	-	7471B	PPB	29 Apr 2022 15:45:26	U	SMPL
PB144477BL - 1	PBS	116	-0.0290	-	7471B	PPB	29 Apr 2022 15:47:43	U	SMPL
PB144477BS - 1	LCSS	20274	3.6994	-	7471B	PPB	29 Apr 2022 15:50:00	U	SMPL
N2604-01 - 1	NB-07-042822	4648	0.8092	-	7471B	PPB	29 Apr 2022 15:52:16	U	SMPL
N2605-01 - 1	TR-04-042822	2034	0.3257	-	7471B	PPB	29 Apr 2022 15:54:33	U	SMPL
N2605-03 - 1	TR-05-042822	1376	0.2040	-	7471B	PPB	29 Apr 2022 15:56:49	U	SMPL
N2605-05 - 1	TR-06-042822	1416	0.2114	-	7471B	PPB	29 Apr 2022 15:59:06	U	SMPL
N2606-01 - 1	WC-3	7364	1.3116	-	7471B	PPB	29 Apr 2022 16:01:21	U	SMPL
CCV59 - 1	CCV59	27655	5.0646	-	7471B	PPB	29 Apr 2022 16:03:37	U	SMPL
CCB59 - 1	CCB59	203	-0.0130	-	7471B	PPB	29 Apr 2022 16:05:51	U	SMPL
N2607-01 - 1	HR-02-042822	855	0.1076	-	7471B	PPB	29 Apr 2022 16:08:07	U	SMPL
N2609-01 - 1	WC-1	940	0.1234	-	7471B	PPB	29 Apr 2022 16:10:22	U	SMPL
N2609-04 - 1	WC-2	3283	0.5567	-	7471B	PPB	29 Apr 2022 16:12:37	U	SMPL
N2609-07 - 1	WC-3	4838	0.8443	-	7471B	PPB	29 Apr 2022 16:14:52	U	SMPL
N2609-10 - 1	WC-4	21921	4.0040	-	7471B	PPB	29 Apr 2022 16:17:08	U	SMPL
N2610-01 - 1	HR-03-042822	41936	7.7060	-	7471B	PPB	29 Apr 2022 16:19:24	U	SMPL
N2611-01 - 1	JC-01-042822	37213	6.8325	-	7471B	PPB	29 Apr 2022 16:21:40	U	SMPL
N2616-01 - 1	MH-18S	4088	0.7056	-	7471B	PPB	29 Apr 2022 16:23:57	U	SMPL
N2616-04 - 1	MH-18D	40166	7.3786	-	7471B	PPB	29 Apr 2022 16:26:14	U	SMPL
N2616-07 - 1	MH-20S	2870	0.4803	-	7471B	PPB	29 Apr 2022 16:28:29	U	SMPL
CCV60 - 1	CCV60	27988	5.1262	-	7471B	PPB	29 Apr 2022 16:30:46	U	SMPL
CCB60 - 1	CCB60	213	-0.0111	-	7471B	PPB	29 Apr 2022 16:33:01	U	SMPL
N2616-10 - 1	MH-20D	1207	0.1727	-	7471B	PPB	29 Apr 2022 16:35:16	U	SMPL
N2616-10DUP - 1	MH-20DDUP	1170	0.1659	-	7471B	PPB	29 Apr 2022 16:37:31	U	SMPL
N2616-10MS - 1	MH-20DMS	21197	3.8701	-	7471B	PPB	29 Apr 2022 16:39:47	U	SMPL
N2616-10MSD - 1	MH-20DMSD	21691	3.9615	-	7471B	PPB	29 Apr 2022 16:42:02	U	SMPL
N2616-10LX5 - 1		375	0.0189	-	7471B	PPB	29 Apr 2022 16:44:18	U	SMPL
N2616-10A - 1		22316	4.0771	-	7471B	PPB	29 Apr 2022 16:46:34	U	SMPL
CCV61 - 1	CCV61	27843	5.0994	-	7471B	PPB	29 Apr 2022 16:48:51	U	SMPL
CCB61 - 1	CCB61	201	-0.0133	-	7471B	PPB	29 Apr 2022 16:51:08	U	SMPL