


LB119977

7471B

INSTRUMENT ID: CV1

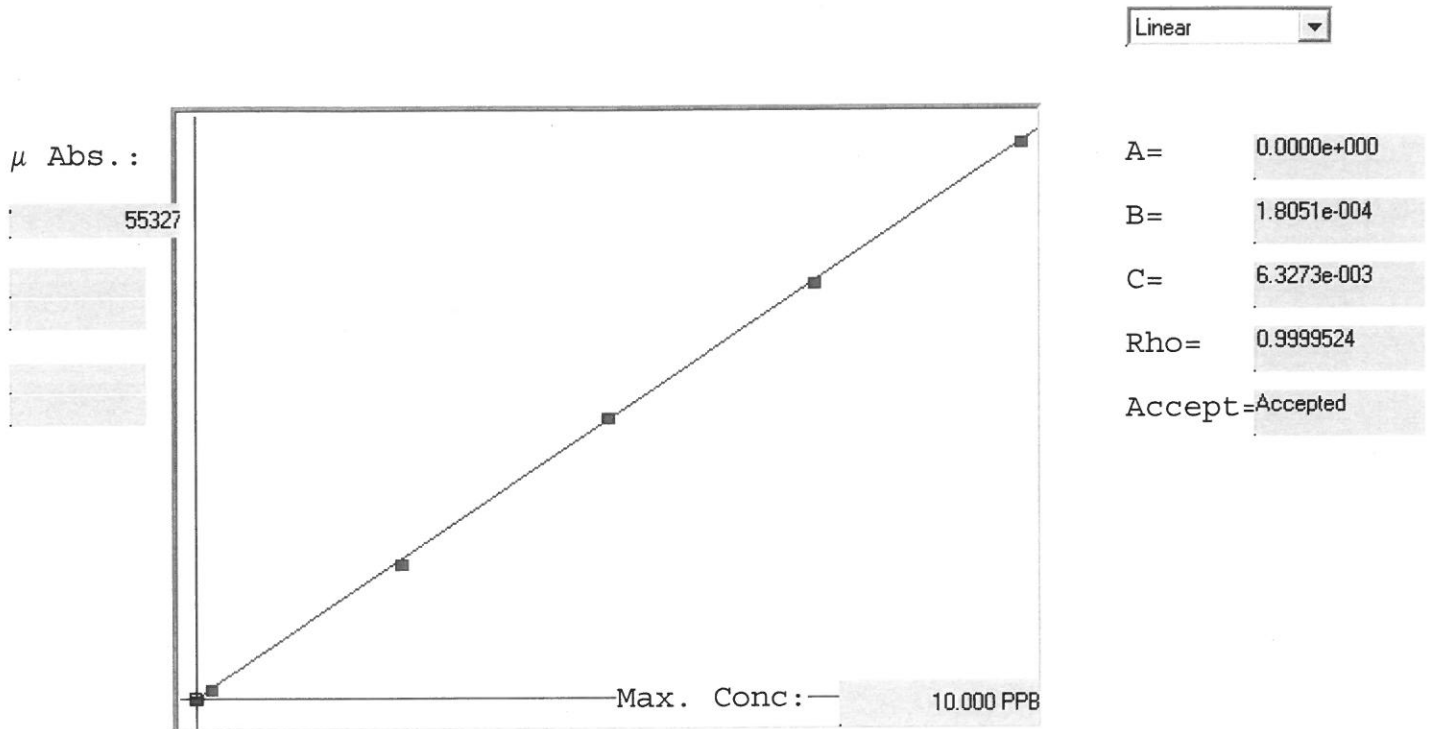

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.013	0.013	39	0.000	39					1
0.2	0.200	0.205	0.005	1102	0.0 %	1102					2
2.5	2.500	2.440	-0.060	13482	0.0 %	13482					-2
5.0	5.000	5.061	0.061	28003	0.0 %	28003					1
7.5	7.500	7.486	-0.014	41438	0.0 %	41438					0
10.0	10.000	9.994	-0.006	55327	0.0 %	55327					0

LB119977 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 04 May 2022 14:55:37

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	39	-	0.0000	7471B	PPB	04 May 2022 14:56:53	S	Std
0.2 - 1	50.2	1102	-	0.2000	7471B	PPB	04 May 2022 14:59:10	S	Std
2.5 - 1	52.5	13482	-	2.5000	7471B	PPB	04 May 2022 15:01:27	S	Std
5.0 - 1	55	28003	-	5.0000	7471B	PPB	04 May 2022 15:03:44	S	Std
7.5 - 1	57.5	41438	-	7.5000	7471B	PPB	04 May 2022 15:06:00	S	Std
10.0 - 1	511	55327	-	10.0000	7471B	PPB	04 May 2022 15:08:17	S	Std
ICV09 - 1	ICV09	21320	3.8549	-	7471B	PPB	04 May 2022 15:11:05	U	SMPL
ICB09 - 1	ICB09	-65	-0.0054	-	7471B	PPB	04 May 2022 15:13:20	U	SMPL
CCV83 - 1	CCV83	28017	5.0638	-	7471B	PPB	04 May 2022 15:15:35	U	SMPL
CCB83 - 1	CCB83	-70	-0.0063	-	7471B	PPB	04 May 2022 15:17:50	U	SMPL
CRA - 1	CRA	1087	0.2025	-	7471B	PPB	04 May 2022 15:20:05	U	SMPL
HighStd - 1	HighStd	55543	10.0326	-	7471B	PPB	04 May 2022 15:22:20	U	SMPL
ChkStd - 1	ChkStd	38528	6.9612	-	7471B	PPB	04 May 2022 15:24:36	U	SMPL
PB144581BL - 1	PBS	-137	-0.0184	-	7471B	PPB	04 May 2022 15:26:53	U	SMPL
PB144581BS - 1	LCSS	19960	3.6094	-	7471B	PPB	04 May 2022 15:29:10	U	SMPL
N2647-01 - 1	357	2309	0.4231	-	7471B	PPB	04 May 2022 15:31:26	U	SMPL
N2648-01 - 1	RBR-346	998	0.1865	-	7471B	PPB	04 May 2022 15:33:42	U	SMPL
N2649-01 - 1	WC-1	597	0.1141	-	7471B	PPB	04 May 2022 15:35:59	U	SMPL
N2650-01 - 1	ETGI-349	1514	0.2796	-	7471B	PPB	04 May 2022 15:38:15	U	SMPL
N2650-03 - 1	ETGI-362	1484	0.2742	-	7471B	PPB	04 May 2022 15:40:30	U	SMPL
CCV84 - 1	CCV84	28159	5.0894	-	7471B	PPB	04 May 2022 15:42:46	U	SMPL
CCB84 - 1	CCB84	-48	-0.0023	-	7471B	PPB	04 May 2022 15:45:01	U	SMPL
N2655-01 - 1	CL-01-050222	4291	0.7809	-	7471B	PPB	04 May 2022 15:47:17	U	SMPL
N2659-01 - 1	22L097-A	3448	0.6287	-	7471B	PPB	04 May 2022 15:49:32	U	SMPL
N2659-02 - 1	22L097-B	2208	0.4049	-	7471B	PPB	04 May 2022 15:51:47	U	SMPL
N2659-03 - 1	22L097-C	3539	0.6452	-	7471B	PPB	04 May 2022 15:54:03	U	SMPL
N2659-04 - 1	22L097-D	3597	0.6556	-	7471B	PPB	04 May 2022 15:56:18	U	SMPL
N2663-01 - 1	TP-25	5243	0.9528	-	7471B	PPB	04 May 2022 16:03:44	U	SMPL
N2663-01DUP - 1	TP-25DUP	5006	0.9100	-	7471B	PPB	04 May 2022 16:06:00	U	SMPL
N2663-01MS - 1	TP-25MS	29464	5.3250	-	7471B	PPB	04 May 2022 16:16:53	U	SMPL
N2663-01MSD - 1	TP-25MSD	28893	5.2219	-	7471B	PPB	04 May 2022 16:19:09	U	SMPL
N2667-01 - 1	75-HALSTAD-ST-STOCK-PILE	8491	1.5391	-	7471B	PPB	04 May 2022 16:21:25	U	SMPL
CCV85 - 1	CCV85	28448	5.1416	-	7471B	PPB	04 May 2022 16:23:40	U	SMPL
CCB85 - 1	CCB85	-66	-0.0056	-	7471B	PPB	04 May 2022 16:25:56	U	SMPL
N2669-01 - 1	OR-03-050322	3892	0.7089	-	7471B	PPB	04 May 2022 16:28:11	U	SMPL
N2673-01 - 1	SWEEPINGS-050322	2588	0.4735	-	7471B	PPB	04 May 2022 16:30:27	U	SMPL
N2674-01 - 1	BU-2-050322	1648	0.3038	-	7471B	PPB	04 May 2022 16:32:42	U	SMPL
N2675-01 - 1	BU-1-050322	1404	0.2598	-	7471B	PPB	04 May 2022 16:34:57	U	SMPL
N2663-01LX5 - 1		985	0.1841	-	7471B	PPB	04 May 2022 16:37:13	U	SMPL
N2663-01A - 1		29269	5.2898	-	7471B	PPB	04 May 2022 16:39:30	U	SMPL
CCV86 - 1	CCV86	28470	5.1456	-	7471B	PPB	04 May 2022 16:41:46	U	SMPL
CCB86 - 1	CCB86	-52	-0.0031	-	7471B	PPB	04 May 2022 16:44:03	U	SMPL