

LB120005

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

5/5/2022 14:07

Test: CNEPA-NEW

Sample Id	Result	Dil. 1 +	Response	Errors
ICV001 ICV001	92.260	0.0	0.097	
ICB001 ICB001	1.071	0.0	0.008	
CCV001 CCV001	237.487	0.0	0.238	
CCB001 CCB001	0.979	0.0	0.008	
PB144608BL PBS608	0.829	0.0	0.008	
N2700-01 BGBP8	0.740	0.0	0.008	
N2700-02 BGBP8D	0.887	0.0	0.008	
N2700-03 BGBP8S	82.923	0.0	0.088	
N2700-04 BGBP9	6.872	0.0	0.014	
N2700-05 BGBQ0	2.353	0.0	0.009	
N2700-06 BGBQ1	2.117	0.0	0.009	
N2700-07 BGBQ2	6.694	0.0	0.014	
CCV002 CCV002	246.844	0.0	0.247	
CCB002 CCB002	1.332	0.0	0.008	

N	14
Mean	48.813
SD	87.4729
CV%	179.20

Aquakem v. 7.2AQ1

Results from time period:

Thu May 05 13:51:16 2022

Thu May 05 13:58:32 2022

Sample Id	Sam/Ctr/c/	Test short Test type	Result	Result unit	Result date and time
S0.0	A	CNEPA-NE\ P	0.6322	µg/l	5/5/2022 12:02:10
S5.0	A	CNEPA-NE\ P	5.6354	µg/l	5/5/2022 12:02:11
S10.0	A	CNEPA-NE\ P	10.2742	µg/l	5/5/2022 12:02:12
S100.0	A	CNEPA-NE\ P	97.5316	µg/l	5/5/2022 12:02:13
S250.0	A	CNEPA-NE\ P	250.8894	µg/l	5/5/2022 12:02:14
S500.0	A	CNEPA-NE\ P	500.0371	µg/l	5/5/2022 12:02:15
ICV001 ICV001	S	CNEPA-NE\ P	92.2598	µg/l	5/5/2022 13:51:17
ICB001 ICB001	S	CNEPA-NE\ P	1.0706	µg/l	5/5/2022 13:51:18
CCV001 CCV001	S	CNEPA-NE\ P	237.4867	µg/l	5/5/2022 13:51:21
CCB001 CCB001	S	CNEPA-NE\ P	0.9785	µg/l	5/5/2022 13:51:23
PB144608BL PBS608	S	CNEPA-NE\ P	0.8291	µg/l	5/5/2022 13:51:25
N2700-01 BGBP8	S	CNEPA-NE\ P	0.7397	µg/l	5/5/2022 13:51:26
N2700-02 BGBP8D	S	CNEPA-NE\ P	0.8869	µg/l	5/5/2022 13:58:23
N2700-03 BGBP8S	S	CNEPA-NE\ P	82.9232	µg/l	5/5/2022 13:58:24
N2700-04 BGBP9	S	CNEPA-NE\ P	6.8719	µg/l	5/5/2022 13:58:26
N2700-05 BGBQ0	S	CNEPA-NE\ P	2.3534	µg/l	5/5/2022 13:58:27
N2700-06 BGBQ1	S	CNEPA-NE\ P	2.1174	µg/l	5/5/2022 13:58:28
N2700-07 BGBQ2	S	CNEPA-NE\ P	6.6935	µg/l	5/5/2022 13:58:29
CCV002 CCV002	S	CNEPA-NE\ P	246.8444	µg/l	5/5/2022 13:58:30
CCB002 CCB002	S	CNEPA-NE\ P	1.3322	µg/l	5/5/2022 13:58:31

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

5/5/2022 12:04


Test CNEPA-NEW

Accepted 5/5/2022 12:04

~~Factor~~ slope ~~1030~~ 0.000971 12
~~Bias~~ Y-intercept 0.007 5/6/22

Coeff. of det. 0.999961

Errors

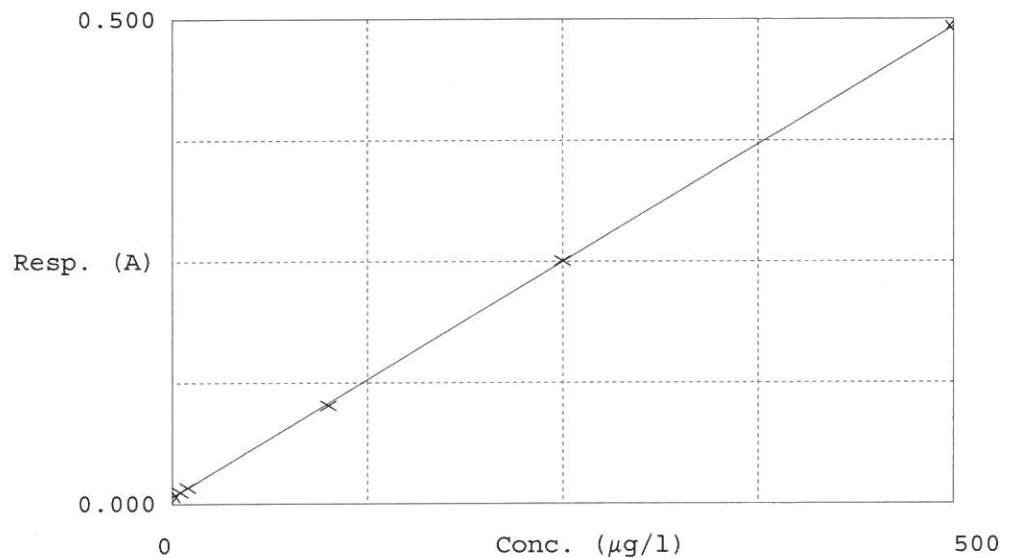

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.008	0.6322	0.0000	-
2	5.0PPBCN	0.012	5.6354	5.0000	12.7
3	10PPBCN	0.017	10.2742	10.0000	2.7
4	100PPBCN	0.102	97.5316	100.0000	-2.5
5	250PPBCN	0.251	250.8894	250.0000	0.4
6	500PPBCN	0.493	500.0371	500.0000	0.0

12
5/5/22