

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

5/6/2022 13:34

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.900	0.0	0.080	
ICB1	0.928	0.0	0.001	
CCV1	247.052	0.0	0.207	
CCB1	0.989	0.0	0.001	
PB144613BL	0.868	0.0	0.001	
N2663-02	1.025	0.0	0.001	
N2663-02DUP	0.778	0.0	0.001	
N2684-01	0.943	0.0	0.001	
N2684-03	0.998	0.0	0.001	
N2685-07	1.054	0.0	0.001	
N2694-01	0.913	0.0	0.001	
N2694-02	1.038	0.0	0.001	
N2694-03	0.908	0.0	0.001	
N2703-02	0.949	0.0	0.001	
CCV2	247.100	0.0	0.207	
CCB2	1.539	0.0	0.001	
N2703-05	0.745	0.0	0.001	
N2703-08	0.770	0.0	0.001	
N2723-02	0.882	0.0	0.001	
N2723-04	0.897	0.0	0.001	
N2723-06	1.002	0.0	0.001	
CCV3	253.770	0.0	0.213	
CCB3	1.028	0.0	0.001	
PB144616BL	0.688	0.0	0.001	
N2694-05	0.835	0.0	0.001	
N2694-06	0.699	0.0	0.001	
N2705-01	0.644	0.0	0.001	
N2712-13	0.855	0.0	0.001	
N2694-04	0.838	0.0	0.001	
N2694-04DUP	1.044	0.0	0.001	
CCV4	258.500	0.0	0.217	
CCB4	1.009	0.0	0.001	

N	32
Mean	35.193
SD	84.7595
CV%	240.84

Aquakem v. 7.2AQ1

Results from time period:

Fri May 06 10:00:21 2022

Fri May 06 13:31:13 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.6262	µg/l	5/6/2022 10:00:21	
5.OPPBCN	A	Total CN	P	5.3783	µg/l	5/6/2022 10:00:22	
10PPBCN	A	Total CN	P	10.3412	µg/l	5/6/2022 10:00:23	
50PPBCN	A	Total CN	P	48.6945	µg/l	5/6/2022 10:00:24	
100PPBCN	A	Total CN	P	98.4852	µg/l	5/6/2022 10:00:25	
250PPBCN	A	Total CN	P	252.1035	µg/l	5/6/2022 10:00:26	
500PPBCN	A	Total CN	P	499.3712	µg/l	5/6/2022 10:00:27	
ICV1	S	Total CN	P	94.8996	µg/l	5/6/2022 12:26:36	
ICB1	S	Total CN	P	0.9281	µg/l	5/6/2022 12:26:37	
CCV1	S	Total CN	P	247.0517	µg/l	5/6/2022 12:26:39	
CCB1	S	Total CN	P	0.9894	µg/l	5/6/2022 12:26:42	
PB144613BL	S	Total CN	P	0.8683	µg/l	5/6/2022 12:26:43	
N2663-02	S	Total CN	P	1.0249	µg/l	5/6/2022 12:26:45	
N2663-02DUP	S	Total CN	P	0.7784	µg/l	5/6/2022 12:34:08	
N2684-01	S	Total CN	P	0.943	µg/l	5/6/2022 12:34:09	
N2684-03	S	Total CN	P	0.9977	µg/l	5/6/2022 12:34:10	
N2685-07	S	Total CN	P	1.0543	µg/l	5/6/2022 12:34:11	
N2694-01	S	Total CN	P	0.9132	µg/l	5/6/2022 12:34:12	
N2694-02	S	Total CN	P	1.0382	µg/l	5/6/2022 12:34:13	
N2694-03	S	Total CN	P	0.9075	µg/l	5/6/2022 12:34:14	
N2703-02	S	Total CN	P	0.9491	µg/l	5/6/2022 12:34:15	
CCV2	S	Total CN	P	247.0996	µg/l	5/6/2022 12:34:17	
CCB2	S	Total CN	P	1.5393	µg/l	5/6/2022 12:34:18	
N2703-05	S	Total CN	P	0.7453	µg/l	5/6/2022 12:39:51	
N2703-08	S	Total CN	P	0.7698	µg/l	5/6/2022 12:39:52	
N2723-02	S	Total CN	P	0.8821	µg/l	5/6/2022 12:39:53	
N2723-04	S	Total CN	P	0.8974	µg/l	5/6/2022 12:39:54	
N2723-06	S	Total CN	P	1.0024	µg/l	5/6/2022 12:39:55	
CCV3	S	Total CN	P	253.7698	µg/l	5/6/2022 12:39:56	
CCB3	S	Total CN	P	1.0276	µg/l	5/6/2022 12:39:57	
PB144616BL	S	Total CN	P	0.6883	µg/l	5/6/2022 13:14:15	
N2694-05	S	Total CN	P	0.8347	µg/l	5/6/2022 13:14:18	
N2694-06	S	Total CN	P	0.6986	µg/l	5/6/2022 13:14:19	
N2705-01	S	Total CN	P	0.6444	µg/l	5/6/2022 13:14:20	
N2712-13	S	Total CN	P	0.8547	µg/l	5/6/2022 13:14:21	
N2694-04	S	Total CN	P	0.8379	µg/l	5/6/2022 13:31:10	
N2694-04DUP	S	Total CN	P	1.0445	µg/l	5/6/2022 13:31:11	
CCV4	S	Total CN	P	258.5004	µg/l	5/6/2022 13:31:12	
CCB4	S	Total CN	P	1.0086	µg/l	5/6/2022 13:31:13	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

5/6/2022 10:12


Test Total CN

Accepted 5/6/2022 10:12

Factor 1192
Bias 0

Coeff. of det. 0.999954

Errors

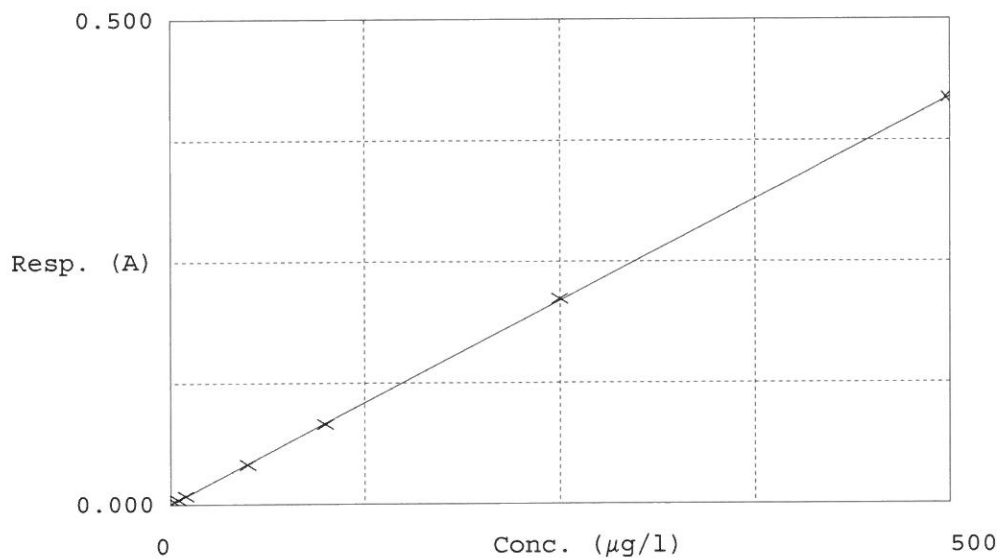

	Calibrator	Response	Calc. con.	Conc.
1	0.0PPBCN	0.001	0.6262	0.0000
2	5.0PPBCN	0.005	5.3783	5.0000
3	10PPBCN	0.009	10.3412	10.0000
4	50PPBCN	0.041	48.6945	50.0000
5	100PPBCN	0.083	98.4852	100.0000
6	250PPBCN	0.212	252.1035	250.0000
7	500PPBCN	0.419	499.3712	500.0000

Re
Errors

-
7.6
3.4
-2.6
-1.5
0.8
-0.1

12
5/6/22