

Clear table

Instrument ID: IC-2										Method:		300.0 / 9056A	
Analyst :										IZ			
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2022-05-02_	5/2/22 18:52		IZ/AP		
STD2	0.4800	0.6730	0.6800	2.2400	0.5710	0.8610	3.5240	0.0000_2022-05-02_	5/2/22 19:21		IZ/AP		
STD3	0.7880	1.2100	1.2100	4.0800	1.0150	1.9540	6.0900	0.0000_2022-05-02_	5/2/22 19:49		IZ/AP		
STD4	1.0150	1.5080	1.4910	4.9920	1.2540	2.6070	7.4970	0.0000_2022-05-02_	5/2/22 20:18		IZ/AP		
STD5	1.9110	2.8980	2.9060	9.6240	2.3960	5.1400	14.2900	0.0000_2022-05-02_	5/2/22 20:47		IZ/AP		
STD6	3.9170	5.9180	5.9280	19.7860	4.9280	10.0090	29.5290	0.0000_2022-05-02_	5/2/22 21:15		IZ/AP		
STD7	5.0890	7.5940	7.5850	25.2780	6.3360	12.4290	38.0700	0.0000_2022-05-02_	5/2/22 21:44		IZ/AP		
ICV	1.9270	2.8530	2.8790	9.4870	2.3700	5.2080	14.0930	0.0000_2022-05-02_	5/2/22 22:13		IZ/AP		
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2022-05-02_	5/2/22 22:41		IZ/AP		
CCV	1.8130	2.8090	2.8200	9.3340	2.3250	4.7530	13.7330	0.0000_2022-05-06_	5/6/22 9:23		IZ/AP		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2022-05-06_	5/6/22 9:59		IZ/AP		
LB120044BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2022-05-06_	5/6/22 10:28		IZ/AP		
LB120044BSW	1.8410	2.7920	2.8270	9.2250	2.3080	5.0730	13.6360	0.0000_2022-05-06_	5/6/22 10:58		IZ/AP		
N2705-01	0.3930	153.9130	0.0000	0.0000	0.3280	0.0000	40.4640	0.0000_2022-05-06_	5/6/22 12:56		IZ/AP		
N2712-13	0.2190	9.6810	0.0000	0.0000	0.5040	0.0000	17.8930	0.0000_2022-05-06_	5/6/22 13:25		IZ/AP		
N2730-01	0.0000	0.0000	0.1410	0.0000	0.2300	0.0000	0.0000	0.0000_2022-05-06_	5/6/22 13:55		IZ/AP		
N2730-01MS	2.1330	2.9840	2.9480	9.3810	2.5480	6.0120	14.3110	0.0000_2022-05-06_	5/6/22 14:25		IZ/AP		
N2730-01MSD	2.0440	2.9130	2.9150	9.5150	2.4980	5.8030	13.9980	0.0000_2022-05-06_	5/6/22 14:54		IZ/AP		
CCV	1.9030	2.8210	2.8340	9.4240	2.3530	5.4260	13.8070	0.0000_2022-05-06_	5/6/22 15:24		IZ/AP		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2022-05-06_	5/6/22 15:54		IZ/AP		
N2741-01	0.3060	99.4240	0.0000	0.0000	1.9500	0.0000	31.5990	0.0000_2022-05-06_	5/6/22 16:24		IZ/AP		
CCV	1.8780	2.8140	2.8300	9.4050	2.3400	5.8630	13.7640	0.0000_2022-05-06_	5/6/22 16:54		IZ/AP		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2022-05-06_	5/6/22 17:23		IZ/AP		

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A


ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-05-02_	5/2/22 18:52		IZ/AP
STD2	0.4800	0.6730	0.6800	2.2400	0.5710	0.8610	3.5240	2022-05-02_	5/2/22 19:21		IZ/AP
STD3	0.7880	1.2100	1.2100	4.0800	1.0150	1.9540	6.0900	2022-05-02_	5/2/22 19:49		IZ/AP
STD4	1.0150	1.5080	1.4910	4.9920	1.2540	2.6070	7.4970	2022-05-02_	5/2/22 20:18		IZ/AP
STD5	1.9110	2.8980	2.9060	9.6240	2.3960	5.1400	14.2900	2022-05-02_	5/2/22 20:47		IZ/AP
STD6	3.9170	5.9180	5.9280	19.7860	4.9280	10.0090	29.5290	2022-05-02_	5/2/22 21:15		IZ/AP
STD7	5.0890	7.5940	7.5850	25.2780	6.3360	12.4290	38.0700	2022-05-02_	5/2/22 21:44		IZ/AP

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1	20.0000	12.1667	13.3333	12.0000	14.2000	-13.9000	17.4667
STD2	-1.5000	0.8333	0.8333	2.0000	1.5000	-2.3000	1.5000
STD3	1.5000	0.5333	-0.6000	-0.1600	0.3200	4.2800	-0.0400
STD4	-4.4500	-3.4000	-3.1333	-3.7600	-4.1600	2.8000	-4.7333
STD5	-2.0750	-1.3667	-1.2000	-1.0700	-1.4400	0.0900	-1.5700
STD6	1.7800	1.2533	1.1333	1.1120	1.3760	-0.5680	2.8919

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-050222.mtw
 Equation: $Q = 0.0670392 \cdot A + 3.11724$
 RSD: 3.903 %
 Correlation coefficient: 0.999170

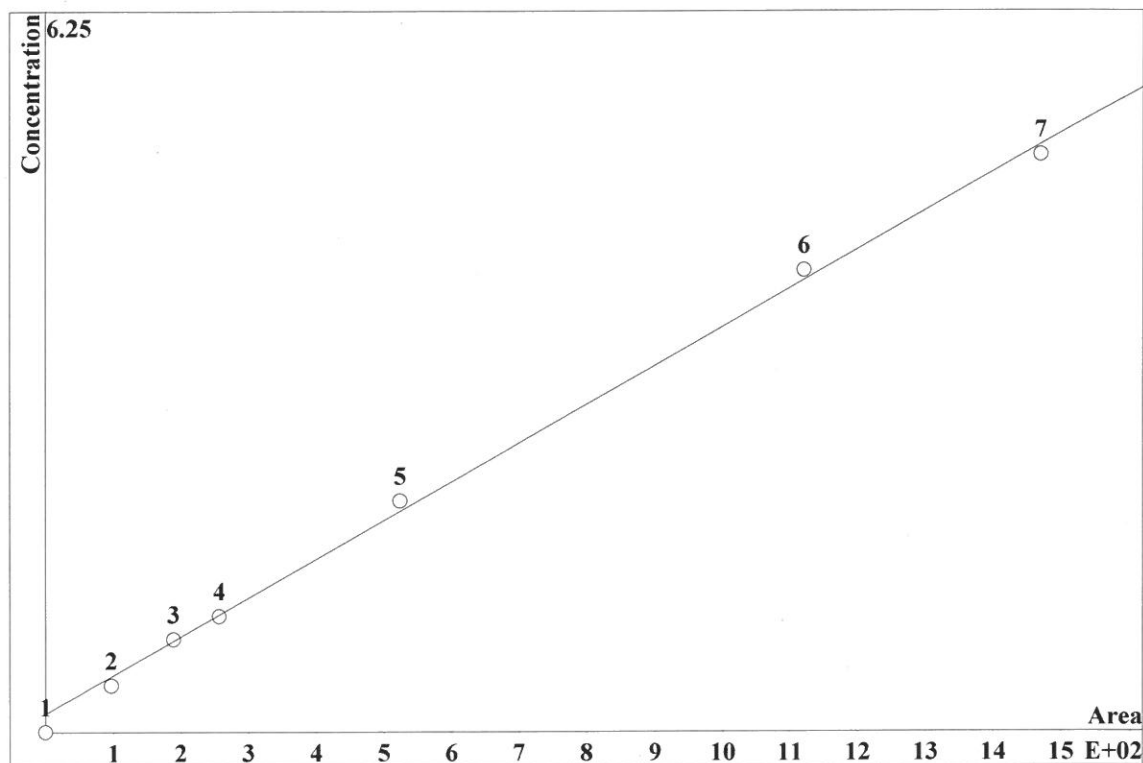


K3 = 0 K2 = 0 K1 = 0.0670392 K0 = 3.11724
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	4.734	96.74	0.4	20	5.653	
3	10.89	188.6	0.8	20	5.653	
4	14.79	256.4	1	20	5.653	
5	31.98	523.5	2	20	5.653	
6	75.3	1122	4	20	5.653	
7	100	1472	5	20	5.653	

1.□

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-050222.mtw
 Equation: $Q = 0.113802 \cdot A + 2.786$
 RSD: 2.688 %
 Correlation coefficient: 0.999606

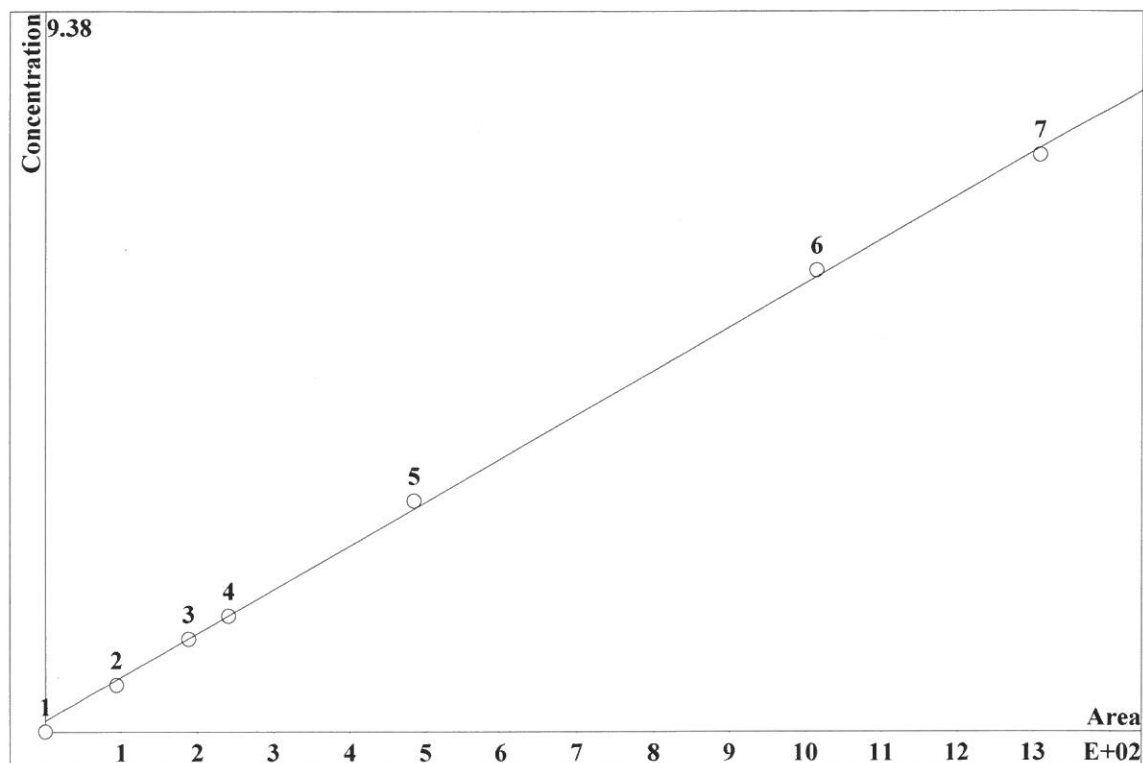

K3 = 0 K2 = 0 K1 = 0.113802 K0 = 2.786

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear


Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.381	93.75	0.6	20	8.643		
3	12.71	188.2	1.2	20	8.643		
4	16.09	240.6	1.5	20	8.643		
5	32.86	484.8	3	20	8.643		
6	70.2	1015	6	20	8.643		
7	89.94	1310	7.5	20	8.643		

*□

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-050222.mtw
 Equation: $Q = 0.0498924 \cdot A + 2.19052$
 RSD: 2.524 %
 Correlation coefficient: 0.999653

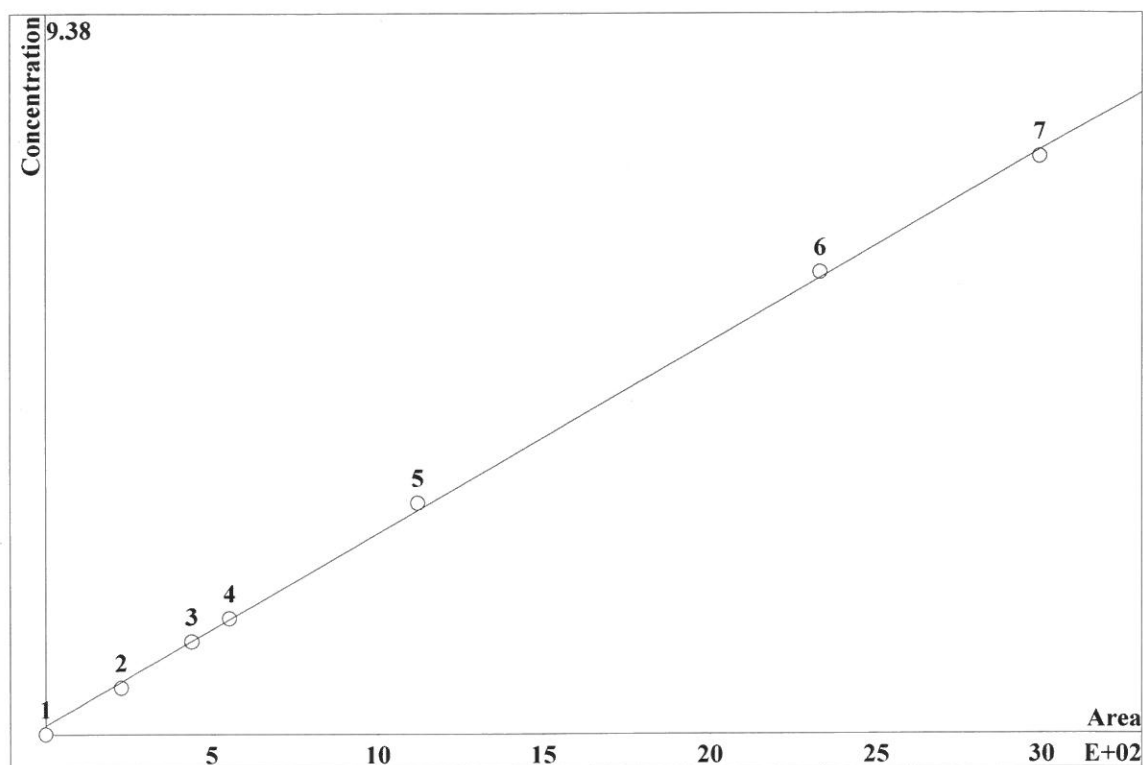


K3 = 0 K2 = 0 K1 = 0.0498924 K0 = 2.19052
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	11.96	228.5	0.6	20	10.45		
3	23.58	441.1	1.2	20	10.45		
4	29.95	553.8	1.5	20	10.45		
5	60.75	1121	3	20	10.45		
6	122.8	2332	6	20	10.45		
7	156	2997	7.5	20	10.45		

□c□

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-050222.mtw
 Equation: $Q = 0.254663 \cdot A + 10.3732$
 RSD: 2.608 %
 Correlation coefficient: 0.999629

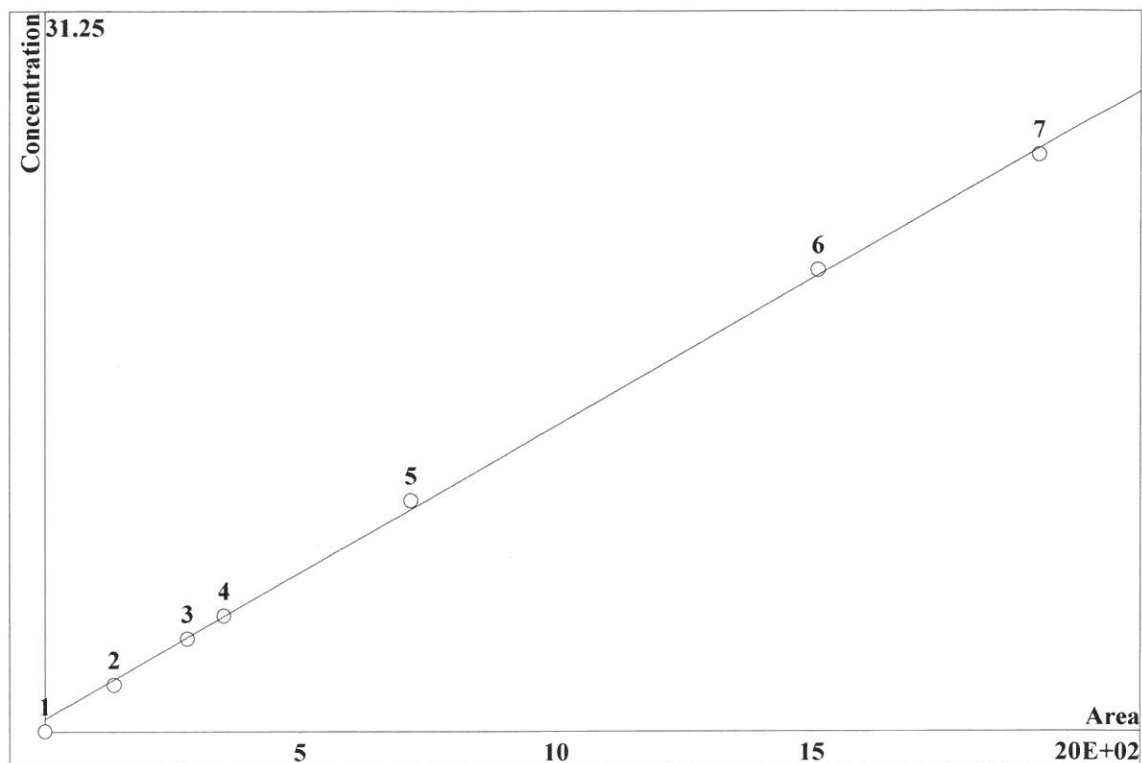

K3 = 0 K2 = 0 K1 = 0.254663 K0 = 10.3732

Base: Area

Ref.channel: chl

ISTD:

Formula: Linear


Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.627	135.2	2	20	13.53		
3	13.52	279.7	4	20	13.53		
4	17.1	351.3	5	20	13.53		
5	35.08	715.1	10	20	13.53		
6	74.18	1513	20	20	13.53		
7	94.44	1945	25	20	13.53		

|□□

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-050222.mtw
 Equation: $Q = 0.0444009 \cdot A + 2.79396$
 RSD: 3.071 %
 Correlation coefficient: 0.999486

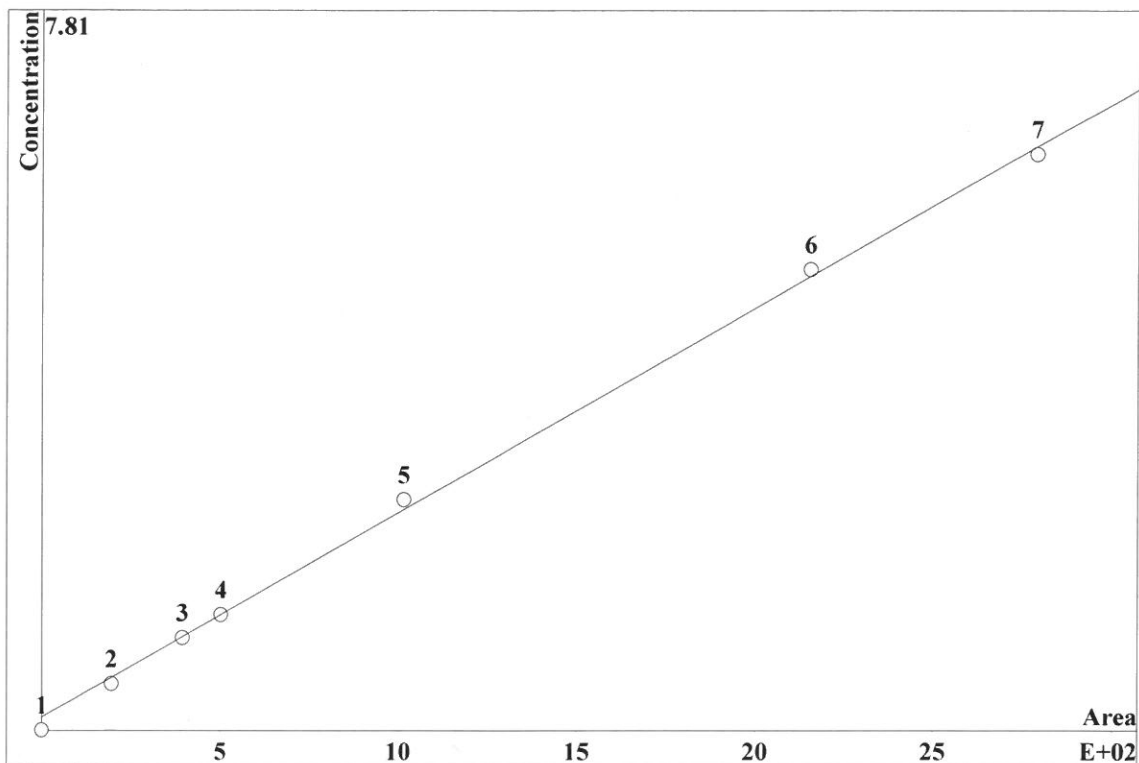

K3 = 0 K2 = 0 K1 = 0.0444009 K0 = 2.79396

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.981	194.3	0.5	20	15.58		
3	16.09	394.5	1	20	15.58		
4	20.37	501.8	1.25	20	15.58		
5	41.68	1016	2.5	20	15.58		
6	88.86	2157	5	20	15.58		
7	114.3	2791	6.25	20	15.58		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-050222.mtw
 Equation: $Q = 0.0826373 \cdot A - 0.871753$
 RSD: 2.181 %
 Correlation coefficient: 0.999741

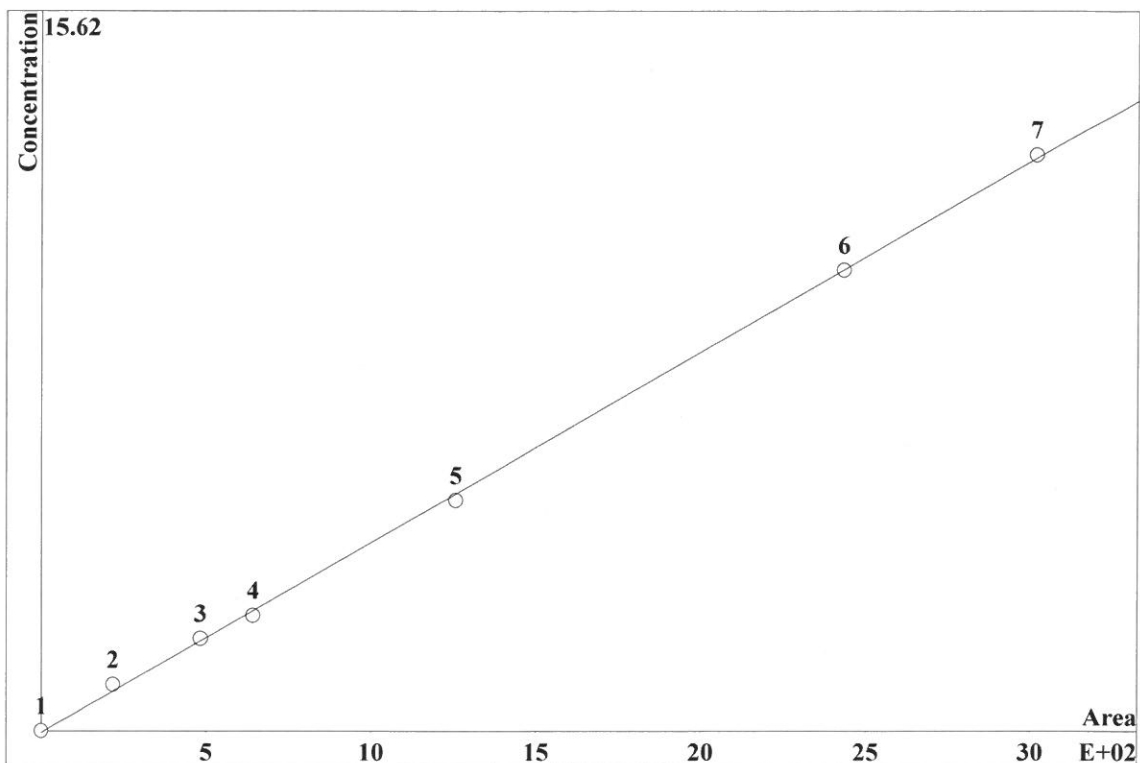

K3 = 0 K2 = 0 K1 = 0.0826373 K0 = -0.871753

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	5.561	218.8	1	20	20.18		
3	12.61	483.6	2	20	20.18		
4	16.77	641.4	2.5	20	20.18		
5	34.26	1255	5	20	20.18		
6	69.58	2433	10	20	20.18		
7	87.09	3019	12.5	20	20.18		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-050222.mtw
 Equation: $Q = 0.145911 \cdot A + 14.1785$
 RSD: 3.499 %
 Correlation coefficient: 0.999332

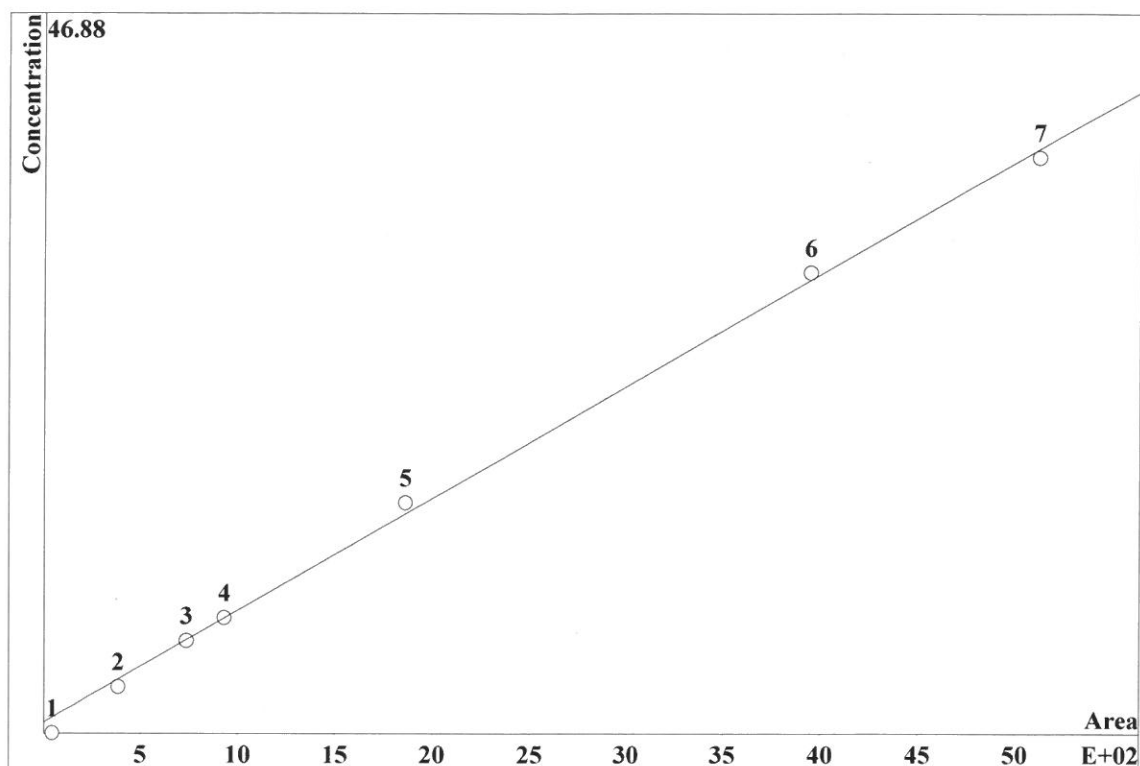

K3 = 0 K2 = 0 K1 = 0.145911 K0 = 14.1785

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	1.157	45.41	0	20	23.09		
2	11.82	385.9	3	20	23.09		
3	23.13	737.5	6	20	23.09		
4	29.3	930.5	7.5	20	23.09		
5	59.9	1862	15	20	23.09		
6	129.2	3950	30	20	23.09		
7	167.1	5121	37.5	20	23.09		

e

Report date: 5/3/2022 9:30:50 AM
Printed by: wet


Ident: STD1
Analysis from: 5/2/2022 6:52:44 PM
File: _2022-05-02_

Last save: 5/3/2022 9:17:07 AM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30204

Last save: 5/2/2022 9:41:5

SAMPLE:
: IZ/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

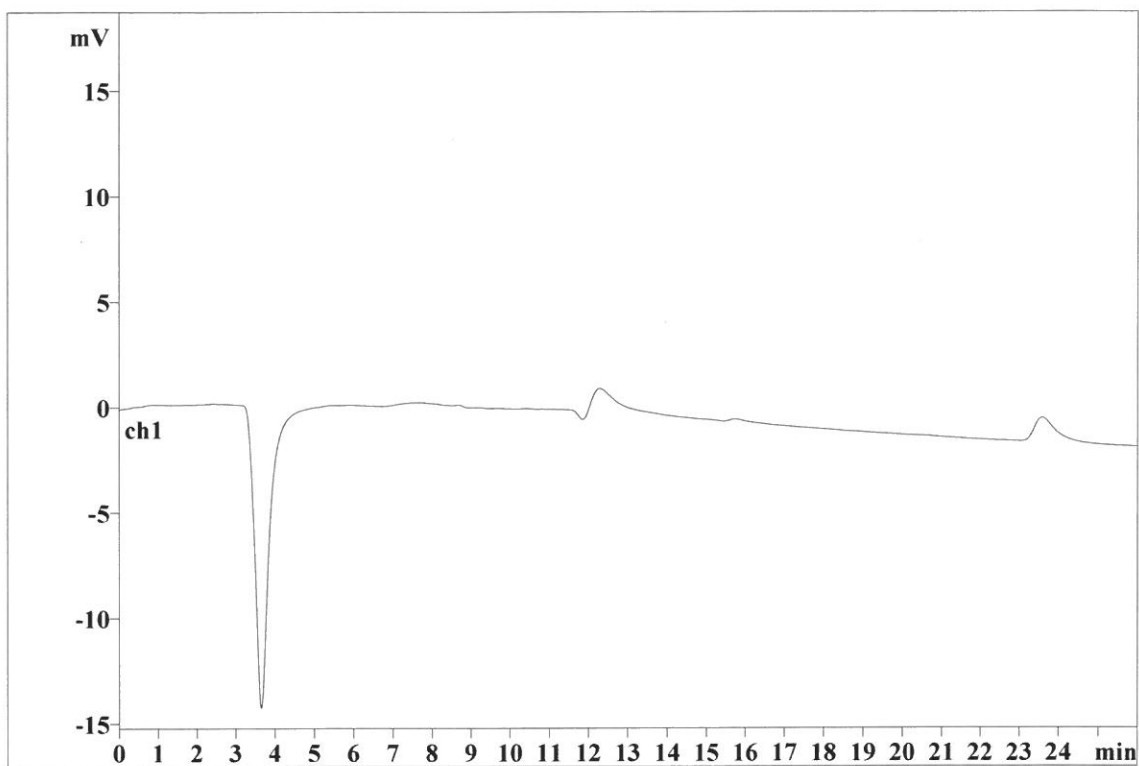

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 5/3/2022 9:31:02 AM
Printed by: wet


Ident: STD2
Analysis from: 5/2/2022 7:21:22 PM
File: _2022-05-02_

Last save: 5/3/2022 9:17:07 AM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30205

Last save: 5/2/2022 9:41:5

SAMPLE:
: IZ/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

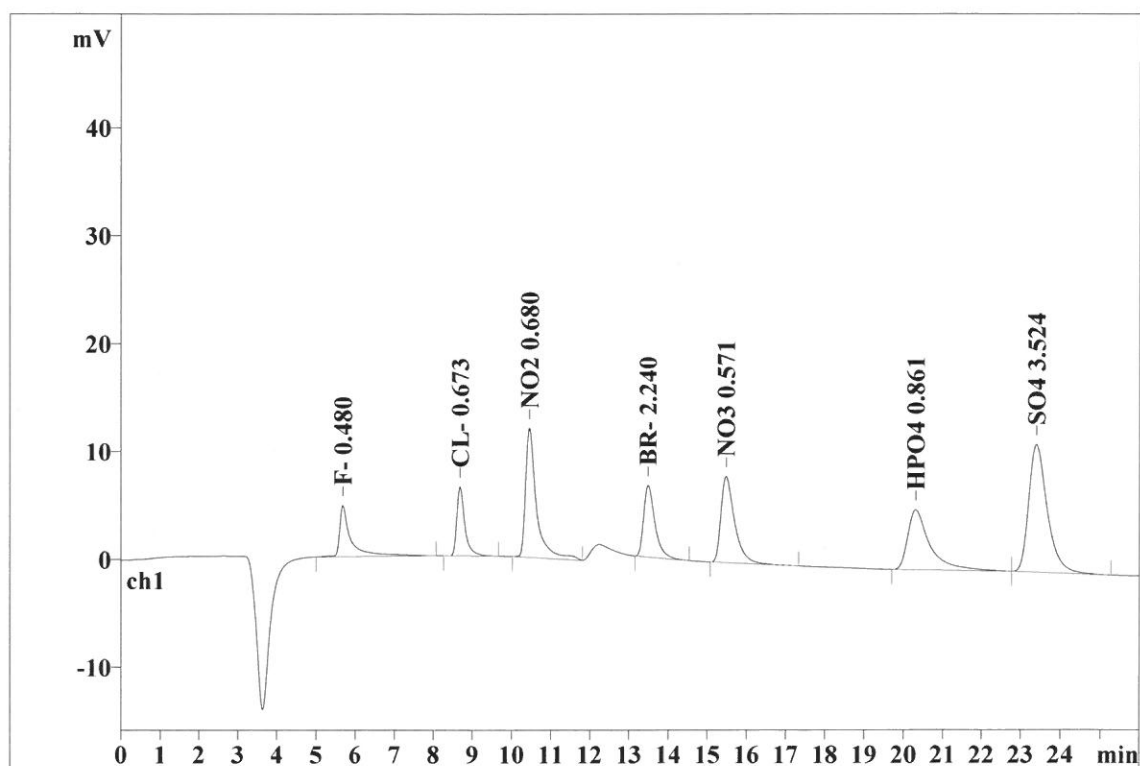

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.68	0.211	4.73	8.60	96.740	7.15
2	8.67	0.207	6.38	11.58	93.753	6.93
3	10.45	0.246	11.96	21.72	228.538	16.89
4	13.49	0.301	6.63	12.03	135.183	9.99
5	15.48	0.356	7.98	14.49	194.270	14.36
6	20.30	0.529	5.56	10.09	218.838	16.17
7	23.40	0.484	11.82	21.47	385.918	28.52
7	26.00	0.334	55.07	99.99	1353.239	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/3/2022 9:31:19 AM
Printed by: wet


Ident: STD3
Analysis from: 5/2/2022 7:49:59 PM
File: _2022-05-02_

Last save: 5/3/2022 9:17:07 AM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30206

Last save: 5/2/2022 9:41:5

SAMPLE:
: IZ/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

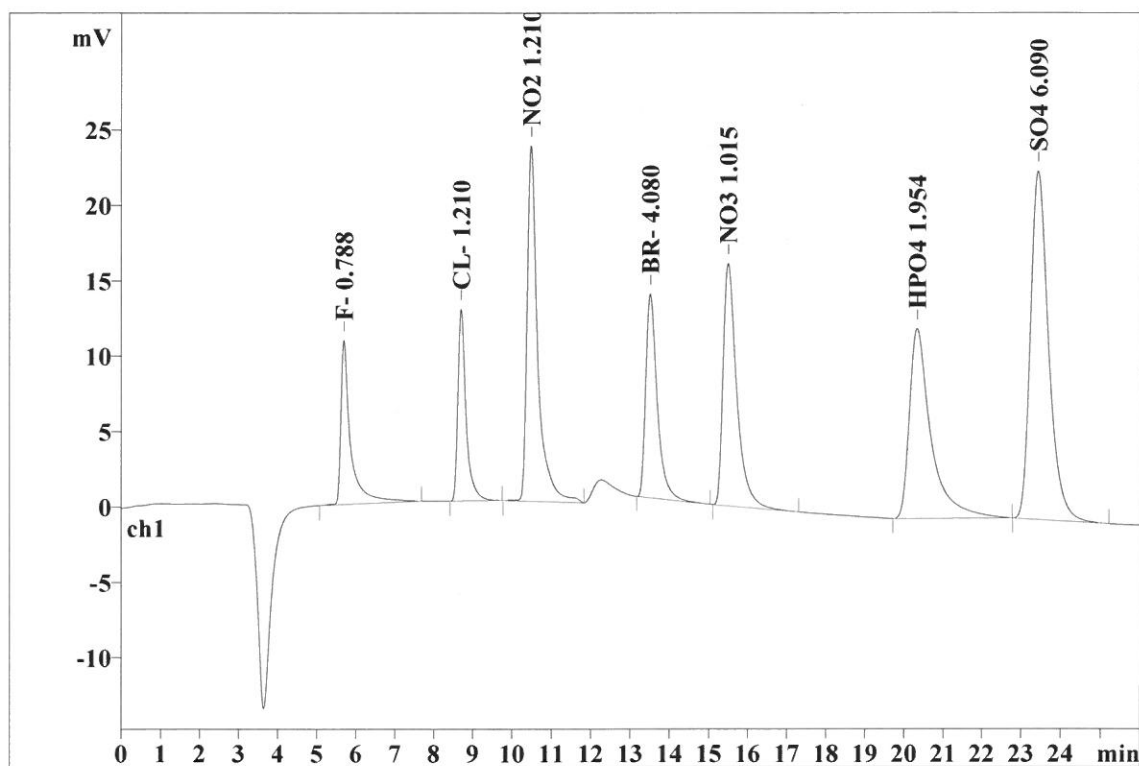

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.69	0.199	10.89	9.67	188.624	6.95
2	8.69	0.209	12.71	11.30	188.217	6.94
3	10.47	0.250	23.58	20.96	441.114	16.26
4	13.50	0.302	13.52	12.02	279.711	10.31
5	15.49	0.357	16.08	14.29	394.471	14.54
6	20.33	0.518	12.61	11.20	483.577	17.82
7	23.43	0.476	23.13	20.55	737.547	27.18
7	26.00	0.330	112.52	99.99	2713.261	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/3/2022 9:31:28 AM
Printed by: wet


Ident: STD4
Analysis from: 5/2/2022 8:18:38 PM
File: _2022-05-02_

Last save: 5/3/2022 9:17:07 AM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30207

Last save: 5/2/2022 9:41:5

SAMPLE:
: IZ/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

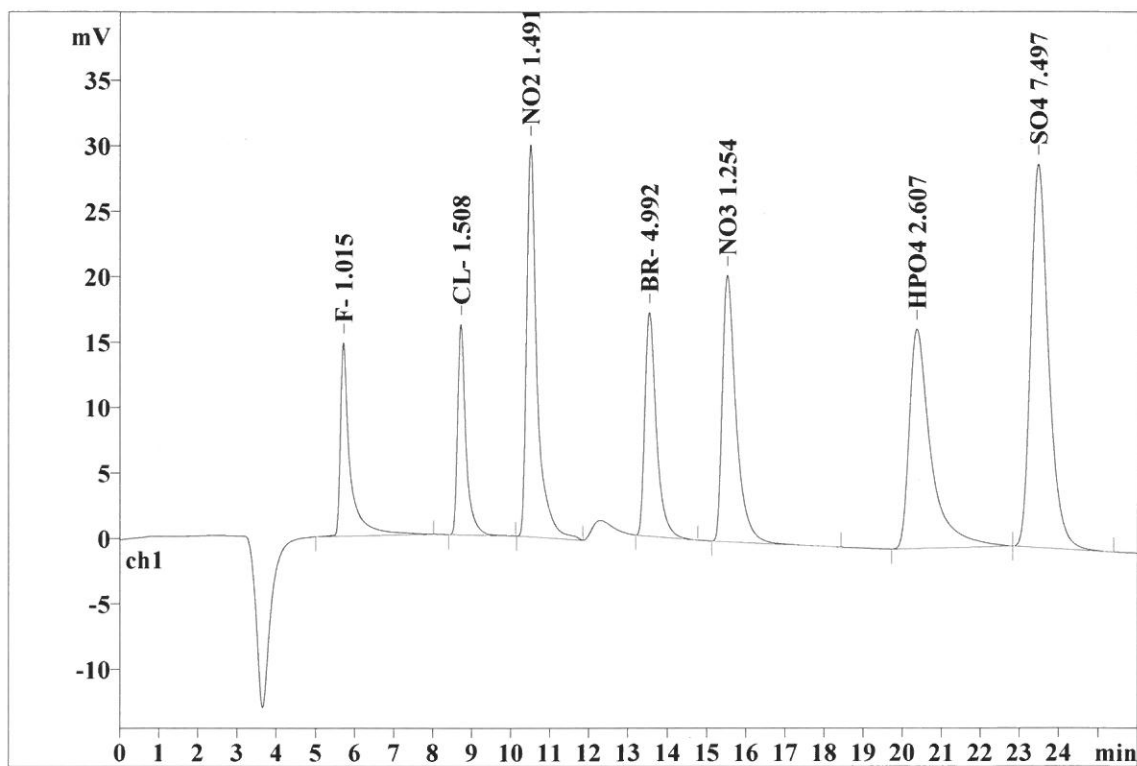

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.70	0.200	14.80	10.25	256.423	7.38
2	8.71	0.209	16.09	11.14	240.554	6.92
3	10.49	0.249	29.95	20.75	553.761	15.93
4	13.54	0.302	17.10	11.85	351.321	10.11
5	15.52	0.358	20.37	14.11	501.780	14.44
6	20.36	0.515	16.77	11.62	641.378	18.45
7	23.47	0.474	29.29	20.29	930.505	26.77
7	26.00	0.330	144.38	100.00	3475.723	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/3/2022 9:31:35 AM
Printed by: wet


Ident: STD5
Analysis from: 5/2/2022 8:47:15 PM
File: _2022-05-02_

Last save: 5/3/2022 9:17:07 AM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30208

Last save: 5/2/2022 9:41:5

SAMPLE: IZ/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

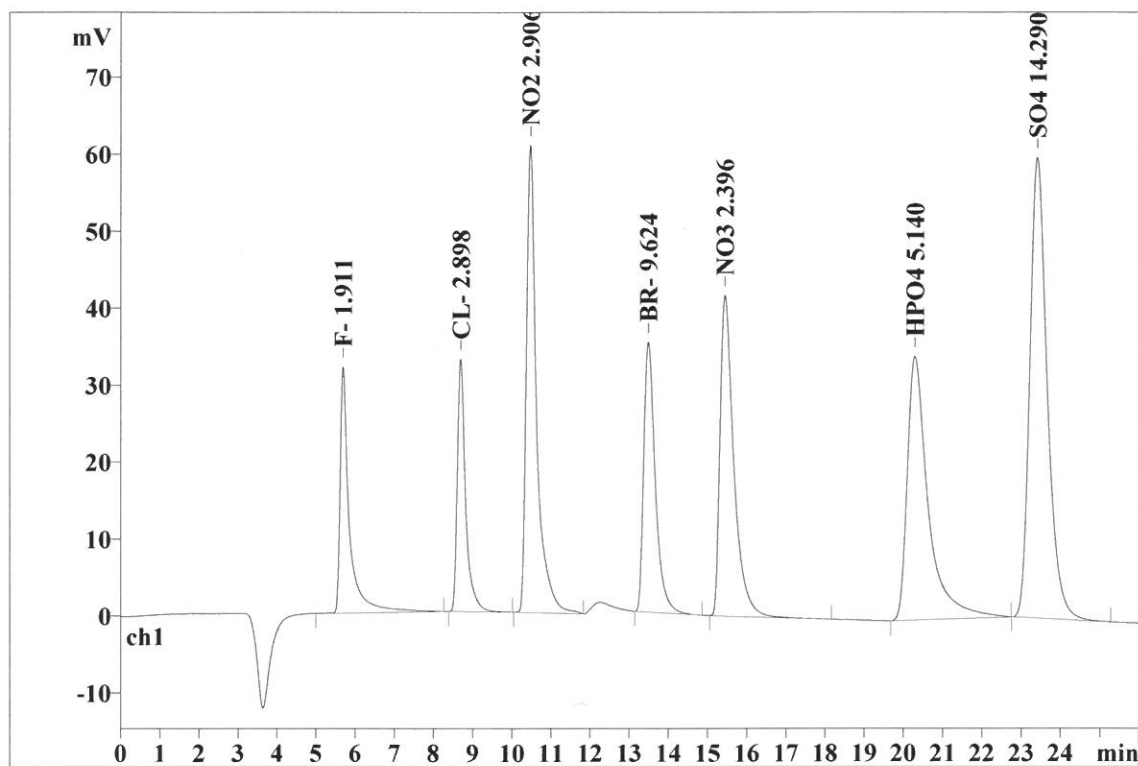

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.68	0.191	31.98	10.79	523.529	7.50
2	8.68	0.207	32.86	11.08	484.781	6.95
3	10.45	0.251	60.75	20.49	1121.069	16.07
4	13.48	0.298	35.08	11.83	715.061	10.25
5	15.43	0.354	41.68	14.06	1016.409	14.57
6	20.28	0.496	34.26	11.55	1254.581	17.98
7	23.39	0.464	59.90	20.20	1861.557	26.68
7	26.00	0.323	296.51	100.00	6976.988	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/3/2022 9:32:02 AM
Printed by: wet


Ident: STD6
Analysis from: 5/2/2022 9:15:54 PM
File: _2022-05-02_

Last save: 5/3/2022 9:17:07 AM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30209

Last save: 5/2/2022 9:41:5

SAMPLE:
: IZ/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

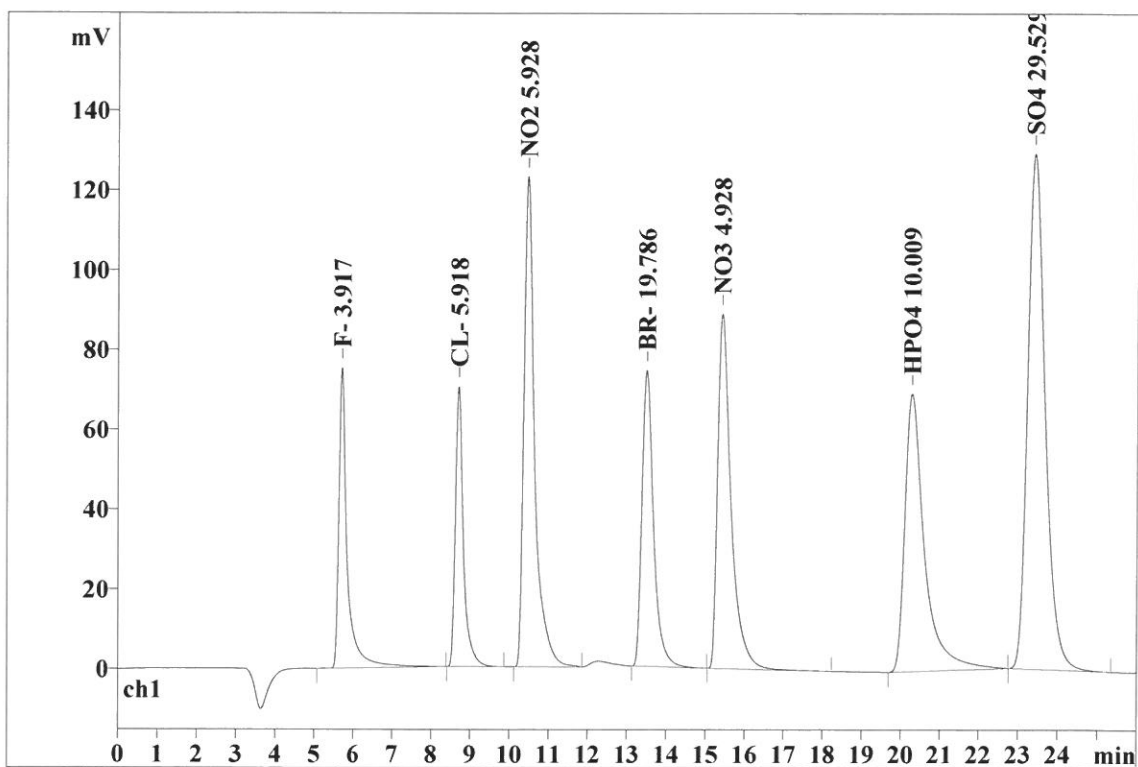

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.69	0.180	75.29	11.95	1122.101	7.73
2	8.69	0.202	70.20	11.14	1015.493	6.99
3	10.45	0.262	122.83	19.49	2332.456	16.06
4	13.49	0.298	74.18	11.77	1513.134	10.42
5	15.42	0.350	88.86	14.10	2156.948	14.85
6	20.28	0.479	69.57	11.04	2432.891	16.75
7	23.41	0.457	129.15	20.50	3950.355	27.20
7	26.00	0.318	630.09	100.00	14523.378	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/3/2022 9:32:12 AM
Printed by: wet


Ident: STD7
Analysis from: 5/2/2022 9:44:32 PM
File: _2022-05-02_

Last save: 5/3/2022 9:17:07 AM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30210

Last save: 5/2/2022 9:41:5

SAMPLE:
: IZ/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

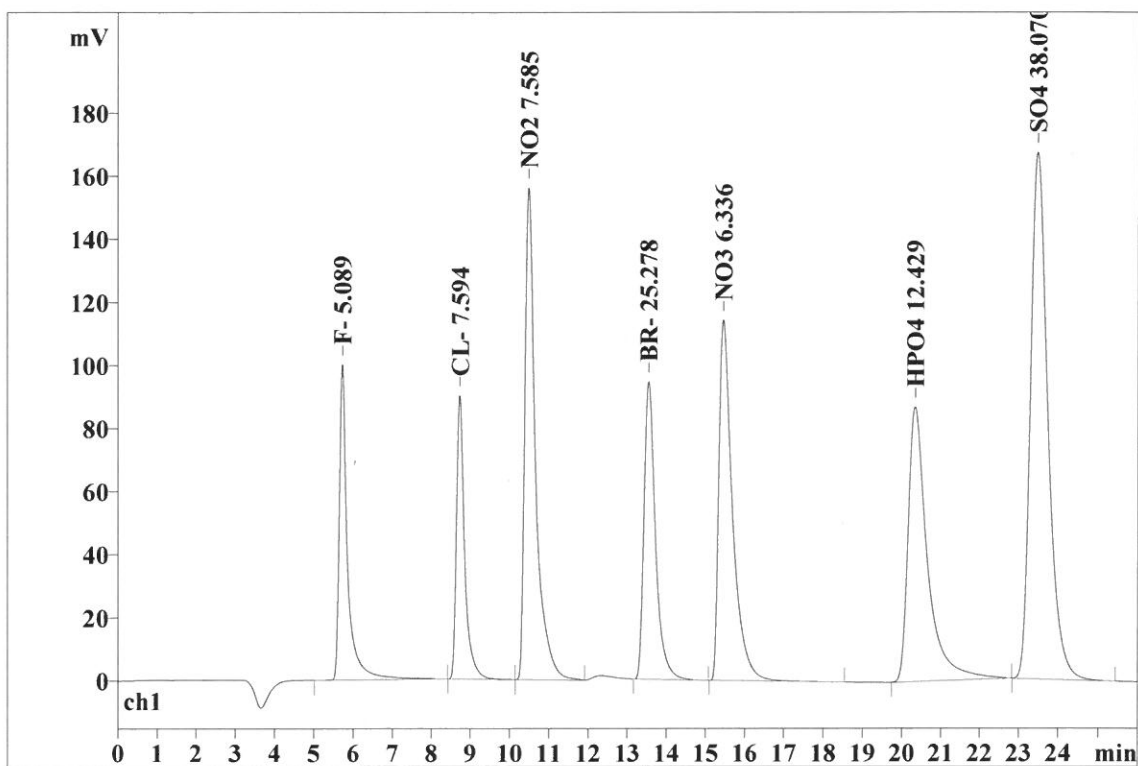

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.182	100.04	12.37	1471.584	7.89
2	8.72	0.203	89.94	11.12	1310.044	7.02
3	10.48	0.265	155.99	19.28	2996.713	16.07
4	13.55	0.301	94.44	11.67	1944.513	10.42
5	15.46	0.351	114.33	14.13	2790.844	14.96
6	20.34	0.476	87.09	10.77	3018.735	16.18
7	23.49	0.458	167.12	20.66	5121.023	27.45
7	26.00	0.320	808.95	100.00	18653.456	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/3/2022 9:32:34 AM
Printed by: wet


Ident: ICV
Analysis from: 5/2/2022 10:13:10 PM
File: _2022-05-02_

Last save: 5/2/2022 10:39:10 PM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30211

Last save: 5/2/2022 10:10:

SAMPLE:
: IZ/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

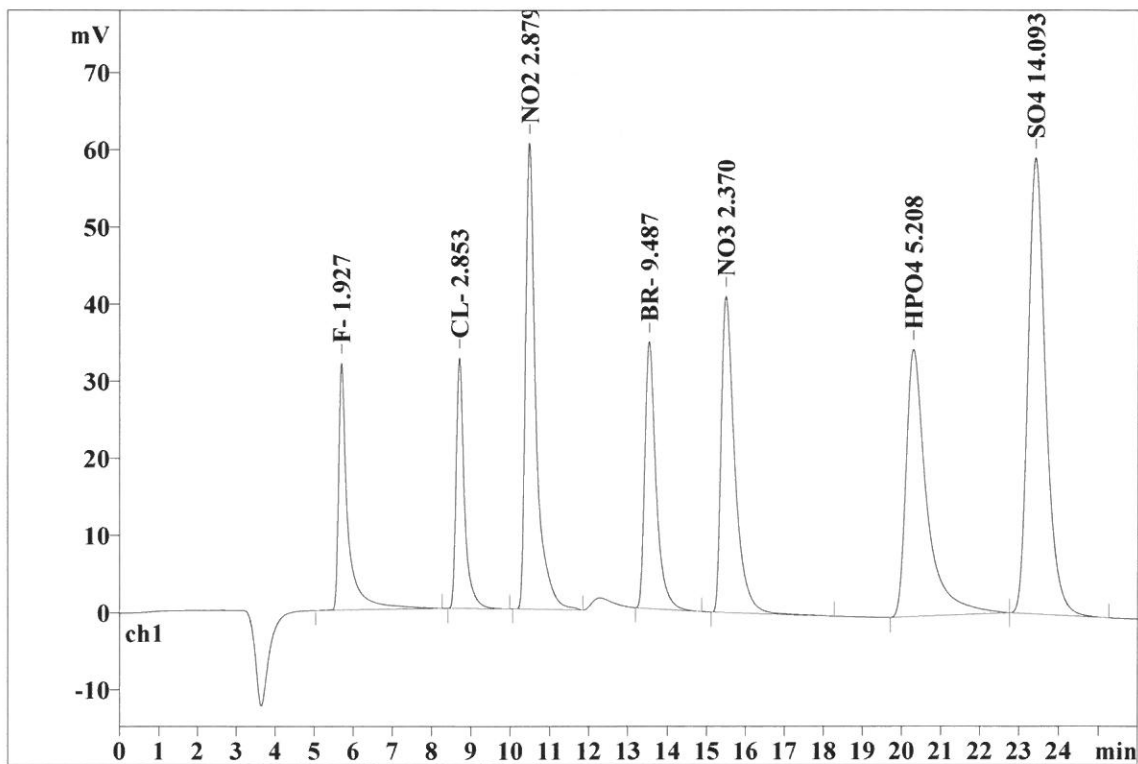

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.69	0.192	32.00	10.87	528.368	7.62
2	8.70	0.206	32.49	11.04	476.870	6.88
3	10.47	0.250	60.43	20.53	1110.239	16.02
4	13.53	0.298	34.60	11.75	704.348	10.16
5	15.49	0.354	41.02	13.93	1004.772	14.50
6	20.30	0.496	34.65	11.77	1271.105	18.34
7	23.41	0.463	59.19	20.11	1834.543	26.47
7	26.00	0.323	294.40	100.00	6930.245	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/3/2022 9:33:10 AM
Printed by: wet


Ident: ICB
Analysis from: 5/2/2022 10:41:47 PM
File: _2022-05-02_

Last save: 5/3/2022 9:33:00 AM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30212

Last save: 5/2/2022 10:10:

SAMPLE:
: IZ/AP
Vial number: 10
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

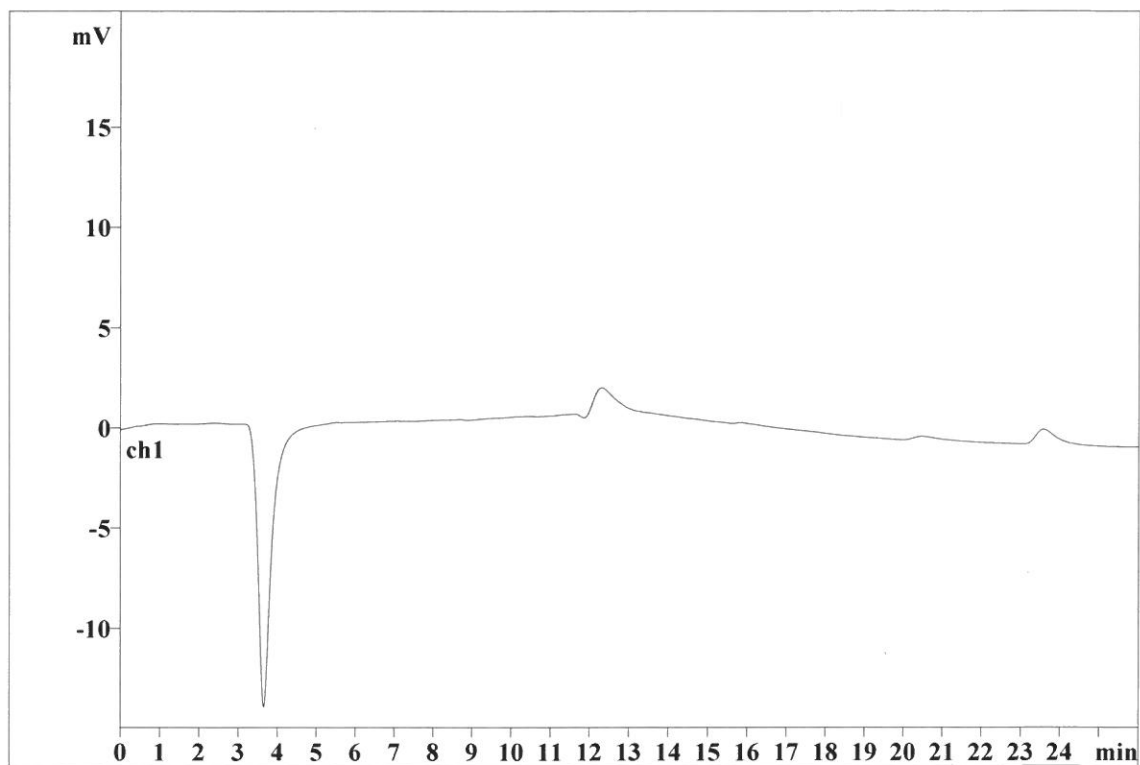

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 5/9/2022 10:11:35 AM
Printed by: wet


Ident: CCV
Analysis from: 5/6/2022 9:23:59 AM
File: _2022-05-06_

Last save: 5/6/2022 9:56:24 AM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30255

Last save: 5/4/2022 10:08:

SAMPLE:
: IZ/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

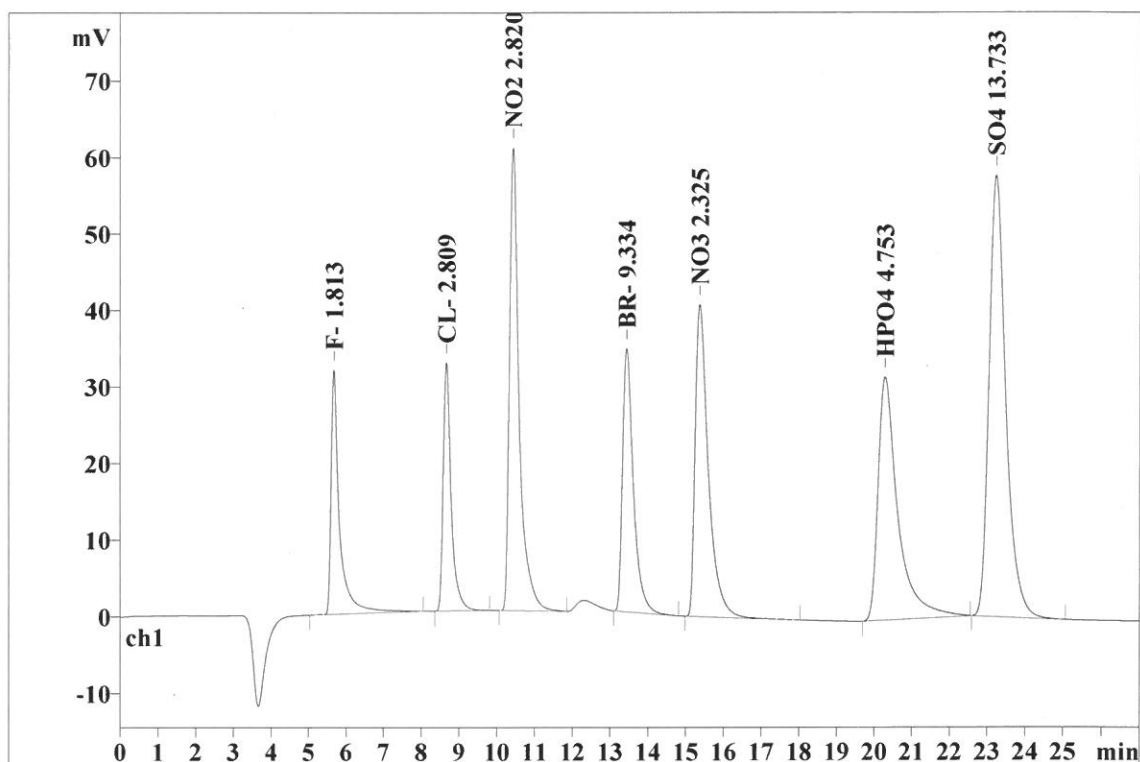

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.68	0.186	31.87	11.01	494.324	7.41
2	8.66	0.203	32.42	11.20	469.182	7.03
3	10.43	0.249	60.50	20.90	1086.377	16.28
4	13.44	0.295	34.42	11.89	692.349	10.38
5	15.37	0.349	40.81	14.10	984.446	14.75
6	20.29	0.497	31.76	10.97	1160.852	17.40
7	23.24	0.459	57.68	19.93	1785.270	26.75
7	27.00	0.320	289.46	100.00	6672.799	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/9/2022 10:11:43 AM
Printed by: wet


Ident: CCB
Analysis from: 5/6/2022 9:59:16 AM
File: _2022-05-06_

Last save: 5/6/2022 10:26:16 AM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30256

Last save: 5/4/2022 10:08:

SAMPLE:
: IZ/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

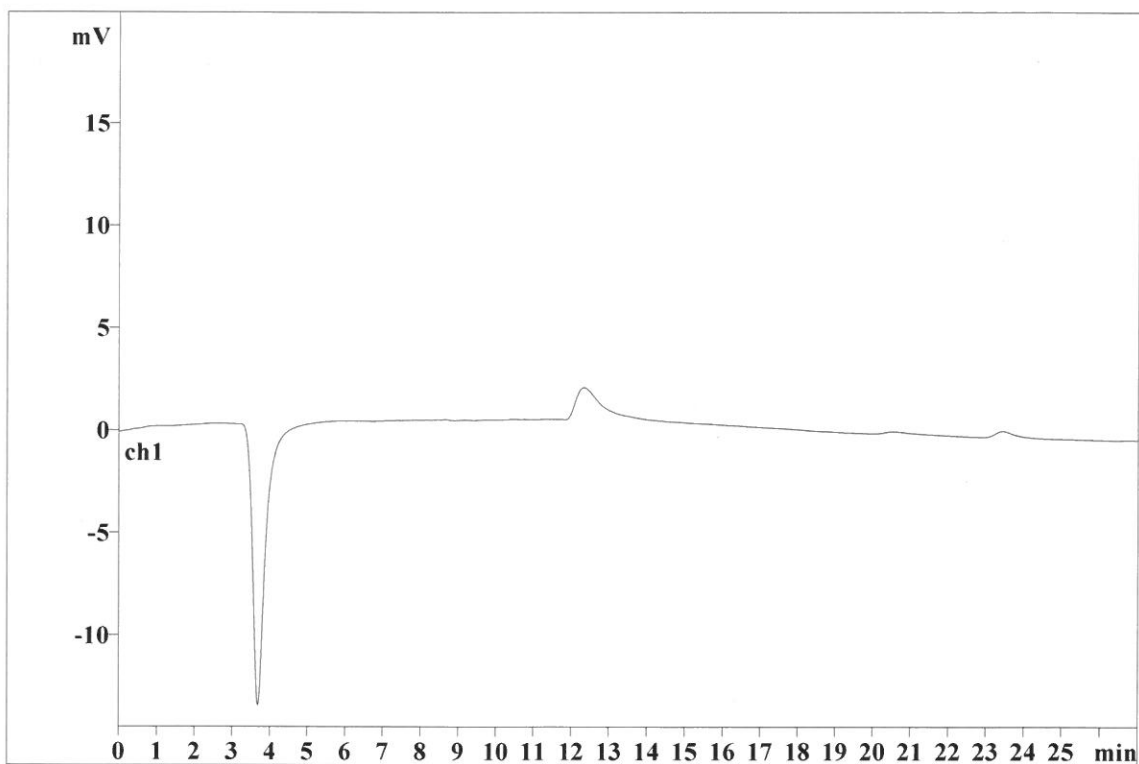

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 5/9/2022 10:11:51 AM
Printed by: wet


Ident: LB120044BLW
Analysis from: 5/6/2022 10:28:51 AM
File: _2022-05-06_

Last save: 5/6/2022 3:13:59 PM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30257

Last save: 5/4/2022 10:08:

SAMPLE:
: IZ/AP
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

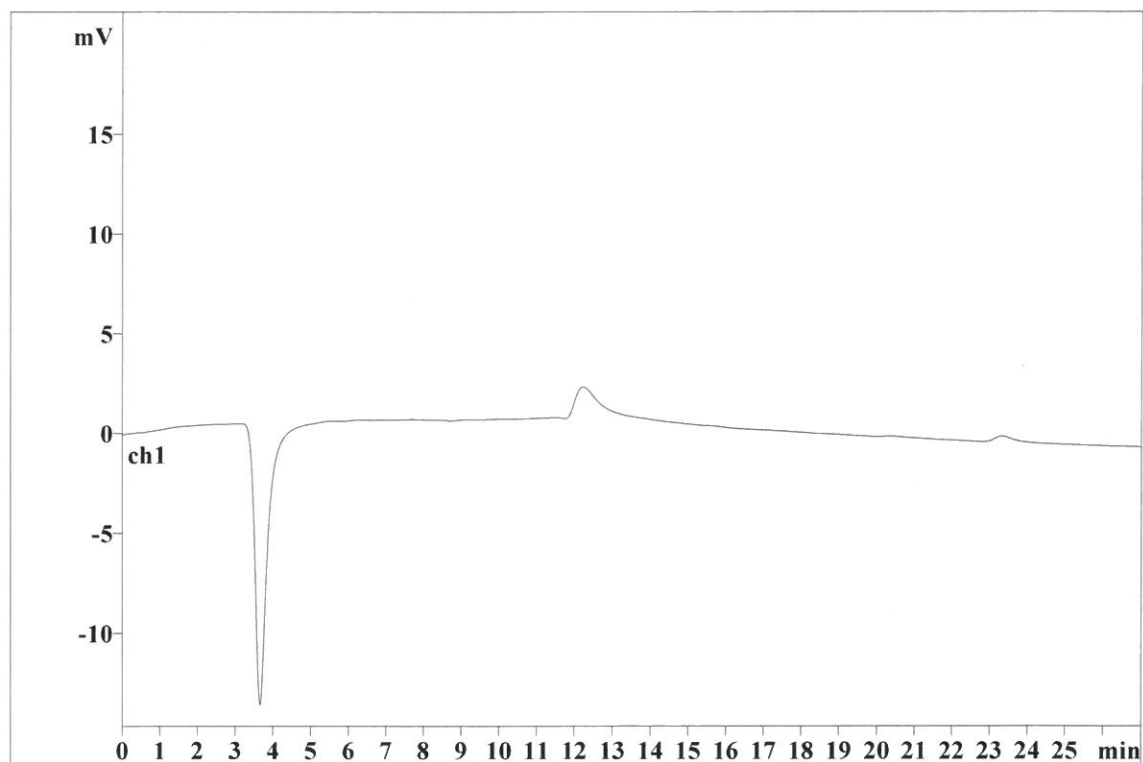

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 5/9/2022 10:11:59 AM
Printed by: wet


Ident: LB120044BSW
Analysis from: 5/6/2022 10:58:26 AM
File: _2022-05-06_

Last save: 5/6/2022 3:13:59 PM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30258

Last save: 5/4/2022 10:08:

SAMPLE:
: IZ/AP
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

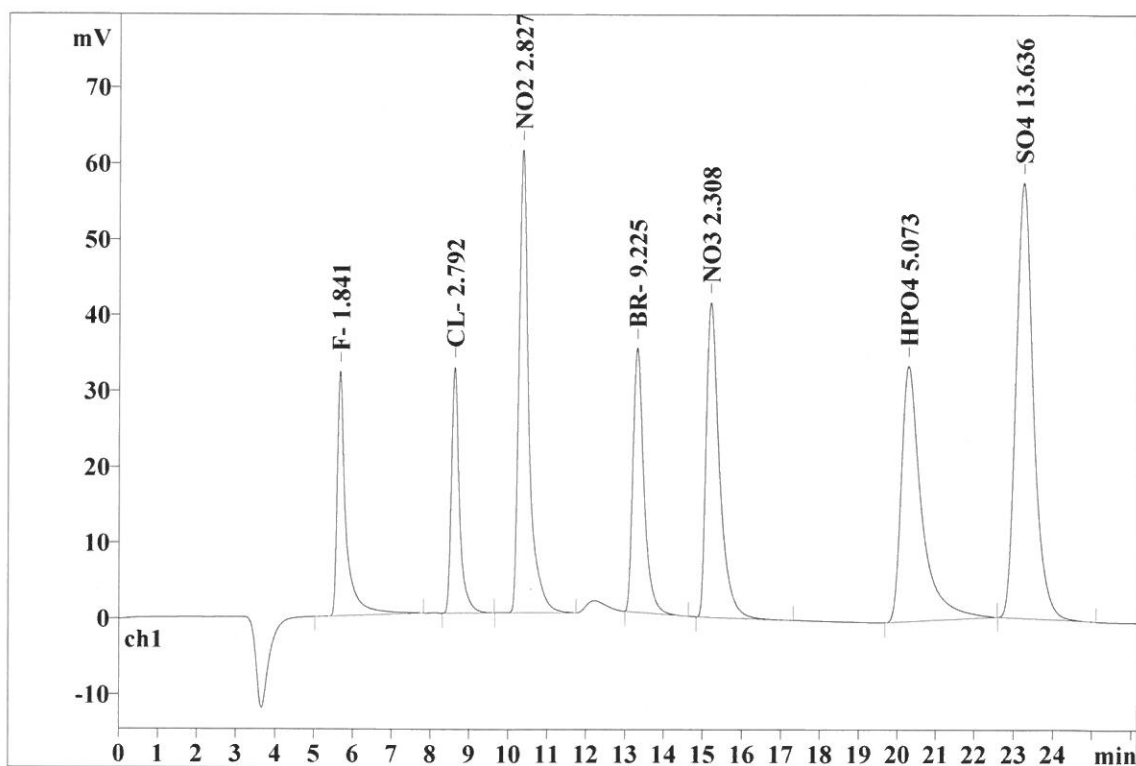

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.66	0.187	32.25	11.00	502.761	7.47
2	8.61	0.202	32.43	11.06	466.175	6.93
3	10.35	0.246	61.06	20.83	1089.208	16.19
4	13.30	0.289	34.83	11.88	683.745	10.16
5	15.19	0.342	41.49	14.15	976.477	14.51
6	20.28	0.499	33.67	11.49	1238.432	18.41
7	23.22	0.459	57.43	19.59	1771.916	26.33
7	26.16	0.318	293.18	100.00	6728.714	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/9/2022 10:12:17 AM
Printed by: wet


Ident: N2705-01
Analysis from: 5/6/2022 12:56:03 PM
File: _2022-05-06_

Last save: 5/6/2022 1:23:04 PM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30262

Last save: 5/4/2022 10:08:

SAMPLE:
: IZ/AP
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

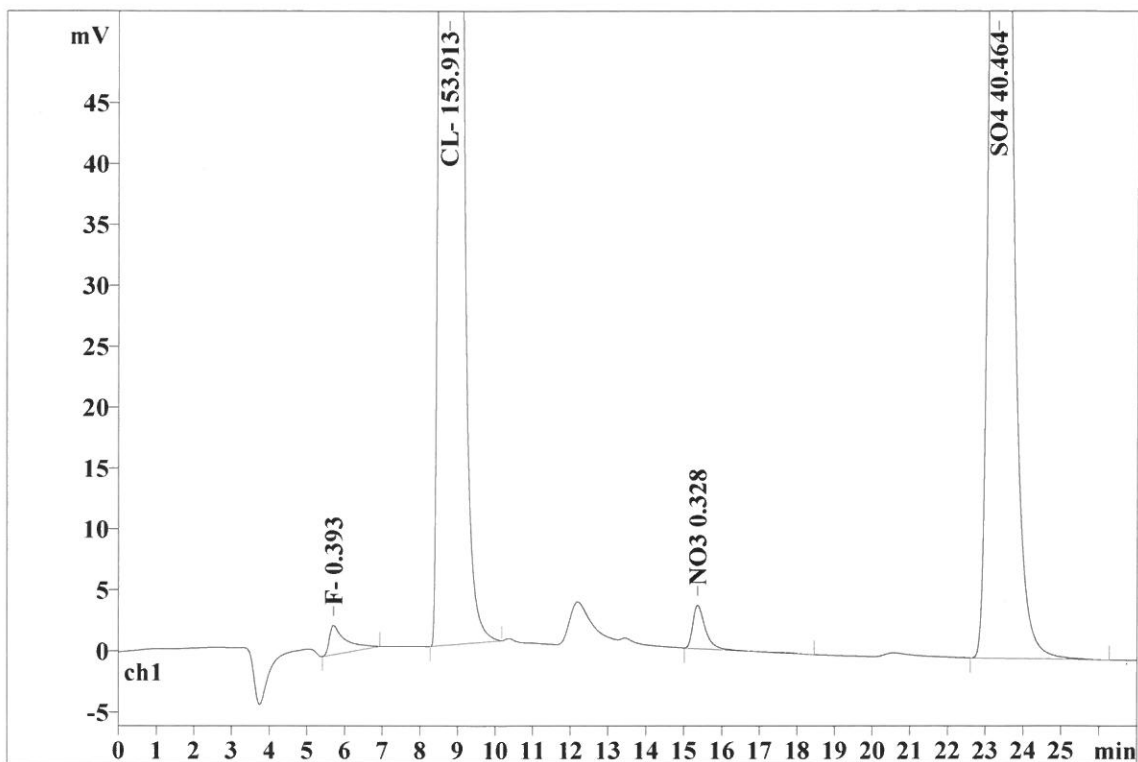

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.70	0.377	2.40	0.15	70.754	0.22
2	8.74	0.282	1442.10	88.46	27024.816	82.82
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.36	0.336	3.56	0.22	84.600	0.26
6	0.00	0.000	0.00	0.00	0.000	0.00
7	23.32	0.445	182.28	11.18	5449.276	16.70
7	27.00	0.206	1630.33	100.00	32629.447	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/9/2022 10:12:29 AM
Printed by: wet


Ident: N2712-13
Analysis from: 5/6/2022 1:25:40 PM
File: _2022-05-06_

Last save: 5/6/2022 1:52:40 PM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30263

Last save: 5/4/2022 10:08:

SAMPLE:
: IZ/AP
Vial number: 21
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

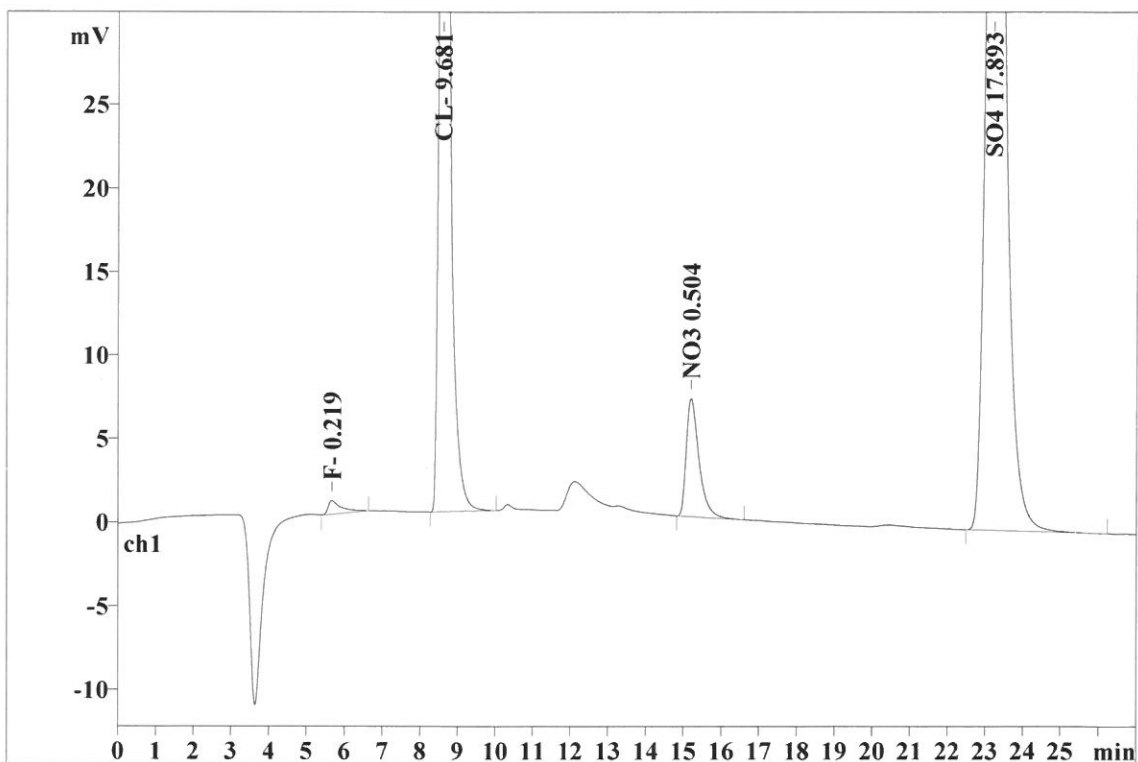

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.67	0.302	0.81	0.39	18.817	0.45
2	8.57	0.192	122.04	59.02	1676.941	39.78
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.19	0.342	7.05	3.41	164.074	3.89
6	0.00	0.000	0.00	0.00	0.000	0.00
7	23.20	0.455	76.86	37.17	2355.419	55.88
7	27.00	0.184	206.76	100.00	4215.251	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/9/2022 10:12:39 AM
Printed by: wet


Ident: N2730-01
Analysis from: 5/6/2022 1:55:24 PM
File: _2022-05-06_

Last save: 5/6/2022 2:22:24 PM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30264

Last save: 5/4/2022 10:08:

SAMPLE:
: IZ/AP
Vial number: 22
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

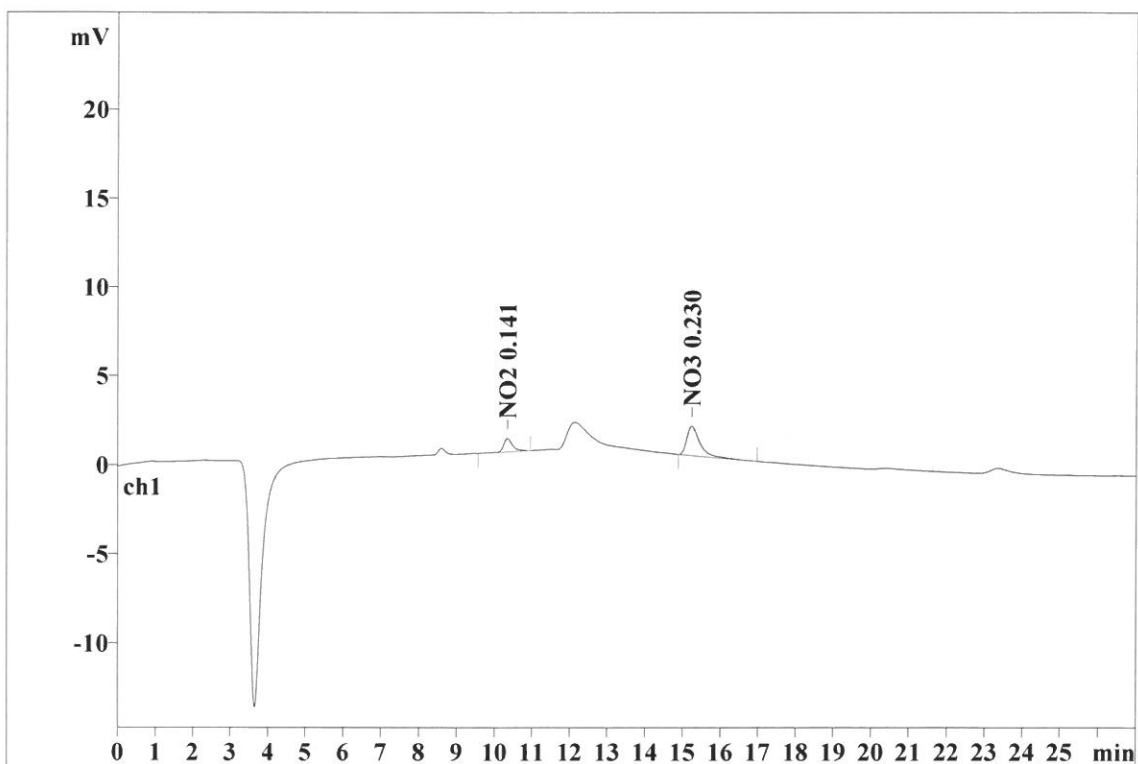

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	10.33	0.238	0.75	31.24	12.509	23.58
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.24	0.350	1.64	68.66	40.542	76.42
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	27.00	0.084	2.39	99.89	53.051	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/9/2022 10:13:51 AM
Printed by: wet


Ident: N2730-01MS
Analysis from: 5/6/2022 2:25:00 PM
File: _2022-05-06_

Last save: 5/6/2022 2:52:00 PM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30265

Last save: 5/4/2022 10:08:

SAMPLE:
: IZ/AP
Vial number: 23
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

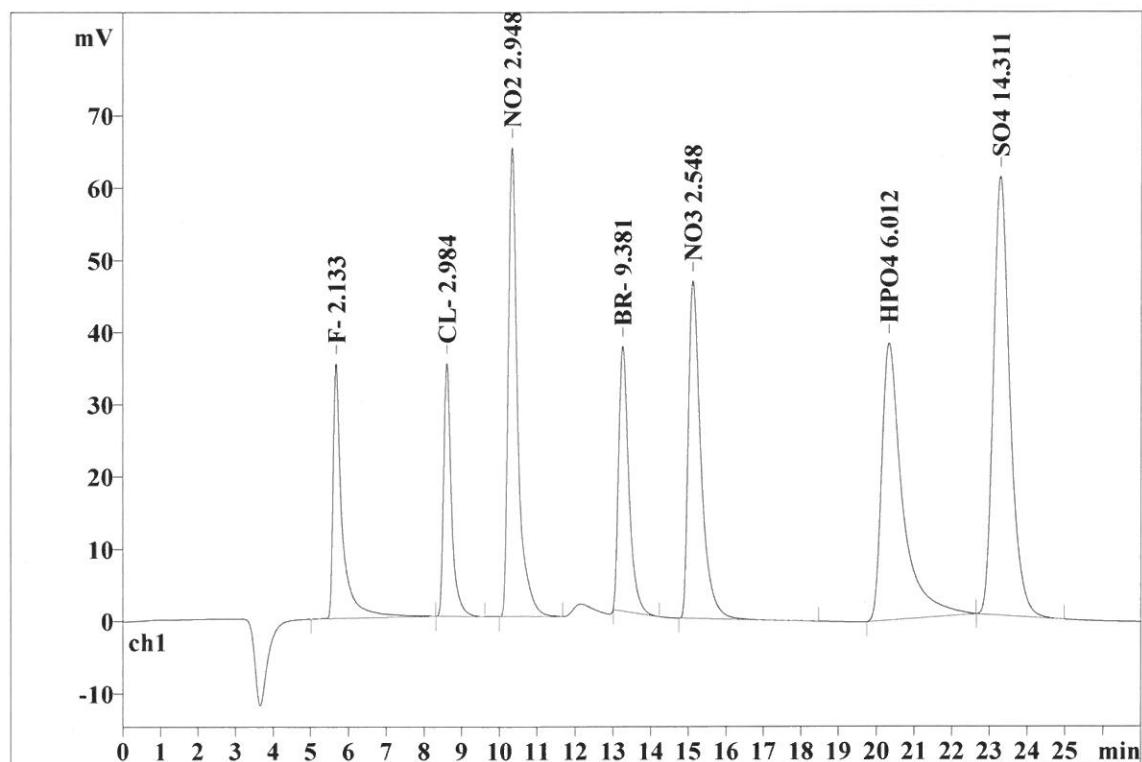

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.68	0.197	35.25	11.09	589.741	8.04
2	8.60	0.201	35.05	11.03	499.895	6.81
3	10.32	0.242	64.96	20.44	1137.766	15.51
4	13.25	0.283	36.67	11.54	695.996	9.48
5	15.12	0.337	46.75	14.71	1084.613	14.78
6	20.33	0.513	38.36	12.07	1465.514	19.97
7	23.28	0.458	60.74	19.11	1864.387	25.41
7	27.00	0.319	317.78	100.00	7337.913	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/9/2022 10:15:08 AM
Printed by: wet


Ident: N2730-01MSD
Analysis from: 5/6/2022 2:54:37 PM
File: _2022-05-06_

Last save: 5/9/2022 10:15:04 AM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30266

Last save: 5/4/2022 10:08:

SAMPLE:
: IZ/AP
Vial number: 24
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

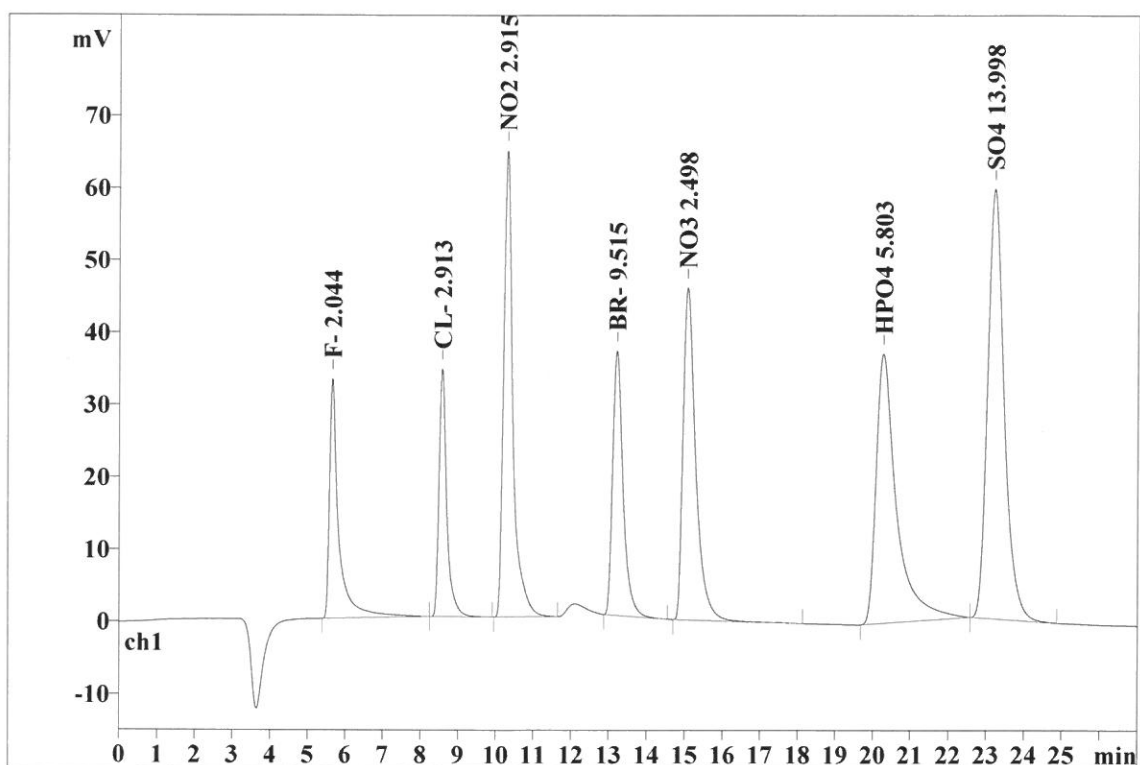

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.65	0.196	33.19	10.66	563.322	7.84
2	8.56	0.199	34.31	11.02	487.510	6.79
3	10.28	0.240	64.55	20.73	1124.520	15.66
4	13.20	0.284	36.58	11.75	706.561	9.84
5	15.06	0.335	45.95	14.76	1062.362	14.79
6	20.26	0.510	37.27	11.97	1414.906	19.70
7	23.21	0.457	59.47	19.10	1821.491	25.37
7	27.00	0.317	311.34	100.00	7180.673	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/9/2022 10:15:29 AM
Printed by: wet


Ident: CCV
Analysis from: 5/6/2022 3:24:18 PM
File: _2022-05-06_

Last save: 5/6/2022 3:53:55 PM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30267

Last save: 5/4/2022 10:08:

SAMPLE:
: IZ/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

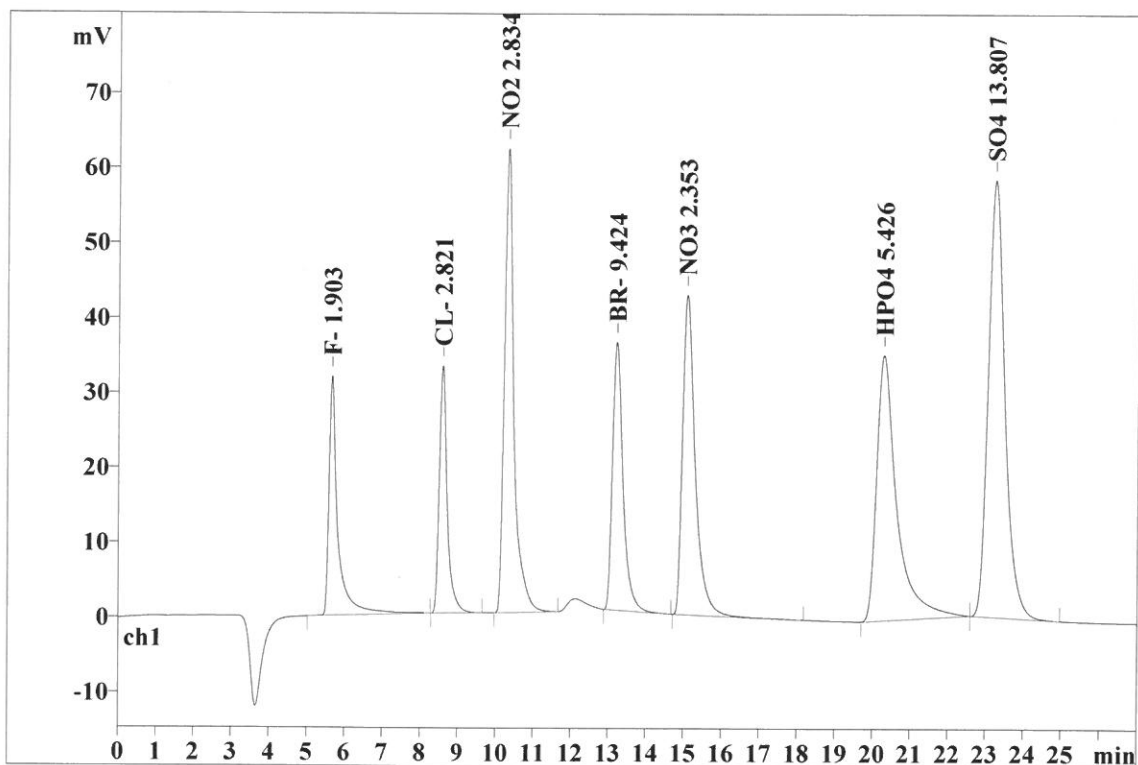

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.65	0.190	32.00	10.69	521.176	7.55
2	8.57	0.201	33.01	11.03	471.369	6.83
3	10.29	0.244	61.94	20.70	1092.205	15.83
4	13.21	0.286	35.82	11.97	699.406	10.14
5	15.08	0.338	42.72	14.28	996.853	14.45
6	20.28	0.505	35.43	11.84	1323.766	19.18
7	23.23	0.459	58.31	19.49	1795.391	26.02
7	27.00	0.318	299.23	100.00	6900.165	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/9/2022 10:15:38 AM
Printed by: wet


Ident: CCB
Analysis from: 5/6/2022 3:54:48 PM
File: _2022-05-06_

Last save: 5/6/2022 4:21:48 PM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30268

Last save: 5/4/2022 10:08:

SAMPLE:
: IZ/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

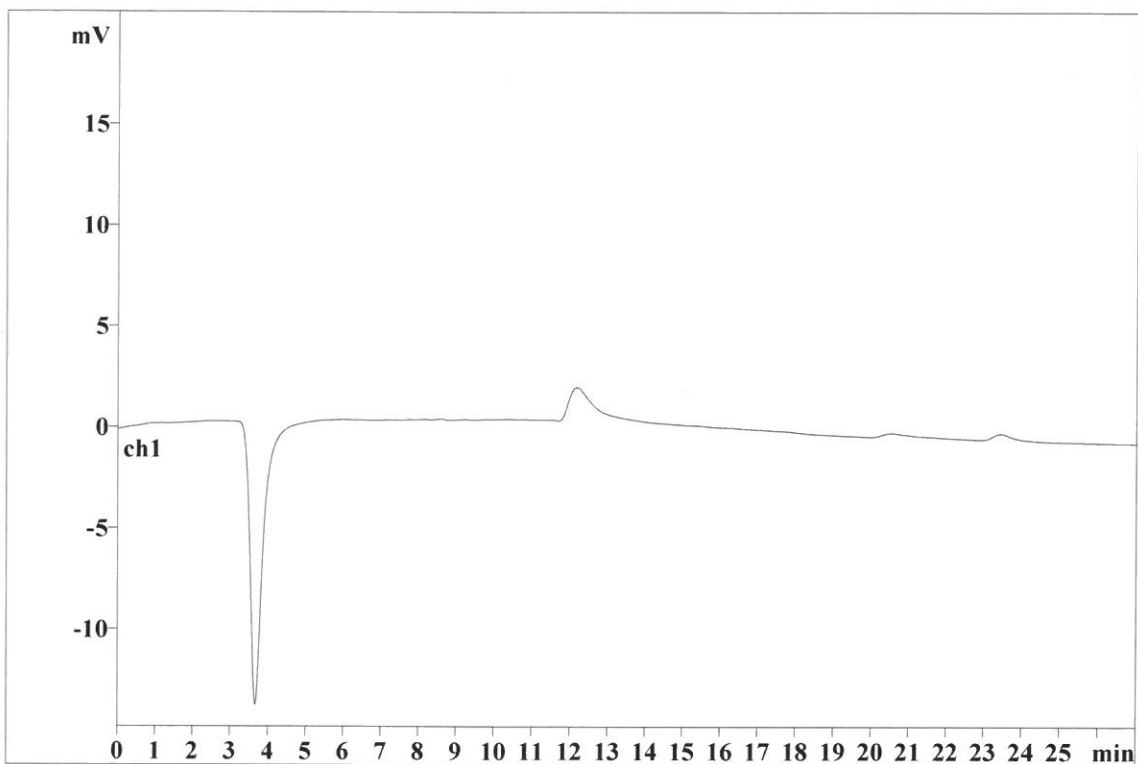

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 5/9/2022 10:15:50 AM
Printed by: wet


Ident: N2741-01
Analysis from: 5/6/2022 4:24:27 PM
File: _2022-05-06_

Last save: 5/6/2022 4:51:27 PM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30269

Last save: 5/6/2022 3:54:2

SAMPLE:
: IZ/AP
Vial number: 25
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

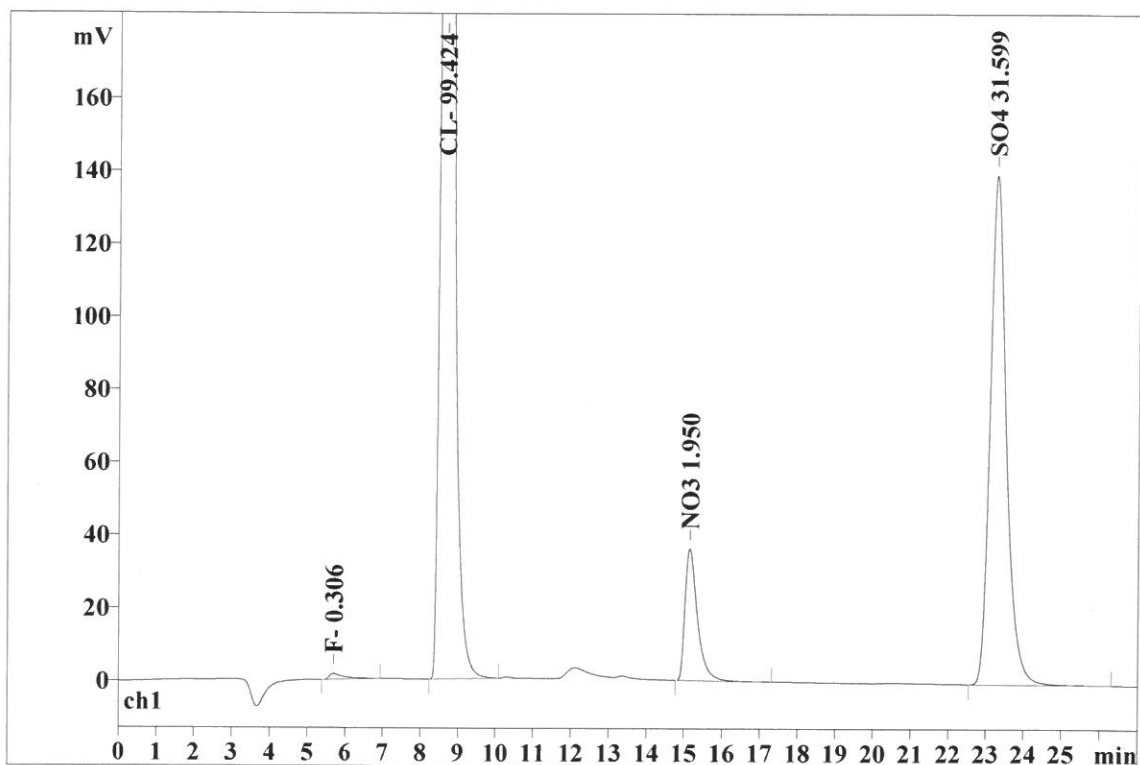

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.70	0.359	1.62	0.12	44.790	0.20
2	8.64	0.204	1218.73	87.30	17448.727	77.40
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.14	0.329	36.09	2.59	815.435	3.62
6	0.00	0.000	0.00	0.00	0.000	0.00
7	23.26	0.449	139.70	10.01	4234.087	18.78
7	27.00	0.192	1396.14	100.01	22543.038	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/9/2022 10:16:08 AM
Printed by: wet


Ident: CCV
Analysis from: 5/6/2022 4:54:08 PM
File: _2022-05-06_

Last save: 5/6/2022 5:21:08 PM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30270

Last save: 5/6/2022 3:54:2

SAMPLE:
: IZ/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

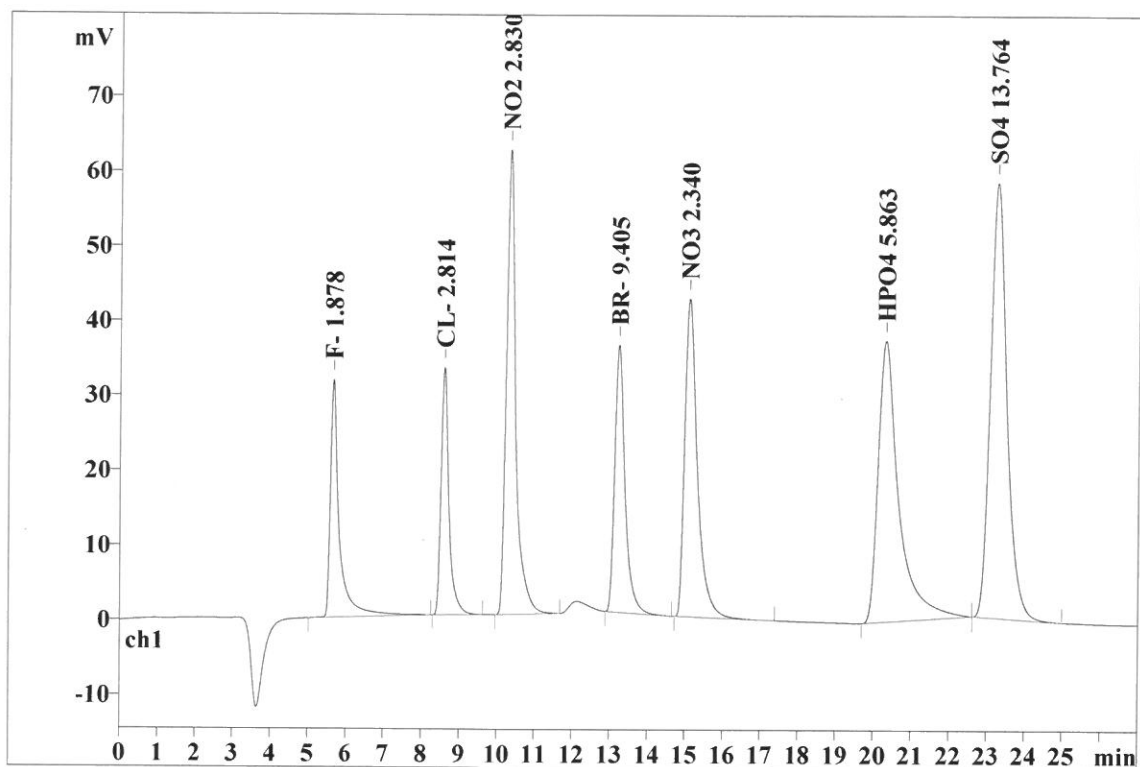

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.66	0.189	31.76	10.56	513.669	7.36
2	8.58	0.200	33.04	10.98	470.081	6.73
3	10.30	0.244	62.08	20.63	1090.711	15.62
4	13.22	0.286	35.70	11.87	697.909	10.00
5	15.09	0.338	42.53	14.13	990.947	14.19
6	20.30	0.513	37.56	12.48	1429.414	20.47
7	23.25	0.460	58.20	19.34	1789.480	25.63
7	27.00	0.319	300.87	100.00	6982.212	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/9/2022 10:16:16 AM
Printed by: wet


Ident: CCB
Analysis from: 5/6/2022 5:23:44 PM
File: _2022-05-06_

Last save: 5/6/2022 5:50:44 PM

Method: AnionsIC2-050222.mtw
Run operator: wet
Analysis number: 30271

Last save: 5/6/2022 3:54:2

SAMPLE:
: IZ/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

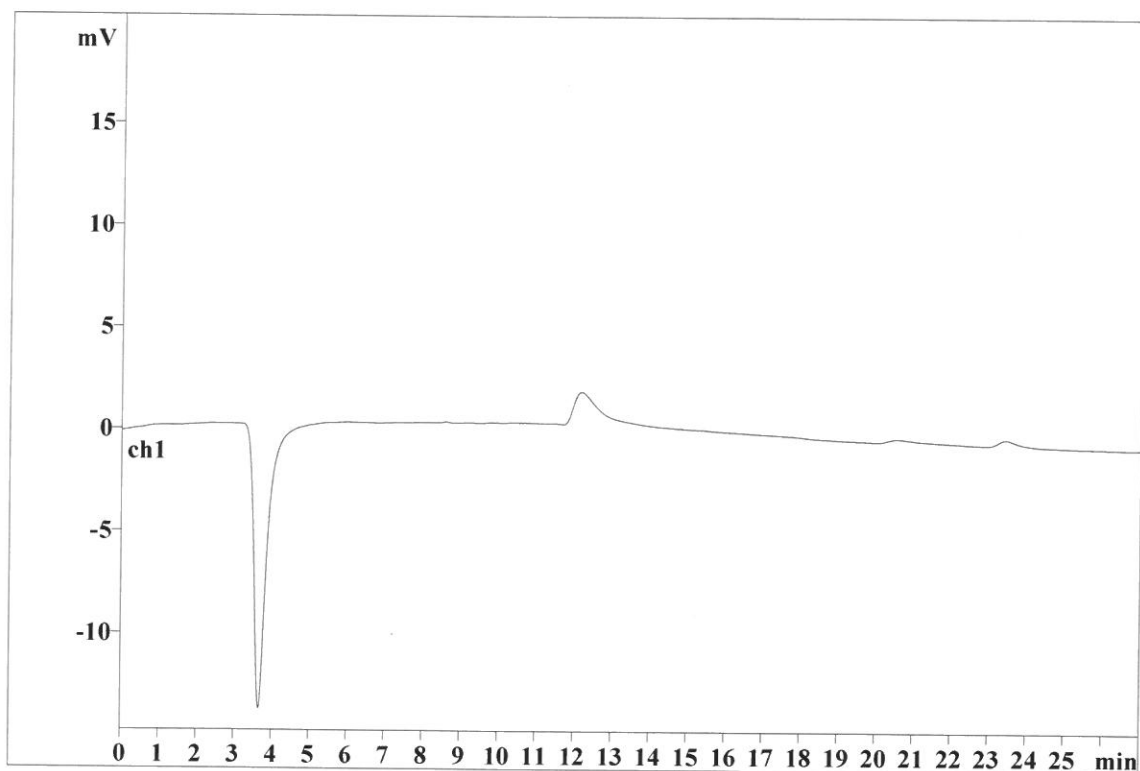

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD