


CB120110

7471B

INSTRUMENT ID: CV2

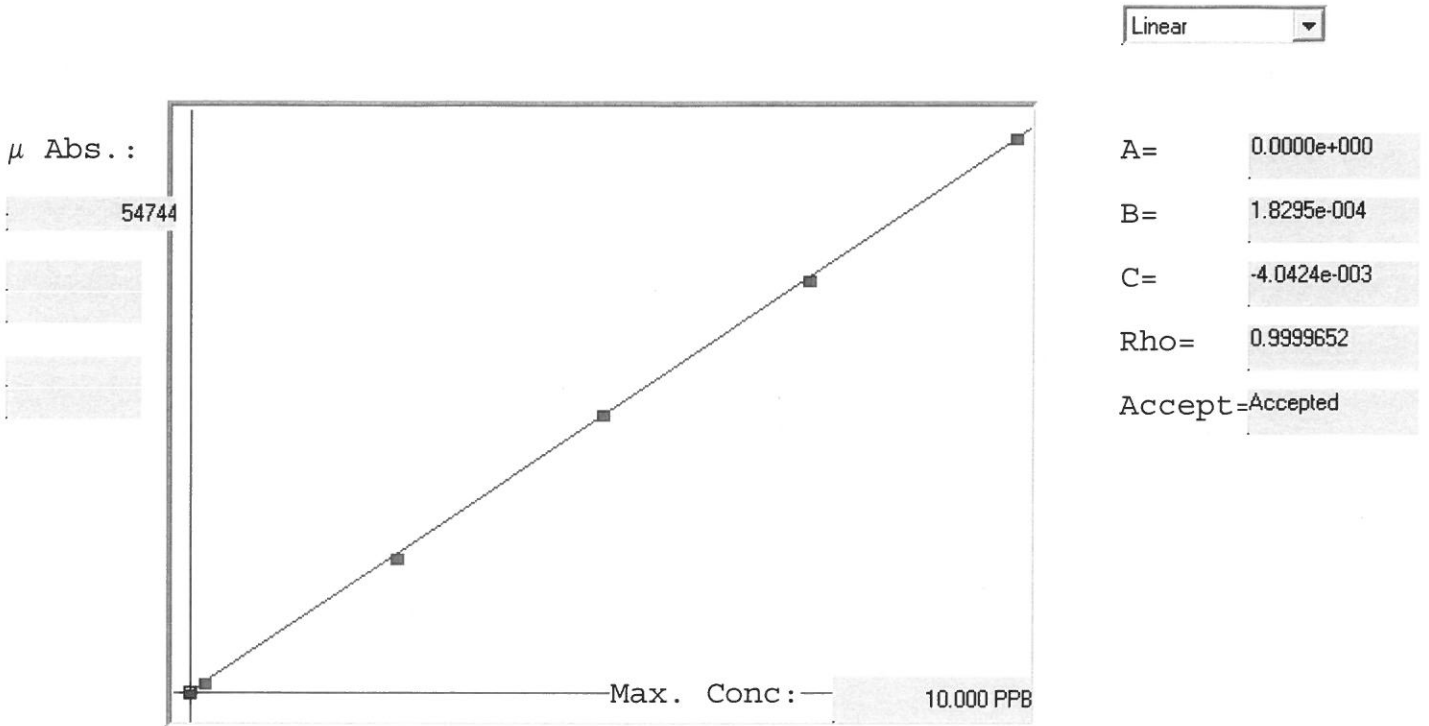

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	6/01
0.0	0.000	0.018	0.018	119	0.000	119					8
0.2	0.200	0.200	0.000	1118	0.0 %	1118					-2
2.5	2.500	2.456	-0.044	13446	0.0 %	13446					1
5.0	5.000	5.047	0.047	27610	0.0 %	27610					0
7.5	7.500	7.467	-0.033	40838	0.0 %	40838					0
10.0	10.000	10.011	0.011	54744	0.0 %	54744					0

LB120110 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 11 May 2022 14:41:16

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	119	-	0.0000	7471B	PPB	11 May 2022 14:42:42	S	Std
0.2 - 1	50.2	1118	-	0.2000	7471B	PPB	11 May 2022 14:44:59	S	Std
2.5 - 1	52.5	13446	-	2.5000	7471B	PPB	11 May 2022 14:47:16	S	Std
5.0 - 1	55	27610	-	5.0000	7471B	PPB	11 May 2022 14:49:32	S	Std
7.5 - 1	57.5	40838	-	7.5000	7471B	PPB	11 May 2022 14:51:48	S	Std
10.0 - 1	510	54744	-	10.0000	7471B	PPB	11 May 2022 14:54:05	S	Std
ICV20 - 1	ICV20	22097	4.0386	-	7471B	PPB	11 May 2022 14:56:44	U	SMPL
ICB20 - 1	ICB20	-32	-0.0099	-	7471B	PPB	11 May 2022 14:58:59	U	SMPL
CCV34 - 1	CCV34	27374	5.0040	-	7471B	PPB	11 May 2022 15:02:48	U	SMPL
CCB34 - 1	CCB34	-56	-0.0143	-	7471B	PPB	11 May 2022 15:05:03	U	SMPL
CRA - 1	CRA	1125	0.2018	-	7471B	PPB	11 May 2022 15:07:18	U	SMPL
HighStd - 1	HighStd	54633	9.9911	-	7471B	PPB	11 May 2022 15:09:33	U	SMPL
ChkStd - 1	ChkStd	38164	6.9781	-	7471B	PPB	11 May 2022 15:11:49	U	SMPL
PB144754BL - 1	PB144754BL	-92	-0.0209	-	7471B	PPB	11 May 2022 15:14:06	U	SMPL
PB144754BS - 1	PB144754BS	19838	3.6253	-	7471B	PPB	11 May 2022 15:16:23	U	SMPL
N2769-01 - 1	CL-02-051022	10629	1.9405	-	7471B	PPB	11 May 2022 15:34:23	U	SMPL
N2769-01DUP - 1	CL-02-051022DUP	10121	1.8476	-	7471B	PPB	11 May 2022 15:36:38	U	SMPL
N2769-01MS - 1	CL-02-051022MS	32415	5.9263	-	7471B	PPB	11 May 2022 15:38:55	U	SMPL
N2769-01MSD - 1	CL-02-051022MSD	30747	5.6211	-	7471B	PPB	11 May 2022 15:41:12	U	SMPL
N2775-01 - 1	MH-35S	32367	5.9175	-	7471B	PPB	11 May 2022 15:43:28	U	SMPL
CCV35 - 1	CCV35	26922	4.9213	-	7471B	PPB	11 May 2022 15:59:56	U	SMPL
CCB35 - 1	CCB35	8	-0.0026	-	7471B	PPB	11 May 2022 16:02:11	U	SMPL
N2775-04 - 1	MH-35D	6474	1.1804	-	7471B	PPB	11 May 2022 16:04:26	U	SMPL
N2776-01 - 1	CF-280MER-8-15	8066	1.4716	-	7471B	PPB	11 May 2022 16:06:41	U	SMPL
N2776-02 - 1	CF-280MER-9-5	2337	0.4235	-	7471B	PPB	11 May 2022 16:08:56	U	SMPL
N2776-03 - 1	CF-280MER-10-15	3677	0.6687	-	7471B	PPB	11 May 2022 16:11:12	U	SMPL
N2777-01 - 1	P-PARK-1-A	159	0.0250	-	7471B	PPB	11 May 2022 16:13:28	U	SMPL
N2769-01LX5 - 1		1713	0.3094	-	7471B	PPB	11 May 2022 16:20:54	U	SMPL
N2769-01A - 1		32690	5.9766	-	7471B	PPB	11 May 2022 16:23:11	U	SMPL
CCV36 - 1	CCV36	27390	5.0070	-	7471B	PPB	11 May 2022 16:25:27	U	SMPL
CCB36 - 1	CCB36	9	-0.0024	-	7471B	PPB	11 May 2022 16:27:44	U	SMPL