

LB 120129

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

5/12/2022 13:00

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.998	0.0	0.107	
ICB1	0.005	0.0	0.004	
CCV1	0.980	0.0	0.105	
CCB1	0.003	0.0	0.004	
PB144750BL	0.002	0.0	0.004	
PB144750BS	0.997	0.0	0.107	
N2761-01	0.098	0.0	0.014	
N2761-01DUP	0.090	0.0	0.013	
N2761-01MS	1.138	0.0	0.121	
N2761-01MSD	1.137	0.0	0.121	
N2761-02	0.101	0.0	0.014	
CCV2	0.980	0.0	0.105	
CCB2	0.001	0.0	0.004	

N	13
Mean	0.502
SD	0.5202
CV%	103.54

Aquakem v. 7.2AQ1

Results from time period:

Thu May 12 12:14:11 2022

Thu May 12 12:53:09 2022

Sample Id	Sam/Ctr/c	Test short na	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0007	mg/l	5/12/2022 12:14:11	
0.05PPM	A	Phenolics-	P	0.0538	mg/l	5/12/2022 12:14:12	
0.1PPM	A	Phenolics-	P	0.1033	mg/l	5/12/2022 12:14:13	
0.25PPM	A	Phenolics-	P	0.2576	mg/l	5/12/2022 12:14:14	
0.50PPM	A	Phenolics-	P	0.4995	mg/l	5/12/2022 12:14:15	
1.0PPM	A	Phenolics-	P	0.9723	mg/l	5/12/2022 12:14:16	
2.0PPM	A	Phenolics-	P	2.0128	mg/l	5/12/2022 12:14:17	
ICV1	S	Phenolics-	P	0.998	mg/l	5/12/2022 12:46:46	
ICB1	S	Phenolics-	P	0.0051	mg/l	5/12/2022 12:46:47	
CCV1	S	Phenolics-	P	0.9804	mg/l	5/12/2022 12:46:50	
CCB1	S	Phenolics-	P	0.0031	mg/l	5/12/2022 12:46:52	
PB144750BL	S	Phenolics-	P	0.0023	mg/l	5/12/2022 12:46:53	
PB144750BS	S	Phenolics-	P	0.9975	mg/l	5/12/2022 12:46:56	
N2761-01	S	Phenolics-	P	0.0985	mg/l	5/12/2022 12:53:03	
N2761-01DUP	S	Phenolics-	P	0.0902	mg/l	5/12/2022 12:53:04	
N2761-01MS	S	Phenolics-	P	1.1382	mg/l	5/12/2022 12:53:05	
N2761-01MSD	S	Phenolics-	P	1.1367	mg/l	5/12/2022 12:53:06	
N2761-02	S	Phenolics-	P	0.1006	mg/l	5/12/2022 12:53:07	
CCV2	S	Phenolics-	P	0.9803	mg/l	5/12/2022 12:53:08	
CCB2	S	Phenolics-	P	0.0007	mg/l	5/12/2022 12:53:09	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

5/12/2022 12:21


Test Phenolics-

Accepted 5/12/2022 12:21

Factor 9.698
Bias 0.004

Coeff. of det. 0.999679

Errors

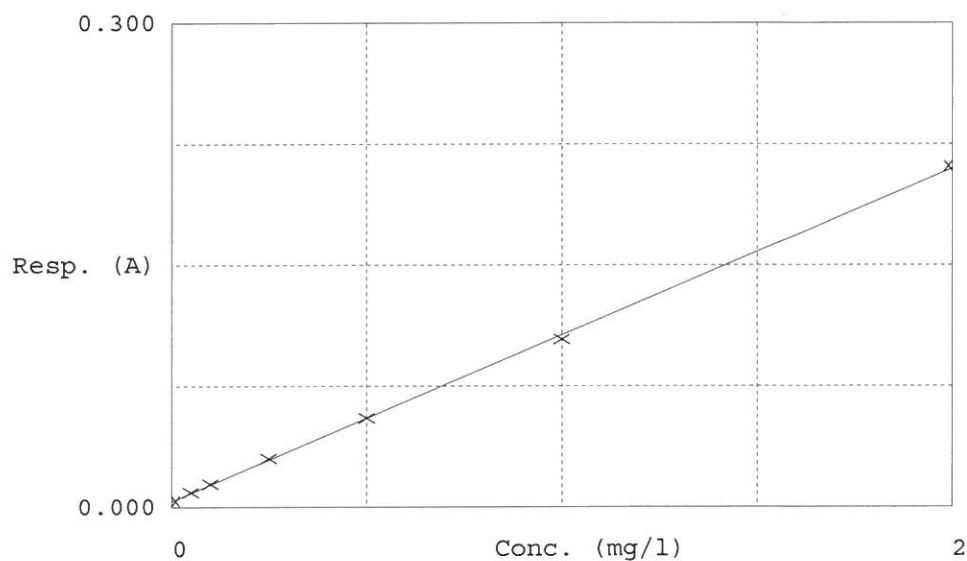

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.004	0.0007	0.0000	-
2	Phenol-2	0.009	0.0538	0.0500	7.6
3	Phenol-2	0.014	0.1033	0.1000	3.3
4	Phenol-2	0.030	0.2576	0.2500	3.0
5	Phenol-2	0.055	0.4995	0.5000	-0.1
6	Phenol-2	0.104	0.9723	1.0000	-2.8
7	Phenol-2	0.211	2.0128	2.0000	0.6

12
5/12/22