

LB120223

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

5/17/2022 16:50

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.802	0.0	0.076	
ICB1	0.835	0.0	0.001	
CCV1	245.698	0.0	0.195	
CCB1	0.837	0.0	0.001	
PB144897BL	0.673	0.0	0.001	
N2858-02	0.561	0.0	0.001	
N2858-02DUP	0.414	0.0	0.001	
N2879-02	0.515	0.0	0.001	
N2879-05	0.573	0.0	0.001	
N2879-08	0.557	0.0	0.001	
N2879-11	0.404	0.0	0.001	
N2881-03	0.522	0.0	0.001	
N2882-02	0.658	0.0	0.001	
CCV2	250.181	0.0	0.199	
CCB2	0.771	0.0	0.001	

N	15
Mean	39.867
SD	87.8756
CV%	220.42

Aquakem v. 7.2AQ1

Results from time period:

Tue May 17 16:33:49 2022

Tue May 17 16:40:36 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.2417	µg/l	5/17/2022 11:30:42	
5.0PPBCN	A	Total CN	P	4.8368	µg/l	5/17/2022 11:30:43	
10PPBCN	A	Total CN	P	9.7927	µg/l	5/17/2022 11:30:44	
50PPBCN	A	Total CN	P	49.7349	µg/l	5/17/2022 11:30:45	
100PPBCN	A	Total CN	P	99.3876	µg/l	5/17/2022 11:30:46	
250PPBCN	A	Total CN	P	251.7028	µg/l	5/17/2022 11:30:47	
500PPBCN	A	Total CN	P	499.3033	µg/l	5/17/2022 11:30:48	
ICV1	S	Total CN	P	94.802	µg/l	5/17/2022 16:33:50	
ICB1	S	Total CN	P	0.8353	µg/l	5/17/2022 16:33:52	
CCV1	S	Total CN	P	245.6976	µg/l	5/17/2022 16:33:54	
CCB1	S	Total CN	P	0.8366	µg/l	5/17/2022 16:33:55	
PB144897BL	S	Total CN	P	0.673	µg/l	5/17/2022 16:33:57	
N2858-02	S	Total CN	P	0.5614	µg/l	5/17/2022 16:33:59	
N2858-02DUP	S	Total CN	P	0.4138	µg/l	5/17/2022 16:40:28	
N2879-02	S	Total CN	P	0.5153	µg/l	5/17/2022 16:40:29	
N2879-05	S	Total CN	P	0.5733	µg/l	5/17/2022 16:40:30	
N2879-08	S	Total CN	P	0.5571	µg/l	5/17/2022 16:40:31	
N2879-11	S	Total CN	P	0.4041	µg/l	5/17/2022 16:40:32	
N2881-03	S	Total CN	P	0.522	µg/l	5/17/2022 16:40:33	
N2882-02	S	Total CN	P	0.6583	µg/l	5/17/2022 16:40:34	
CCV2	S	Total CN	P	250.1815	µg/l	5/17/2022 16:40:35	
CCB2	S	Total CN	P	0.7709	µg/l	5/17/2022 16:40:36	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

5/17/2022 11:32


Test Total CN

Accepted 5/17/2022 11:32

Factor 1262
Bias 0.001

Coeff. of det. 0.999981

Errors

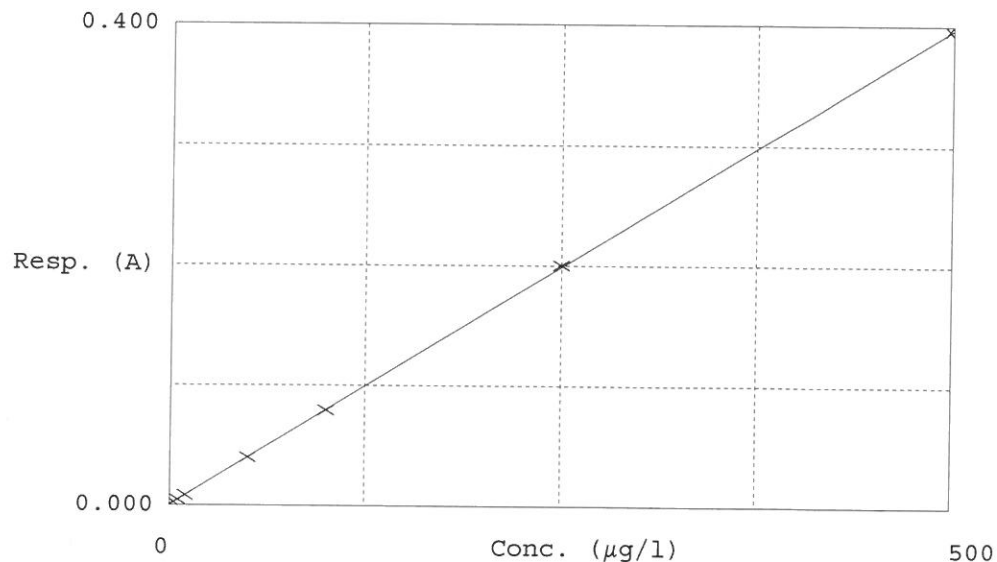

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.2417	0.0000	—
2	5.0PPBCN	0.005	4.8368	5.0000	-3.3
3	10PPBCN	0.008	9.7927	10.0000	-2.1
4	50PPBCN	0.040	49.7349	50.0000	-0.5
5	100PPBCN	0.079	99.3876	100.0000	-0.2
6	250PPBCN	0.200	251.7028	250.0000	0.7
7	500PPBCN	0.396	499.3033	500.0000	-0.1

12
5/17/22