

LB120241

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

5/18/2022 11:57

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.080	0.0	0.077	
ICB1	-0.082	0.0	0.001	
CCV1	244.304	0.0	0.199	
CCB1	0.005	0.0	0.001	
PB144895BL	-0.389	0.0	0.001	
PB144895BS	93.498	0.0	0.077	
MIDPB144895	243.037	0.0	0.198	979/90-110)
N2880-01	0.172	0.0	0.001	
N2880-01DUP	-0.467	0.0	0.001	
N2880-01MS	36.556	0.0	0.031	12
N2880-01MSD	35.790	0.0	0.030	5/19/22
CCV2	241.221	0.0	0.196	
CCB2	-0.534	0.0	0.001	

N 13
Mean 75.861
SD 100.8915
CV% 133.00

Aquakem v. 7.2AQ1

Results from time period:

Wed May 18 10:19:46 2022

Wed May 18 11:10:39 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
0.0PPBCN	A	Total CN	P	-0.6861	µg/l	5/18/2022 10:19:46
5.0PPBCN	A	Total CN	P	4.2354	µg/l	5/18/2022 10:19:47
10PPBCN	A	Total CN	P	9.2302	µg/l	5/18/2022 10:19:48
50PPBCN	A	Total CN	P	49.5003	µg/l	5/18/2022 10:19:49
100PPBCN	A	Total CN	P	98.6508	µg/l	5/18/2022 10:19:50
250PPBCN	A	Total CN	P	257.453	µg/l	5/18/2022 10:19:51
500PPBCN	A	Total CN	P	496.6163	µg/l	5/18/2022 10:19:52
ICV1	S	Total CN	P	93.0799	µg/l	5/18/2022 11:00:17
ICB1	S	Total CN	P	-0.0824	µg/l	5/18/2022 11:00:18
CCV1	S	Total CN	P	244.3036	µg/l	5/18/2022 11:00:22
CCB1	S	Total CN	P	0.0051	µg/l	5/18/2022 11:00:23
PB144895BL	S	Total CN	P	-0.3891	µg/l	5/18/2022 11:00:26
PB144895BS	S	Total CN	P	93.4979	µg/l	5/18/2022 11:07:52
MIDPB144895	S	Total CN	P	243.037	µg/l	5/18/2022 11:07:53
N2880-01	S	Total CN	P	0.1718	µg/l	5/18/2022 11:07:55
N2880-01DUP	S	Total CN	P	-0.467	µg/l	5/18/2022 11:07:56
N2880-01MS	S	Total CN	P	36.5557	µg/l	5/18/2022 11:07:59
N2880-01MSD	S	Total CN	P	35.7898	µg/l	5/18/2022 11:08:00
CCV2	S	Total CN	P	241.2205	µg/l	5/18/2022 11:08:01
CCB2	S	Total CN	P	-0.5338	µg/l	5/18/2022 11:10:39

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

5/18/2022 10:34


Test Total CN

Accepted 5/18/2022 10:34

Factor 1235
Bias 0.001

Coeff. of det. 0.999656

Errors

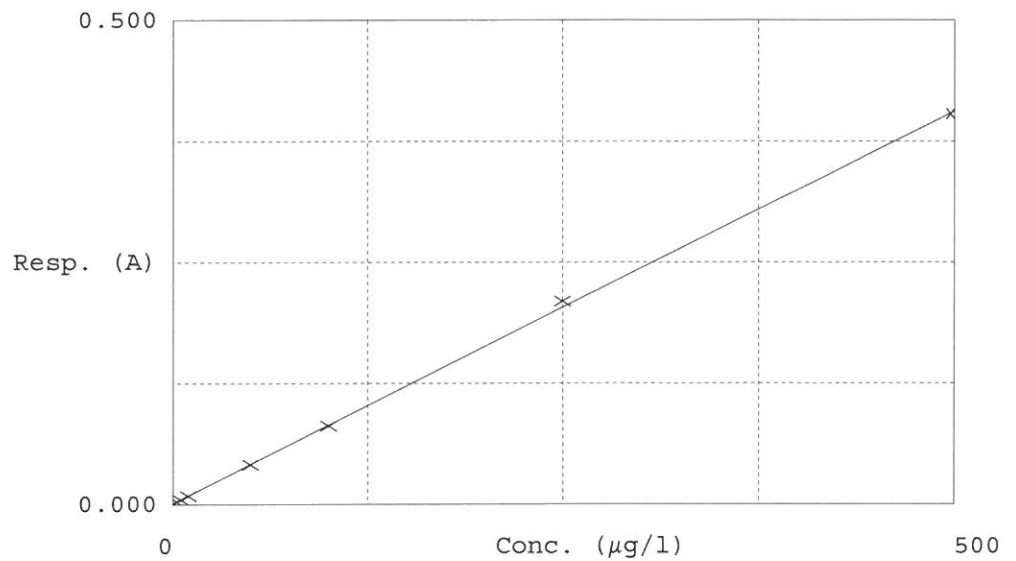

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.6861	0.0000	-
2	5.0PPBCN	0.005	4.2354	5.0000	-15.3
3	10PPBCN	0.009	9.2302	10.0000	-7.7
4	50PPBCN	0.041	49.5003	50.0000	-1.0
5	100PPBCN	0.081	98.6508	100.0000	-1.3
6	250PPBCN	0.210	257.4530	250.0000	3.0
7	500PPBCN	0.403	496.6163	500.0000	-0.7

12
5/19/22