

Clear table

Instrument ID: IC-2											
Method: 300.0 / 9056A											
Analyst : IZ											
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.4040	2022-05-19_	5/19/22 14:22		IZ/AP
STD2	0.4310	0.6260	0.6120	0.4440	0.5170	0.5400	3.1050	2022-05-19_	5/19/22 14:52		IZ/AP
STD3	0.7900	1.1920	1.1940	2.4940	0.9940	1.9330	5.9210	2022-05-19_	5/19/22 15:21		IZ/AP
STD4	0.9500	1.4980	1.4620	3.5370	1.2470	2.6940	7.2920	2022-05-19_	5/19/22 15:51		IZ/AP
STD5	2.0400	2.9910	3.0250	8.8470	2.4990	5.6270	15.3410	2022-05-19_	5/19/22 16:21		IZ/AP
STD6	3.9870	5.9490	5.9560	18.6110	4.9670	10.0490	29.6940	2022-05-19_	5/19/22 16:50		IZ/AP
STD7	5.0020	7.5430	7.4970	24.1550	6.2770	12.1580	37.6460	2022-05-19_	5/19/22 17:20		IZ/AP
ICV	1.9240	2.8640	2.9140	8.0920	2.4010	5.0970	14.2250	2022-05-19_	5/19/22 17:49		IZ/AP
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.7040	2022-05-19_	5/19/22 18:19		IZ/AP
CCV	1.9200	2.8690	2.9290	8.1480	2.3930	6.1240	14.4840	2022-05-19_	5/19/22 18:49		IZ/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.6280	2022-05-19_	5/19/22 19:18		IZ/AP
LB120263BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.5880	2022-05-19_	5/19/22 19:48		IZ/AP
LB120263BSW	1.9280	2.8670	2.9270	8.0970	2.3890	5.4580	14.3140	2022-05-19_	5/19/22 20:18		IZ/AP
N2946-03	0.0000	96.7920	0.0820	0.0000	0.8550	0.2700	8.4570	2022-05-19_	5/19/22 20:47		IZ/AP
N2946-03MS	2.6230	95.7520	3.0360	8.3990	3.2790	9.8990	22.5730	2022-05-19_	5/19/22 21:17		IZ/AP
N2946-03MSD	2.6570	95.8070	3.1290	8.7870	3.3730	10.0300	22.7680	2022-05-19_	5/19/22 21:47		IZ/AP
CCV	1.9820	2.8860	2.9190	8.0680	2.4230	6.1030	13.9660	2022-05-19_	5/19/22 22:16		IZ/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.4290	2022-05-19_	5/19/22 22:46		IZ/AP

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A


ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.4040	2022-05-19_	5/19/22 14:22		IZ/AP
STD2	0.4310	0.6260	0.6120	0.4440	0.5170	0.5400	3.1050	2022-05-19_	5/19/22 14:52		IZ/AP
STD3	0.7900	1.1920	1.1940	2.4940	0.9940	1.9330	5.9210	2022-05-19_	5/19/22 15:21		IZ/AP
STD4	0.9500	1.4980	1.4620	3.5370	1.2470	2.6940	7.2920	2022-05-19_	5/19/22 15:51		IZ/AP
STD5	2.0400	2.9910	3.0250	8.8470	2.4990	5.6270	15.3410	2022-05-19_	5/19/22 16:21		IZ/AP
STD6	3.9870	5.9490	5.9560	18.6110	4.9670	10.0490	29.6940	2022-05-19_	5/19/22 16:50		IZ/AP
STD7	5.0020	7.5430	7.4970	24.1550	6.2770	12.1580	37.6460	2022-05-19_	5/19/22 17:20		IZ/AP

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1							
STD2	7.7500	4.3333	2.0000	-77.8000	3.4000	-46.0000	3.5000
STD3	-1.2500	-0.6667	-0.5000	-37.6500	-0.6000	-3.3500	-1.3167
STD4	-5.0000	-0.1333	-2.5333	-29.2600	-0.2400	7.7600	-2.7733
STD5	2.0000	-0.3000	0.8333	-11.5300	-0.0400	12.5400	2.2733
STD6	-0.3250	-0.8500	-0.7333	-6.9450	-0.6600	0.4900	-1.0200
STD7	0.0400	0.5733	-0.0400	-3.3800	0.4320	-2.7360	1.7459

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-051922.mtw
 Equation: $Q = 0.0542483 \cdot A + 1.82974$
 RSD: 1.659 %
 Correlation coefficient: 0.999850

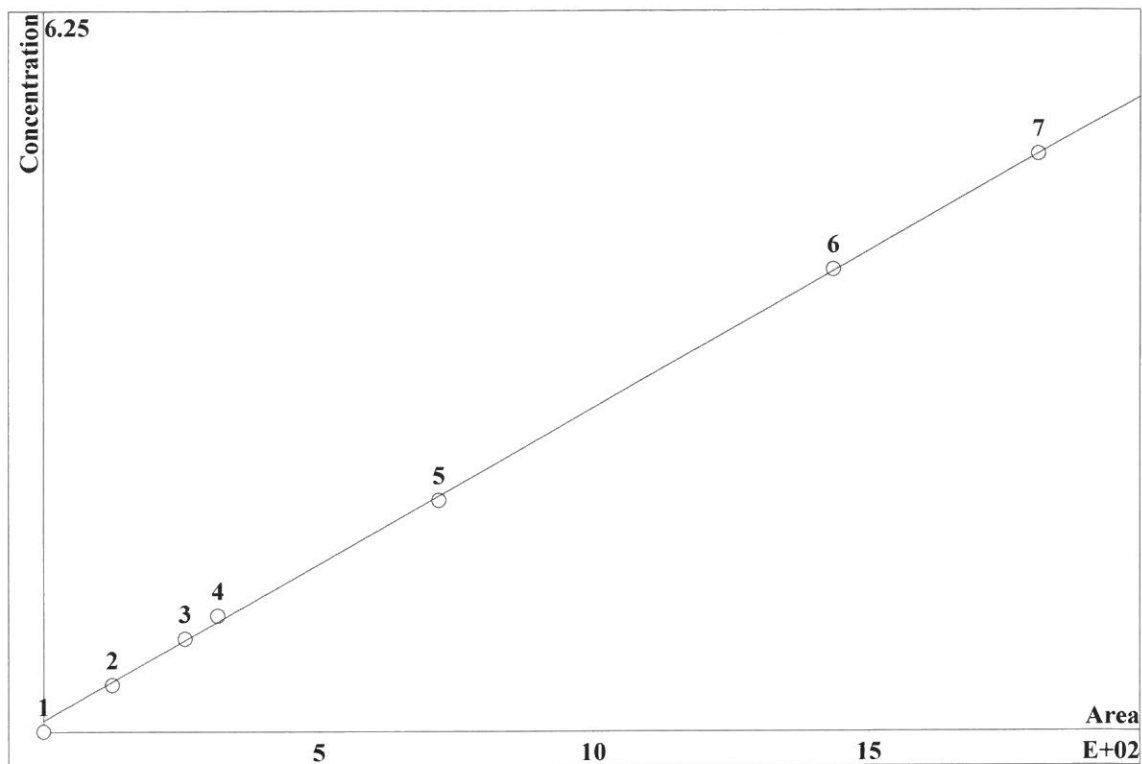


K3 = 0 K2 = 0 K1 = 0.0542483 K0 = 1.82974

Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1		0	0	0	0		0
2	5.701	125.1	0.4	20	5.653		
3	13.76	257.5	0.8	20	5.653		
4	16.31	316.4	1	20	5.653		
5	37.39	718.3	2	20	5.653		
6	81.72	1436	4	20	5.653		
7	102.8	1811	5	20	5.653		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-051922.mtw
 Equation: $Q = 0.0941016 \cdot A + 0.885368$
 RSD: 1.104 %
 Correlation coefficient: 0.999934

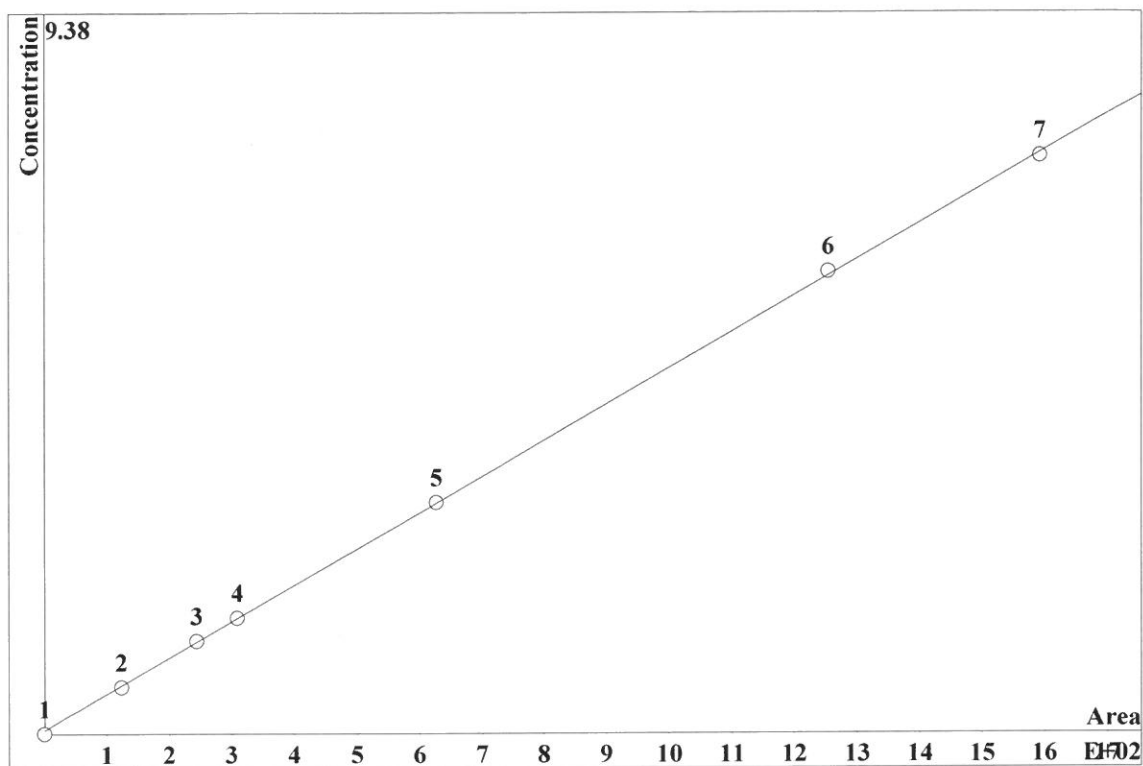


K3 = 0 K2 = 0 K1 = 0.0941016 K0 = 0.885368
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	8.8	123.6	0.6	20	8.643		
3	17.89	244	1.2	20	8.643		
4	21.99	309.1	1.5	20	8.643		
5	45.61	626.3	3	20	8.643		
6	93.42	1255	6	20	8.643		
7	118.4	1594	7.5	20	8.643		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-051922.mtw
 Equation: $Q = 0.0438456 \cdot A + 0.934942$
 RSD: 0.958 %
 Correlation coefficient: 0.999950

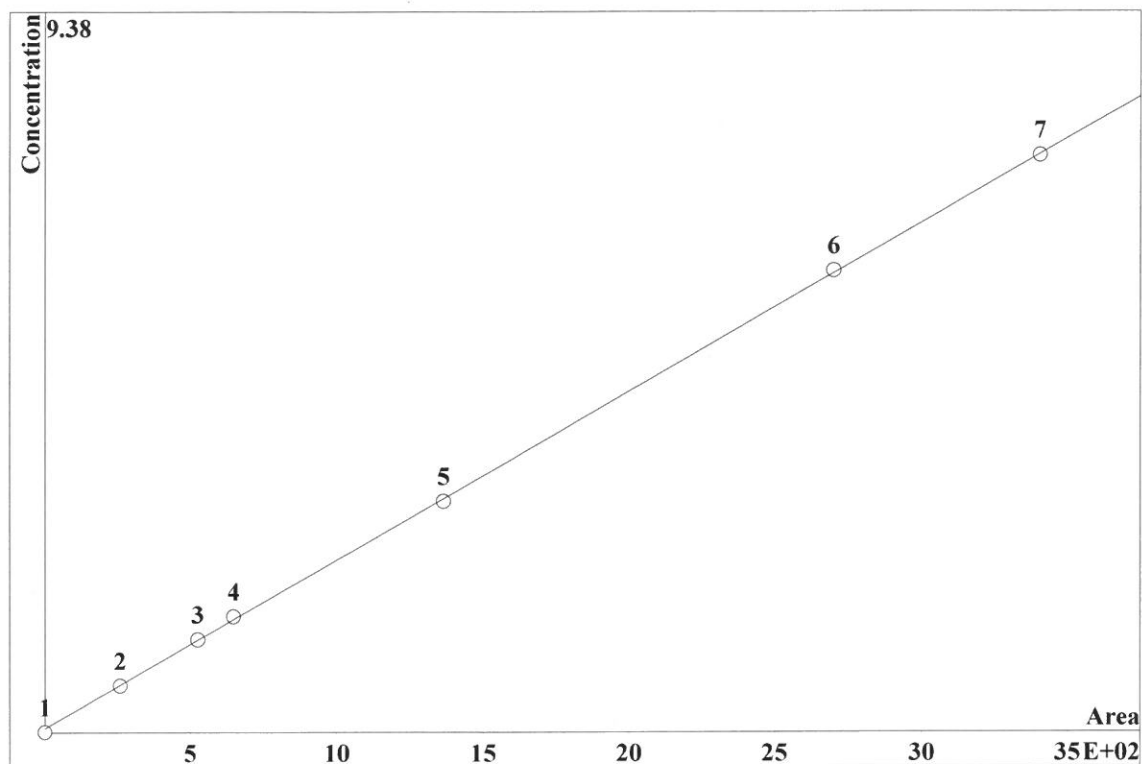

K3 = 0 K2 = 0 K1 = 0.0438456 K0 = 0.934942

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1		0	0	0	0		0
2	15.74	258.5	0.6	20	10.45		
3	32.1	525.4	1.2	20	10.45		
4	38.71	647.7	1.5	20	10.45		
5	80.75	1364	3	20	10.45		
6	156.3	2701	6	20	10.45		
7	190.5	3407	7.5	20	10.45		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-051922.mtw
 Equation: $Q = 0.220573 \cdot A - 34.7134$
 RSD: 3.089 %
 Correlation coefficient: 0.999480

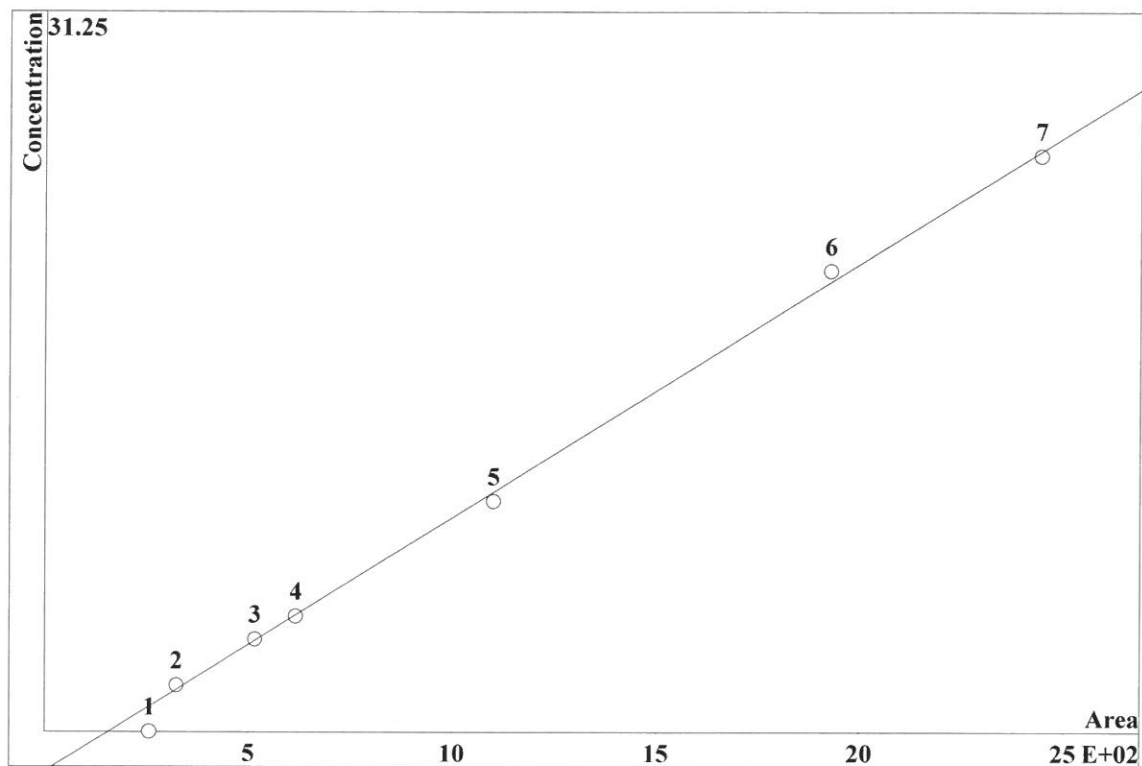


K3 = 0 K2 = 0 K1 = 0.220573 K0 = -34.7134
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	2.328	256.6		0	20		13.53
2	10.32	322.9		2	20		13.53
3	19.61	516.3		4	20		13.53
4	24.14	617.7		5	20		13.53
5	48.05	1101		10	20		13.53
6	93.59	1929		20	20		13.53
7	117.1	2442		25	20		13.53

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-051922.mtw
 Equation: $Q = 0.0372514 \cdot A + 0.553794$
 RSD: 0.845 %
 Correlation coefficient: 0.999961

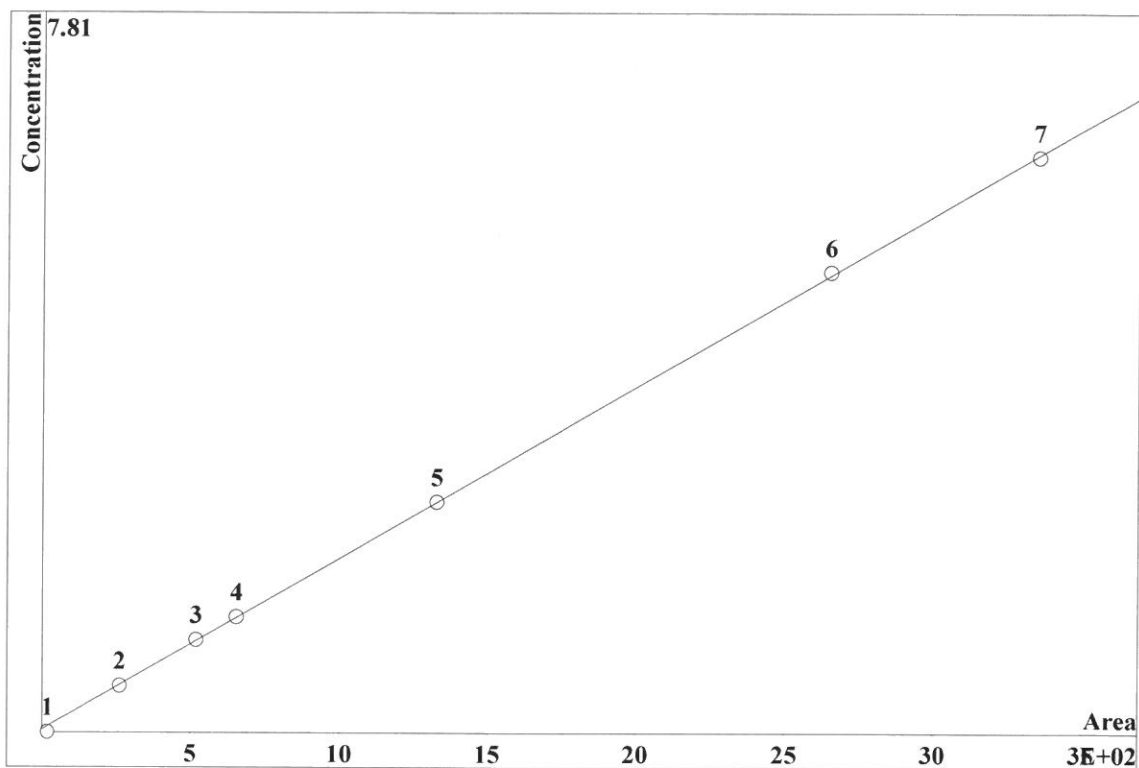


K3 = 0 K2 = 0 K1 = 0.0372514 K0 = 0.553794
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0.5352	19.92		0	20		15.58
2	10.86	262.9		0.5	20		15.58
3	22.12	518.6		1	20		15.58
4	27.45	654.4		1.25	20		15.58
5	56.73	1327		2.5	20		15.58
6	114.4	2652		5	20		15.58
7	144.8	3355		6.25	20		15.58

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-051922.mtw
 Equation: $Q = 0.0519897 \cdot A - 19.1596$
 RSD: 7.958 %
 Correlation coefficient: 0.996542

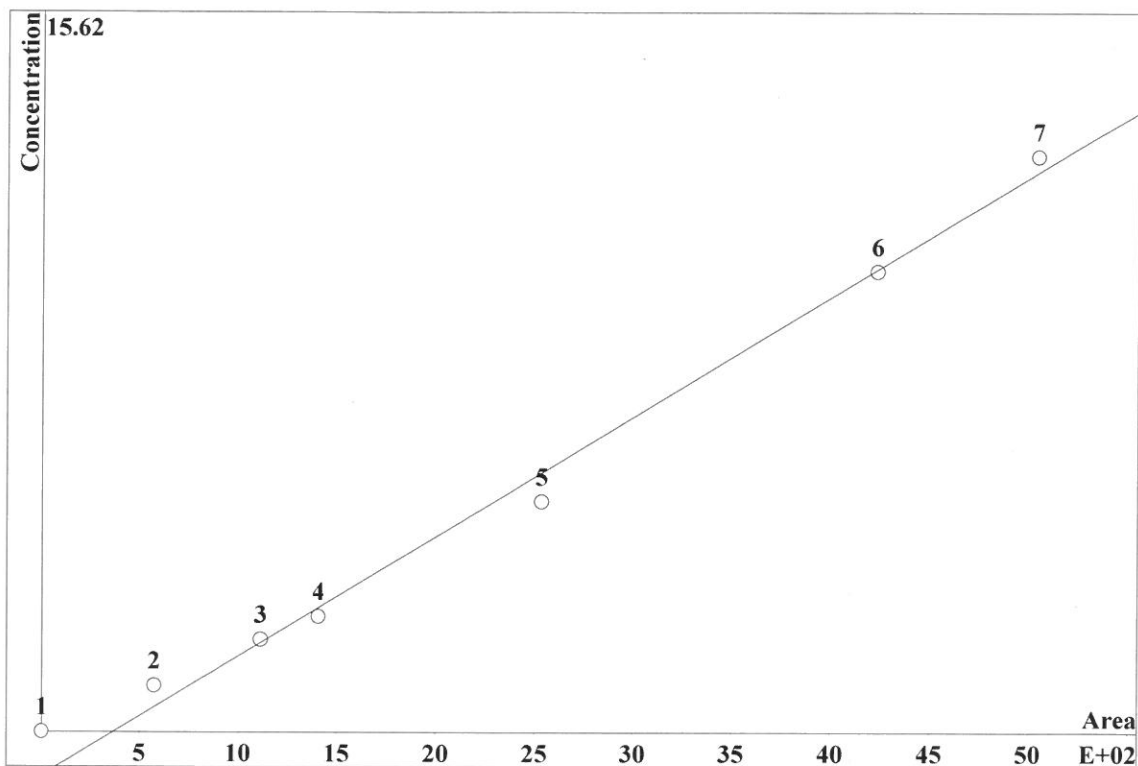


K3 = 0 K2 = 0 K1 = 0.0519897 K0 = -19.1596
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	12.75	576.1	1	20	20.18		
3	26.27	1112	2	20	20.18		
4	33.61	1405	2.5	20	20.18		
5	64.64	2533	5	20	20.18		
6	115.8	4234	10	20	20.18		
7	140.6	5045	12.5	20	20.18		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-051922.mtw
 Equation: $Q = 0.123626 \cdot A - 71.0066$
 RSD: 1.636 %
 Correlation coefficient: 0.999854

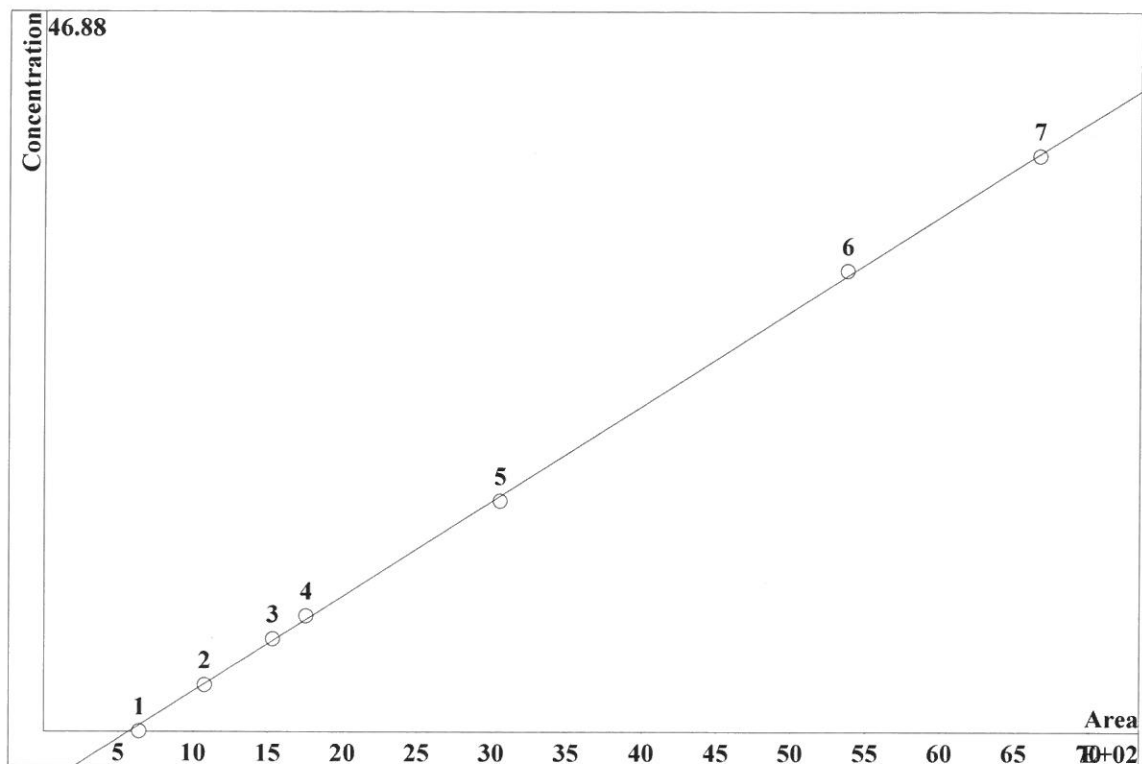

K3 = 0 K2 = 0 K1 = 0.123626 K0 = -71.0066

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	17.37	639.8	0	20	23.09		
2	30.98	1077	3	20	23.09		
3	46.25	1532	6	20	23.09		
4	53.99	1754	7.5	20	23.09		
5	96.8	3056	15	20	23.09		
6	181.5	5378	30	20	23.09		
7	226.3	6665	37.5	20	23.09		

Report date: 5/20/2022 11:04:50 AM
Printed by: wet


Ident: STD1
Analysis from: 5/19/2022 2:22:31 PM
File: _2022-05-19_

Last save: 5/20/2022 9:38:25 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30414

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

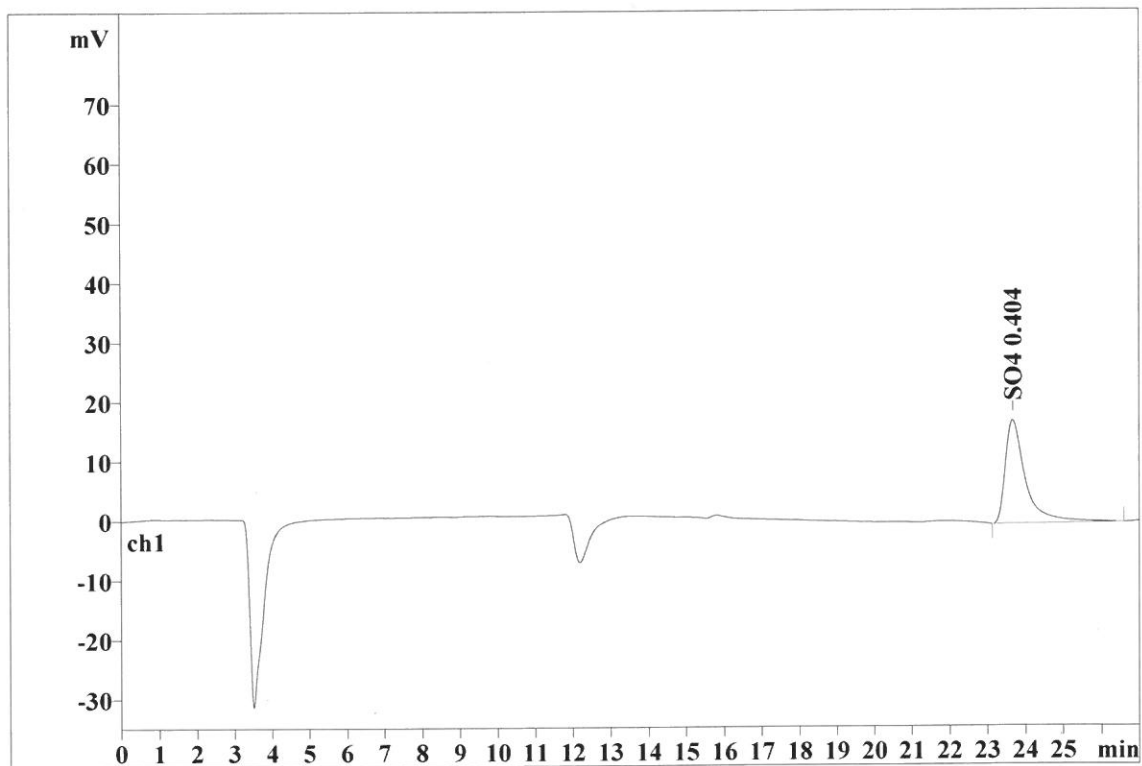

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	23.68	0.498	17.37	99.99	639.772	100.00
7	27.00	0.071	17.37	99.99	639.772	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:05:04 AM
Printed by: wet


Ident: STD2
Analysis from: 5/19/2022 2:52:09 PM
File: _2022-05-19_

Last save: 5/20/2022 9:16:52 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30415

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

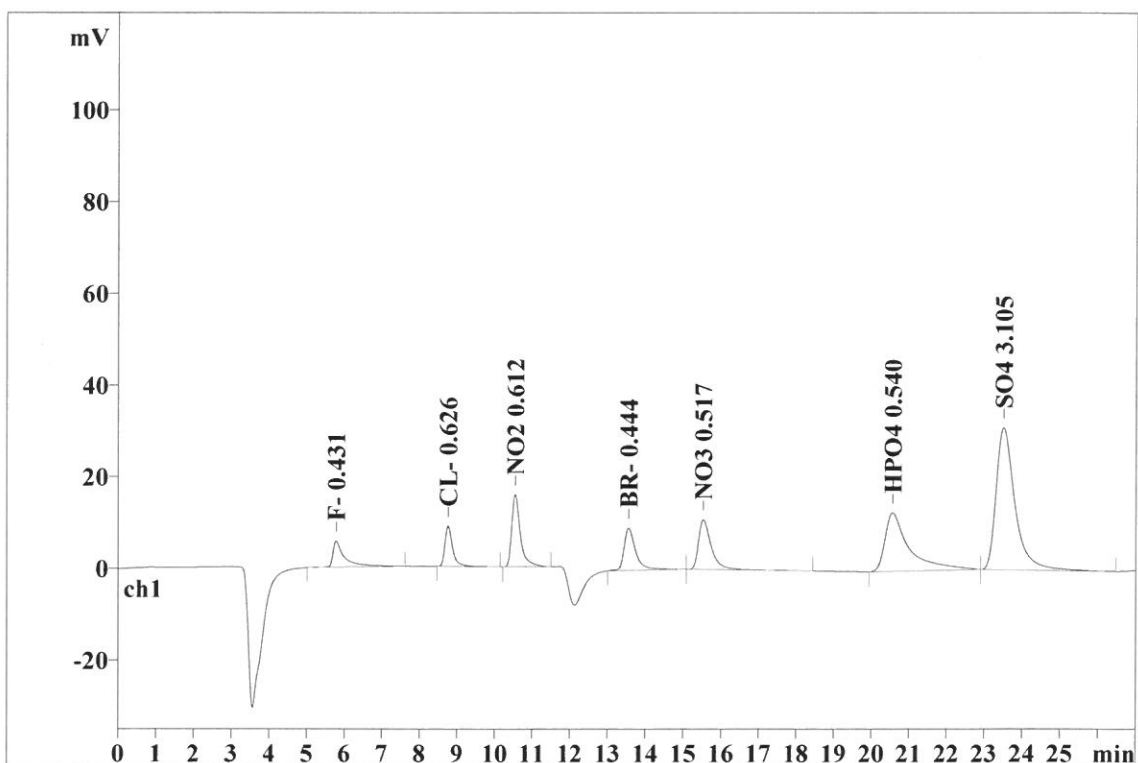

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.78	0.245	5.70	6.06	125.129	4.78
2	8.76	0.197	8.80	9.35	123.646	4.72
3	10.55	0.231	15.74	16.73	258.020	9.85
4	13.56	0.296	9.23	9.81	197.624	7.54
5	15.53	0.342	10.86	11.54	262.850	10.03
6	20.56	0.560	12.75	13.55	576.133	21.99
7	23.52	0.498	30.98	32.94	1076.702	41.09
7	27.00	0.338	94.06	100.00	2620.104	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:05:13 AM
Printed by: wet


Ident: STD3
Analysis from: 5/19/2022 3:21:47 PM
File: _2022-05-19_

Last save: 5/20/2022 9:16:52 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30416

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

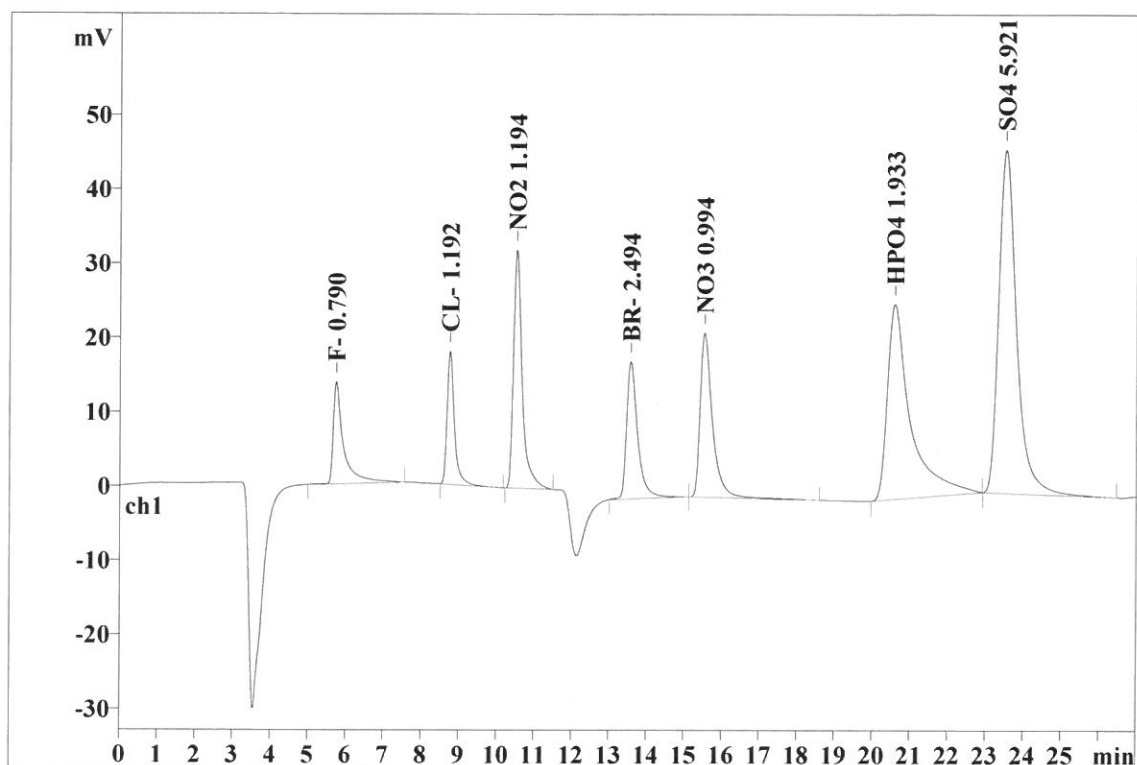

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.75	0.217	13.76	7.78	257.510	5.63
2	8.75	0.193	17.89	10.12	244.036	5.34
3	10.53	0.230	32.08	18.14	523.182	11.45
4	13.58	0.296	18.47	10.45	383.505	8.39
5	15.54	0.335	22.12	12.51	518.591	11.34
6	20.59	0.533	26.27	14.85	1112.134	24.33
7	23.52	0.479	46.25	26.15	1532.301	33.52
7	27.00	0.326	176.84	100.00	4571.259	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:05:22 AM
Printed by: wet


Ident: STD4
Analysis from: 5/19/2022 3:51:25 PM
File: _2022-05-19_

Last save: 5/20/2022 9:16:52 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30417

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

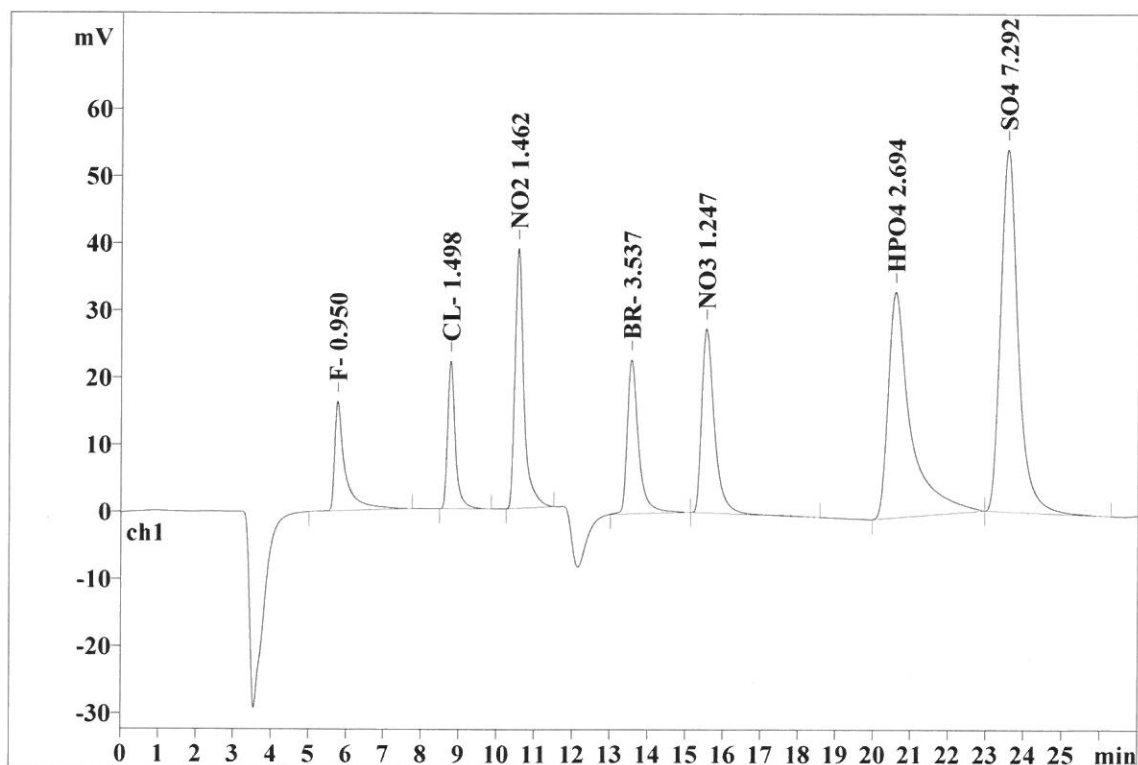

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.76	0.224	16.31	7.59	316.406	5.69
2	8.77	0.200	21.99	10.23	309.071	5.56
3	10.55	0.236	38.69	18.00	645.471	11.60
4	13.55	0.294	22.94	10.67	478.126	8.60
5	15.53	0.345	27.45	12.77	654.376	11.76
6	20.57	0.529	33.61	15.63	1404.978	25.26
7	23.55	0.474	53.99	25.12	1754.100	31.53
7	27.00	0.329	214.97	100.00	5562.528	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:05:30 AM
Printed by: wet


Ident: STD5
Analysis from: 5/19/2022 4:21:03 PM
File: _2022-05-19_

Last save: 5/20/2022 9:16:52 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30418

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

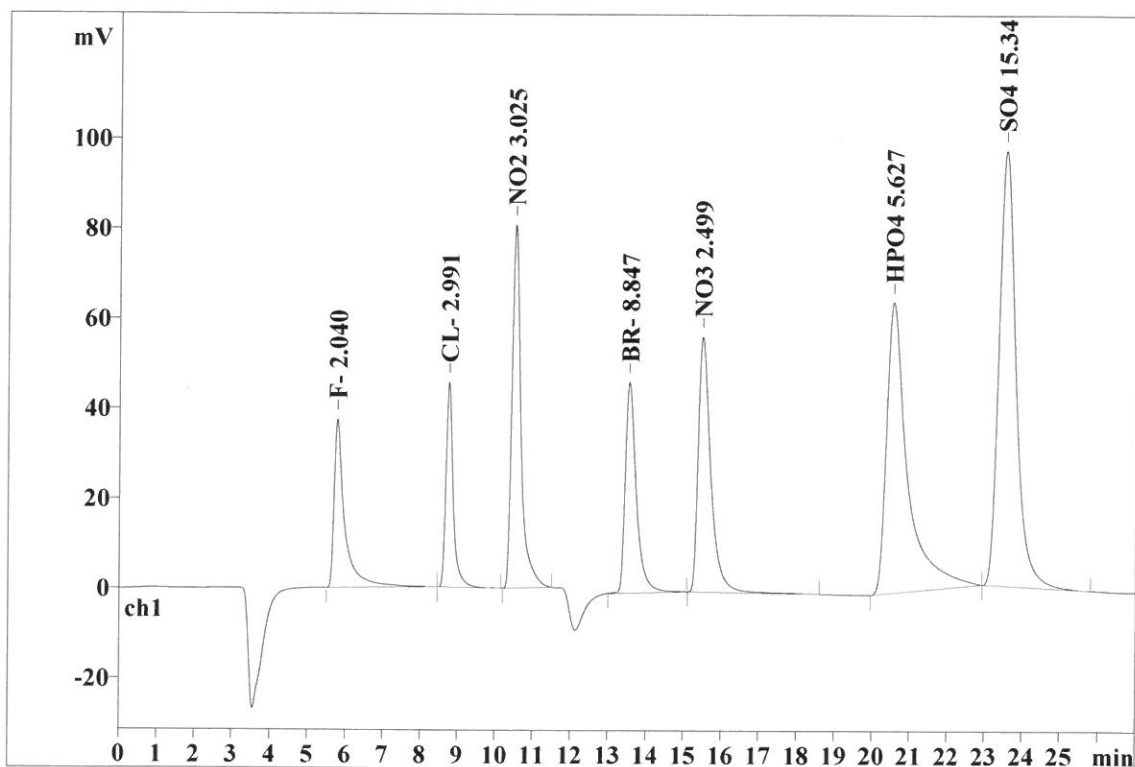

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.78	0.226	37.39	8.72	718.265	6.79
2	8.75	0.194	45.61	10.64	626.259	5.92
3	10.52	0.237	80.72	18.83	1358.313	12.84
4	13.56	0.297	46.82	10.92	959.568	9.07
5	15.49	0.337	56.73	13.23	1326.660	12.54
6	20.55	0.504	64.64	15.08	2533.013	23.95
7	23.54	0.466	96.80	22.58	3056.161	28.89
7	27.00	0.323	428.70	100.00	10578.238	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:05:39 AM
Printed by: wet


Ident: STD6
Analysis from: 5/19/2022 4:50:40 PM
File: _2022-05-19_

Last save: 5/20/2022 9:16:52 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30419

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

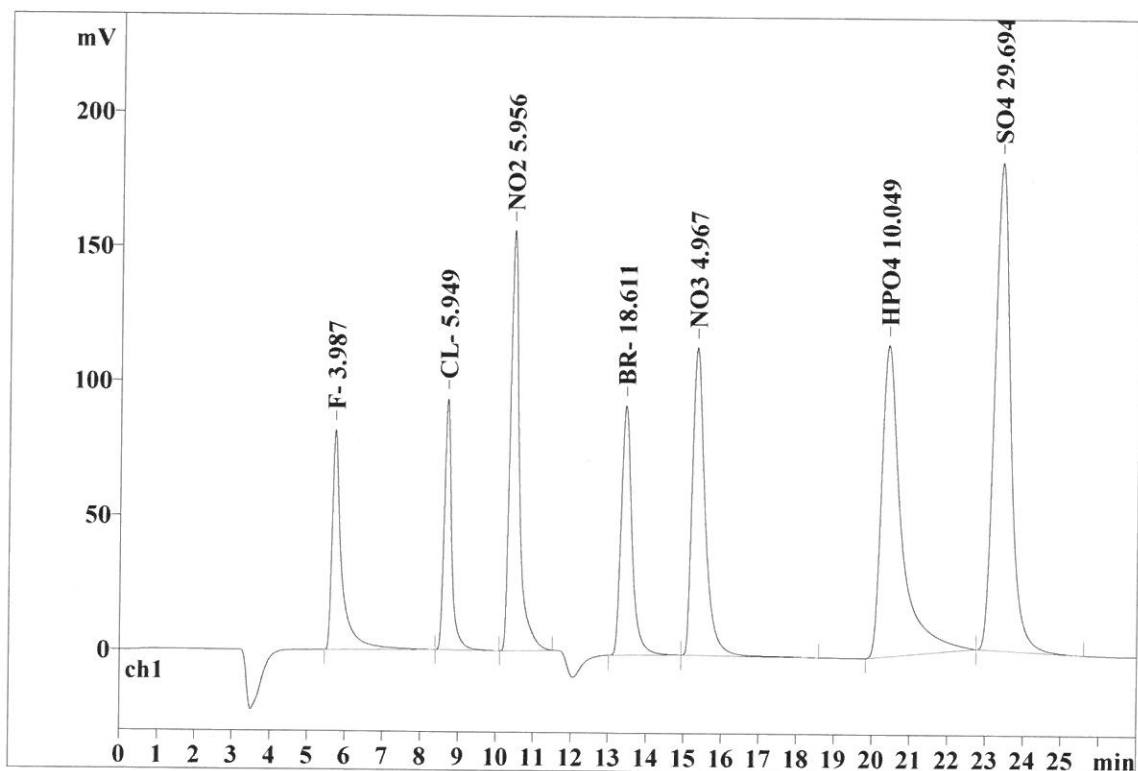

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.212	81.72	9.78	1436.321	7.37
2	8.67	0.190	93.42	11.18	1254.944	6.44
3	10.42	0.245	156.22	18.69	2695.316	13.83
4	13.42	0.292	92.77	11.10	1844.846	9.46
5	15.30	0.335	114.39	13.69	2651.913	13.60
6	20.39	0.478	115.79	13.85	4234.269	21.72
7	23.35	0.440	181.50	21.71	5378.245	27.59
7	27.00	0.313	835.81	100.00	19495.853	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:05:47 AM
Printed by: wet


Ident: STD7
Analysis from: 5/19/2022 5:20:19 PM
File: _2022-05-19_

Last save: 5/20/2022 9:18:02 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30420

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

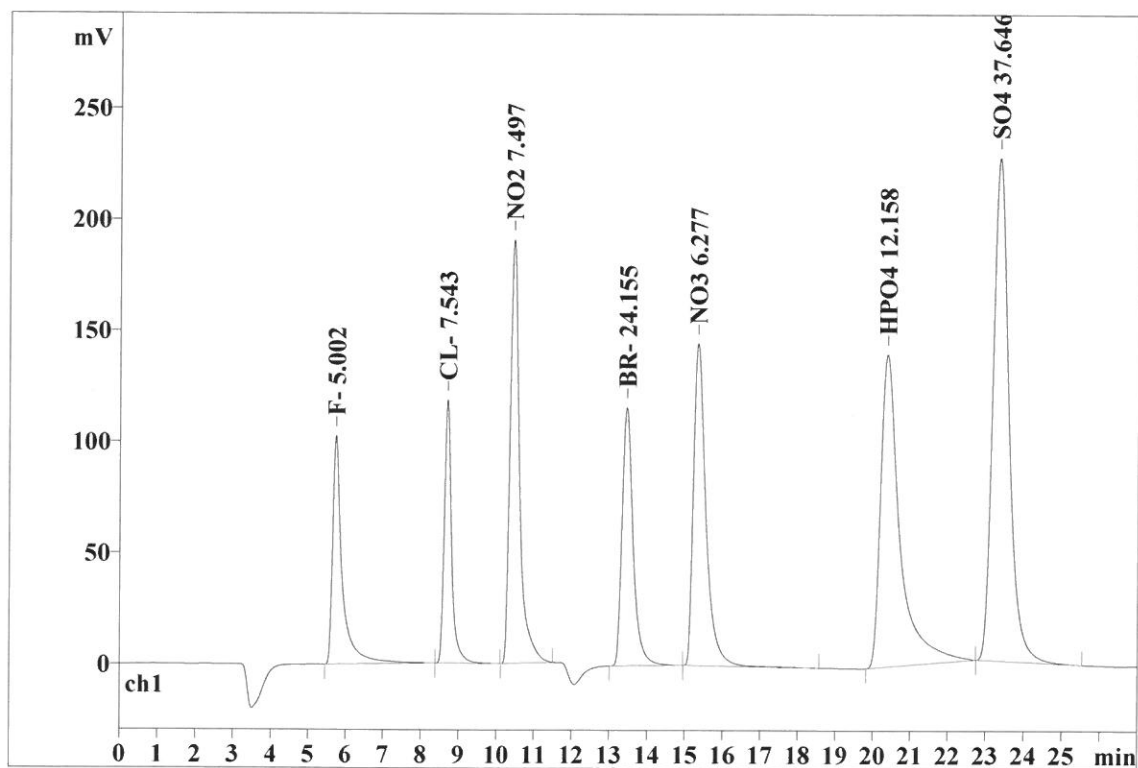

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.73	0.214	102.76	9.89	1810.504	7.48
2	8.69	0.190	118.37	11.39	1593.808	6.58
3	10.44	0.255	190.47	18.32	3398.408	14.03
4	13.45	0.297	116.15	11.17	2347.601	9.69
5	15.32	0.336	144.81	13.93	3355.137	13.86
6	20.37	0.473	140.55	13.52	5045.473	20.84
7	23.34	0.439	226.29	21.77	6664.685	27.52
7	27.00	0.315	1039.41	100.00	24215.617	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:05:56 AM
Printed by: wet


Ident: ICV
Analysis from: 5/19/2022 5:49:57 PM
File: _2022-05-19_

Last save: 5/20/2022 9:18:03 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30421

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

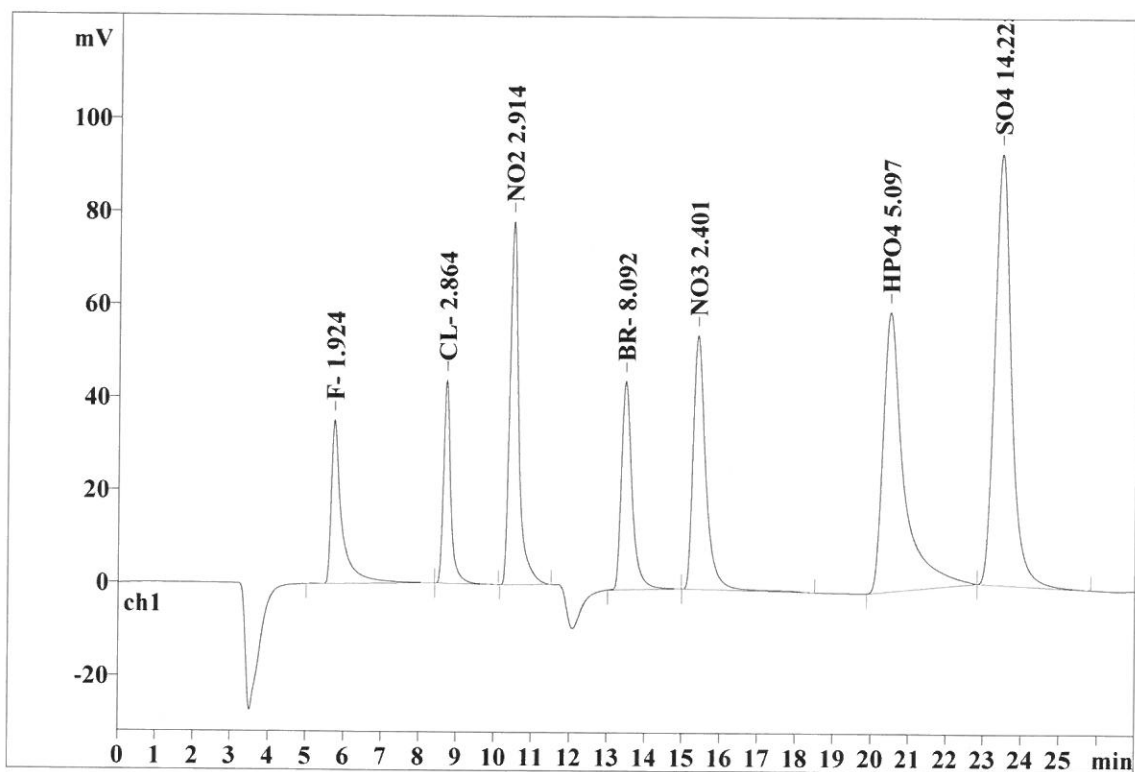

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.74	0.225	35.20	8.59	675.573	6.79
2	8.70	0.194	43.77	10.68	599.271	6.02
3	10.47	0.236	78.25	19.09	1307.665	13.14
4	13.46	0.288	44.91	10.96	891.091	8.95
5	15.38	0.335	54.64	13.33	1274.230	12.80
6	20.47	0.498	60.23	14.69	2329.166	23.40
7	23.43	0.456	92.92	22.67	2875.593	28.89
7	27.00	0.319	409.92	100.00	9952.591	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:06:07 AM
Printed by: wet


Ident: ICB
Analysis from: 5/19/2022 6:19:35 PM
File: _2022-05-19_

Last save: 5/20/2022 9:39:35 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30422

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 10
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

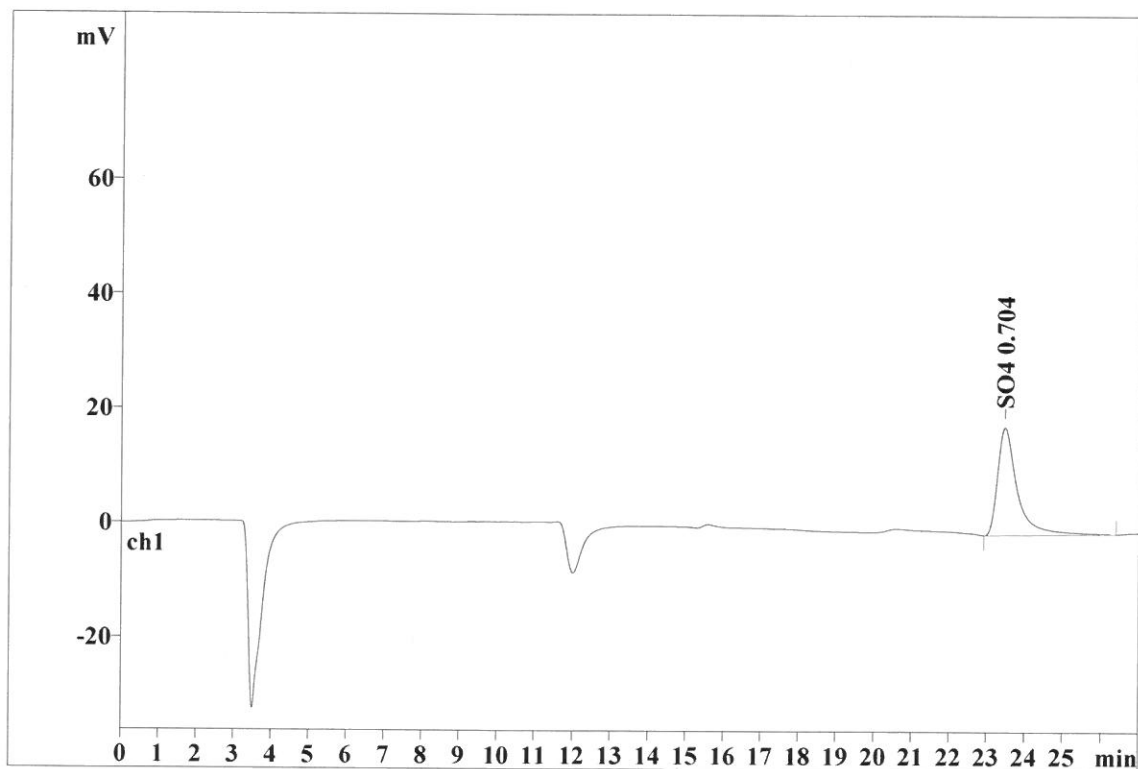

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	23.46	0.497	18.81	99.99	688.220	100.00
7	27.00	0.071	18.81	99.99	688.220	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:06:17 AM
Printed by: wet


Ident: CCV
Analysis from: 5/19/2022 6:49:12 PM
File: _2022-05-19_

Last save: 5/20/2022 9:18:03 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30423

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

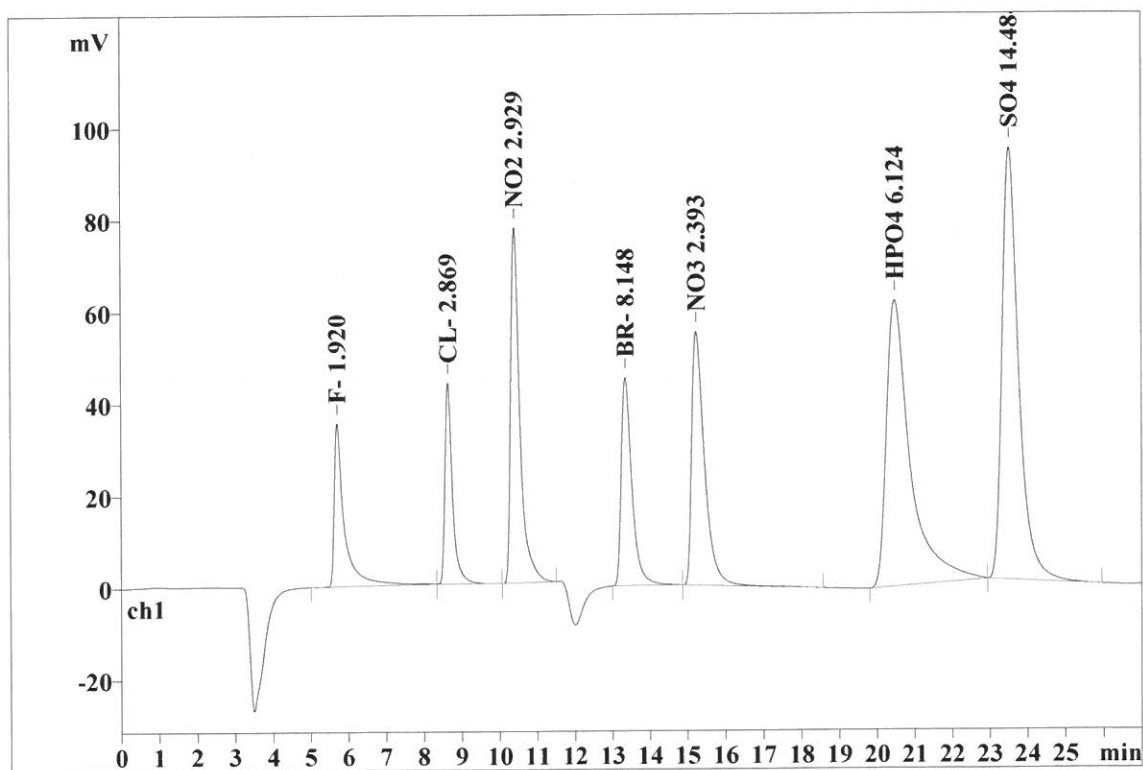

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.71	0.220	35.50	8.59	674.202	6.48
2	8.65	0.194	43.74	10.58	600.429	5.77
3	10.41	0.240	77.35	18.71	1314.707	12.64
4	13.36	0.287	45.29	10.96	896.147	8.62
5	15.25	0.333	55.21	13.36	1269.792	12.21
6	20.49	0.579	62.31	15.08	2724.421	26.20
7	23.54	0.456	93.93	22.73	2917.551	28.06
7	27.00	0.330	413.33	100.00	10397.249	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:06:33 AM
Printed by: wet


Ident: CCB
Analysis from: 5/19/2022 7:18:50 PM
File: _2022-05-19_

Last save: 5/20/2022 9:39:50 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30424

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

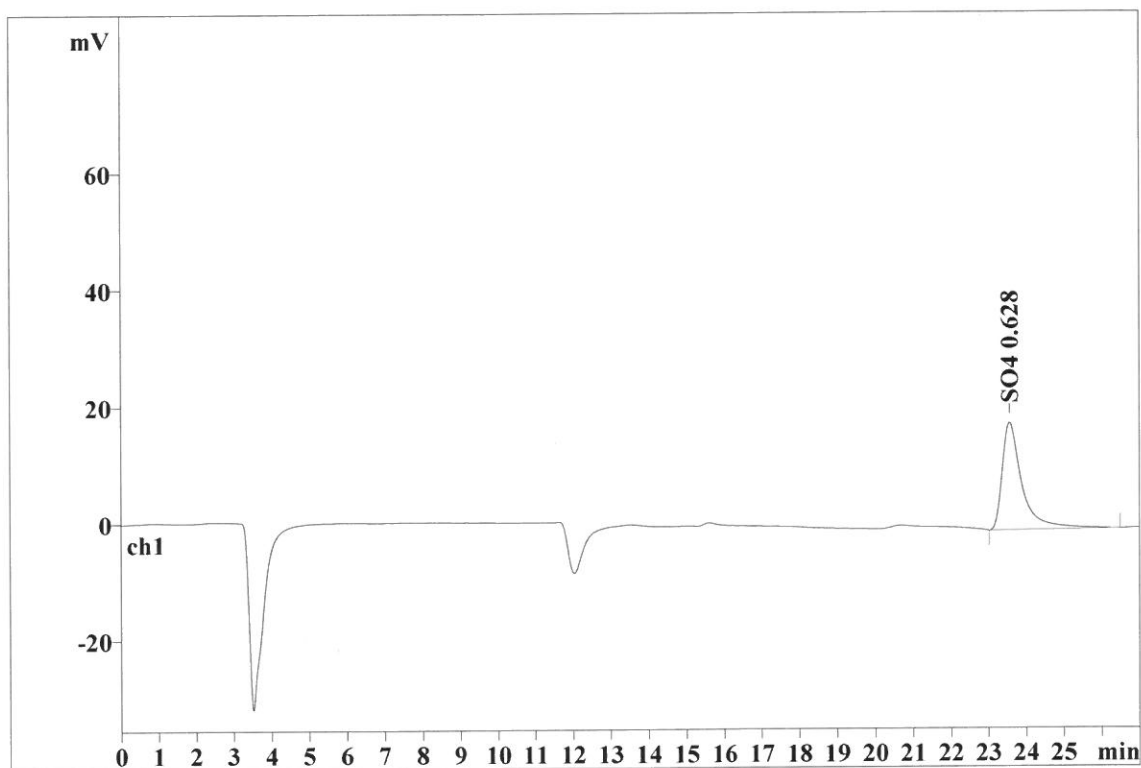

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	23.57	0.500	18.36	99.99	676.015	100.00
7	27.00	0.071	18.36	99.99	676.015	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:06:40 AM
Printed by: wet


Ident: LB120263BLW
Analysis from: 5/19/2022 7:48:28 PM
File: _2022-05-19_

Last save: 5/20/2022 9:40:03 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30425

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

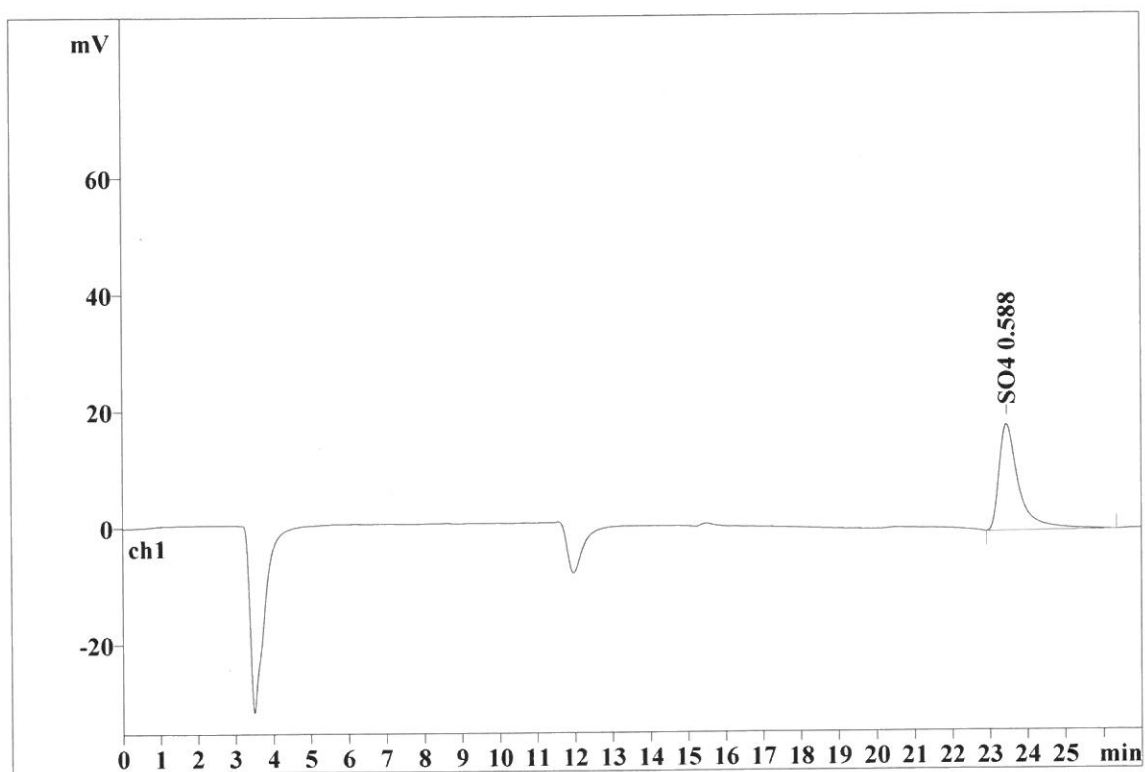

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	23.45	0.499	18.21	100.00	669.463	100.00
7	27.00	0.071	18.21	100.00	669.463	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:06:49 AM
Printed by: wet


Ident: LB120263BSW
Analysis from: 5/19/2022 8:18:06 PM
File: _2022-05-19_

Last save: 5/20/2022 9:18:03 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30426

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

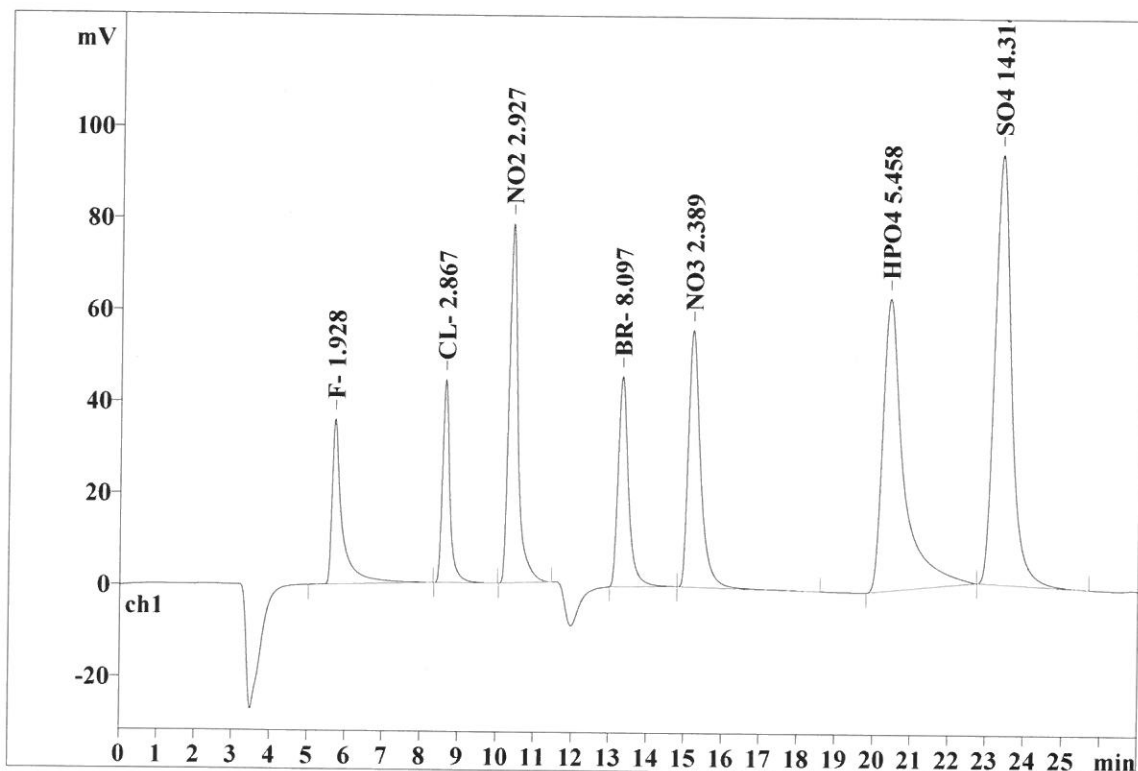

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.71	0.219	35.93	8.60	677.059	6.70
2	8.63	0.192	44.27	10.60	599.973	5.94
3	10.38	0.238	78.27	18.74	1313.734	13.00
4	13.31	0.284	45.78	10.96	891.562	8.82
5	15.18	0.329	55.97	13.40	1267.555	12.54
6	20.40	0.499	63.71	15.25	2468.250	24.42
7	23.35	0.455	93.73	22.44	2890.065	28.59
7	27.00	0.316	417.66	100.00	10108.199	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:10:04 AM
Printed by: wet


Ident: N2946-03
Analysis from: 5/19/2022 8:47:44 PM
File: _2022-05-19_

Last save: 5/20/2022 9:40:31 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30427

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

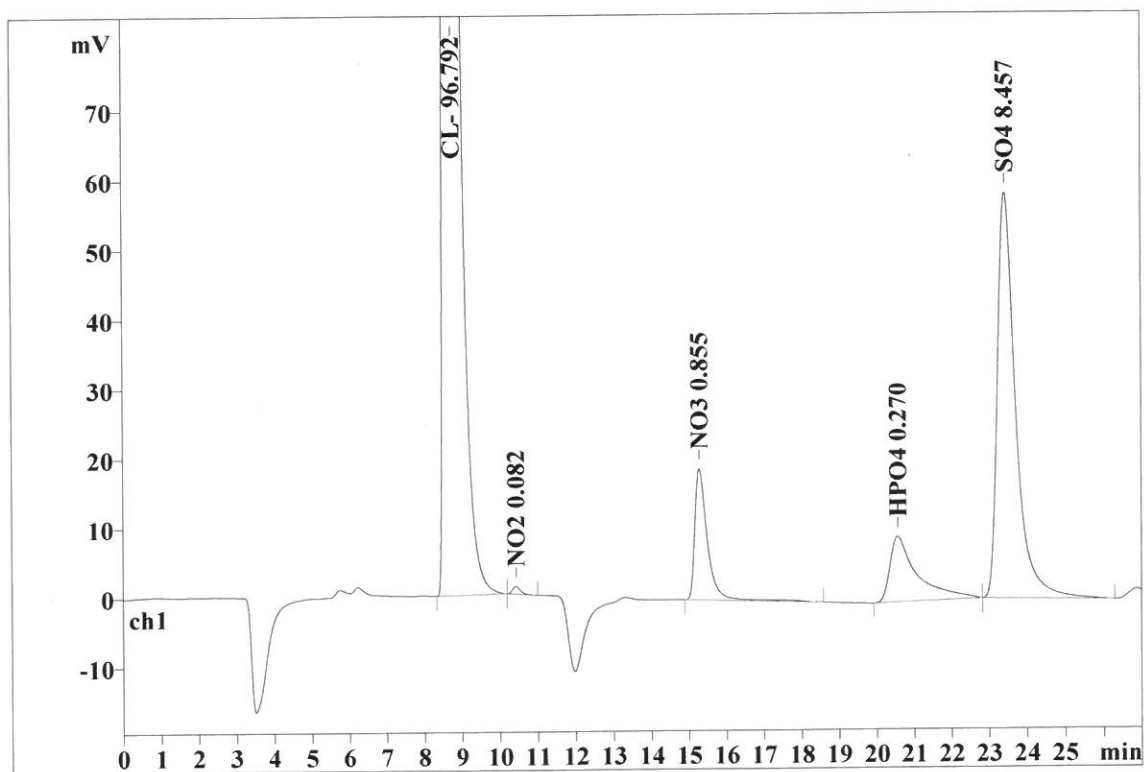

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.74	0.239	1271.50	93.55	20562.348	87.73
3	10.43	0.221	1.09	0.08	15.941	0.07
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.29	0.328	18.84	1.39	444.401	1.90
6	20.57	0.621	9.39	0.69	472.470	2.02
7	23.45	0.475	58.33	4.29	1942.467	8.29
7	27.00	0.269	1359.15	100.00	23437.627	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:10:14 AM
Printed by: wet


Ident: N2946-03MS
Analysis from: 5/19/2022 9:17:22 PM
File: _2022-05-19_

Last save: 5/20/2022 9:18:03 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30428

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 16
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

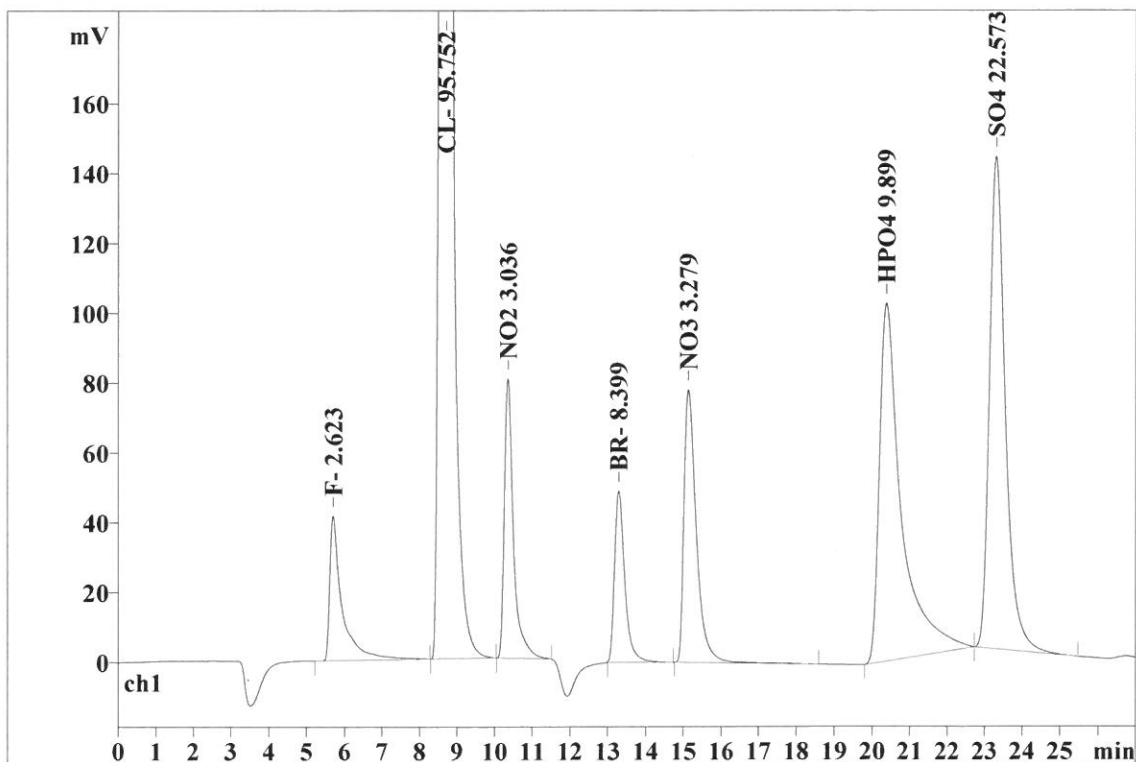

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.70	0.257	41.45	2.35	933.283	2.77
2	8.70	0.237	1269.68	72.07	20341.275	60.35
3	10.35	0.238	80.00	4.54	1363.331	4.04
4	13.29	0.275	48.99	2.78	918.934	2.73
5	15.13	0.323	78.08	4.43	1745.760	5.18
6	20.37	0.518	102.55	5.82	4176.708	12.39
7	23.31	0.443	141.09	8.01	4226.216	12.54
7	27.00	0.327	1761.83	100.00	33705.507	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:10:28 AM
Printed by: wet


Ident: N2946-03MSD
Analysis from: 5/19/2022 9:47:00 PM
File: 2022-05-19

Last save: 5/20/2022 9:18:03 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30429

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 17
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

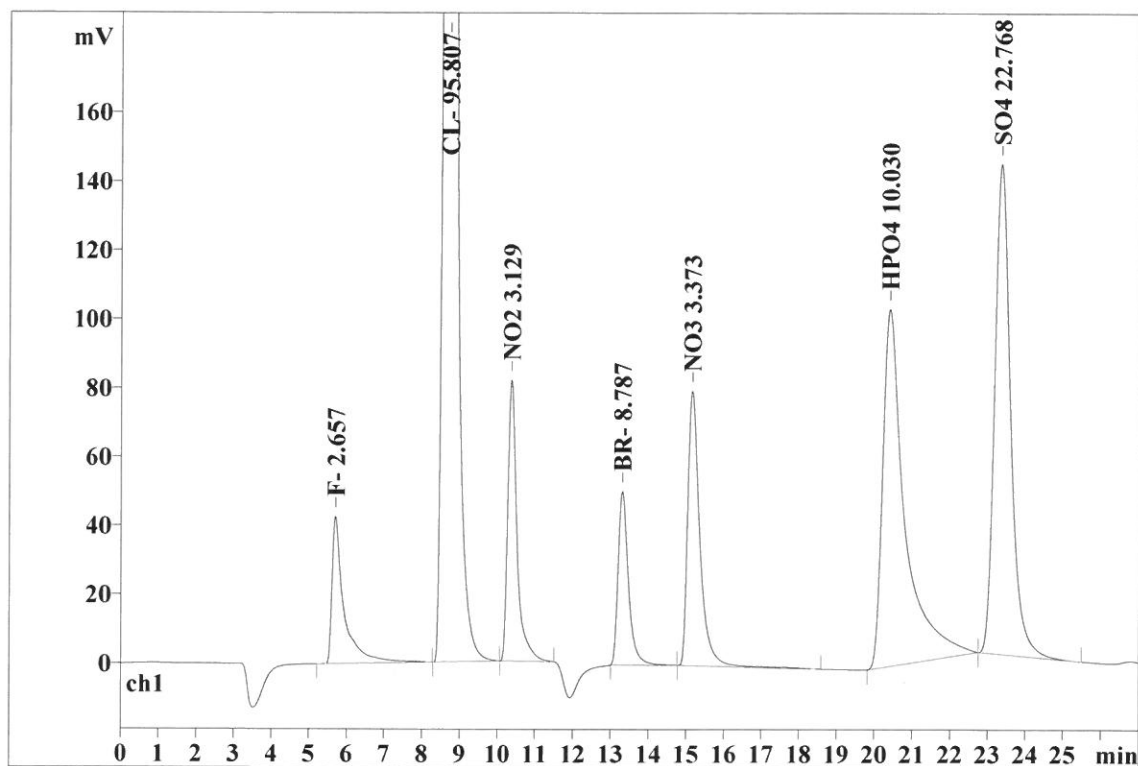

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.70	0.253	42.75	2.42	945.790	2.79
2	8.71	0.237	1269.60	71.73	20352.949	59.97
3	10.37	0.241	81.62	4.61	1406.062	4.14
4	13.30	0.276	50.41	2.85	954.131	2.81
5	15.15	0.324	79.67	4.50	1795.997	5.29
6	20.39	0.519	103.64	5.86	4226.815	12.45
7	23.34	0.443	142.33	8.04	4257.651	12.54
7	27.00	0.328	1770.01	100.00	33939.395	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:10:42 AM
Printed by: wet


Ident: CCV
Analysis from: 5/19/2022 10:16:41 PM
File: _2022-05-19_

Last save: 5/20/2022 9:18:03 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30430

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

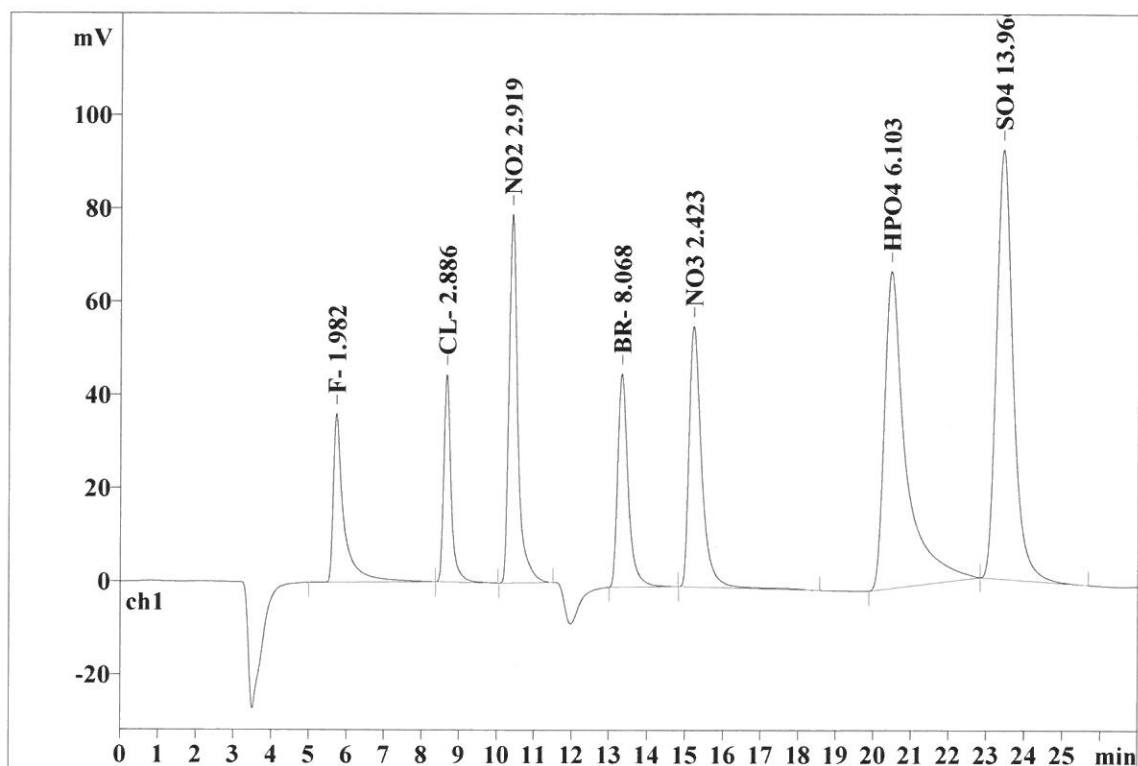

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.73	0.225	36.16	8.58	697.134	6.74
2	8.66	0.192	44.51	10.56	603.907	5.84
3	10.40	0.234	79.08	18.76	1310.312	12.68
4	13.33	0.283	45.73	10.85	888.911	8.60
5	15.21	0.329	55.92	13.26	1286.104	12.44
6	20.46	0.511	68.05	16.14	2716.436	26.28
7	23.43	0.454	92.16	21.86	2833.778	27.42
7	27.00	0.318	421.61	100.00	10336.582	100.00

This report has been created by IC Net
METROHM LTD

Report date: 5/20/2022 11:11:09 AM
Printed by: wet


Ident: CCB
Analysis from: 5/19/2022 10:46:18 PM
File: _2022-05-19_

Last save: 5/20/2022 9:41:31 AM

Method: AnionsIC2-051922.mtw
Run operator: wet
Analysis number: 30431

Last save: 5/19/2022 5:17:

SAMPLE:
: IZ/AP
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

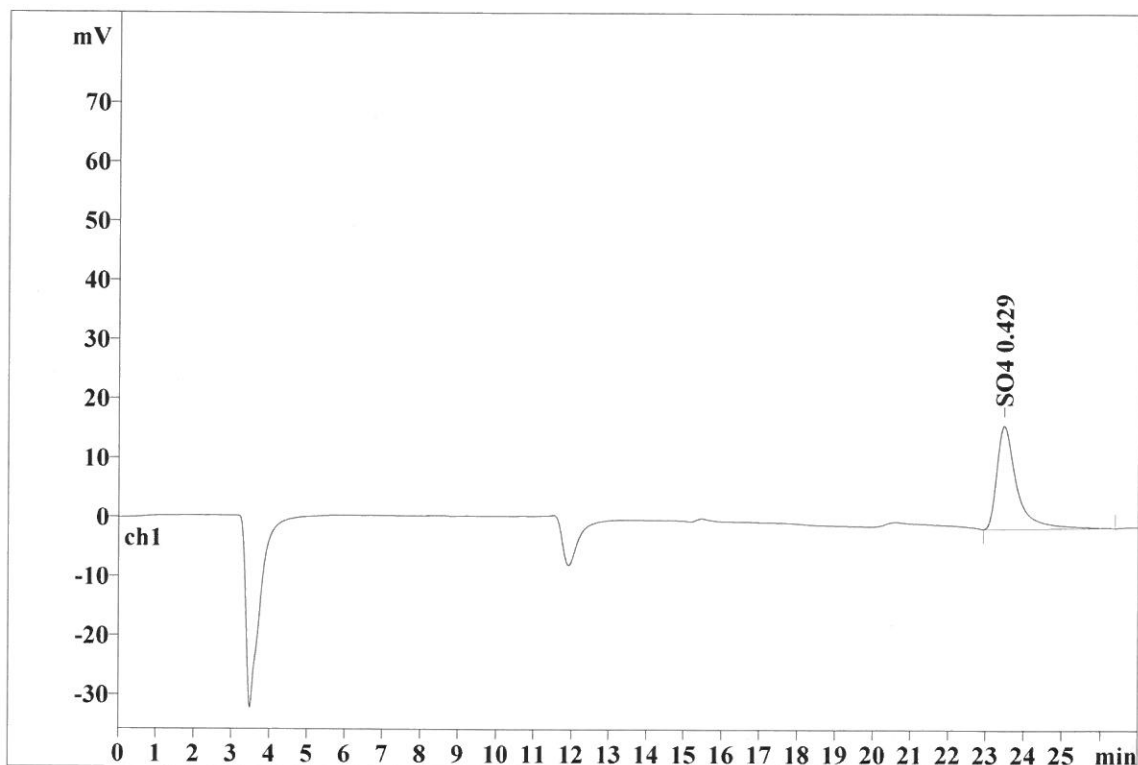

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	23.46	0.502	17.43	100.01	643.831	100.00
7	27.00	0.072	17.43	100.01	643.831	100.00

This report has been created by IC Net
METROHM LTD